

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011320\
 Data File : PS008393.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jan 2020 16:22
 Operator : DD\AJ
 Sample : PB126035BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 14 08:54:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.280	5.968	887.1E6	428.6E6	502.426	452.342
Target Compounds							
1) T	Dalapon	2.509	2.186	483.7E6	103.9E6	188.680	81.969 #
2) T	3,5-DICHL...	0.000	5.153	0	80154875	N.D.	57.369
7) T	MCPA	6.775	0.000	19293804	0	2.640	N.D. #
8) T	DICHLORPROP	0.000	6.789	0	14402199	N.D.	14.907
9) T	2,4-D	0.000	7.036	0	17300976	N.D.	14.759
10) T	Pentachlo...	7.765	7.486	49305992	13745706	2.028	1.018 #
11) T	2,4,5-TP ...	0.000	7.893	0	1529388	N.D.	<MDL
12) T	2,4,5-T	8.482	8.283	89283736	52695281	9.677	9.965
13) T	2,4-DB	9.070	0.000	27715107	0	19.993	N.D. #
14) T	DINOSEB	10.216	9.078	42208515	28412910	5.883	7.521 #
15) T	Picloram	10.063	10.054	427.5E6	243.8E6	34.251	32.822
16) T	DCPA	0.000	10.005	0	21047748	N.D.	3.230



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011320\
Data File : PS008393.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jan 2020 16:22
Operator : DD\AJ
Sample : PB126035BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 14 08:54:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

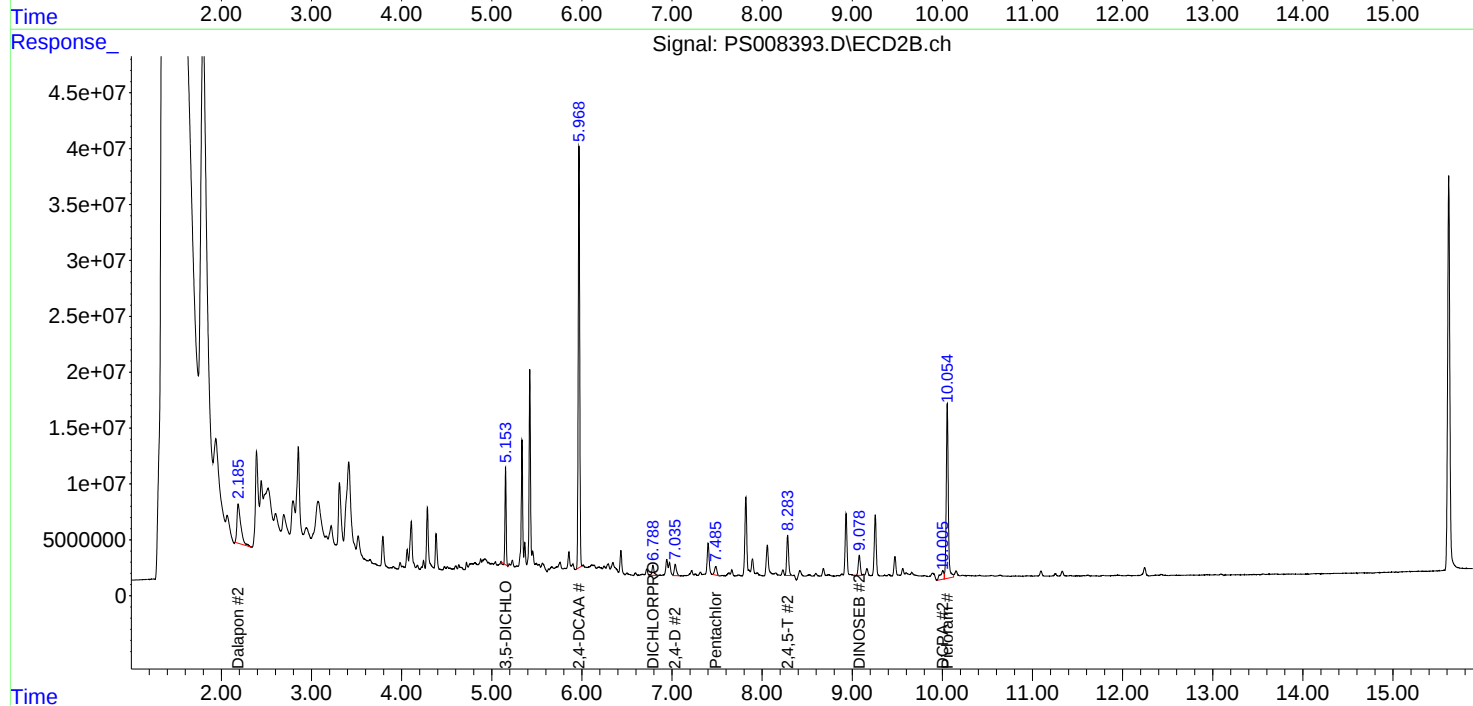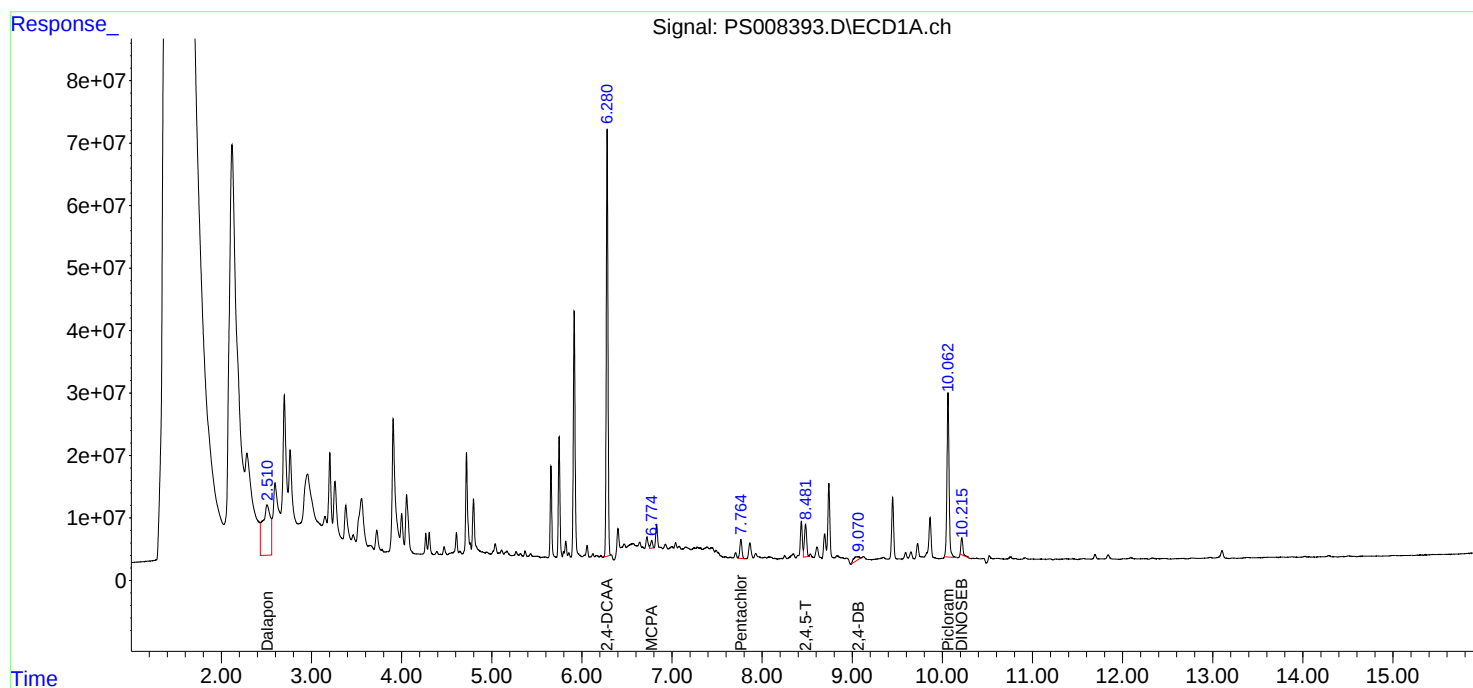


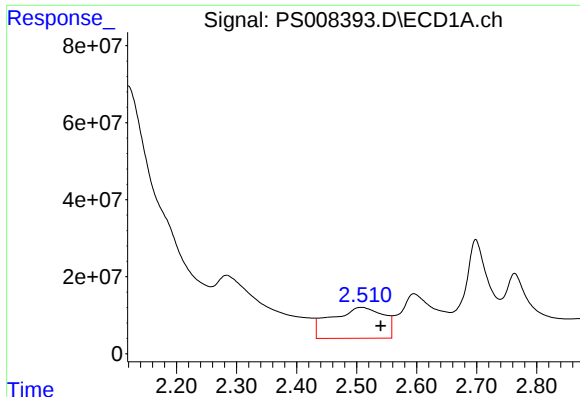

#1 Dalapon


R.T.: 2.509 min
Delta R.T.: -0.031 min
Response: 483746430
Conc: 188.68 ng/ml

Instrument :
ECD_O
ClientSampleId :

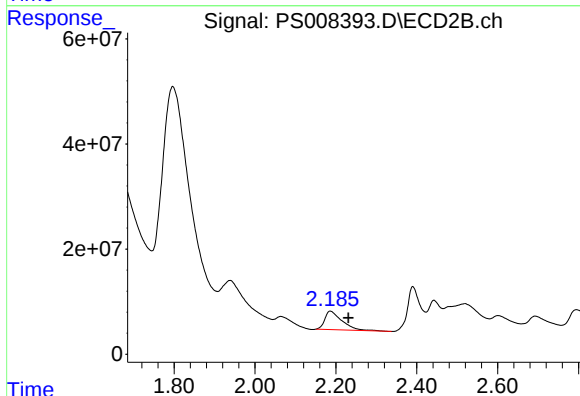


#1 Dalapon

R.T.: 2.186 min
Delta R.T.: -0.045 min
Response: 103915795
Conc: 81.97 ng/ml

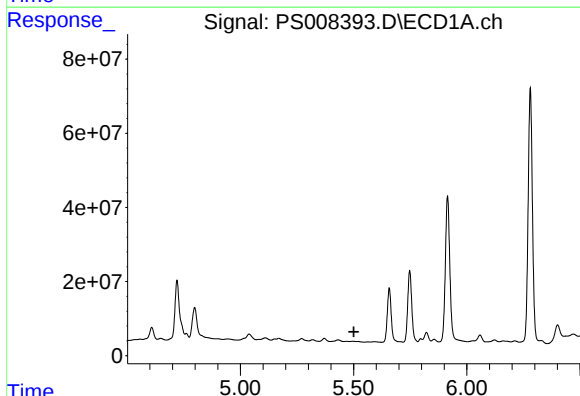


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

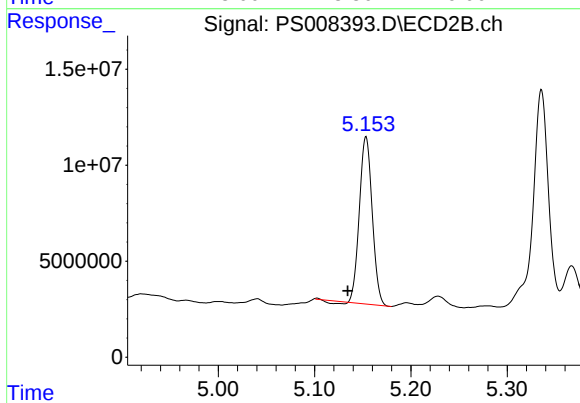

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.153 min
Delta R.T.: 0.019 min
Response: 80154875
Conc: 57.37 ng/ml

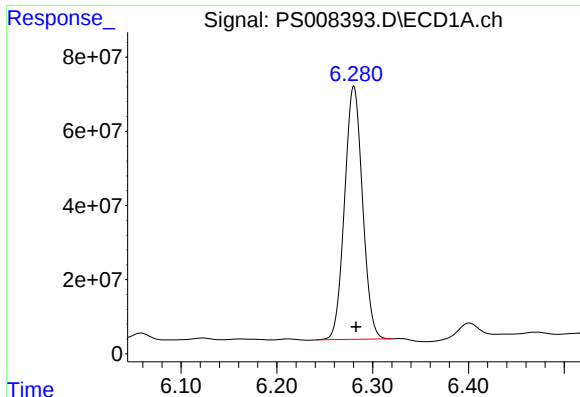

#4 2,4-DCAA


R.T.: 6.280 min
Delta R.T.: -0.002 min
Response: 887135310
Conc: 502.43 ng/ml

Instrument :
ECD_O
ClientSampleId :

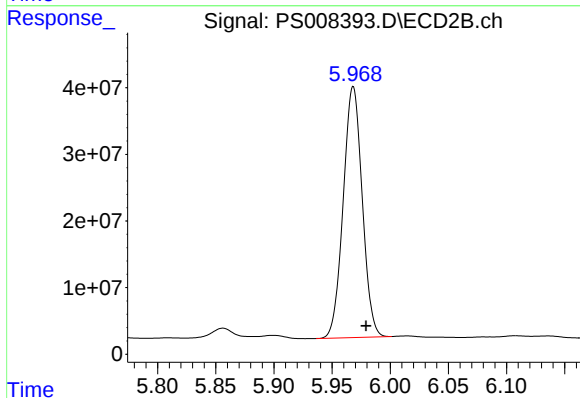


#4 2,4-DCAA

R.T.: 5.968 min
Delta R.T.: -0.011 min
Response: 428577288
Conc: 452.34 ng/ml

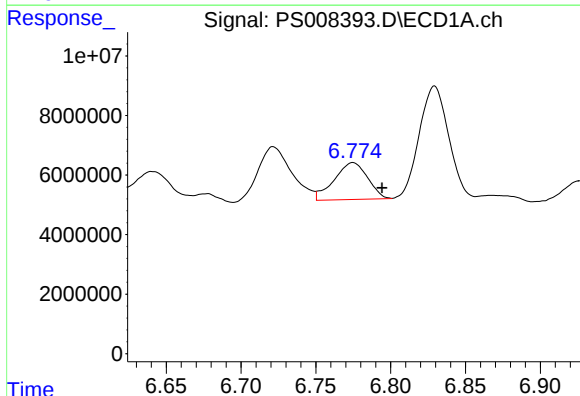


#7 MCPA

R.T.: 6.775 min
Delta R.T.: -0.019 min
Response: 19293804
Conc: 2.64 ug/ml

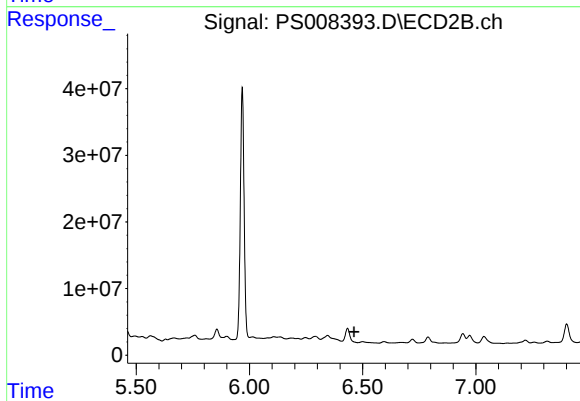

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.462 min
Response: 0
Conc: N.D.

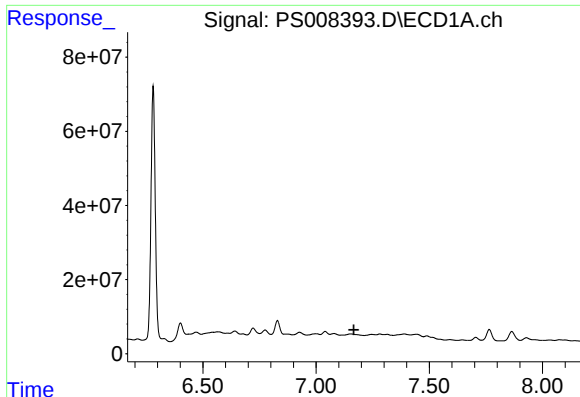

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.167 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

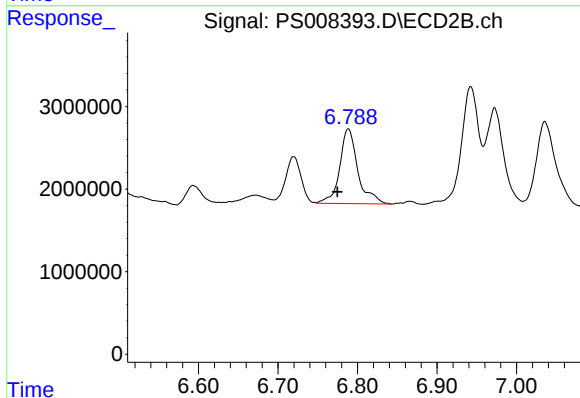


#8 DICHLORPROP

R.T.: 6.789 min
Delta R.T.: 0.014 min
Response: 14402199
Conc: 14.91 ng/ml

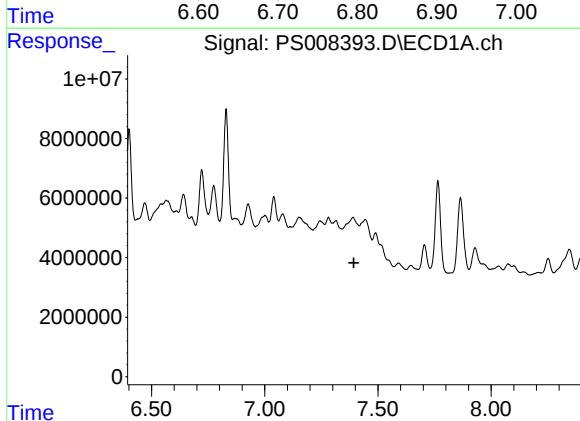


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 7.394 min
Response: 0
Conc: N.D.

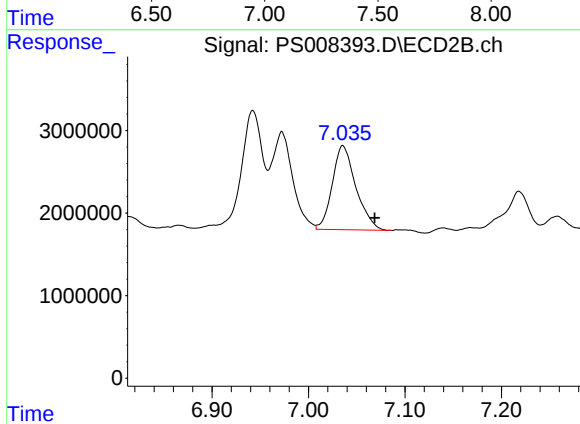

#9 2,4-D


R.T.: 7.036 min
Delta R.T.: -0.033 min
Response: 17300976
Conc: 14.76 ng/ml

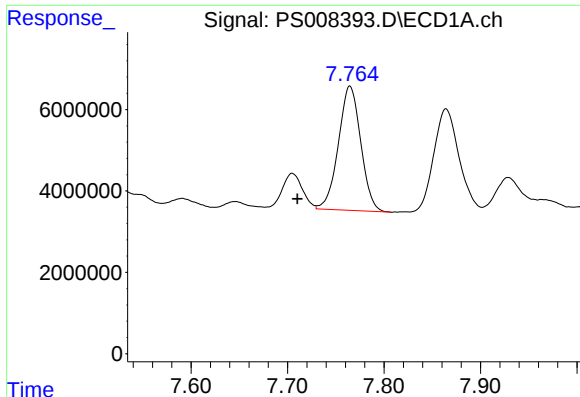

#10 Pentachlorophenol


R.T.: 7.765 min
Delta R.T.: 0.054 min
Response: 49305992
Conc: 2.03 ng/ml

Instrument :
ECD_O
ClientSampleId :

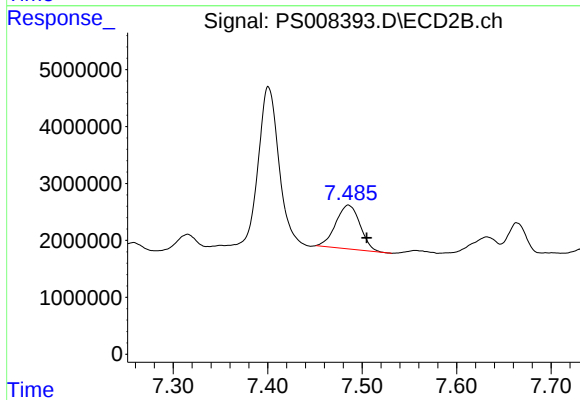


#10 Pentachlorophenol

R.T.: 7.486 min
Delta R.T.: -0.019 min
Response: 13745706
Conc: 1.02 ng/ml

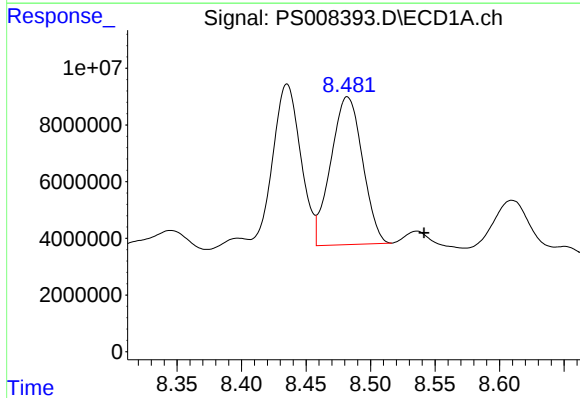


#12 2,4,5-T

R.T.: 8.482 min
Delta R.T.: -0.059 min
Response: 89283736
Conc: 9.68 ng/ml

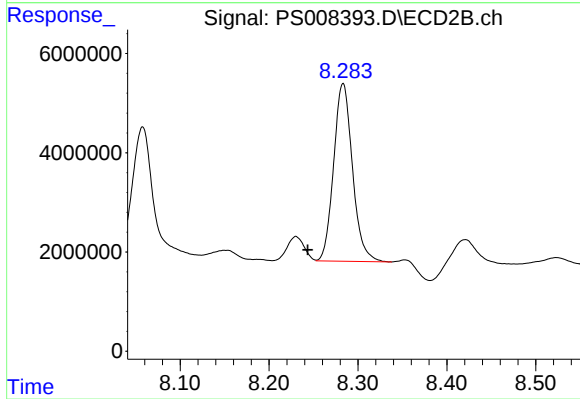

#12 2,4,5-T


R.T.: 8.283 min
Delta R.T.: 0.040 min
Response: 52695281
Conc: 9.96 ng/ml

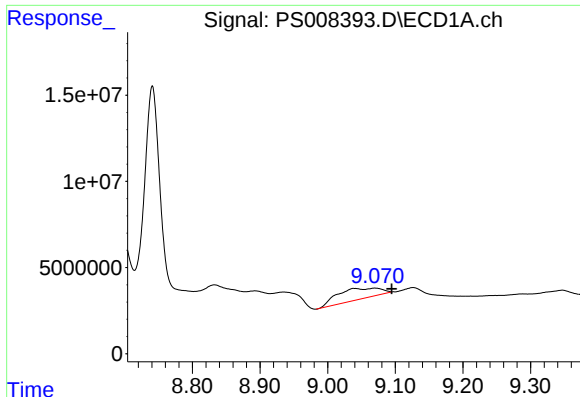

#13 2,4-DB


R.T.: 9.070 min
Delta R.T.: -0.025 min
Response: 27715107
Conc: 19.99 ng/ml

Instrument :
ECD_O
ClientSampleId :

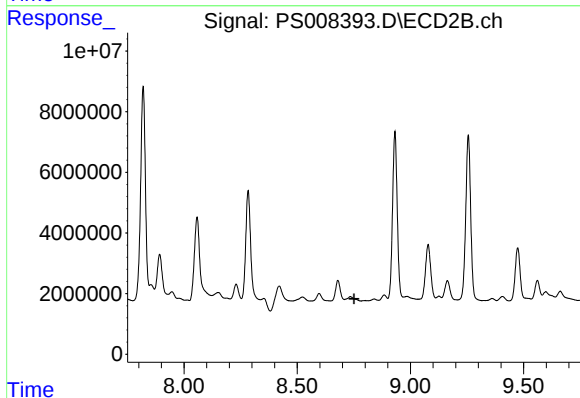


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 8.751 min
Response: 0
Conc: N.D.

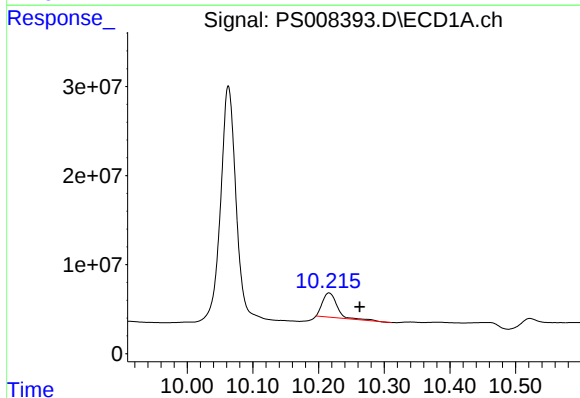


#14 DINOSEB

R.T.: 10.216 min
Delta R.T.: -0.047 min
Response: 42208515
Conc: 5.88 ng/ml

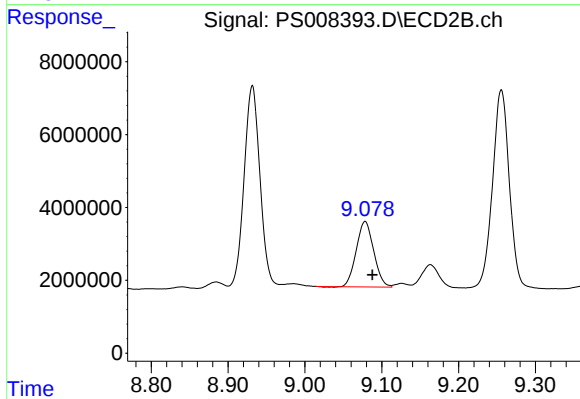

#14 DINOSEB


R.T.: 9.078 min
Delta R.T.: -0.009 min
Response: 28412910
Conc: 7.52 ng/ml

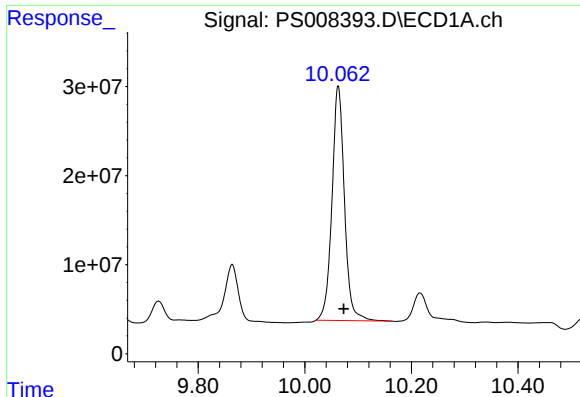

#15 Picloram


R.T.: 10.063 min
Delta R.T.: -0.010 min
Response: 427507932
Conc: 34.25 ng/ml

Instrument :
ECD_O
ClientSampleId :

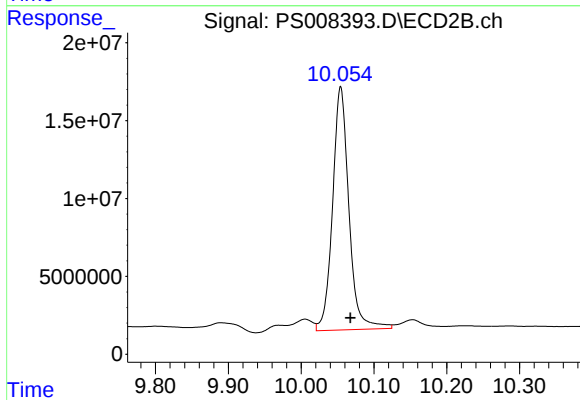


#15 Picloram

R.T.: 10.054 min
Delta R.T.: -0.013 min
Response: 243846054
Conc: 32.82 ng/ml

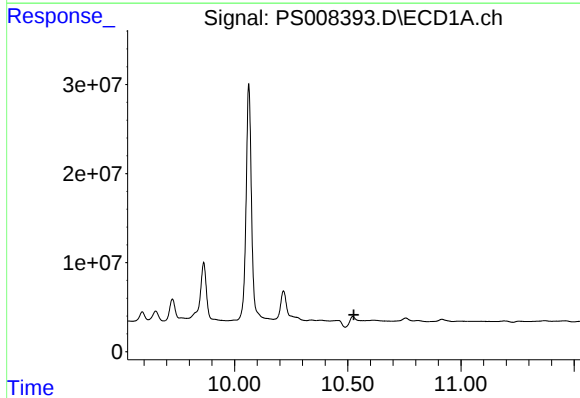

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.527 min
Response: 0
Conc: N.D.

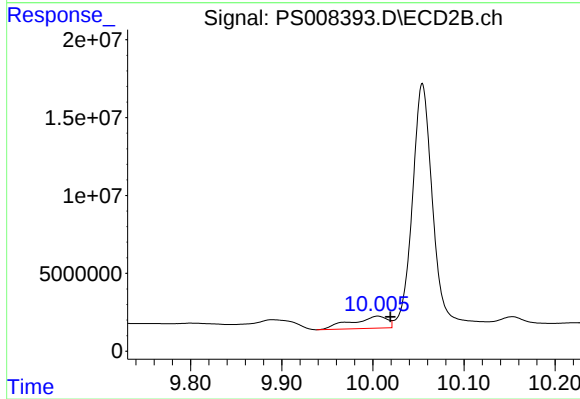

#16 DCPA

R.T.: 10.005 min
Delta R.T.: -0.014 min
Response: 21047748
Conc: 3.23 ng/ml