

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011321\
 Data File : P0074591.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Jan 2021 12:54
 Operator : AJ/MA
 Sample : M1092-07
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 263K-3A

Manual Integrations
 APPROVED

Ankita
 1/15/2021 12:30:38 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 15:26:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.931	4.005	2523631	1370883	23.917	24.370
2)	SA Decachlor...	10.949	9.257	2303581	1296867	22.697	23.620
Target Compounds							
26)	L6 AR-1254-1	7.167	6.113	461712	252056	104.979	69.783 #
27)	L6 AR-1254-2	7.397	6.272	815464	301092	119.732	96.611
28)	L6 AR-1254-3	7.780	6.688	1372036	1039977	195.605	212.070
29)	L6 AR-1254-4	8.075	6.926	953708	478012	157.256	137.844
30)	L6 AR-1254-5	8.511	7.352	2669227	15334725	459.503m	3388.185 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011321\
Data File : PO074591.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jan 2021 12:54
Operator : AJ/MA
Sample : M1092-07
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
263K-3A


Manual Integrations
APPROVED

Ankita
1/15/2021 12:30:38 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 15:26:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

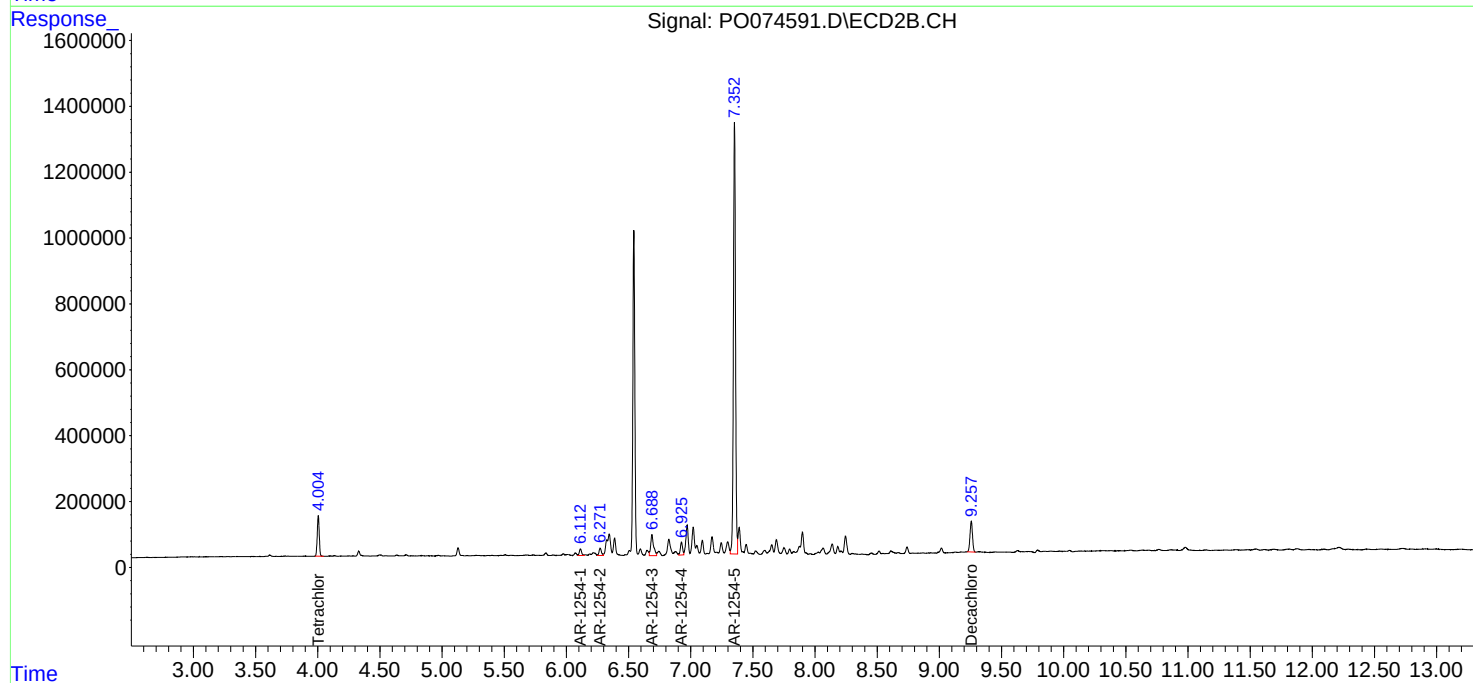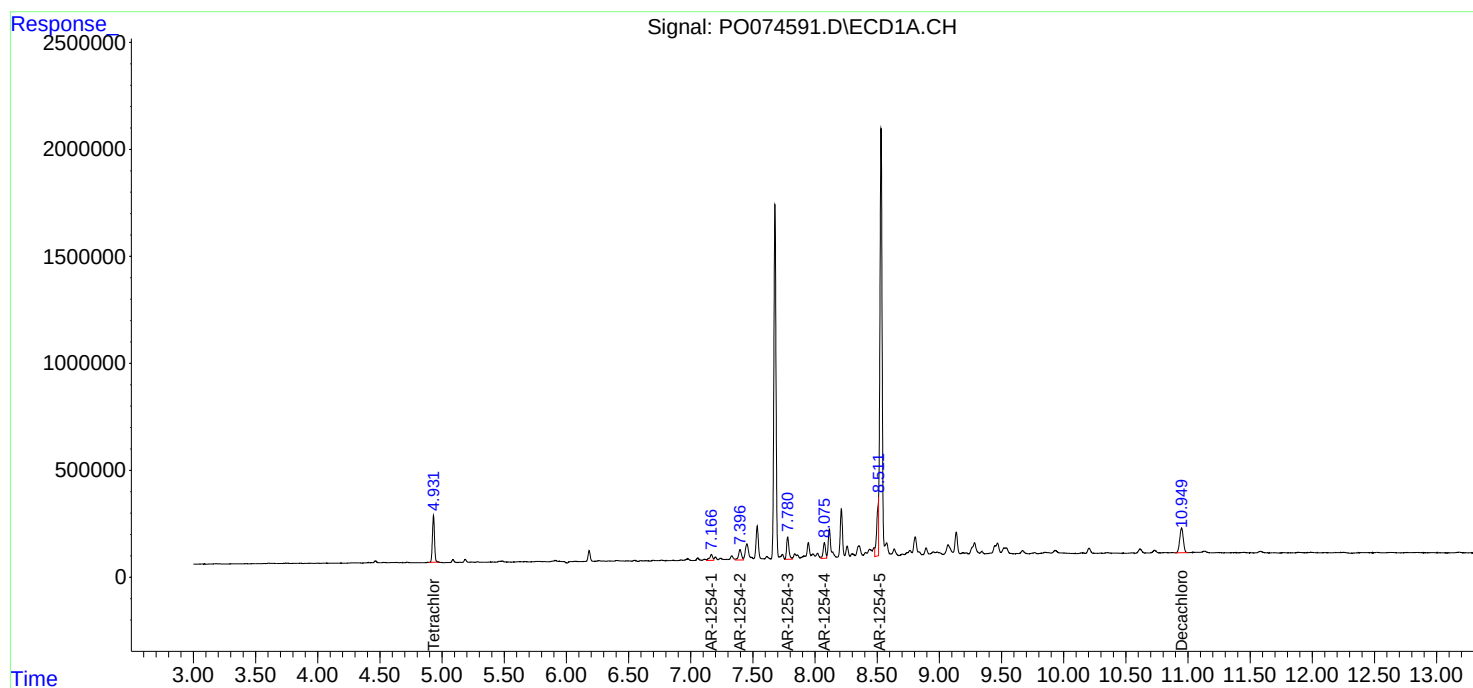

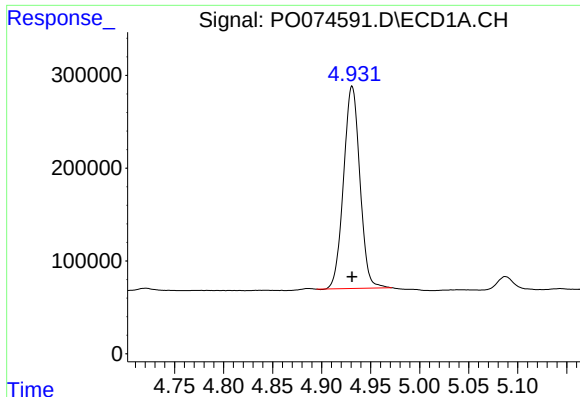


#1 Tetrachloro-m-xylene

R.T.: 4.931 min
Delta R.T.: 0.000 min
Response: 2523631
Conc: 23.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-3A


Manual Integrations
APPROVED

Ankita
1/15/2021 12:30:38 PM

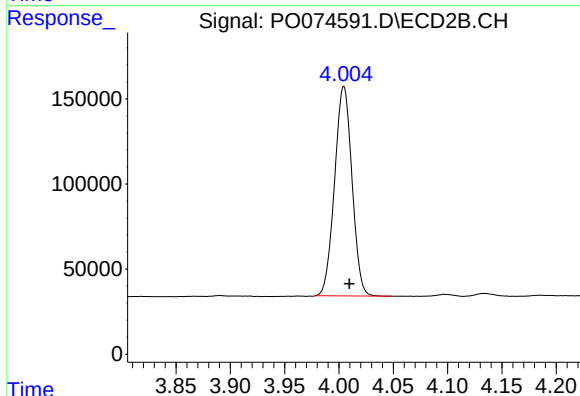


#1 Tetrachloro-m-xylene

R.T.: 4.005 min
Delta R.T.: -0.005 min
Response: 1370883
Conc: 24.37 ng/ml

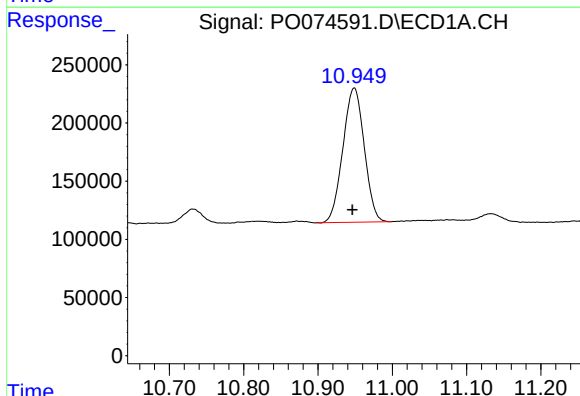


#2 Decachlorobiphenyl

R.T.: 10.949 min
Delta R.T.: 0.002 min
Response: 2303581
Conc: 22.70 ng/ml

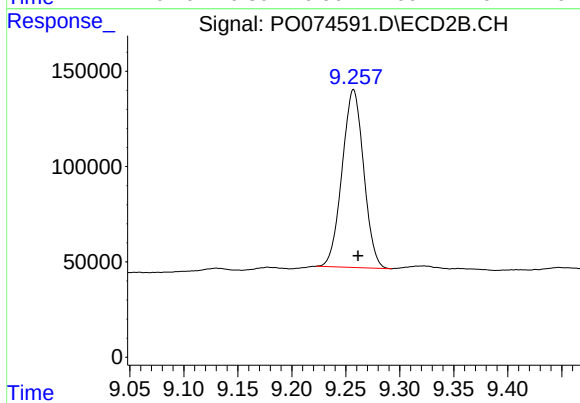

#2 Decachlorobiphenyl

R.T.: 9.257 min
Delta R.T.: -0.004 min
Response: 1296867
Conc: 23.62 ng/ml

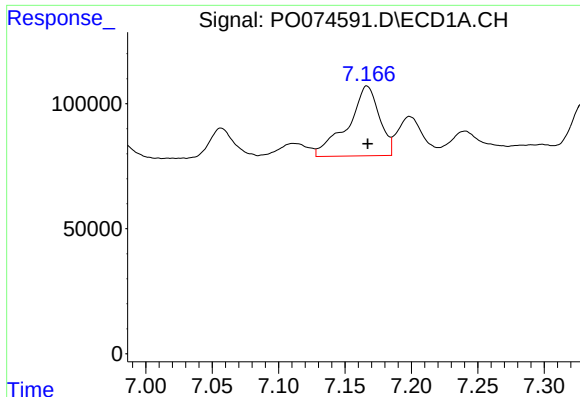


#26 AR-1254-1

R.T.: 7.167 min
Delta R.T.: 0.000 min
Response: 461712
Conc: 104.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-3A


Manual Integrations
APPROVED

Ankita
1/15/2021 12:30:38 PM

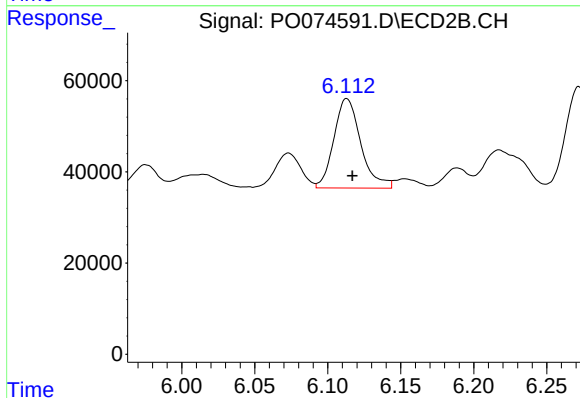


#26 AR-1254-1

R.T.: 6.113 min
Delta R.T.: -0.004 min
Response: 252056
Conc: 69.78 ng/ml

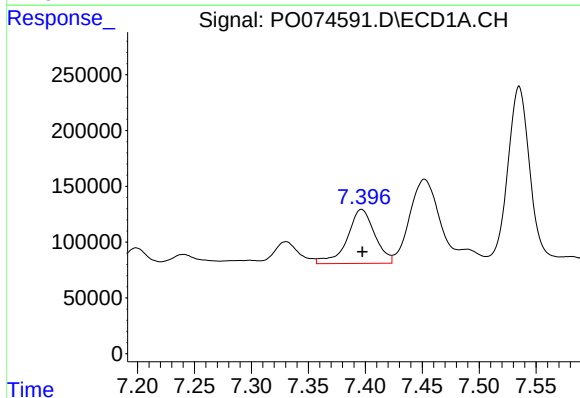


#27 AR-1254-2

R.T.: 7.397 min
Delta R.T.: 0.000 min
Response: 815464
Conc: 119.73 ng/ml

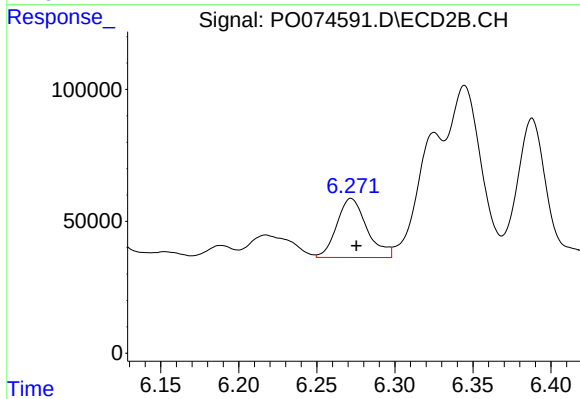

#27 AR-1254-2

R.T.: 6.272 min
Delta R.T.: -0.003 min
Response: 301092
Conc: 96.61 ng/ml

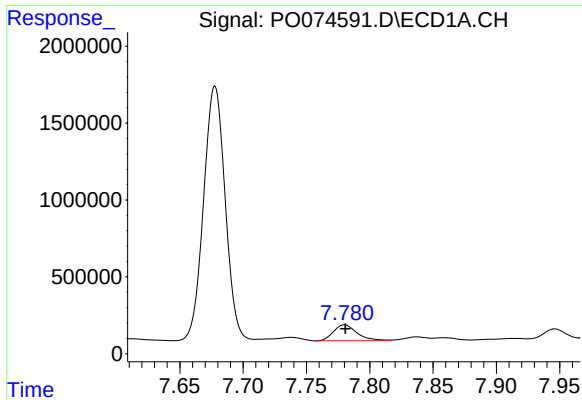


#28 AR-1254-3

R.T.: 7.780 min
Delta R.T.: 0.000 min
Response: 1372036
Conc: 195.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-3A


Manual Integrations
APPROVED

Ankita
1/15/2021 12:30:38 PM

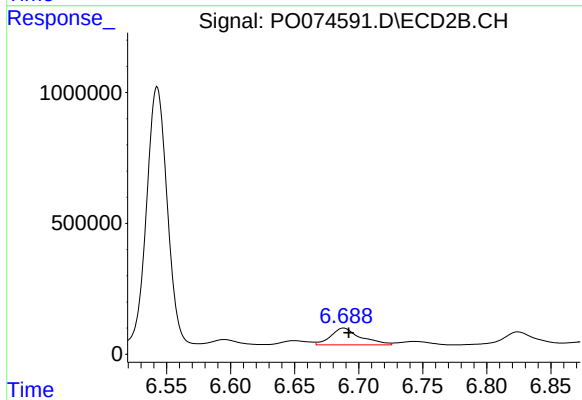


#28 AR-1254-3

R.T.: 6.688 min
Delta R.T.: -0.004 min
Response: 1039977
Conc: 212.07 ng/ml

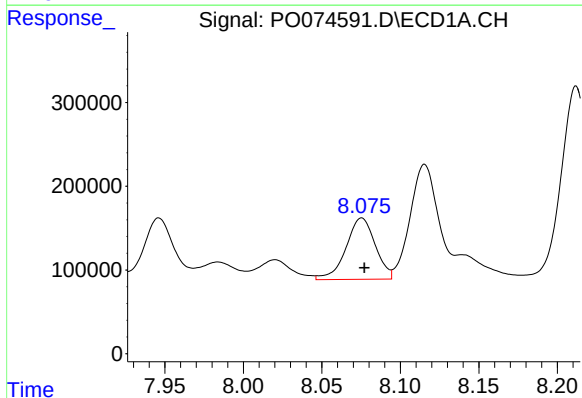


#29 AR-1254-4

R.T.: 8.075 min
Delta R.T.: -0.002 min
Response: 953708
Conc: 157.26 ng/ml

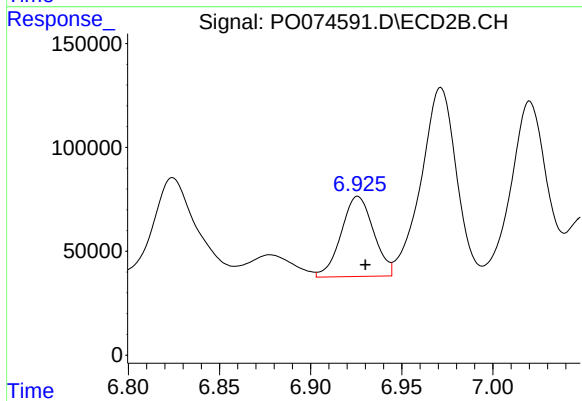

#29 AR-1254-4

R.T.: 6.926 min
Delta R.T.: -0.004 min
Response: 478012
Conc: 137.84 ng/ml

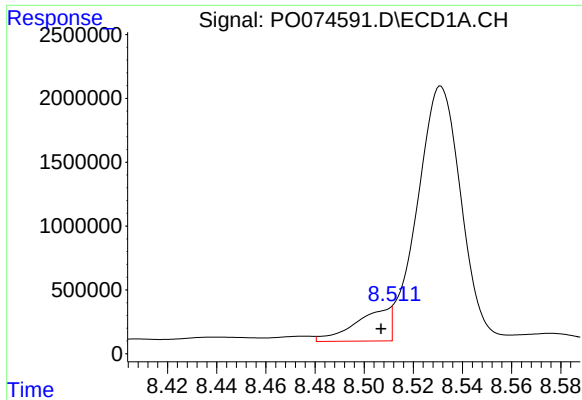


#30 AR-1254-5

R.T.: 8.511 min
Delta R.T.: 0.004 min
Response: 2669227
Conc: 459.50 ng/ml m

Instrument :
ECD_O
ClientSampleId :
263K-3A

Manual Integrations
APPROVED

Ankita
1/15/2021 12:30:38 PM

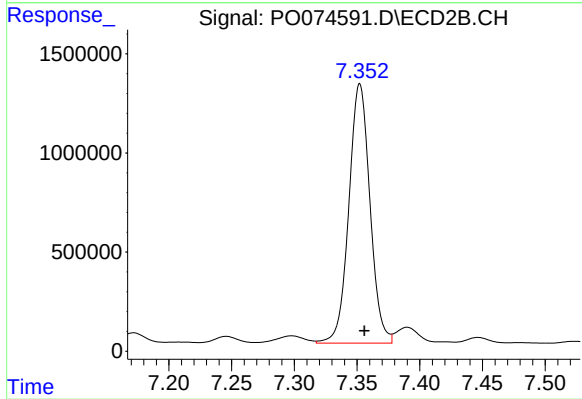

#30 AR-1254-5

R.T.: 7.352 min
Delta R.T.: -0.004 min
Response: 15334725
Conc: 3388.18 ng/ml