

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011321\
 Data File : P0074592.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Jan 2021 13:11
 Operator : AJ/MA
 Sample : M1092-10
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 263K-4A

Manual Integrations
 APPROVED

Ankita
 1/15/2021 12:30:39 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 15:26:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.933	4.005	2344289	1301193	22.217	23.131
2) SA Decachlor...	10.950	9.259	2116518	1179720	20.854	21.487
Target Compounds						
26) L6 AR-1254-1	7.168	6.115	272393	219567	61.934	60.788
27) L6 AR-1254-2	7.398	6.273	679146	225702	99.716	72.421 #
28) L6 AR-1254-3	7.782	6.690	981417	818034	139.916	166.812
29) L6 AR-1254-4	8.077	6.928	735637	360101	121.299	103.842
30) L6 AR-1254-5	8.514	7.354	2331206	8247367	401.314m	1822.244 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011321\
Data File : PO074592.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jan 2021 13:11
Operator : AJ/MA
Sample : M1092-10
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
263K-4A


Manual Integrations
APPROVED

Ankita
1/15/2021 12:30:39 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 15:26:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

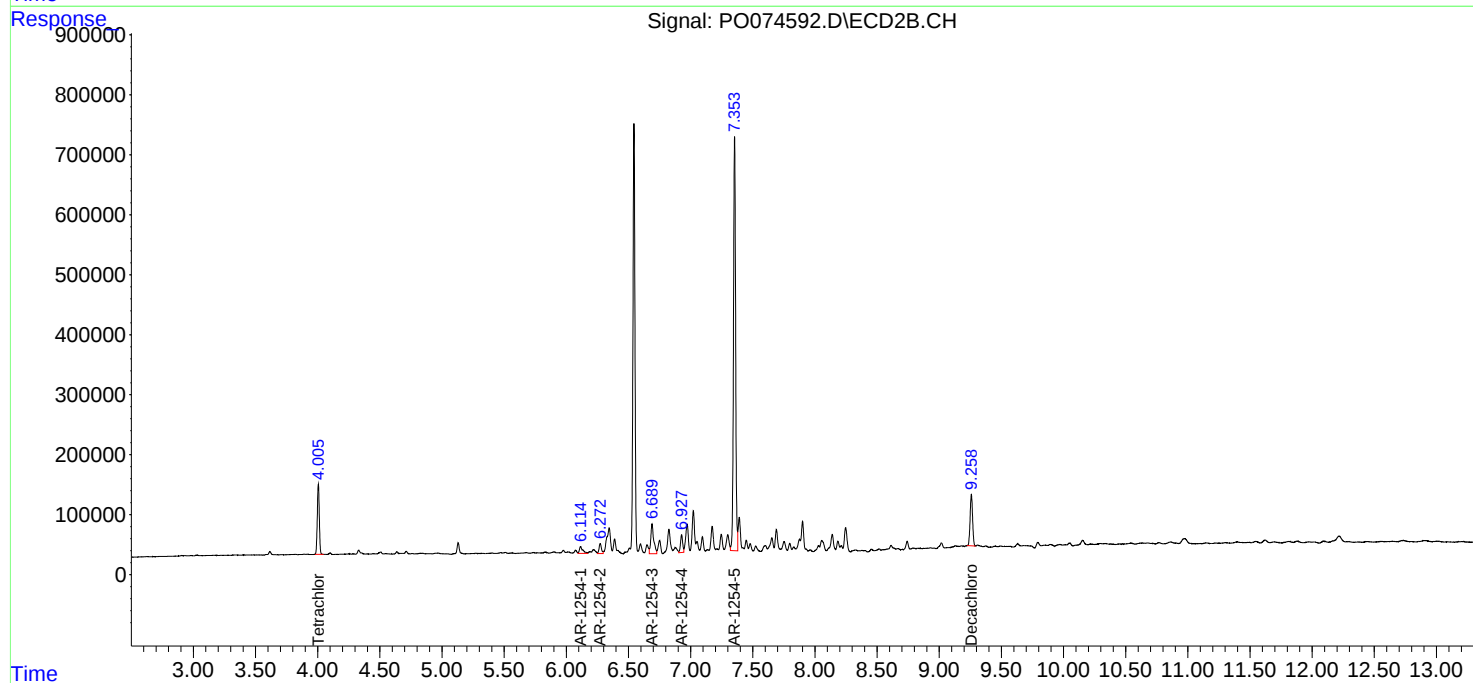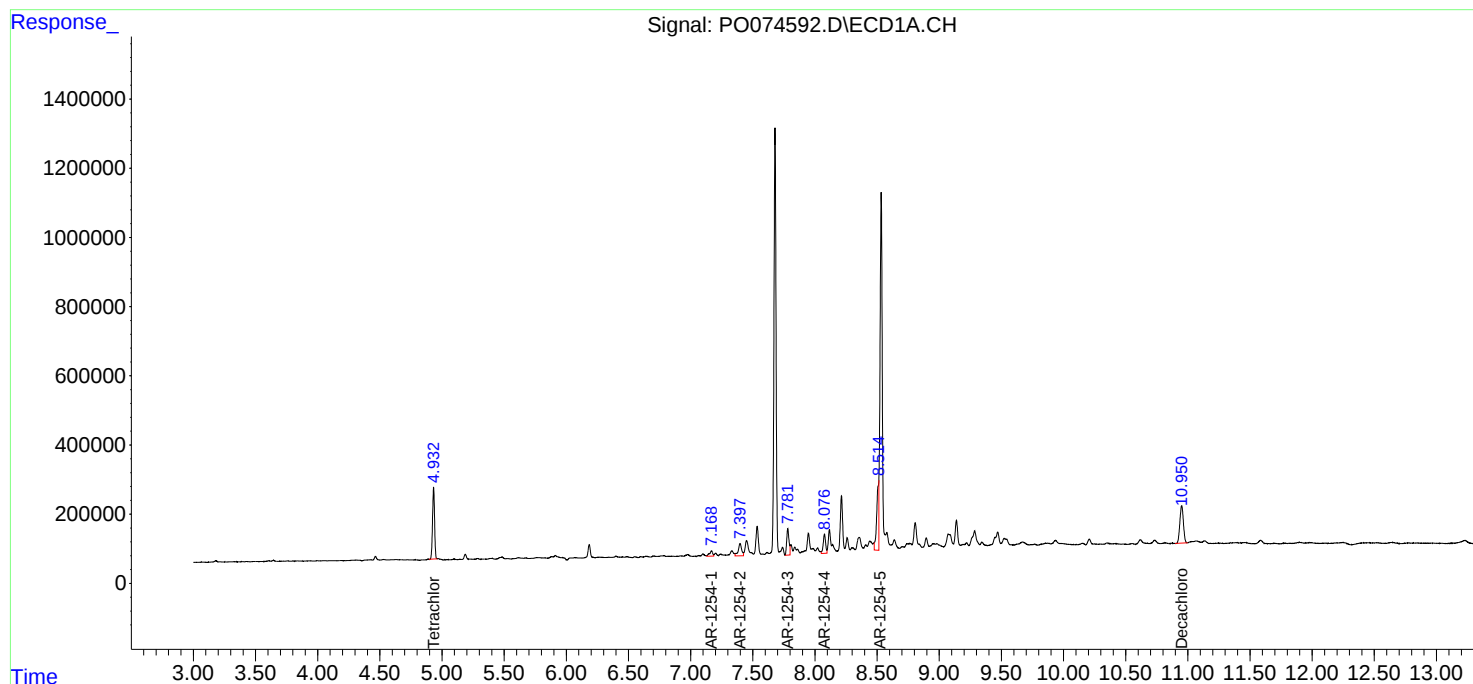

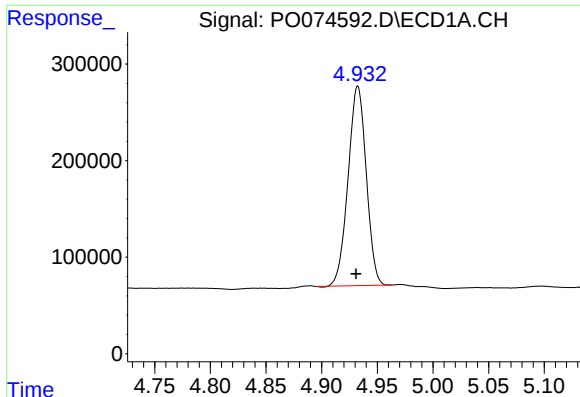


#1 Tetrachloro-m-xylene

R.T.: 4.933 min
Delta R.T.: 0.002 min
Response: 2344289
Conc: 22.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-4A


Manual Integrations
APPROVED

Ankita
1/15/2021 12:30:39 PM

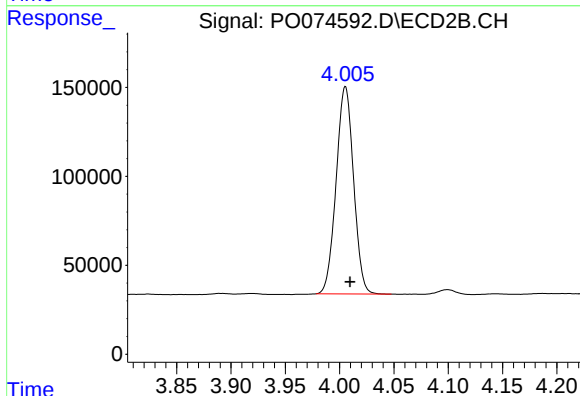


#1 Tetrachloro-m-xylene

R.T.: 4.005 min
Delta R.T.: -0.004 min
Response: 1301193
Conc: 23.13 ng/ml

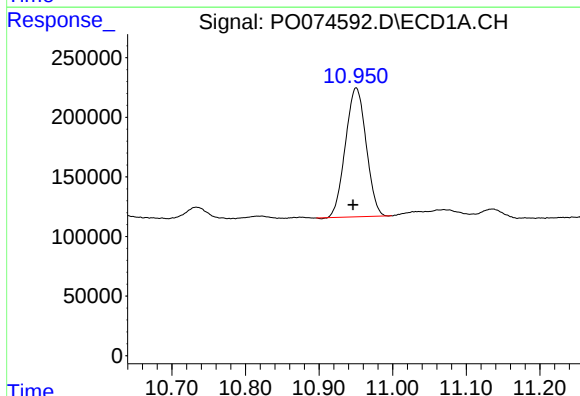


#2 Decachlorobiphenyl

R.T.: 10.950 min
Delta R.T.: 0.004 min
Response: 2116518
Conc: 20.85 ng/ml

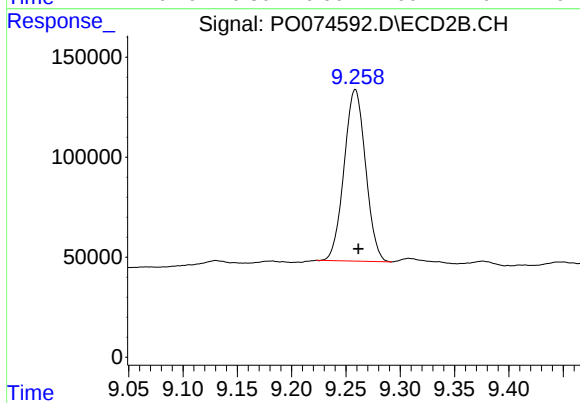

#2 Decachlorobiphenyl

R.T.: 9.259 min
Delta R.T.: -0.003 min
Response: 1179720
Conc: 21.49 ng/ml

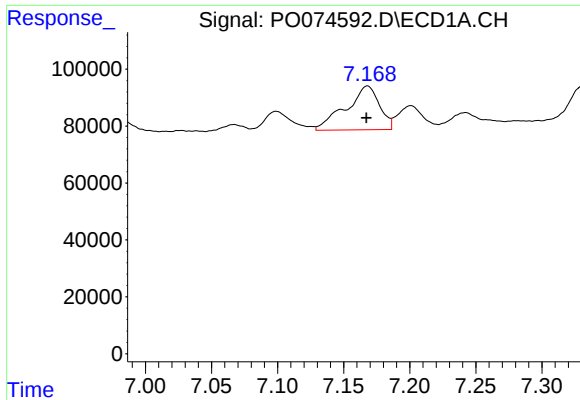


#26 AR-1254-1

R.T.: 7.168 min
Delta R.T.: 0.000 min
Response: 272393
Conc: 61.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-4A


Manual Integrations
APPROVED

Ankita
1/15/2021 12:30:39 PM

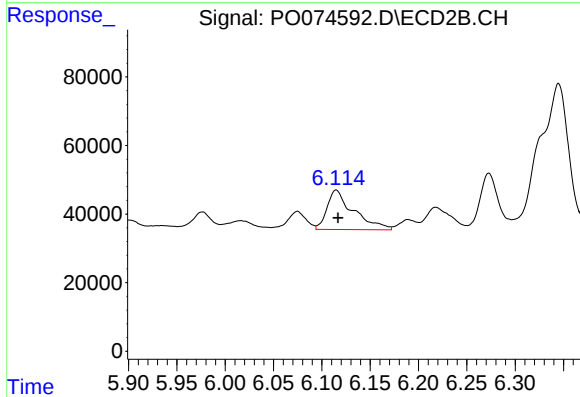


#26 AR-1254-1

R.T.: 6.115 min
Delta R.T.: -0.002 min
Response: 219567
Conc: 60.79 ng/ml

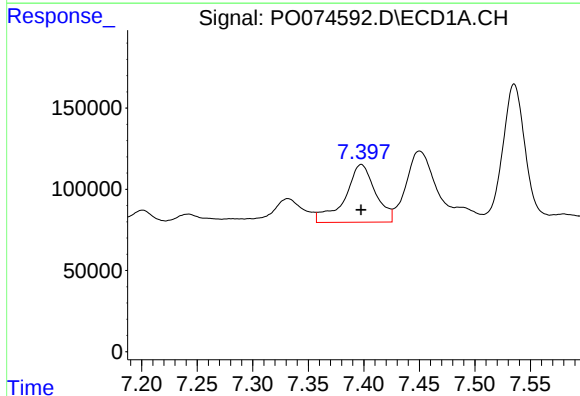


#27 AR-1254-2

R.T.: 7.398 min
Delta R.T.: 0.000 min
Response: 679146
Conc: 99.72 ng/ml

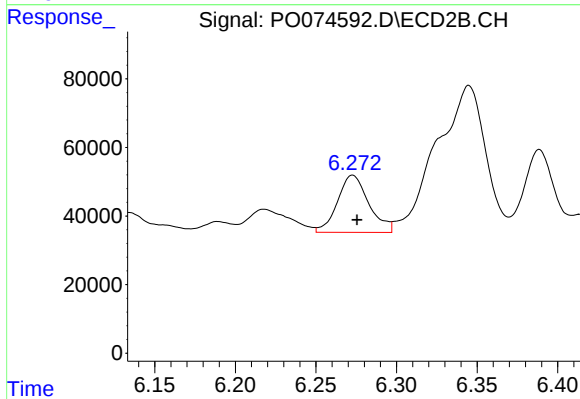

#27 AR-1254-2

R.T.: 6.273 min
Delta R.T.: -0.003 min
Response: 225702
Conc: 72.42 ng/ml

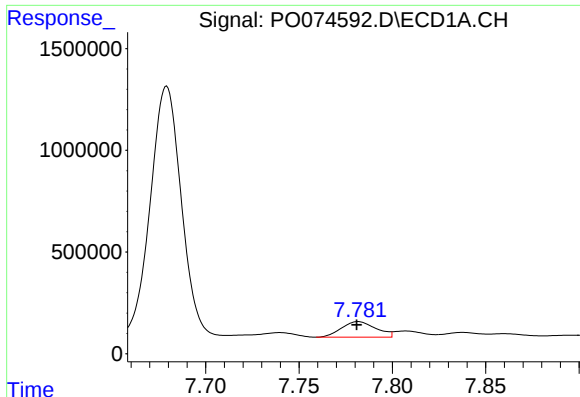


#28 AR-1254-3

R.T.: 7.782 min
Delta R.T.: 0.000 min
Response: 981417
Conc: 139.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-4A


Manual Integrations
APPROVED

Ankita
1/15/2021 12:30:39 PM

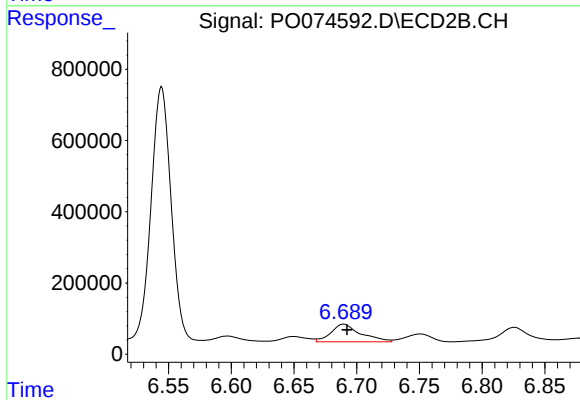


#28 AR-1254-3

R.T.: 6.690 min
Delta R.T.: -0.003 min
Response: 818034
Conc: 166.81 ng/ml

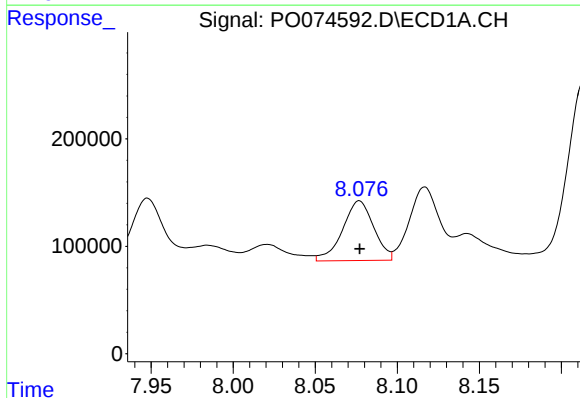


#29 AR-1254-4

R.T.: 8.077 min
Delta R.T.: 0.000 min
Response: 735637
Conc: 121.30 ng/ml

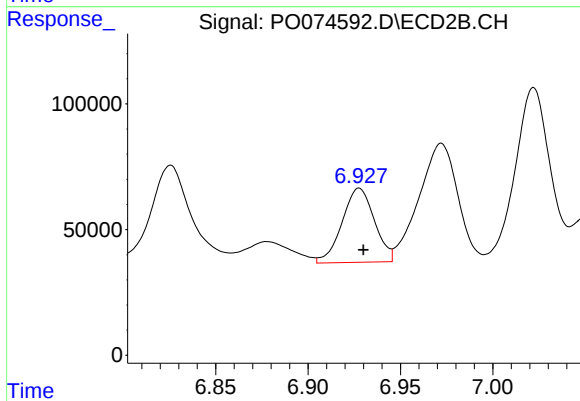

#29 AR-1254-4

R.T.: 6.928 min
Delta R.T.: -0.002 min
Response: 360101
Conc: 103.84 ng/ml

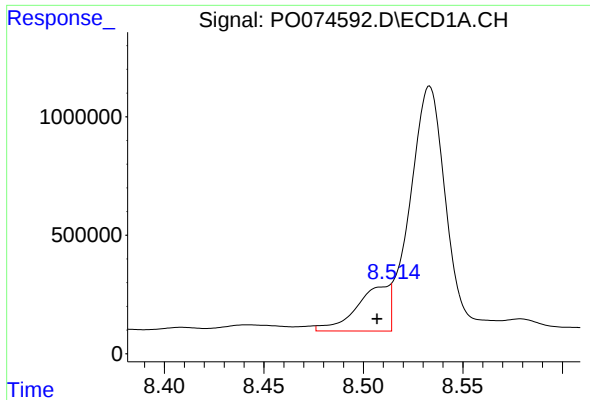


#30 AR-1254-5

R.T.: 8.514 min
Delta R.T.: 0.007 min
Response: 2331206
Conc: 401.31 ng/ml m

Instrument :
ECD_O
ClientSampleId :
263K-4A

Manual Integrations
APPROVED

Ankita
1/15/2021 12:30:39 PM

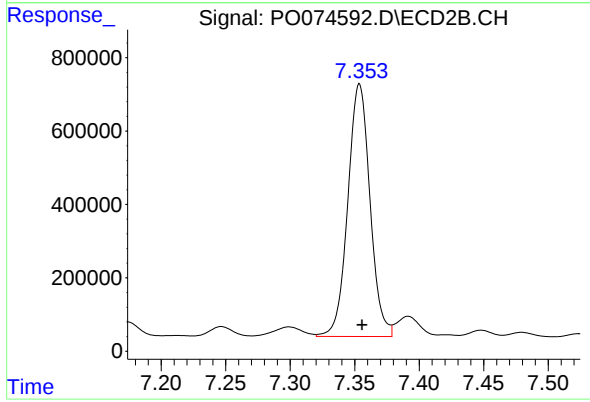

#30 AR-1254-5

R.T.: 7.354 min
Delta R.T.: -0.002 min
Response: 8247367
Conc: 1822.24 ng/ml