

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011321\
 Data File : P0074593.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Jan 2021 13:28
 Operator : AJ/MA
 Sample : M1092-13
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 263K-5A

Manual Integrations
 APPROVED

Ankita
 1/15/2021 12:30:41 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 15:26:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.933	4.006	2390729	1369967	22.657	24.354
2) SA Decachlor...	10.951	9.259	1838124	1010520	18.111	18.405
Target Compounds						
26) L6 AR-1254-1	7.168	6.114	333257	245754	75.772	68.038
27) L6 AR-1254-2	7.398	6.274	682937	294930	100.273	94.634
28) L6 AR-1254-3	7.783	6.690	1249205	895556	178.093	182.620
29) L6 AR-1254-4	8.078	6.928	852416	406874	140.554	117.330
30) L6 AR-1254-5	8.513	7.354	1998692	10490321	344.072m	2317.821 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011321\
Data File : PO074593.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jan 2021 13:28
Operator : AJ/MA
Sample : M1092-13
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
263K-5A


Manual Integrations
APPROVED

Ankita
1/15/2021 12:30:41 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 15:26:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

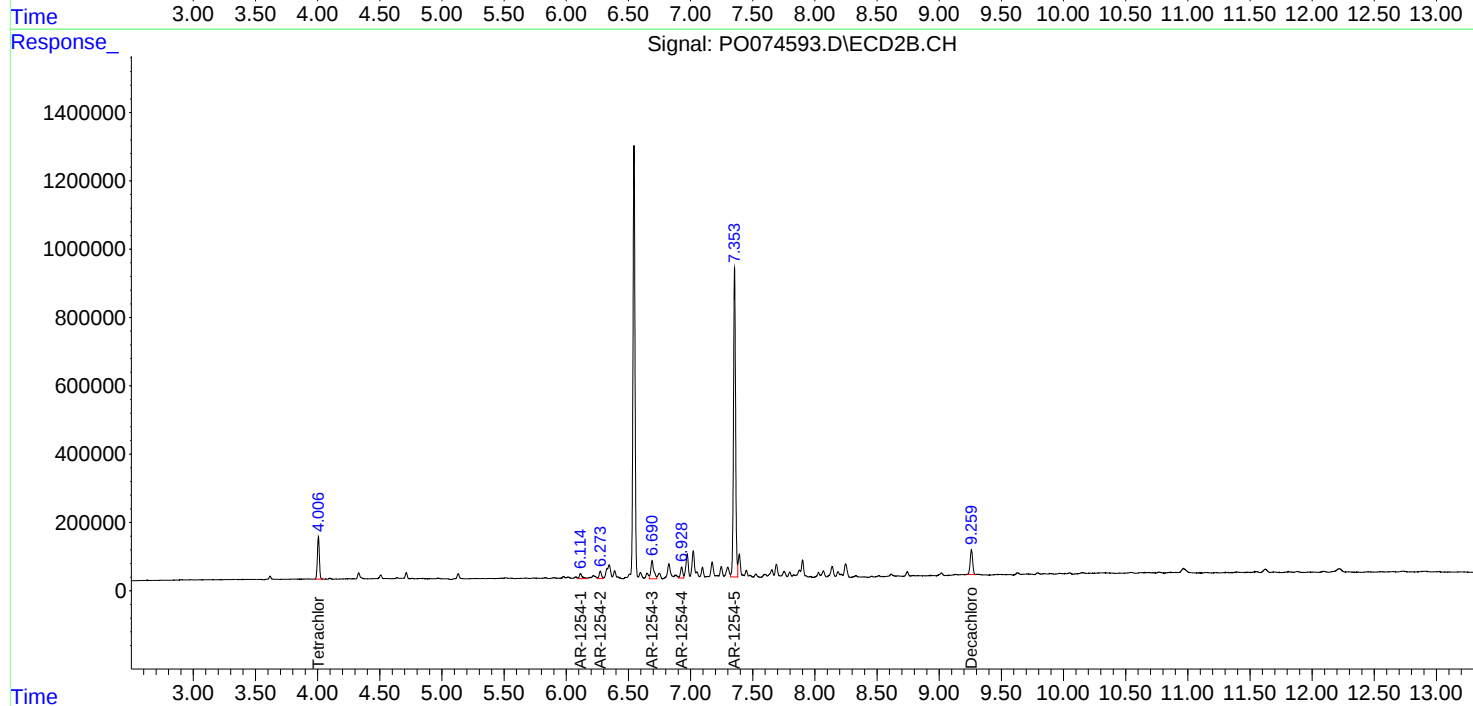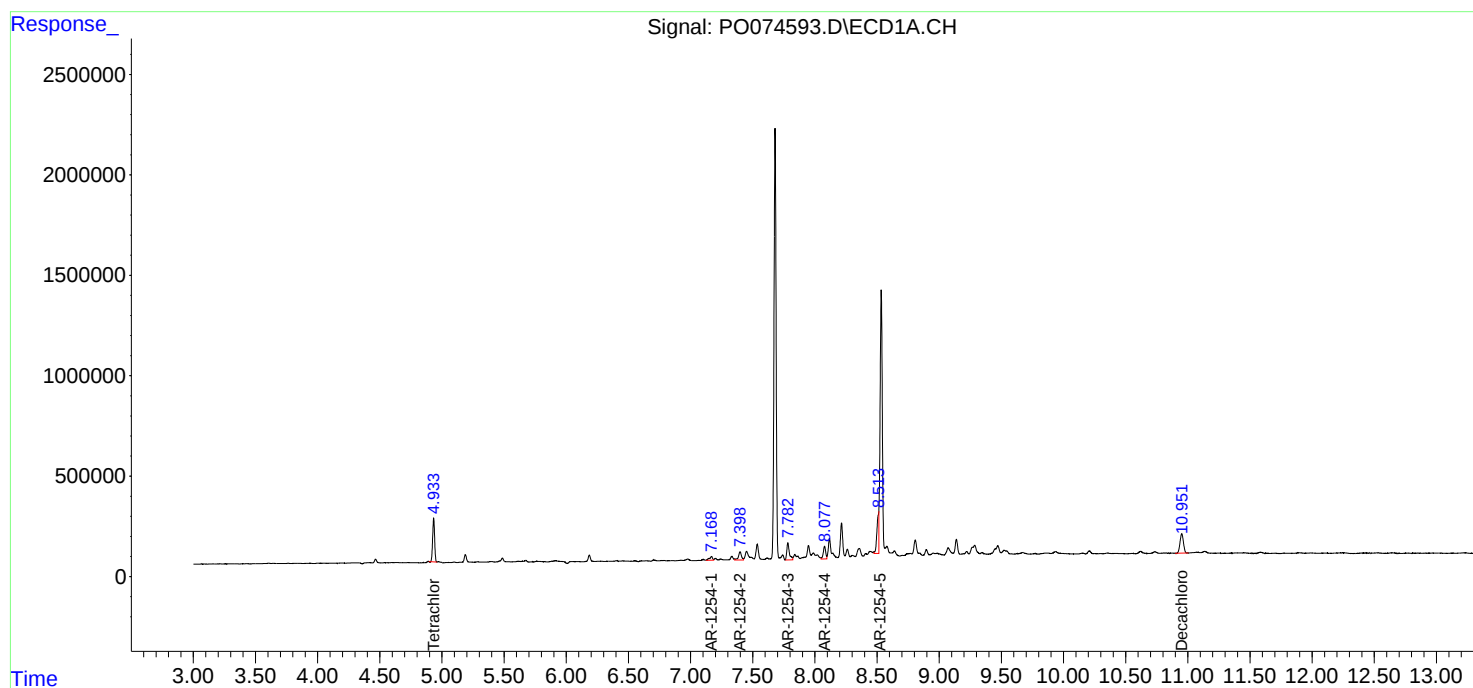

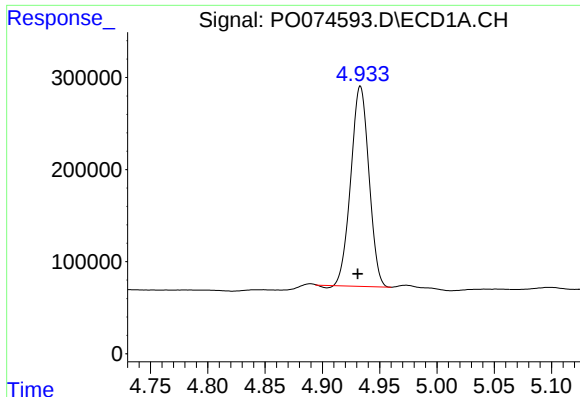


#1 Tetrachloro-m-xylene

R.T.: 4.933 min
Delta R.T.: 0.002 min
Response: 2390729
Conc: 22.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-5A


Manual Integrations
APPROVED

Ankita
1/15/2021 12:30:41 PM

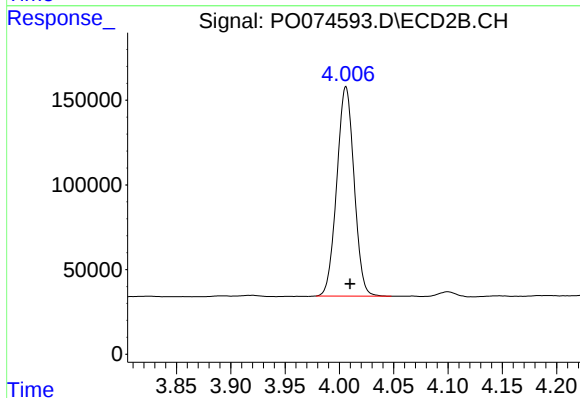


#1 Tetrachloro-m-xylene

R.T.: 4.006 min
Delta R.T.: -0.004 min
Response: 1369967
Conc: 24.35 ng/ml

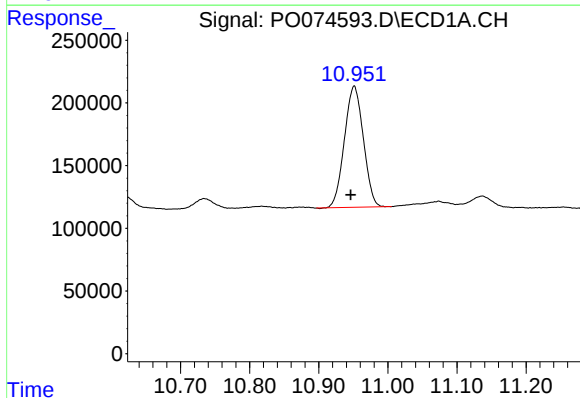


#2 Decachlorobiphenyl

R.T.: 10.951 min
Delta R.T.: 0.005 min
Response: 1838124
Conc: 18.11 ng/ml

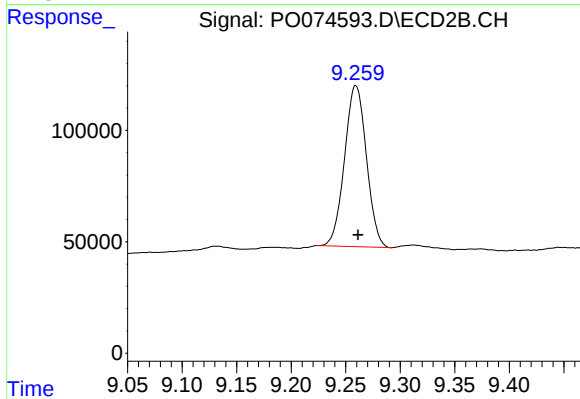

#2 Decachlorobiphenyl

R.T.: 9.259 min
Delta R.T.: -0.002 min
Response: 1010520
Conc: 18.41 ng/ml

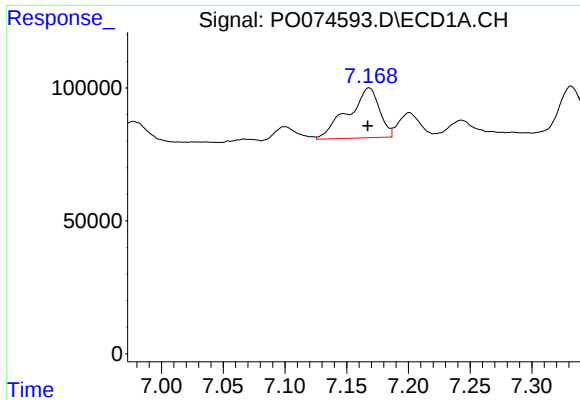


#26 AR-1254-1

R.T.: 7.168 min
Delta R.T.: 0.000 min
Response: 333257
Conc: 75.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-5A


Manual Integrations
APPROVED

Ankita
1/15/2021 12:30:41 PM

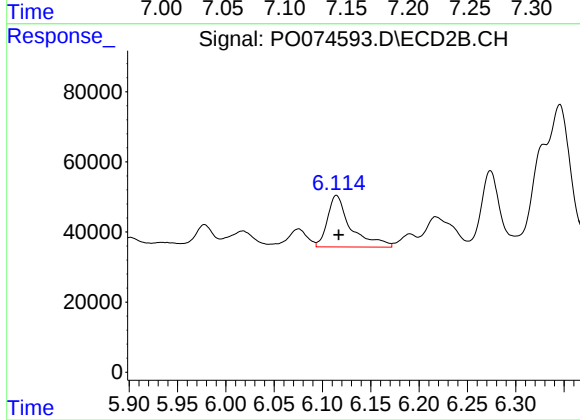


#26 AR-1254-1

R.T.: 6.114 min
Delta R.T.: -0.002 min
Response: 245754
Conc: 68.04 ng/ml

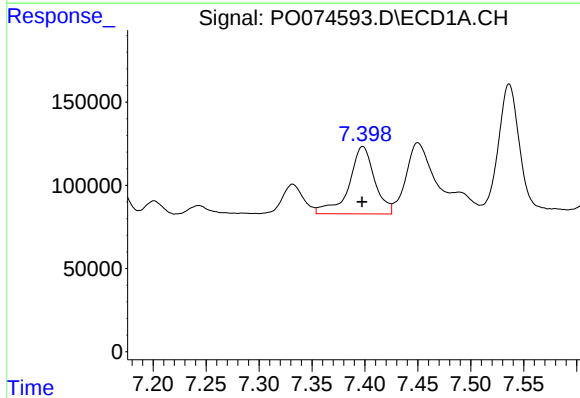


#27 AR-1254-2

R.T.: 7.398 min
Delta R.T.: 0.000 min
Response: 682937
Conc: 100.27 ng/ml

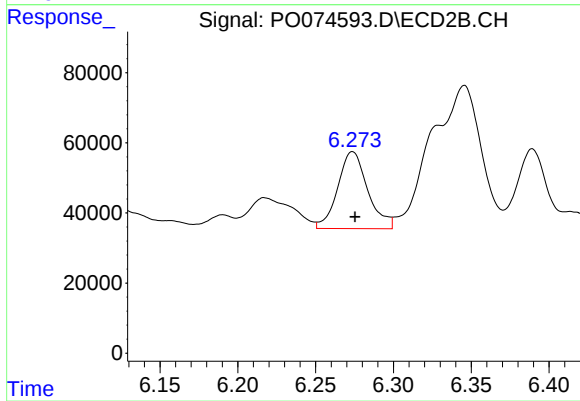

#27 AR-1254-2

R.T.: 6.274 min
Delta R.T.: -0.002 min
Response: 294930
Conc: 94.63 ng/ml

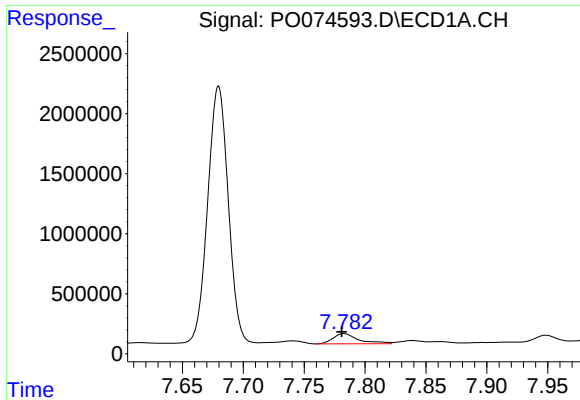


#28 AR-1254-3

R.T.: 7.783 min
Delta R.T.: 0.002 min
Response: 1249205
Conc: 178.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-5A


Manual Integrations
APPROVED

Ankita
1/15/2021 12:30:41 PM

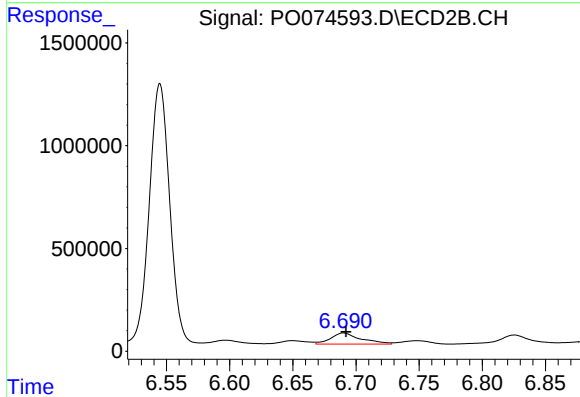


#28 AR-1254-3

R.T.: 6.690 min
Delta R.T.: -0.002 min
Response: 895556
Conc: 182.62 ng/ml

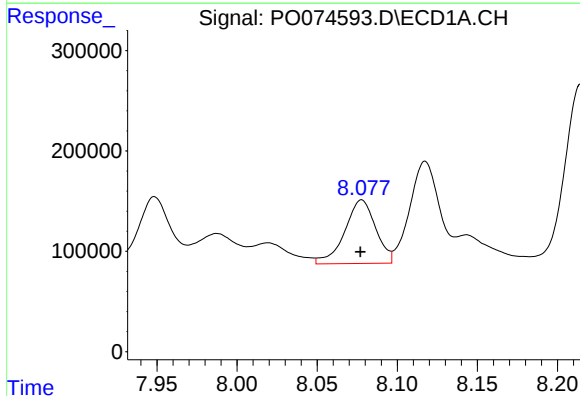


#29 AR-1254-4

R.T.: 8.078 min
Delta R.T.: 0.000 min
Response: 852416
Conc: 140.55 ng/ml

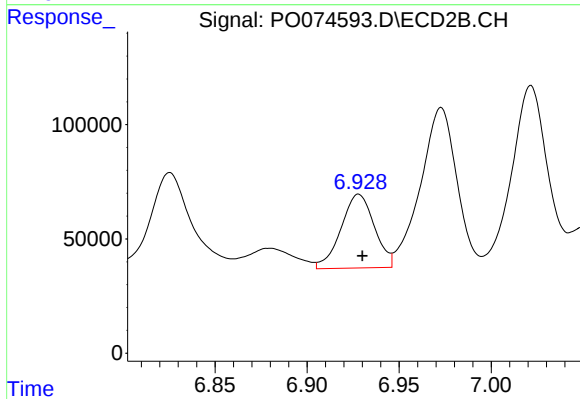

#29 AR-1254-4

R.T.: 6.928 min
Delta R.T.: -0.002 min
Response: 406874
Conc: 117.33 ng/ml

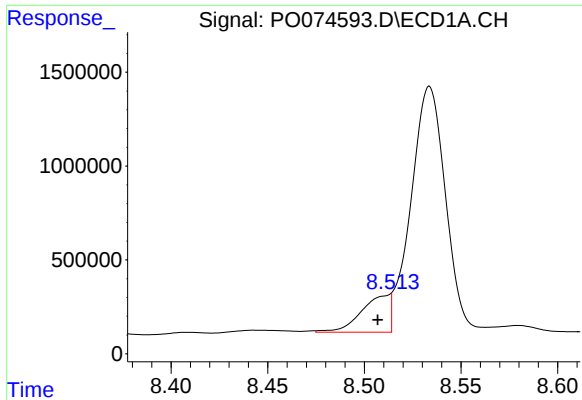


#30 AR-1254-5

R.T.: 8.513 min
Delta R.T.: 0.006 min
Response: 1998692
Conc: 344.07 ng/ml m

Instrument :
ECD_O
ClientSampleId :
263K-5A

Manual Integrations
APPROVED

Ankita
1/15/2021 12:30:41 PM

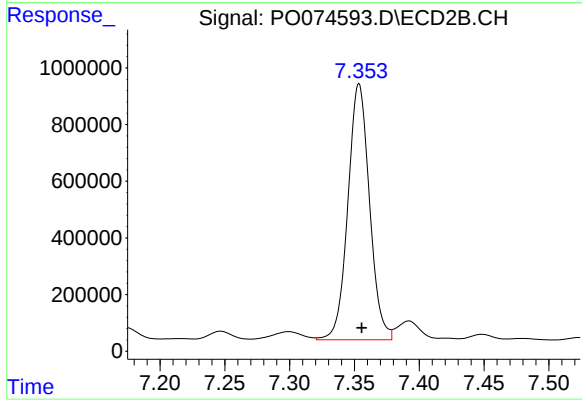

#30 AR-1254-5

R.T.: 7.354 min
Delta R.T.: -0.002 min
Response: 10490321
Conc: 2317.82 ng/ml