

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011321\
 Data File : P0074611.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Jan 2021 18:36
 Operator : AJ/MA
 Sample : M1098-03
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 263K-DUP1

Manual Integrations
 APPROVED

Ankita
 1/15/2021 8:56:06 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 18:54:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.932	4.005	2639957	1435815	25.019	25.525
2) SA Decachlor...	10.949	9.258	2069449	1135715	20.390	20.685
Target Compounds						
26) L6 AR-1254-1	7.167	6.113	153576	177264	34.918	49.076 #
27) L6 AR-1254-2	7.397	6.272	571145	181546	83.859	58.252 #
28) L6 AR-1254-3	7.781	6.688	752888	608465	107.336	124.077
29) L6 AR-1254-4	8.077	6.926	438869	242840	72.365	70.028
30) L6 AR-1254-5	8.508	7.352	1344370	4386735	231.431m	969.243 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011321\
Data File : PO074611.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jan 2021 18:36
Operator : AJ/MA
Sample : M1098-03
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
263K-DUP1


Manual Integrations
APPROVED

Ankita
1/15/2021 8:56:06 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 18:54:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

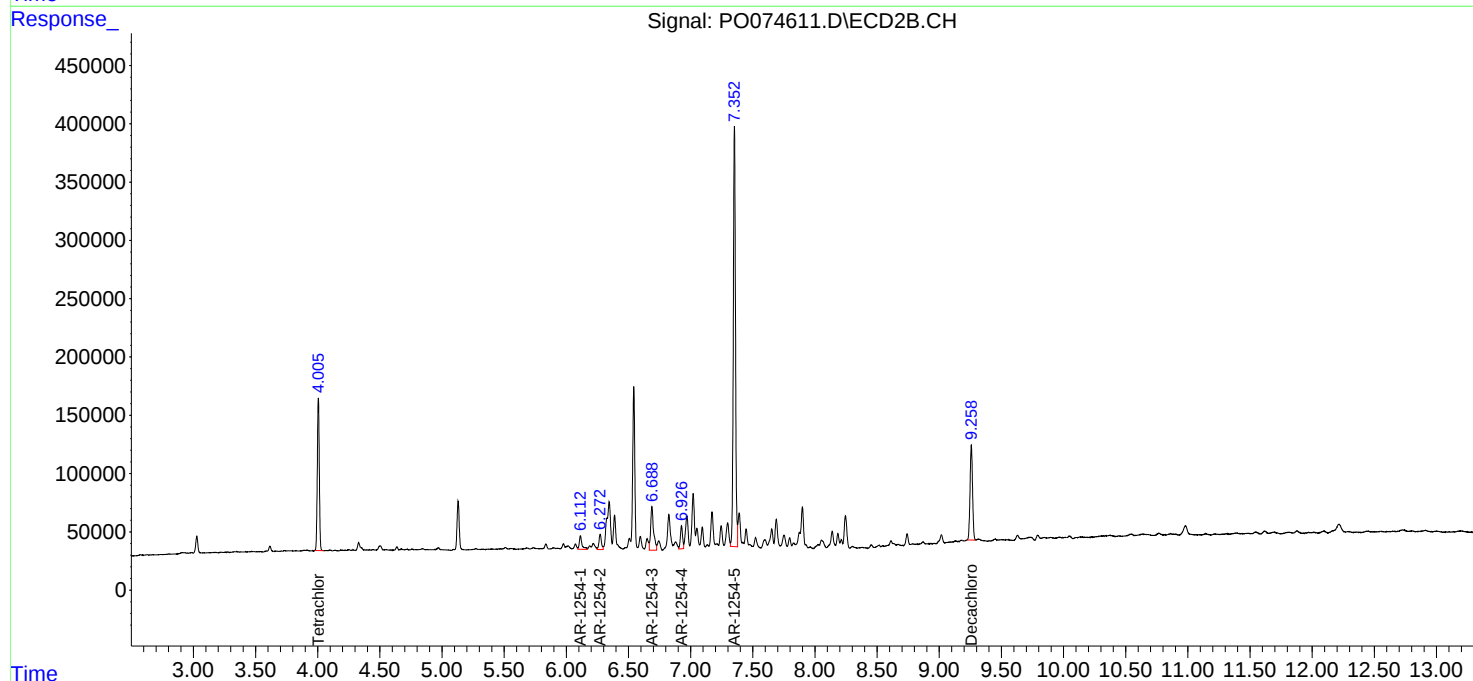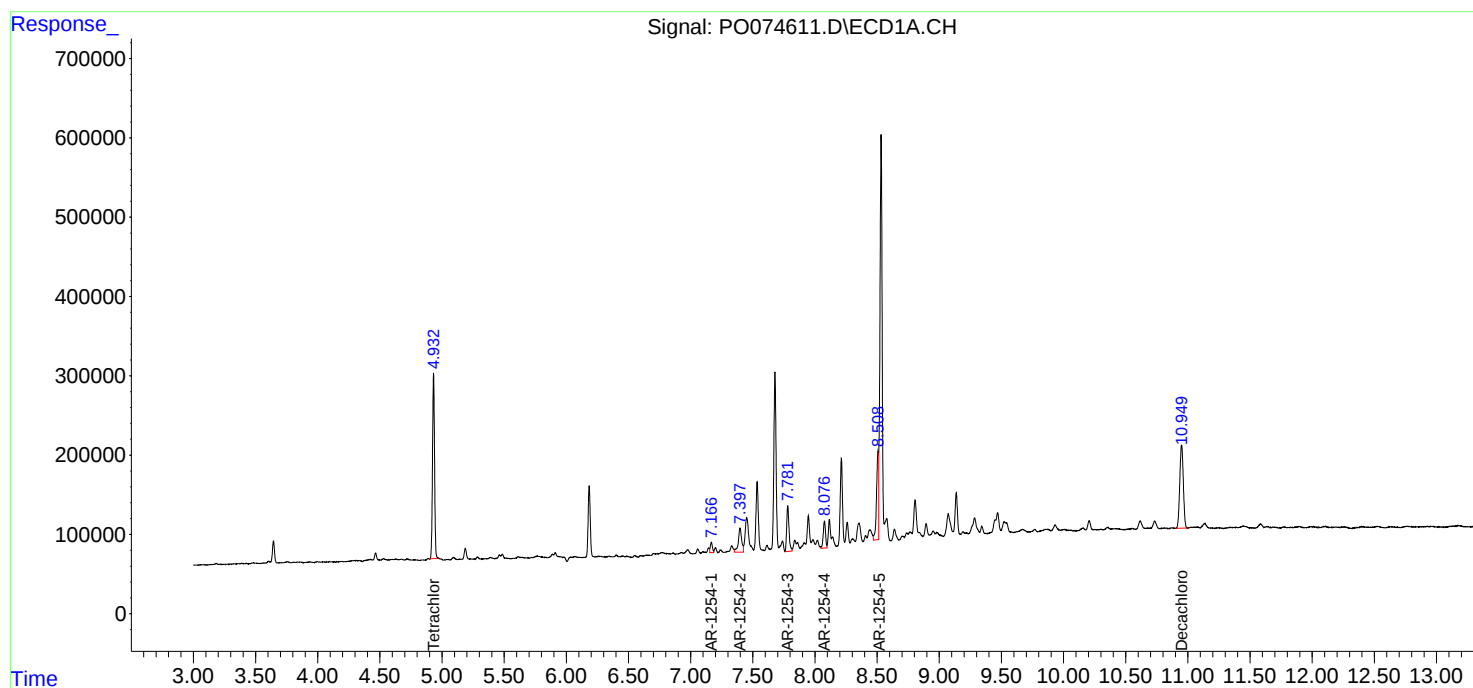

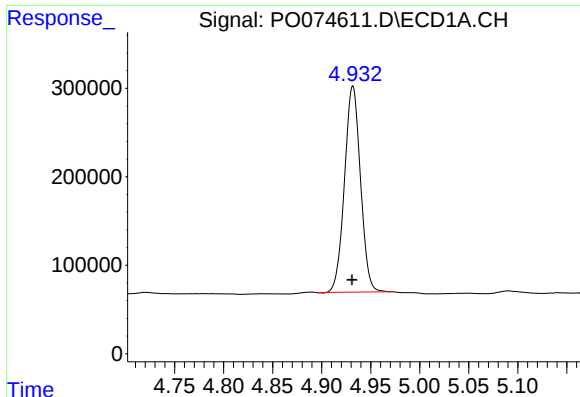


#1 Tetrachloro-m-xylene

R.T.: 4.932 min
Delta R.T.: 0.000 min
Response: 2639957
Conc: 25.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-DUP1


Manual Integrations
APPROVED

Ankita
1/15/2021 8:56:06 AM

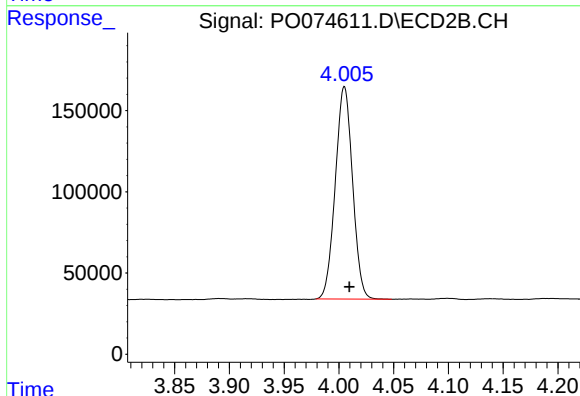


#1 Tetrachloro-m-xylene

R.T.: 4.005 min
Delta R.T.: -0.005 min
Response: 1435815
Conc: 25.52 ng/ml

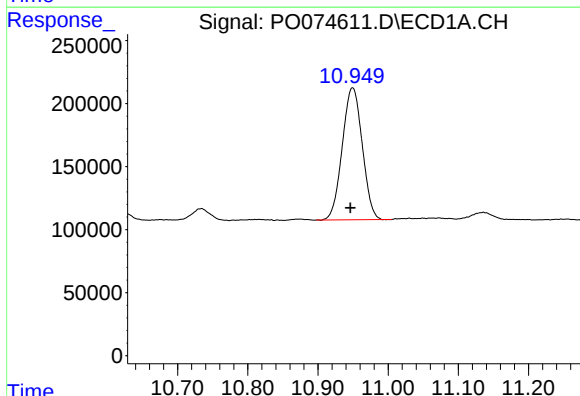


#2 Decachlorobiphenyl

R.T.: 10.949 min
Delta R.T.: 0.003 min
Response: 2069449
Conc: 20.39 ng/ml

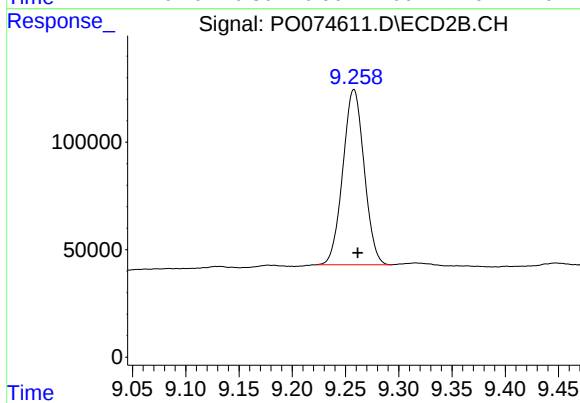

#2 Decachlorobiphenyl

R.T.: 9.258 min
Delta R.T.: -0.004 min
Response: 1135715
Conc: 20.69 ng/ml

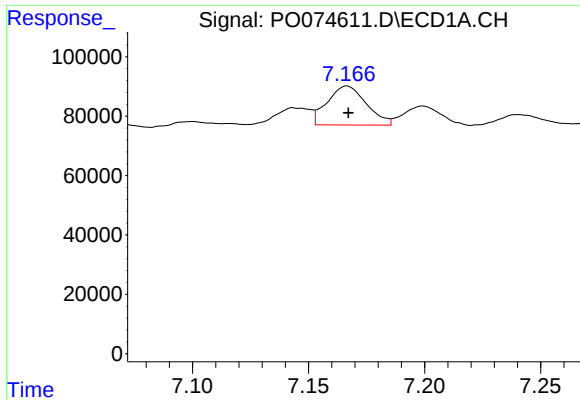


#26 AR-1254-1

R.T.: 7.167 min
Delta R.T.: 0.000 min
Response: 153576
Conc: 34.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-DUP1


Manual Integrations
APPROVED

Ankita
1/15/2021 8:56:06 AM

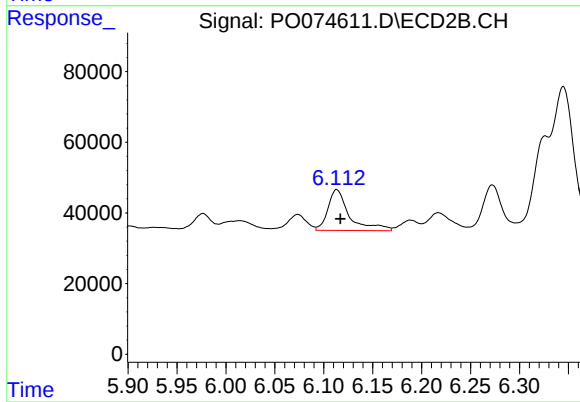


#26 AR-1254-1

R.T.: 6.113 min
Delta R.T.: -0.004 min
Response: 177264
Conc: 49.08 ng/ml

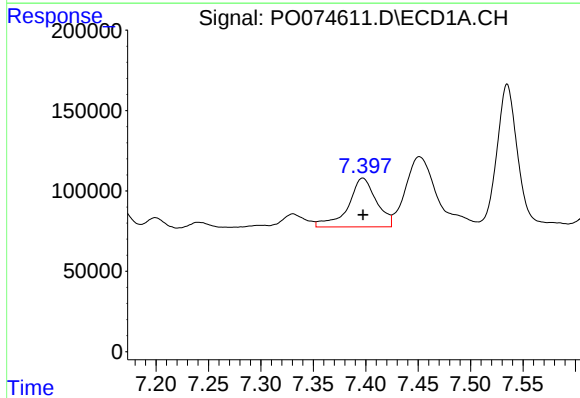


#27 AR-1254-2

R.T.: 7.397 min
Delta R.T.: 0.000 min
Response: 571145
Conc: 83.86 ng/ml

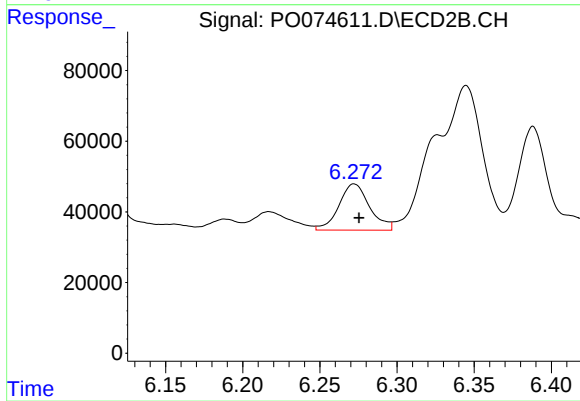

#27 AR-1254-2

R.T.: 6.272 min
Delta R.T.: -0.003 min
Response: 181546
Conc: 58.25 ng/ml

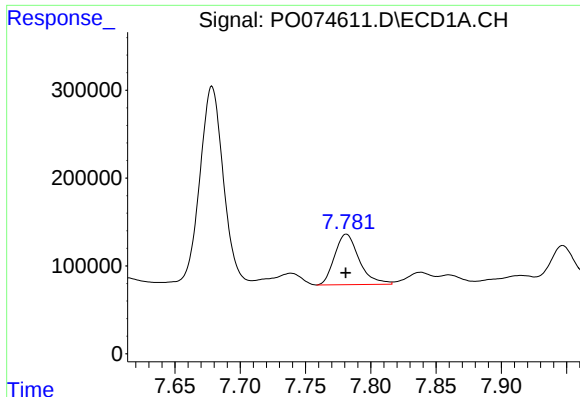


#28 AR-1254-3

R.T.: 7.781 min
Delta R.T.: 0.000 min
Response: 752888
Conc: 107.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-DUP1


Manual Integrations
APPROVED

Ankita
1/15/2021 8:56:06 AM

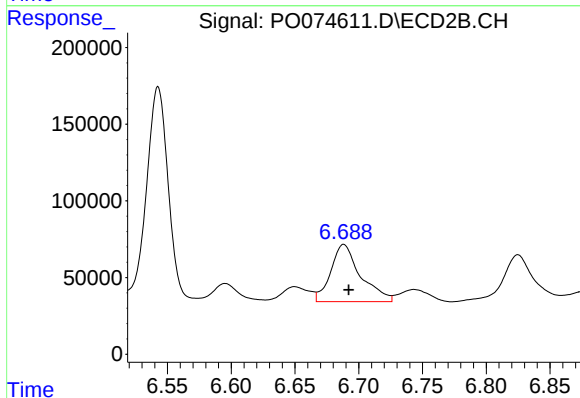


#28 AR-1254-3

R.T.: 6.688 min
Delta R.T.: -0.004 min
Response: 608465
Conc: 124.08 ng/ml

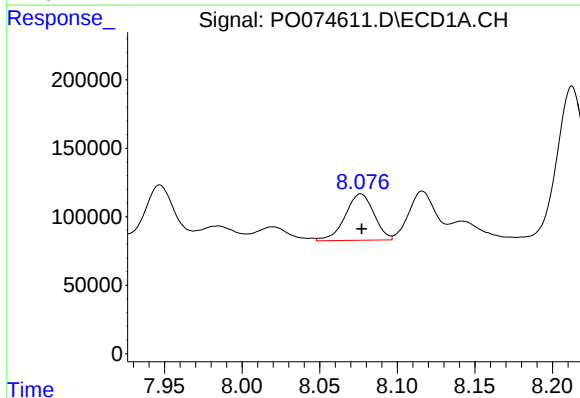


#29 AR-1254-4

R.T.: 8.077 min
Delta R.T.: 0.000 min
Response: 438869
Conc: 72.36 ng/ml

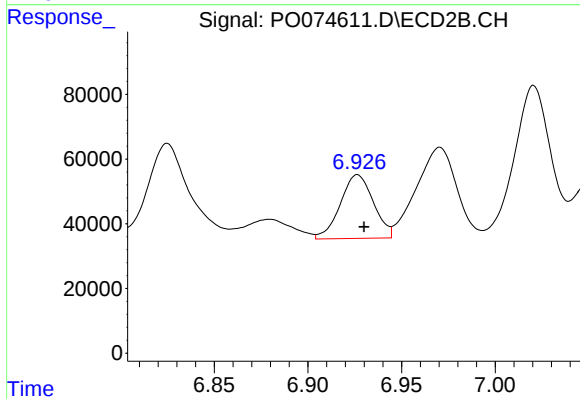

#29 AR-1254-4

R.T.: 6.926 min
Delta R.T.: -0.004 min
Response: 242840
Conc: 70.03 ng/ml

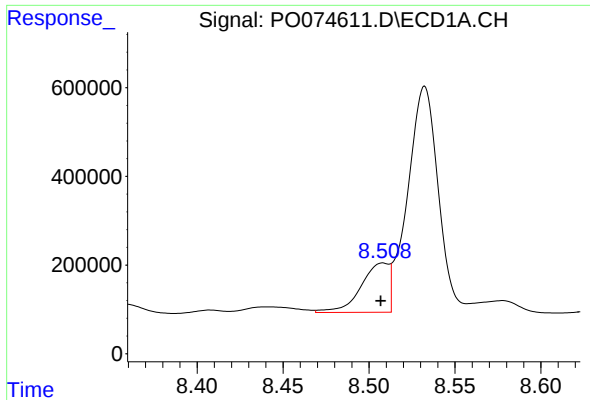


#30 AR-1254-5

R.T.: 8.508 min
Delta R.T.: 0.000 min
Response: 1344370
Conc: 231.43 ng/ml m

Instrument :
ECD_O
ClientSampleId :
263K-DUP1

Manual Integrations
APPROVED

Ankita
1/15/2021 8:56:06 AM

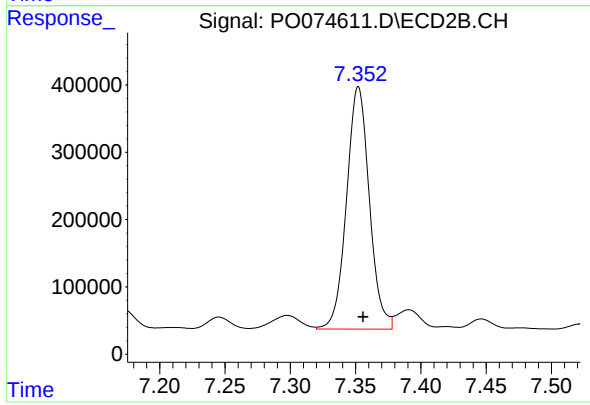

#30 AR-1254-5

R.T.: 7.352 min
Delta R.T.: -0.004 min
Response: 4386735
Conc: 969.24 ng/ml