

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011321\
 Data File : P0074612.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Jan 2021 18:53
 Operator : AJ/MA
 Sample : M1095-15
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 263K-27A

Manual Integrations
 APPROVED

Ankita
 1/15/2021 8:56:08 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 14 09:40:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.932	4.005	1896327	1094063	17.972	19.449
2) SA Decachlor...	10.951	9.258	1413053	807433	13.923	14.706
Target Compounds						
26) L6 AR-1254-1	7.167	6.114	58508	96483	13.303	26.712m#
27) L6 AR-1254-2	7.399	6.273	362530	177201	53.229	56.858
28) L6 AR-1254-3	7.782	6.689	626360	455315	89.297	92.847
29) L6 AR-1254-4	8.076	6.927	373587	207450	61.601	59.822
30) L6 AR-1254-5	8.506	7.353	1193191	2356375	205.406	520.638 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011321\
Data File : PO074612.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jan 2021 18:53
Operator : AJ/MA
Sample : M1095-15
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
263K-27A


Manual Integrations
APPROVED

Ankita
1/15/2021 8:56:08 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 14 09:40:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

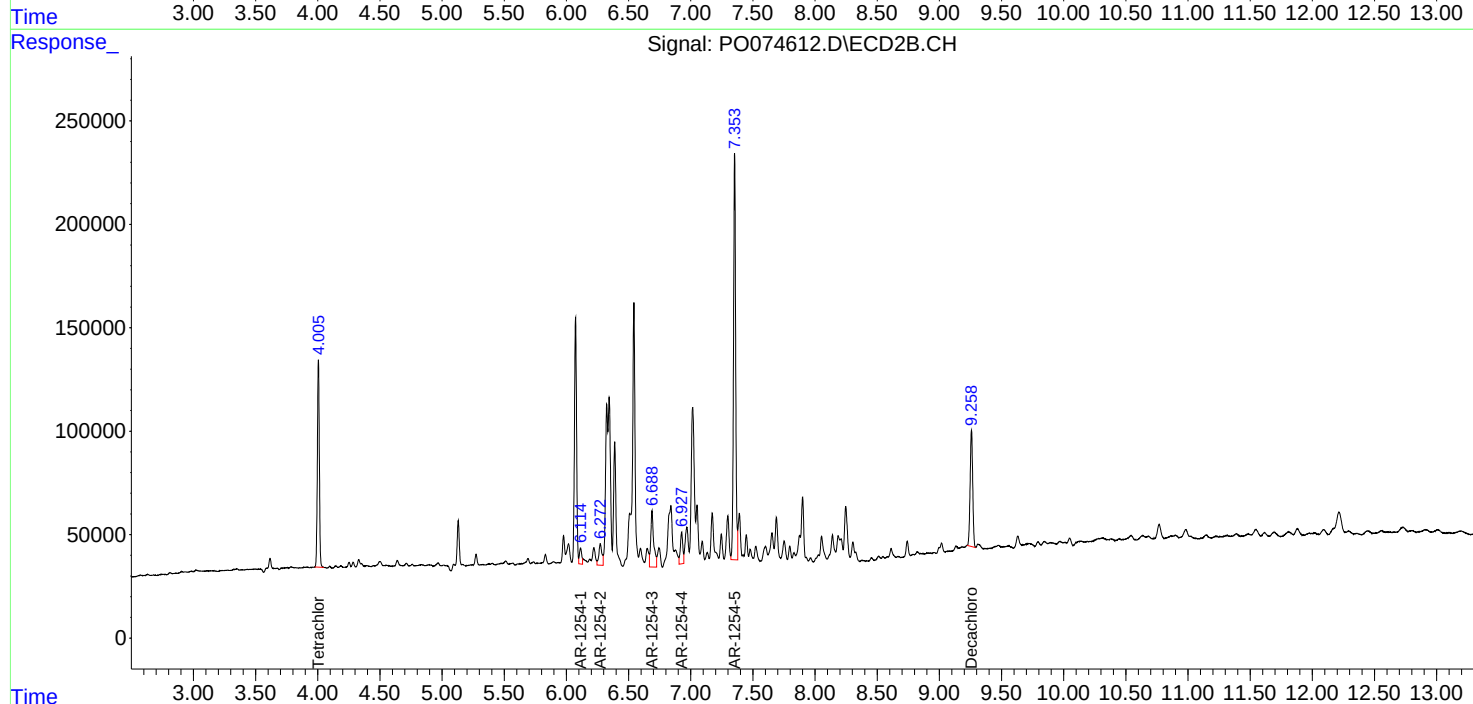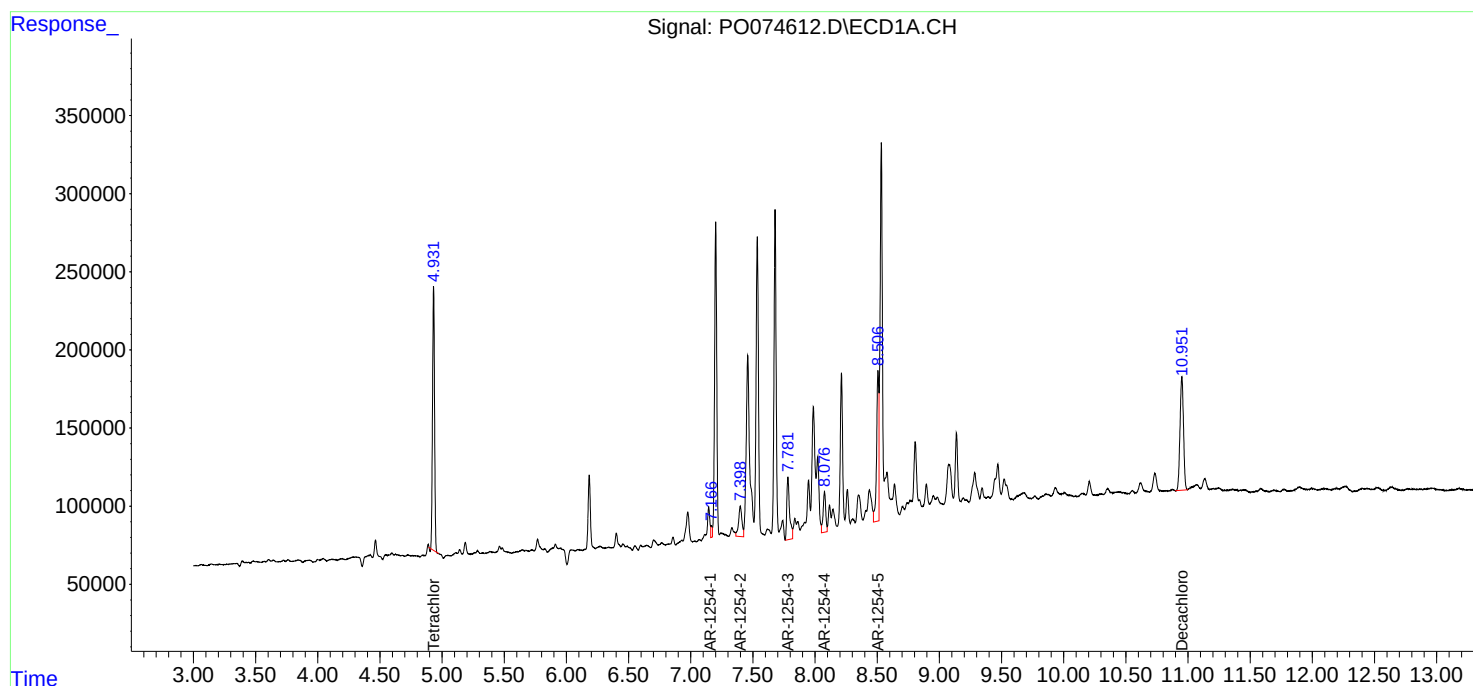

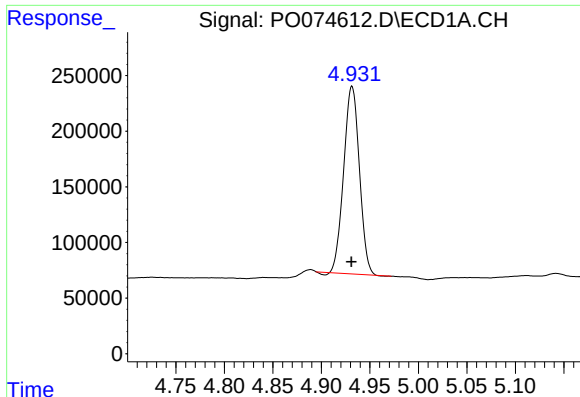


#1 Tetrachloro-m-xylene

R.T.: 4.932 min
Delta R.T.: 0.000 min
Response: 1896327
Conc: 17.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-27A


Manual Integrations
APPROVED

Ankita
1/15/2021 8:56:08 AM

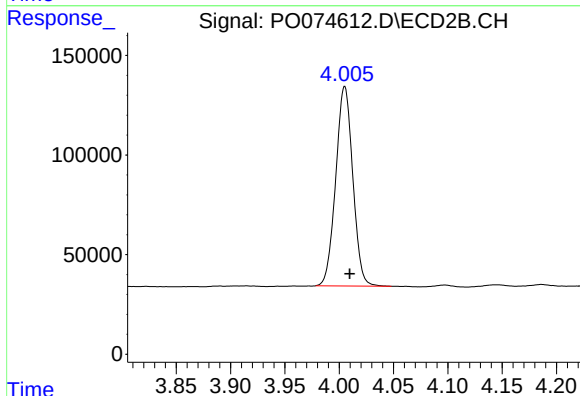


#1 Tetrachloro-m-xylene

R.T.: 4.005 min
Delta R.T.: -0.005 min
Response: 1094063
Conc: 19.45 ng/ml

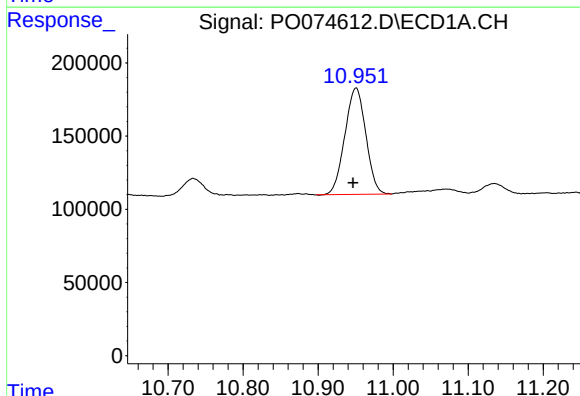


#2 Decachlorobiphenyl

R.T.: 10.951 min
Delta R.T.: 0.004 min
Response: 1413053
Conc: 13.92 ng/ml

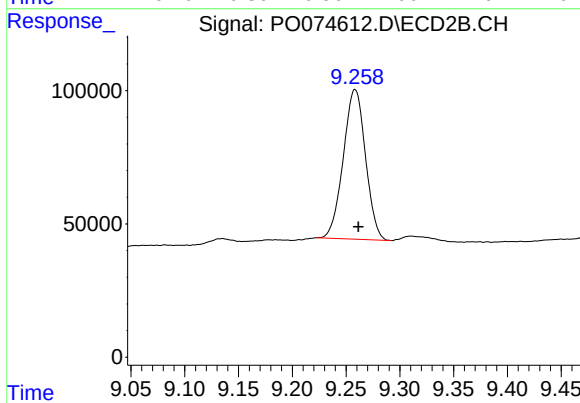

#2 Decachlorobiphenyl

R.T.: 9.258 min
Delta R.T.: -0.003 min
Response: 807433
Conc: 14.71 ng/ml

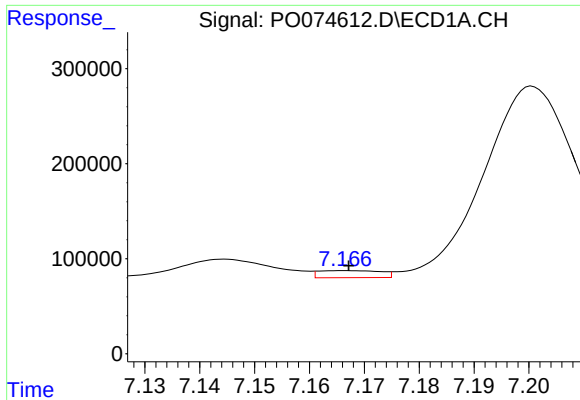


#26 AR-1254-1

R.T.: 7.167 min
Delta R.T.: 0.000 min
Response: 58508
Conc: 13.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-27A


Manual Integrations
APPROVED

Ankita
1/15/2021 8:56:08 AM

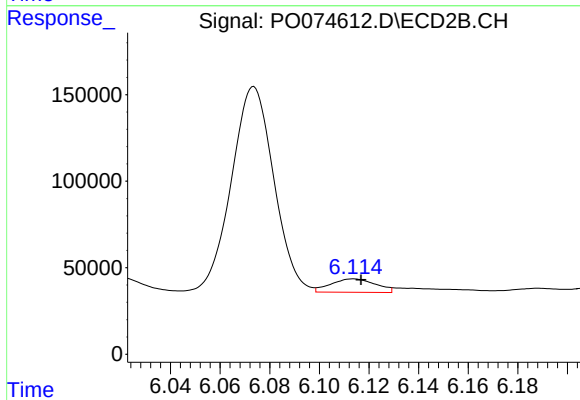


#26 AR-1254-1

R.T.: 6.114 min
Delta R.T.: -0.003 min
Response: 96483
Conc: 26.71 ng/ml m

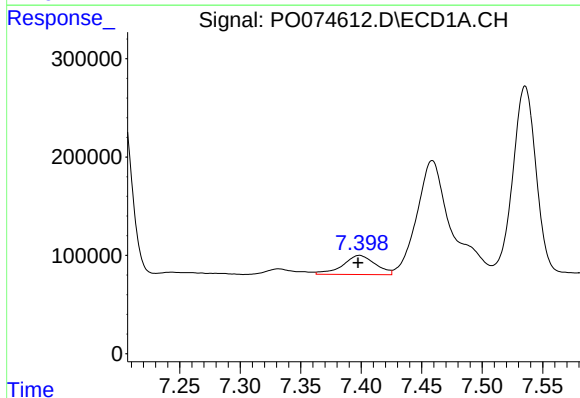


#27 AR-1254-2

R.T.: 7.399 min
Delta R.T.: 0.001 min
Response: 362530
Conc: 53.23 ng/ml

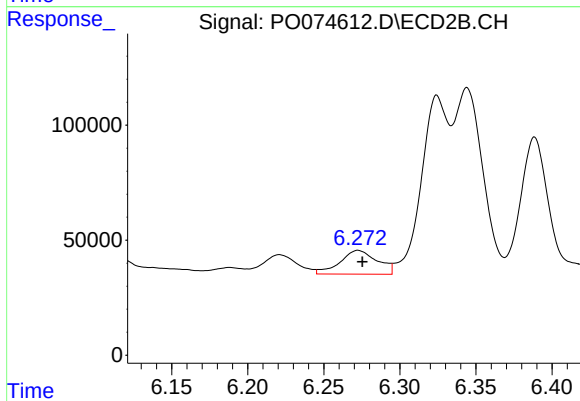

#27 AR-1254-2

R.T.: 6.273 min
Delta R.T.: -0.003 min
Response: 177201
Conc: 56.86 ng/ml

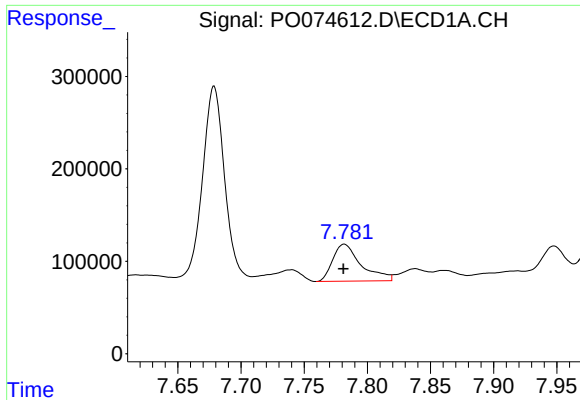


#28 AR-1254-3

R.T.: 7.782 min
Delta R.T.: 0.000 min
Response: 626360
Conc: 89.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-27A


Manual Integrations
APPROVED

Ankita
1/15/2021 8:56:08 AM

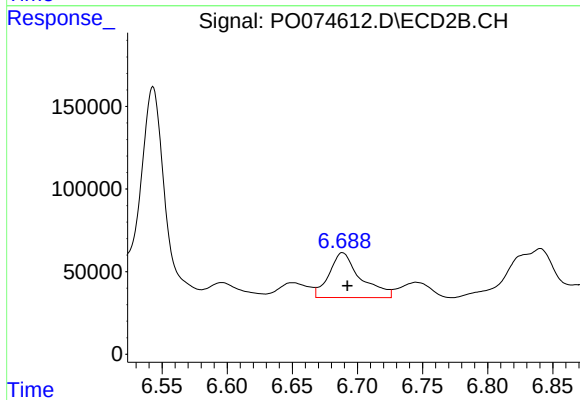


#28 AR-1254-3

R.T.: 6.689 min
Delta R.T.: -0.004 min
Response: 455315
Conc: 92.85 ng/ml

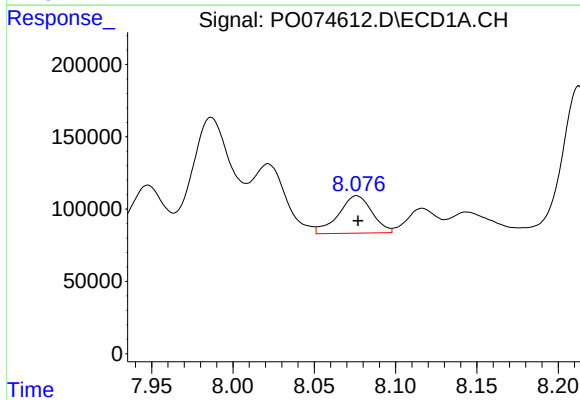


#29 AR-1254-4

R.T.: 8.076 min
Delta R.T.: 0.000 min
Response: 373587
Conc: 61.60 ng/ml

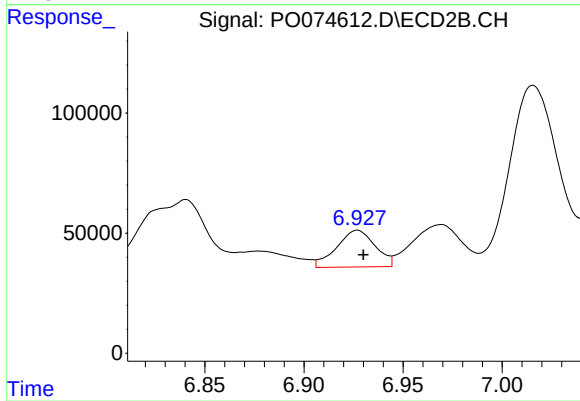

#29 AR-1254-4

R.T.: 6.927 min
Delta R.T.: -0.003 min
Response: 207450
Conc: 59.82 ng/ml

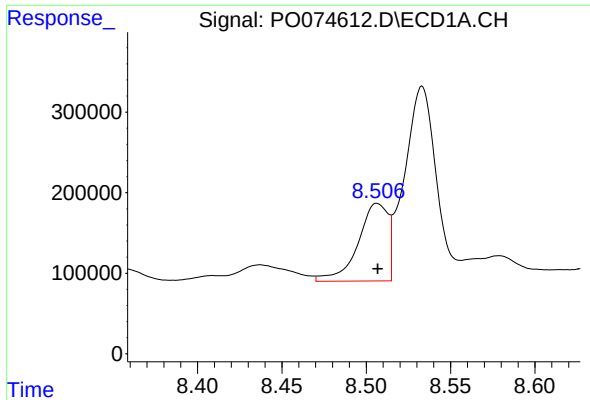


#30 AR-1254-5

R.T.: 8.506 min
Delta R.T.: 0.000 min
Response: 1193191
Conc: 205.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-27A

Manual Integrations
APPROVED

Ankita
1/15/2021 8:56:08 AM

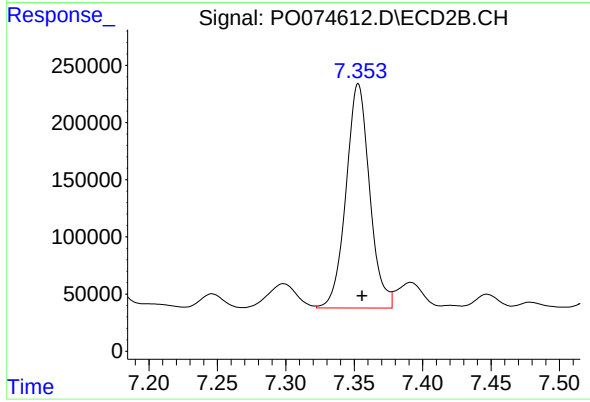

#30 AR-1254-5

R.T.: 7.353 min
Delta R.T.: -0.003 min
Response: 2356375
Conc: 520.64 ng/ml