

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011321\
 Data File : P0074625.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Jan 2021 22:36
 Operator : AJ/MA
 Sample : M1107-06 5X
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S19-06-B

Manual Integrations
 APPROVED

Ankita
 1/14/2021 2:19:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 14 00:30:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.932	4.004	456645	256949	4.328	4.568
2) SA Decachlor...	10.951	9.258	1407448	756466	13.868	13.778
Target Compounds						
41) L9 AR-1268-1	9.448	8.184	4146117	2333622	221.914	208.457
42) L9 AR-1268-2	9.544	8.249	3079822	1809817	193.033	189.169
43) L9 AR-1268-3	9.769	8.454	2556320	1443219	179.997	173.696
44) L9 AR-1268-4	10.206	8.741	956926	551122	163.339	158.864
45) L9 AR-1268-5	10.618	9.018	7320794	3901307	175.188	164.759

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011321\
Data File : P0074625.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jan 2021 22:36
Operator : AJ/MA
Sample : M1107-06 5X
Misc :
ALS Vial : 46 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S19-06-B


Manual Integrations
APPROVED

Ankita
1/14/2021 2:19:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 14 00:30:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

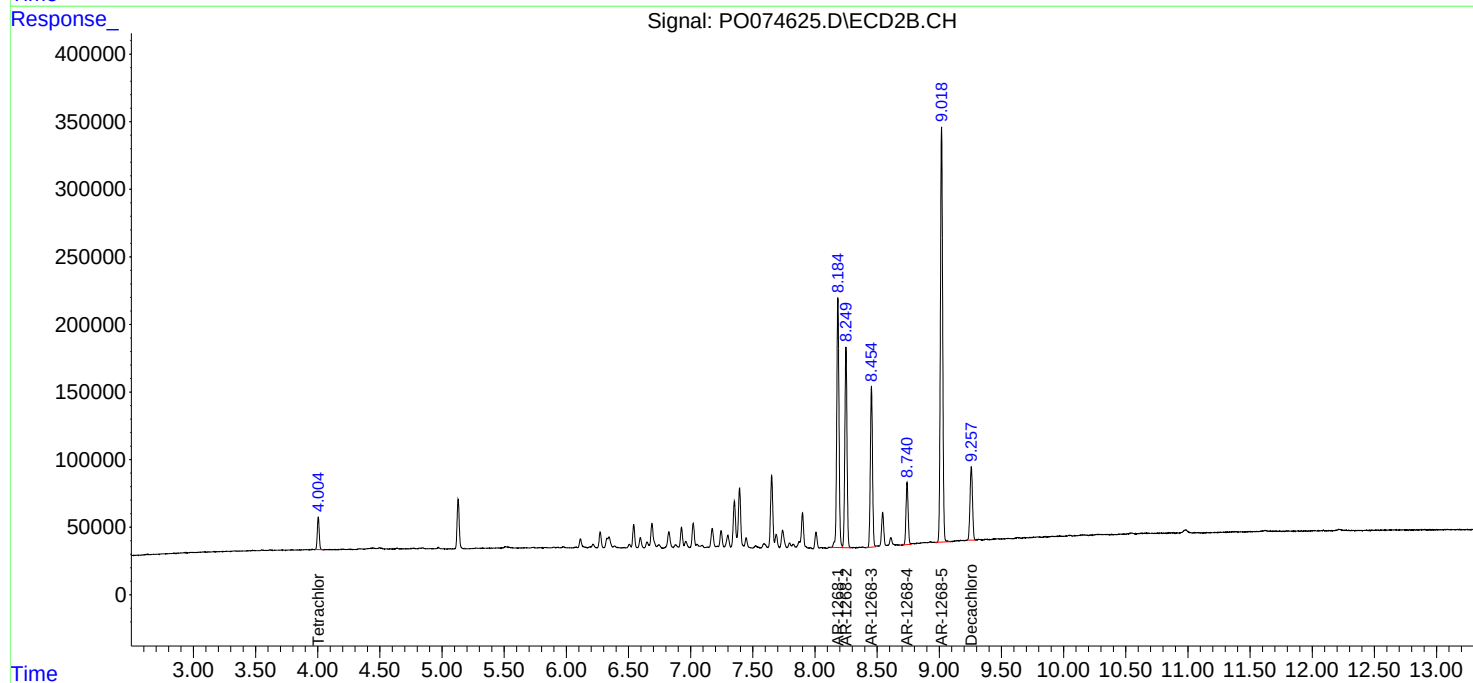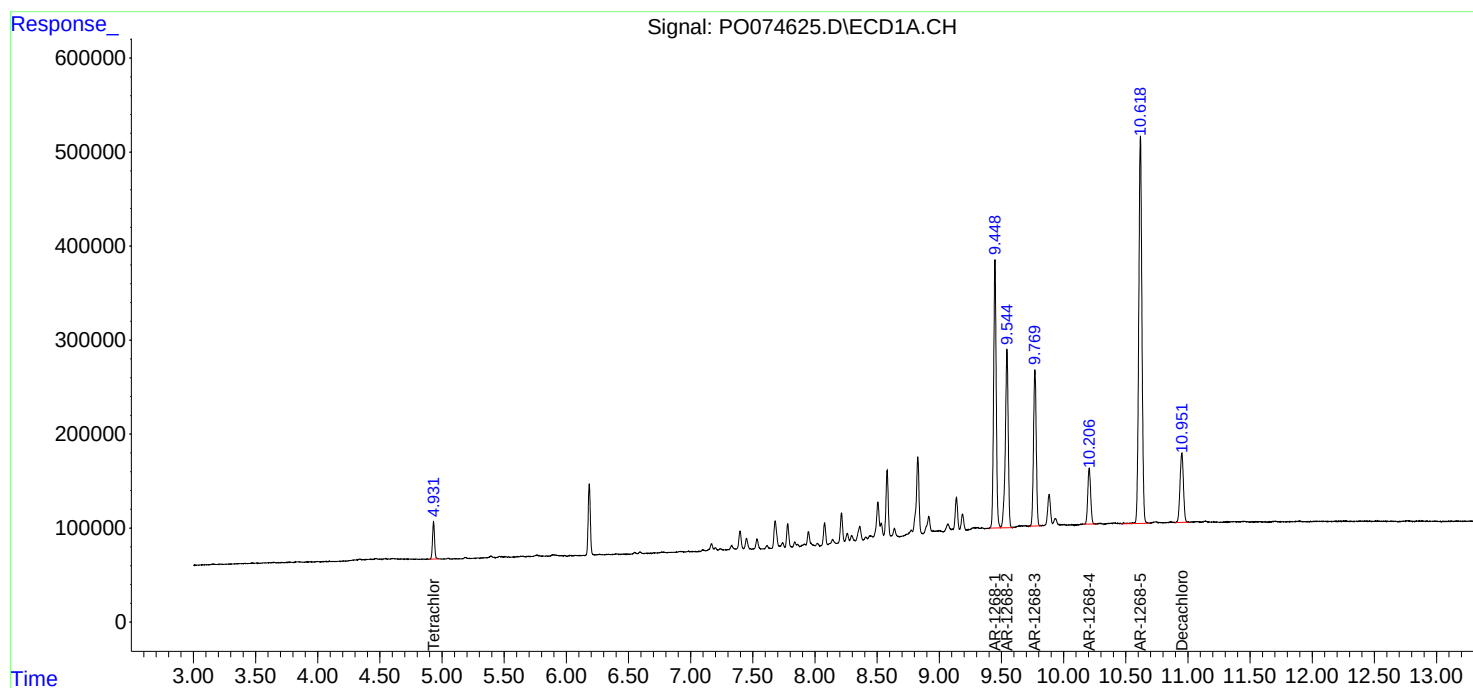

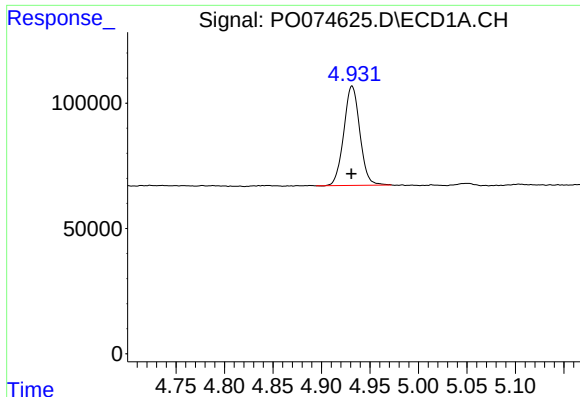


#1 Tetrachloro-m-xylene

R.T.: 4.932 min
Delta R.T.: 0.000 min
Response: 456645
Conc: 4.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
S19-06-B


Manual Integrations
APPROVED

Ankita
1/14/2021 2:19:55 PM

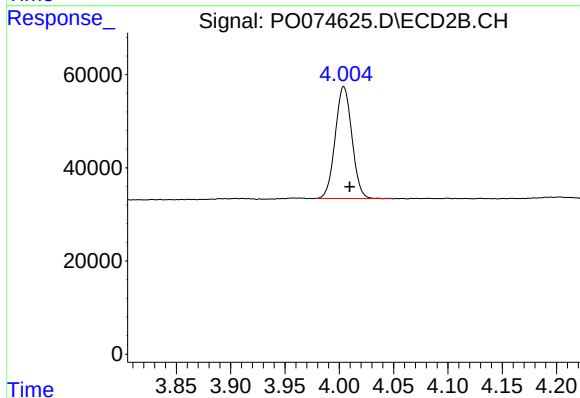


#1 Tetrachloro-m-xylene

R.T.: 4.004 min
Delta R.T.: -0.006 min
Response: 256949
Conc: 4.57 ng/ml

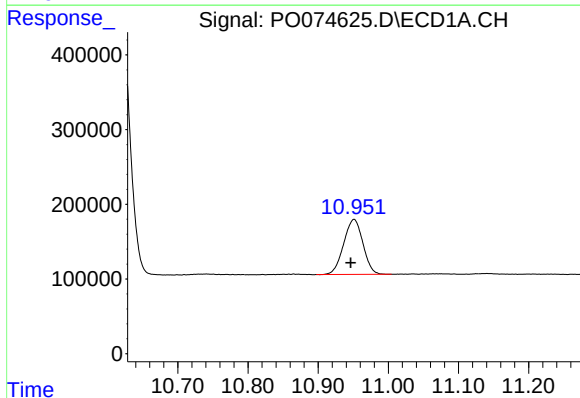


#2 Decachlorobiphenyl

R.T.: 10.951 min
Delta R.T.: 0.005 min
Response: 1407448
Conc: 13.87 ng/ml

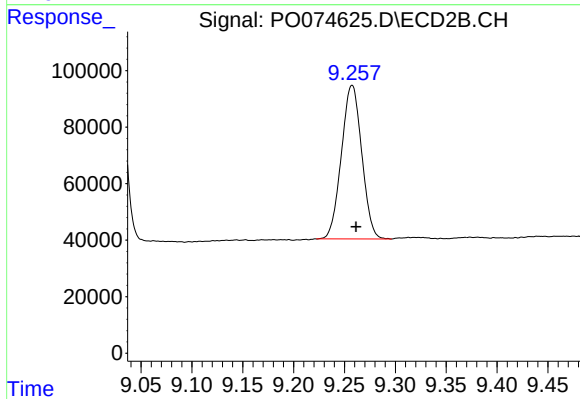

#2 Decachlorobiphenyl

R.T.: 9.258 min
Delta R.T.: -0.004 min
Response: 756466
Conc: 13.78 ng/ml

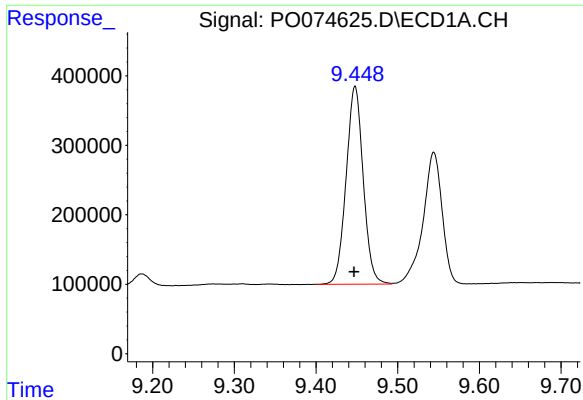


#41 AR-1268-1

R.T.: 9.448 min
Delta R.T.: 0.001 min
Response: 4146117
Conc: 221.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
S19-06-B


Manual Integrations
APPROVED

Ankita
1/14/2021 2:19:55 PM

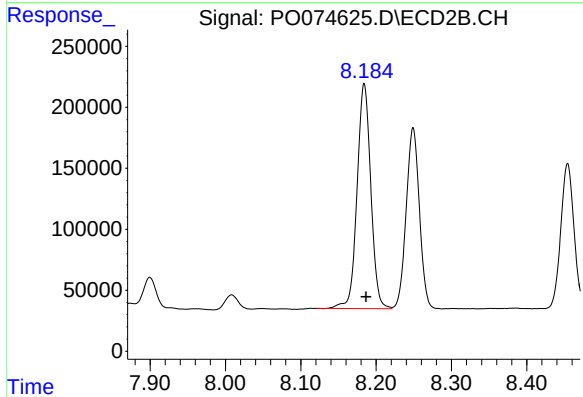


#41 AR-1268-1

R.T.: 8.184 min
Delta R.T.: -0.003 min
Response: 2333622
Conc: 208.46 ng/ml

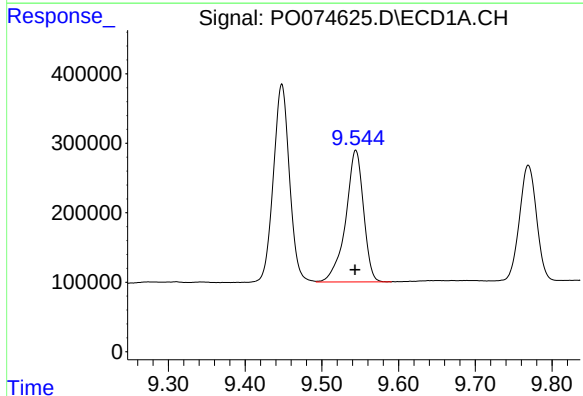


#42 AR-1268-2

R.T.: 9.544 min
Delta R.T.: 0.000 min
Response: 3079822
Conc: 193.03 ng/ml

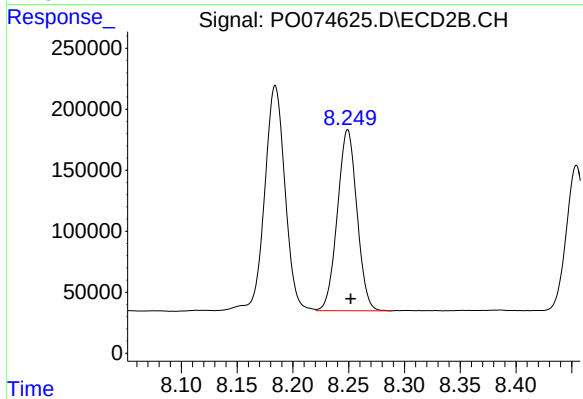

#42 AR-1268-2

R.T.: 8.249 min
Delta R.T.: -0.003 min
Response: 1809817
Conc: 189.17 ng/ml

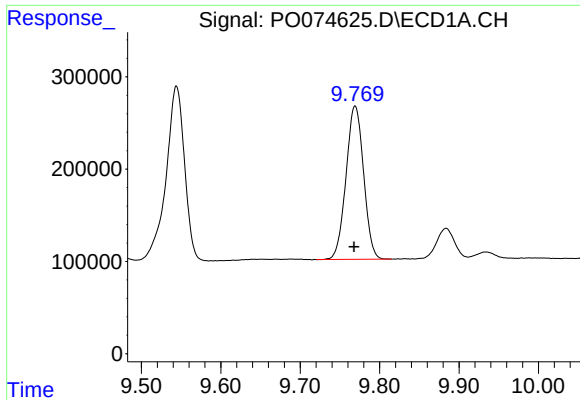


#43 AR-1268-3

R.T.: 9.769 min
Delta R.T.: 0.001 min
Response: 2556320
Conc: 180.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
S19-06-B


Manual Integrations
APPROVED

Ankita
1/14/2021 2:19:55 PM

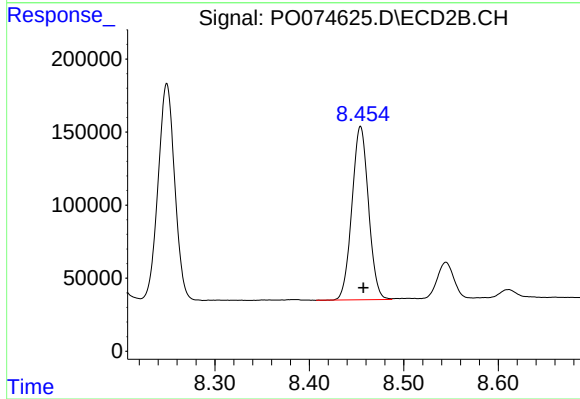


#43 AR-1268-3

R.T.: 8.454 min
Delta R.T.: -0.003 min
Response: 1443219
Conc: 173.70 ng/ml

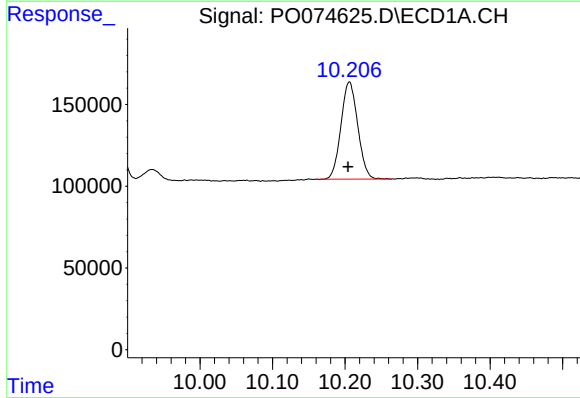


#44 AR-1268-4

R.T.: 10.206 min
Delta R.T.: 0.002 min
Response: 956926
Conc: 163.34 ng/ml

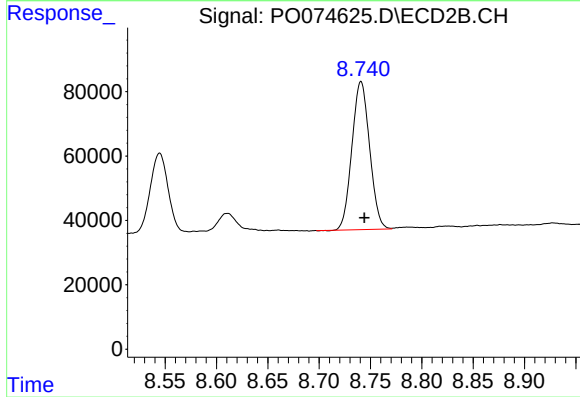

#44 AR-1268-4

R.T.: 8.741 min
Delta R.T.: -0.003 min
Response: 551122
Conc: 158.86 ng/ml

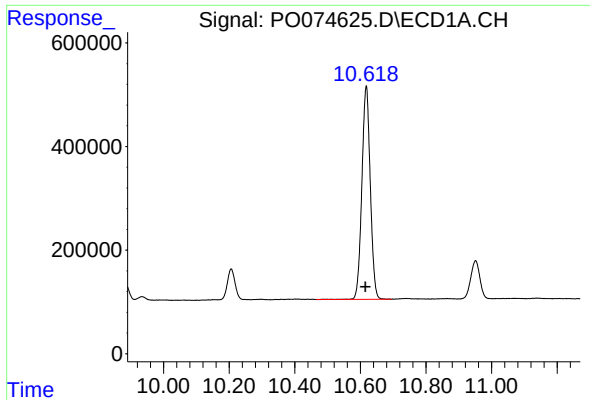


#45 AR-1268-5

R.T.: 10.618 min
Delta R.T.: 0.002 min
Response: 7320794
Conc: 175.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
S19-06-B

Manual Integrations
APPROVED

Ankita
1/14/2021 2:19:55 PM

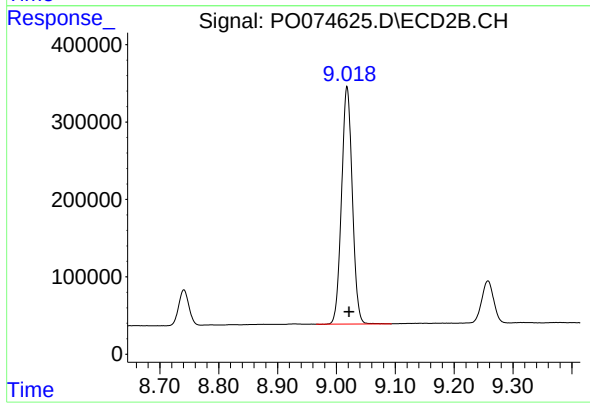

#45 AR-1268-5

R.T.: 9.018 min
Delta R.T.: -0.003 min
Response: 3901307
Conc: 164.76 ng/ml