

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011321\
 Data File : P0074627.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Jan 2021 23:10
 Operator : AJ/MA
 Sample : M1107-16 5X
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DUP-37

Manual Integrations
 APPROVED

Ankita
 1/14/2021 2:19:57 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 14 00:31:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.932	4.004	486233	277316	4.608	4.930
2) SA Decachlor...	10.950	9.258	1249512	681288	12.311	12.409
Target Compounds						
41) L9 AR-1268-1	9.448	8.185	4312232	2423510	230.805	216.486
42) L9 AR-1268-2	9.544	8.249	2806690	1641810	175.914	171.608
43) L9 AR-1268-3	9.769	8.454	3188471	1815119	224.509	218.456
44) L9 AR-1268-4	10.207	8.741	813309	478003	138.824	137.787
45) L9 AR-1268-5	10.618	9.019	8572661	4579122	205.145	193.385

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011321\
Data File : PO074627.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jan 2021 23:10
Operator : AJ/MA
Sample : M1107-16 5X
Misc :
ALS Vial : 48 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
DUP-37


Manual Integrations
APPROVED

Ankita
1/14/2021 2:19:57 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 14 00:31:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

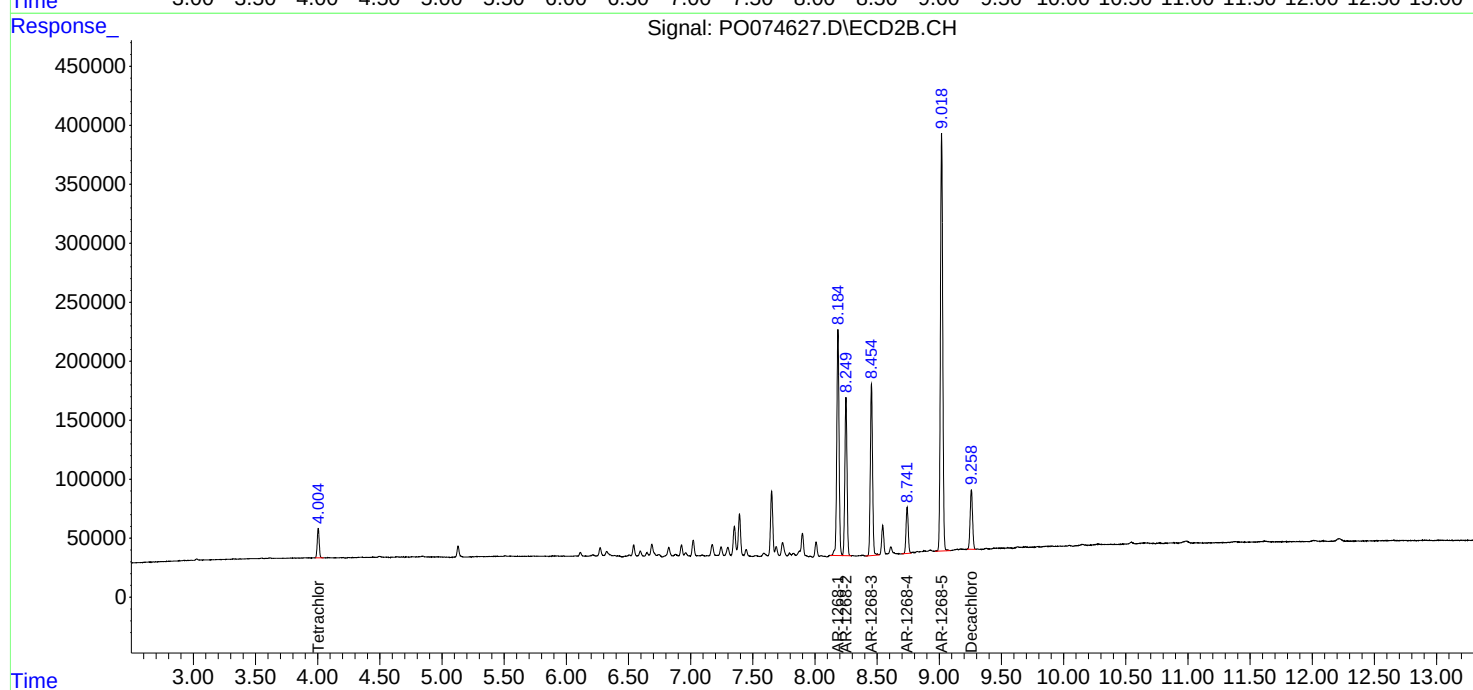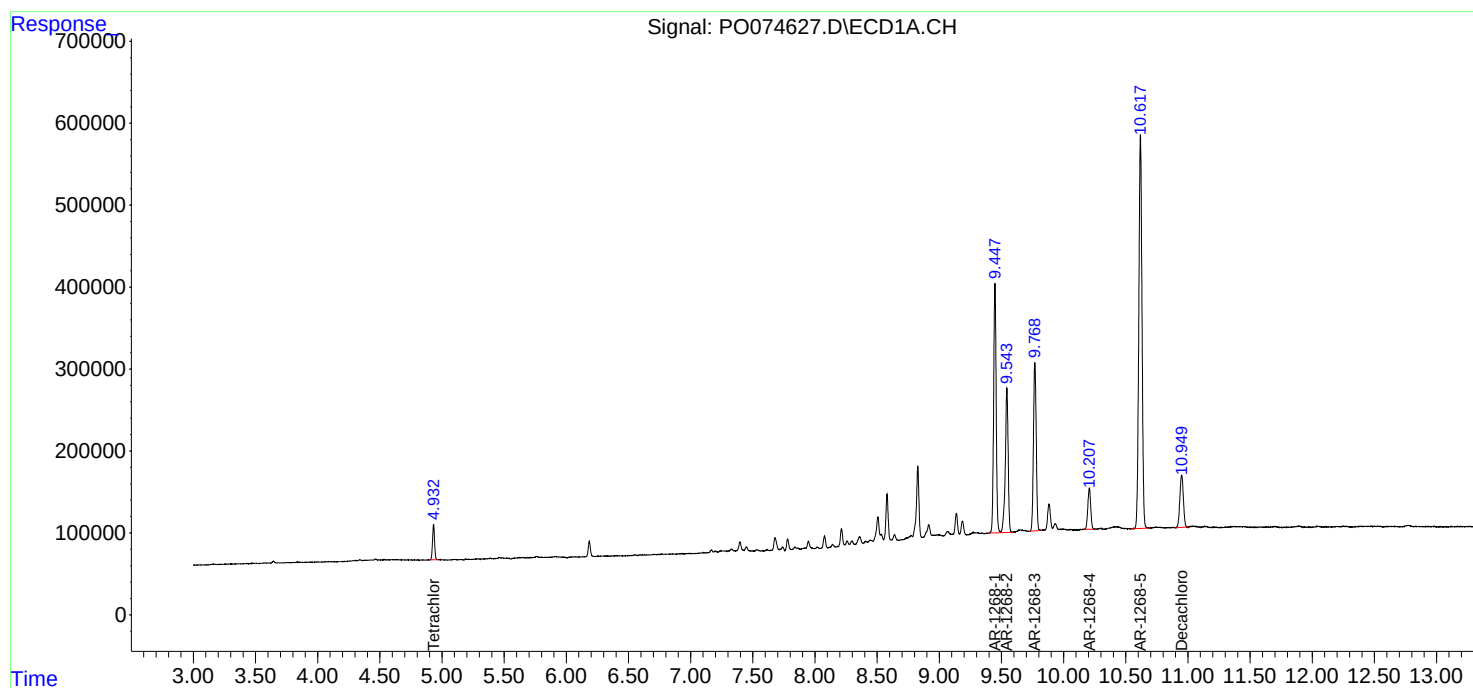

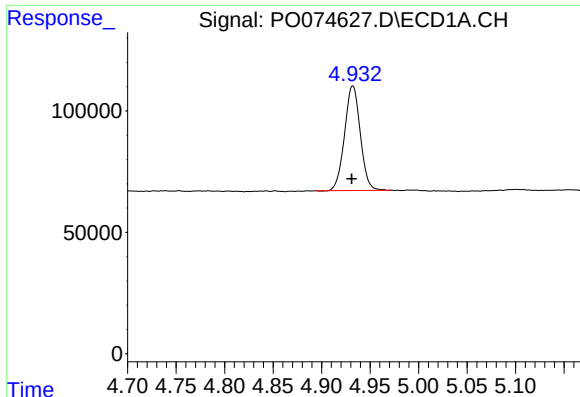


#1 Tetrachloro-m-xylene

R.T.: 4.932 min
Delta R.T.: 0.001 min
Response: 486233
Conc: 4.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
DUP-37


Manual Integrations
APPROVED

Ankita
1/14/2021 2:19:57 PM

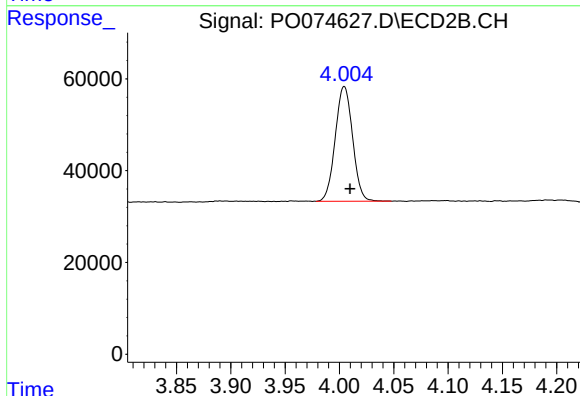


#1 Tetrachloro-m-xylene

R.T.: 4.004 min
Delta R.T.: -0.005 min
Response: 277316
Conc: 4.93 ng/ml

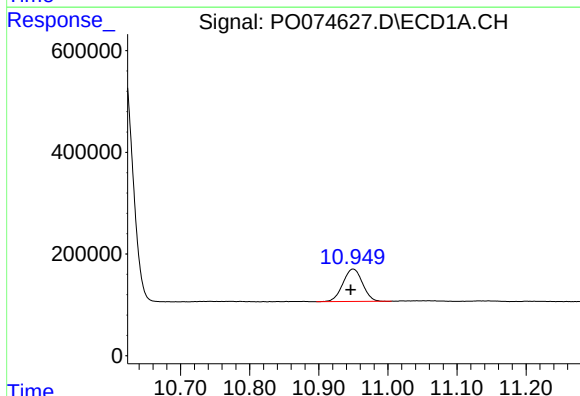


#2 Decachlorobiphenyl

R.T.: 10.950 min
Delta R.T.: 0.003 min
Response: 1249512
Conc: 12.31 ng/ml

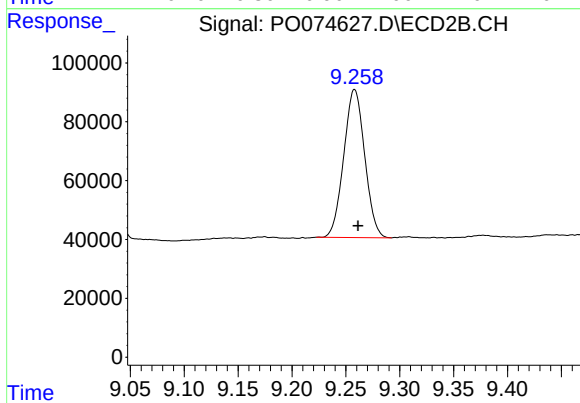

#2 Decachlorobiphenyl

R.T.: 9.258 min
Delta R.T.: -0.003 min
Response: 681288
Conc: 12.41 ng/ml

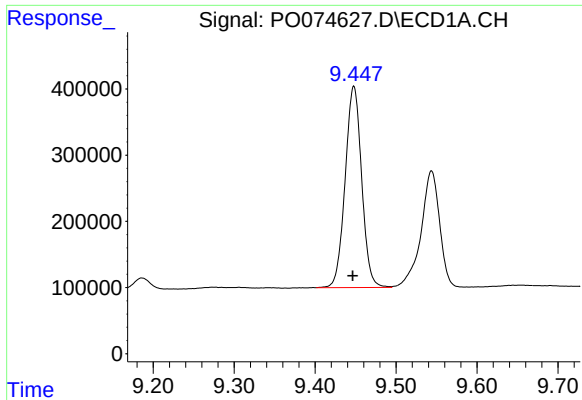


#41 AR-1268-1

R.T.: 9.448 min
Delta R.T.: 0.001 min
Response: 4312232
Conc: 230.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
DUP-37


Manual Integrations
APPROVED

Ankita
1/14/2021 2:19:57 PM

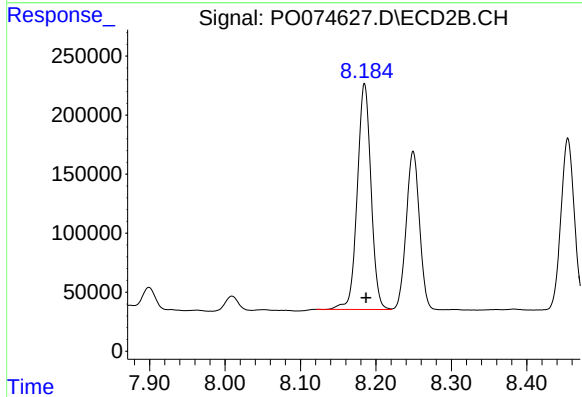


#41 AR-1268-1

R.T.: 8.185 min
Delta R.T.: -0.002 min
Response: 2423510
Conc: 216.49 ng/ml

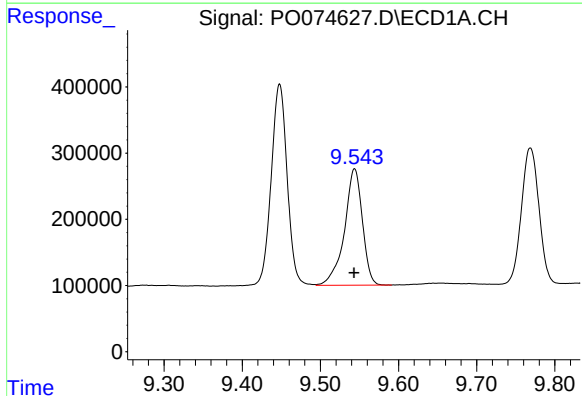


#42 AR-1268-2

R.T.: 9.544 min
Delta R.T.: 0.000 min
Response: 2806690
Conc: 175.91 ng/ml

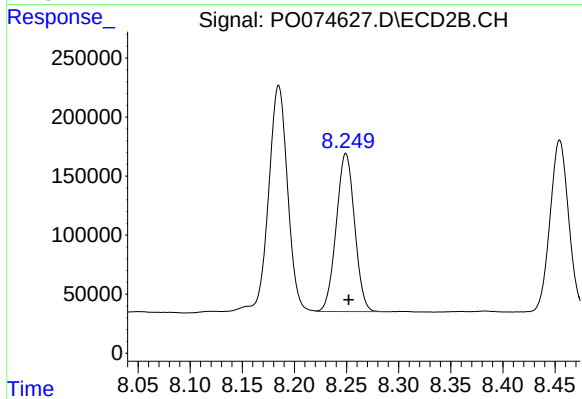

#42 AR-1268-2

R.T.: 8.249 min
Delta R.T.: -0.003 min
Response: 1641810
Conc: 171.61 ng/ml

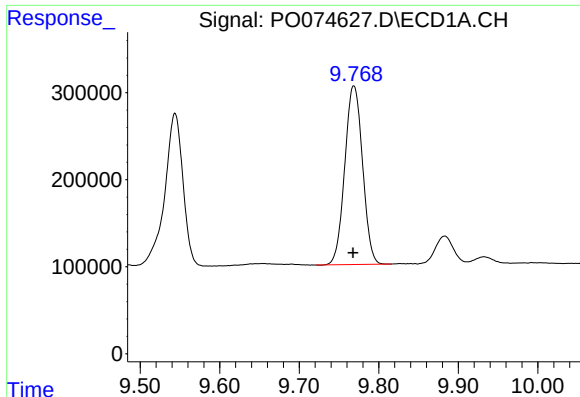


#43 AR-1268-3

R.T.: 9.769 min
Delta R.T.: 0.000 min
Response: 3188471
Conc: 224.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
DUP-37


Manual Integrations
APPROVED

Ankita
1/14/2021 2:19:57 PM

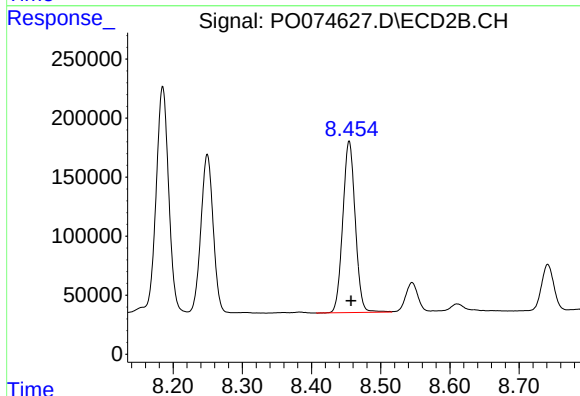


#43 AR-1268-3

R.T.: 8.454 min
Delta R.T.: -0.003 min
Response: 1815119
Conc: 218.46 ng/ml

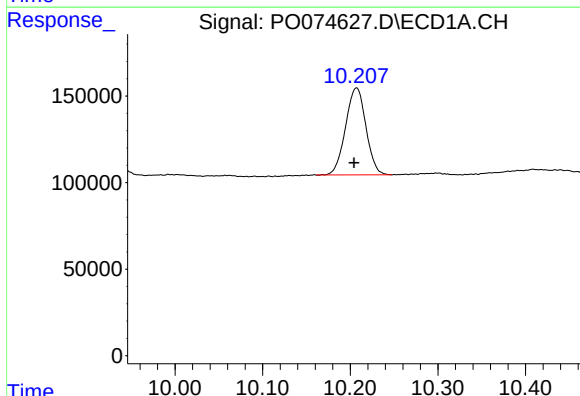


#44 AR-1268-4

R.T.: 10.207 min
Delta R.T.: 0.003 min
Response: 813309
Conc: 138.82 ng/ml

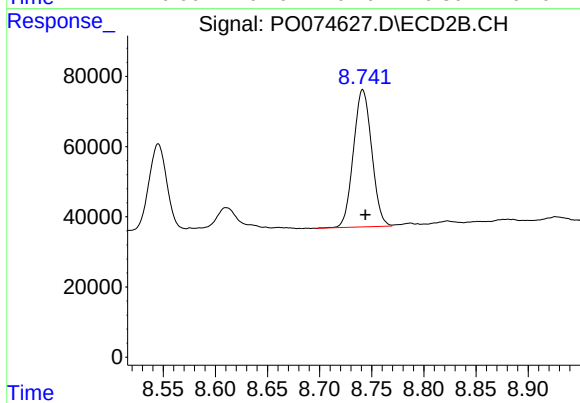

#44 AR-1268-4

R.T.: 8.741 min
Delta R.T.: -0.003 min
Response: 478003
Conc: 137.79 ng/ml

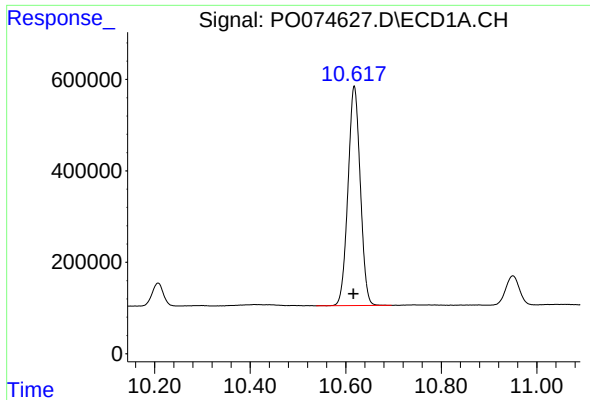


#45 AR-1268-5

R.T.: 10.618 min
Delta R.T.: 0.002 min
Response: 8572661
Conc: 205.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
DUP-37

Manual Integrations
APPROVED

Ankita
1/14/2021 2:19:57 PM

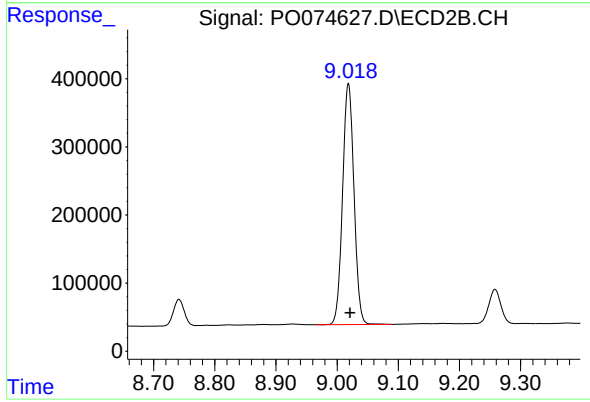

#45 AR-1268-5

R.T.: 9.019 min
Delta R.T.: -0.003 min
Response: 4579122
Conc: 193.38 ng/ml