

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011322\
 Data File : P0084233.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Jan 2022 2:20
 Operator : AJ\MA
 Sample : AR1254ICC750
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC750

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/14/2022
 Supervised By :mohammad ahmed 01/14/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 14 03:05:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011322.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 14 02:57:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	6.522	5.309	6953898	1673060	71.579	71.717
2)	SA Decachlor...	13.778	11.320	4405281	1409518	75.962	76.905
Target Compounds							
26)	L6 AR-1254-1	8.943	7.740	2293616	814854	738.918m	736.380
27)	L6 AR-1254-2	9.181	7.908	3109451	700371	727.870	740.413
28)	L6 AR-1254-3	9.580	8.362	3200979	1137102	733.595	742.661
29)	L6 AR-1254-4	9.898	8.610	2309768	721477	739.350	747.361
30)	L6 AR-1254-5	10.398	9.062	2885668	982033	744.694	754.970

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011322\
Data File : PO084233.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jan 2022 2:20
Operator : AJ\MA
Sample : AR1254ICC750
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1254ICC750


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/14/2022
Supervised By :mohammad ahmed 01/14/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 14 03:05:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011322.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 14 02:57:46 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

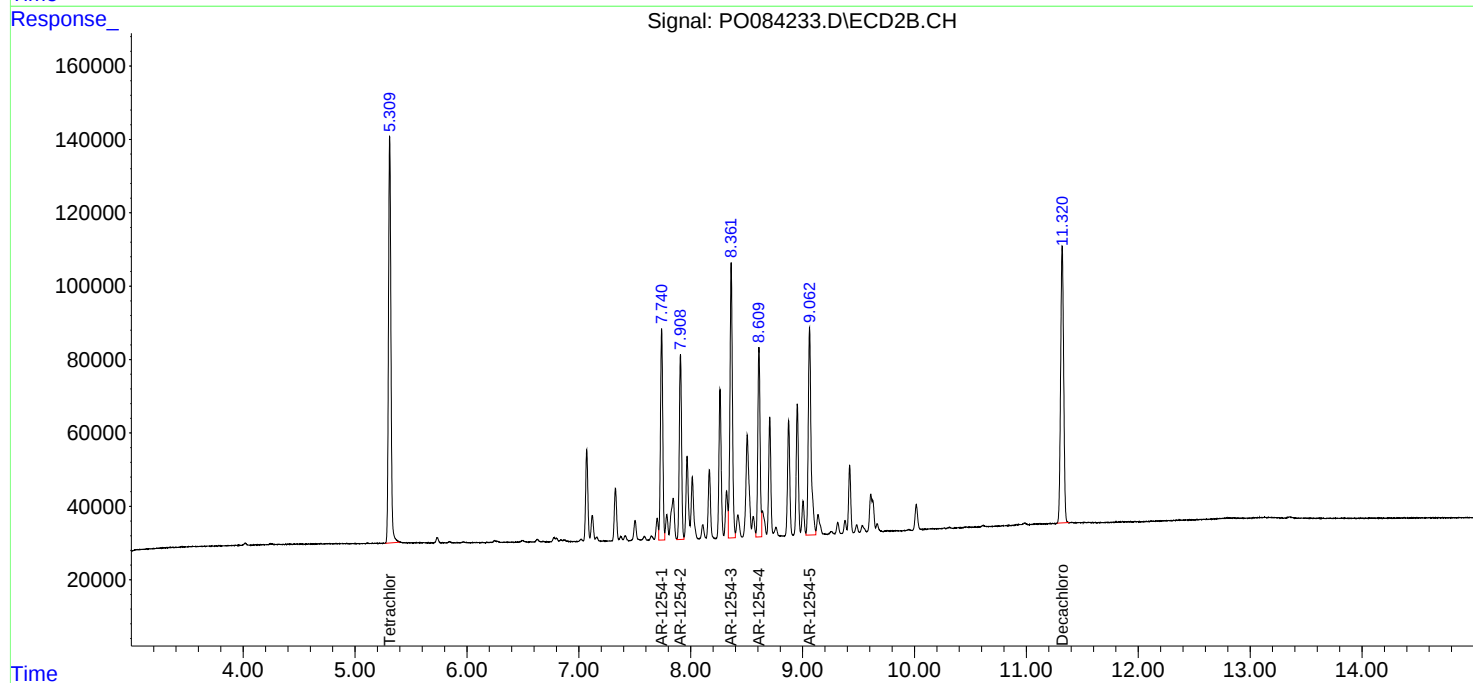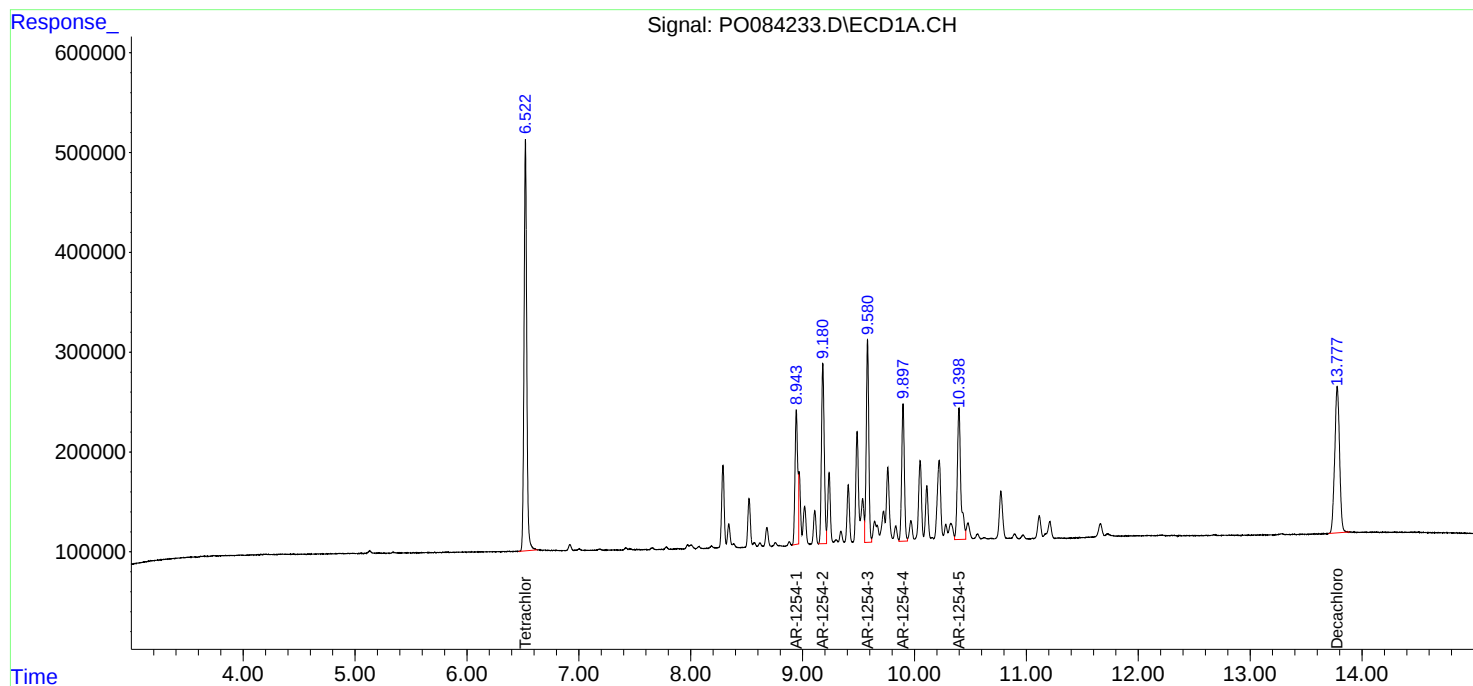

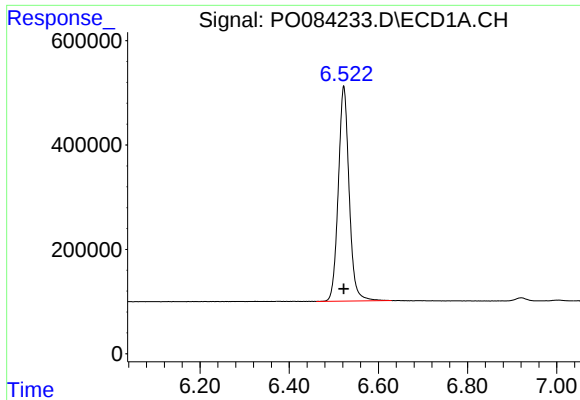


#1 Tetrachloro-m-xylene

R.T.: 6.522 min
Delta R.T.: 0.000 min
Response: 6953898
Conc: 71.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254ICC750


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/14/2022
Supervised By :mohammad ahmed 01/14/2022

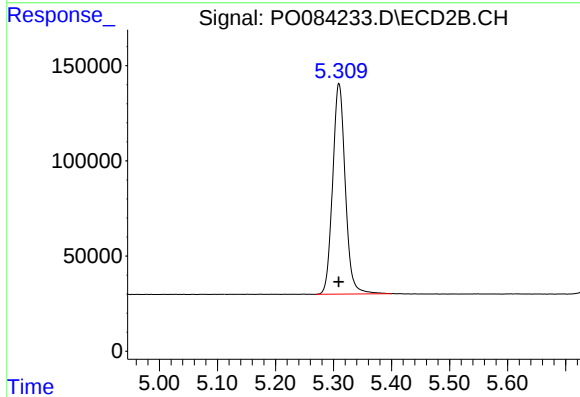


#1 Tetrachloro-m-xylene

R.T.: 5.309 min
Delta R.T.: 0.000 min
Response: 1673060
Conc: 71.72 ng/ml

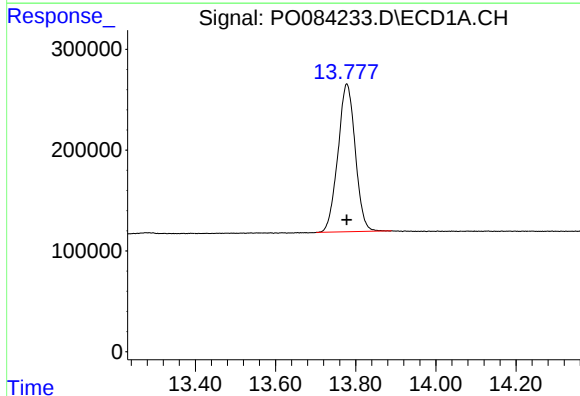


#2 Decachlorobiphenyl

R.T.: 13.778 min
Delta R.T.: 0.000 min
Response: 4405281
Conc: 75.96 ng/ml

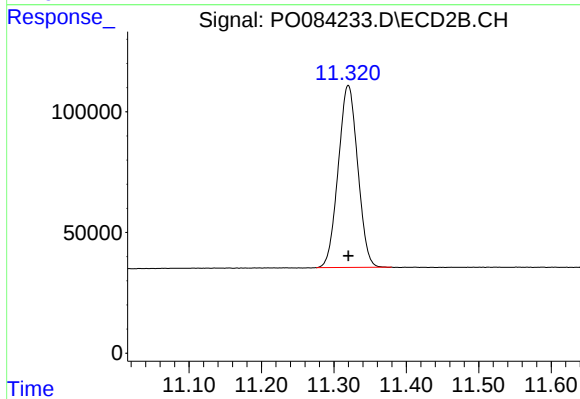

#2 Decachlorobiphenyl

R.T.: 11.320 min
Delta R.T.: 0.000 min
Response: 1409518
Conc: 76.90 ng/ml

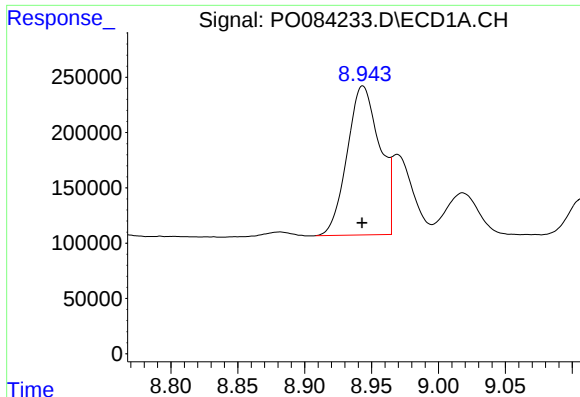


#26 AR-1254-1

R.T.: 8.943 min
Delta R.T.: 0.000 min
Response: 2293616
Conc: 738.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254ICC750


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/14/2022
Supervised By :mohammad ahmed 01/14/2022

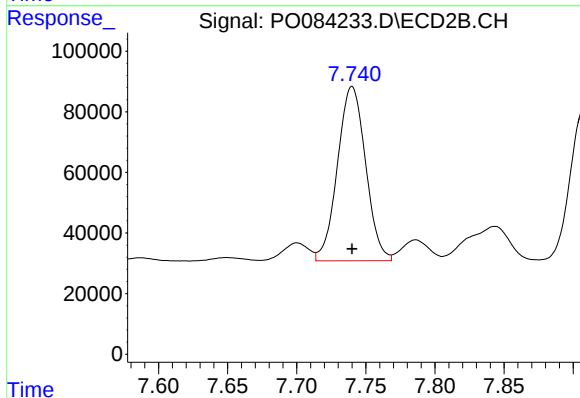


#26 AR-1254-1

R.T.: 7.740 min
Delta R.T.: 0.000 min
Response: 814854
Conc: 736.38 ng/ml

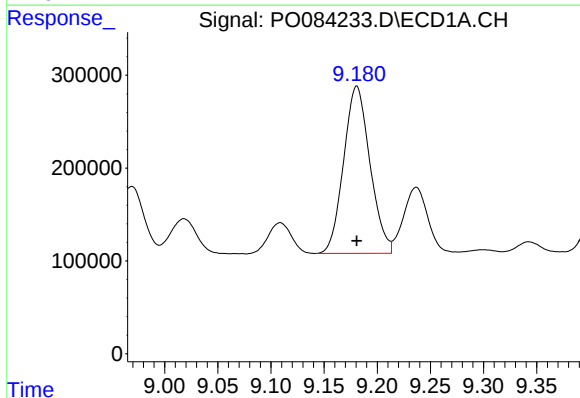


#27 AR-1254-2

R.T.: 9.181 min
Delta R.T.: 0.000 min
Response: 3109451
Conc: 727.87 ng/ml

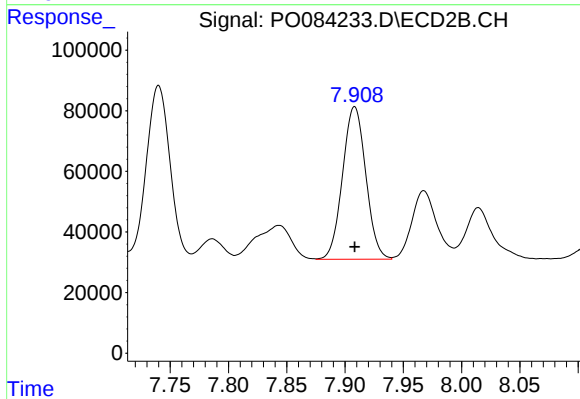

#27 AR-1254-2

R.T.: 7.908 min
Delta R.T.: 0.000 min
Response: 700371
Conc: 740.41 ng/ml

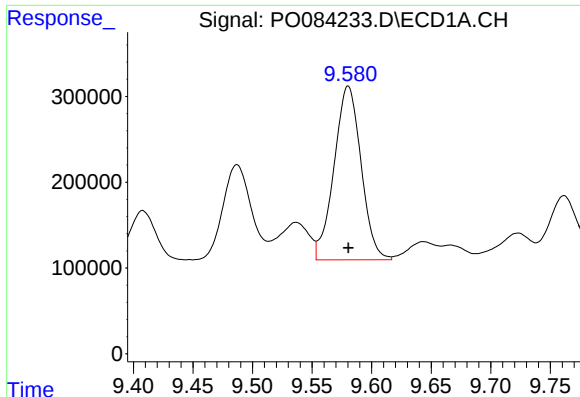


#28 AR-1254-3

R.T.: 9.580 min
Delta R.T.: 0.000 min
Response: 3200979
Conc: 733.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254ICC750


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/14/2022
Supervised By :mohammad ahmed 01/14/2022

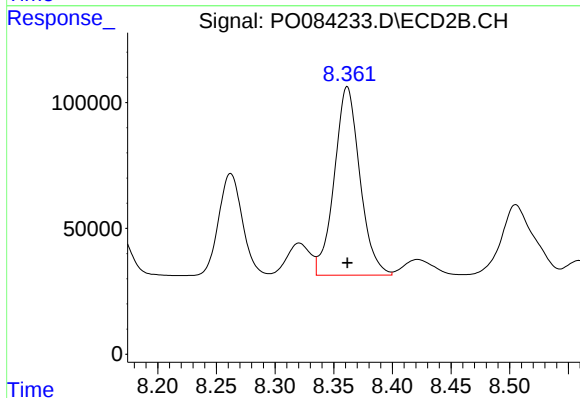


#28 AR-1254-3

R.T.: 8.362 min
Delta R.T.: 0.000 min
Response: 1137102
Conc: 742.66 ng/ml

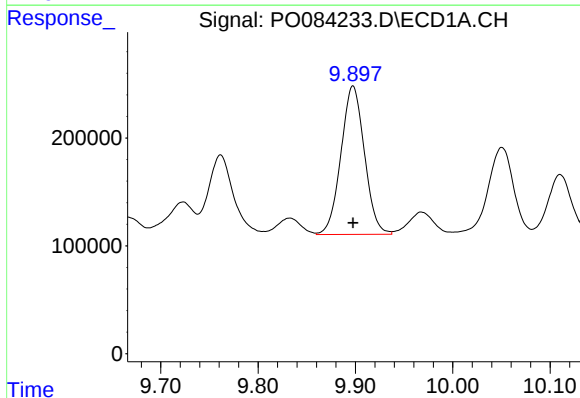


#29 AR-1254-4

R.T.: 9.898 min
Delta R.T.: 0.000 min
Response: 2309768
Conc: 739.35 ng/ml

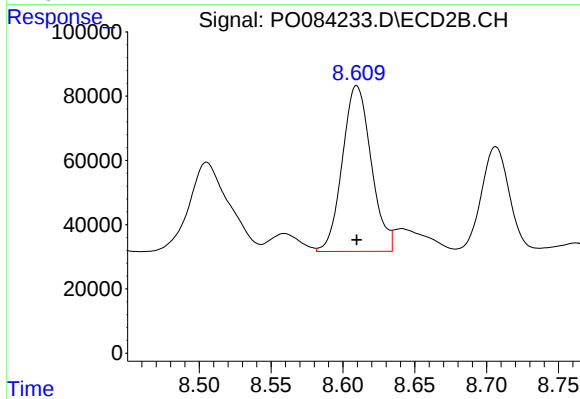

#29 AR-1254-4

R.T.: 8.610 min
Delta R.T.: 0.000 min
Response: 721477
Conc: 747.36 ng/ml

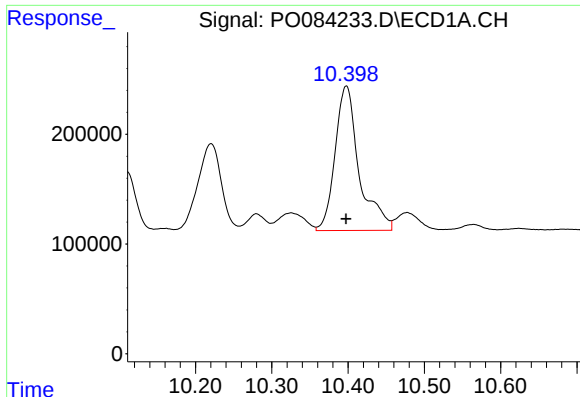


#30 AR-1254-5

R.T.: 10.398 min
Delta R.T.: 0.000 min
Response: 2885668
Conc: 744.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254ICC750

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/14/2022
Supervised By :mohammad ahmed 01/14/2022

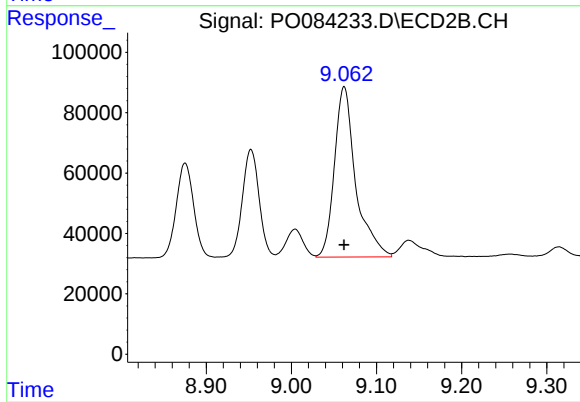

#30 AR-1254-5

R.T.: 9.062 min
Delta R.T.: 0.000 min
Response: 982033
Conc: 754.97 ng/ml