

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011322\
 Data File : P0084236.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Jan 2022 3:16
 Operator : AJ\MA
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC050

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/14/2022
 Supervised By :mohammad ahmed 01/14/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 14 03:39:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011322.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 14 03:38:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	6.522	5.308	615122	122688	6.016	5.285
2) SA Decachlor...	13.777	11.319	320547	93416	5.317	5.017
Target Compounds						
26) L6 AR-1254-1	8.945	7.741	218293	67388	63.087m	58.238
27) L6 AR-1254-2	9.181	7.908	281185	57804	61.249	58.221
28) L6 AR-1254-3	9.580	8.362	320873	93092	66.201	58.038
29) L6 AR-1254-4	9.897	8.611	217450	56874	63.732	56.353
30) L6 AR-1254-5	10.397	9.062	277045	81251	64.928	59.098

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011322\
Data File : P0084236.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jan 2022 3:16
Operator : AJ\MA
Sample : AR1254ICC050
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/14/2022
Supervised By :mohammad ahmed 01/14/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 14 03:39:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011322.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 14 03:38:49 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

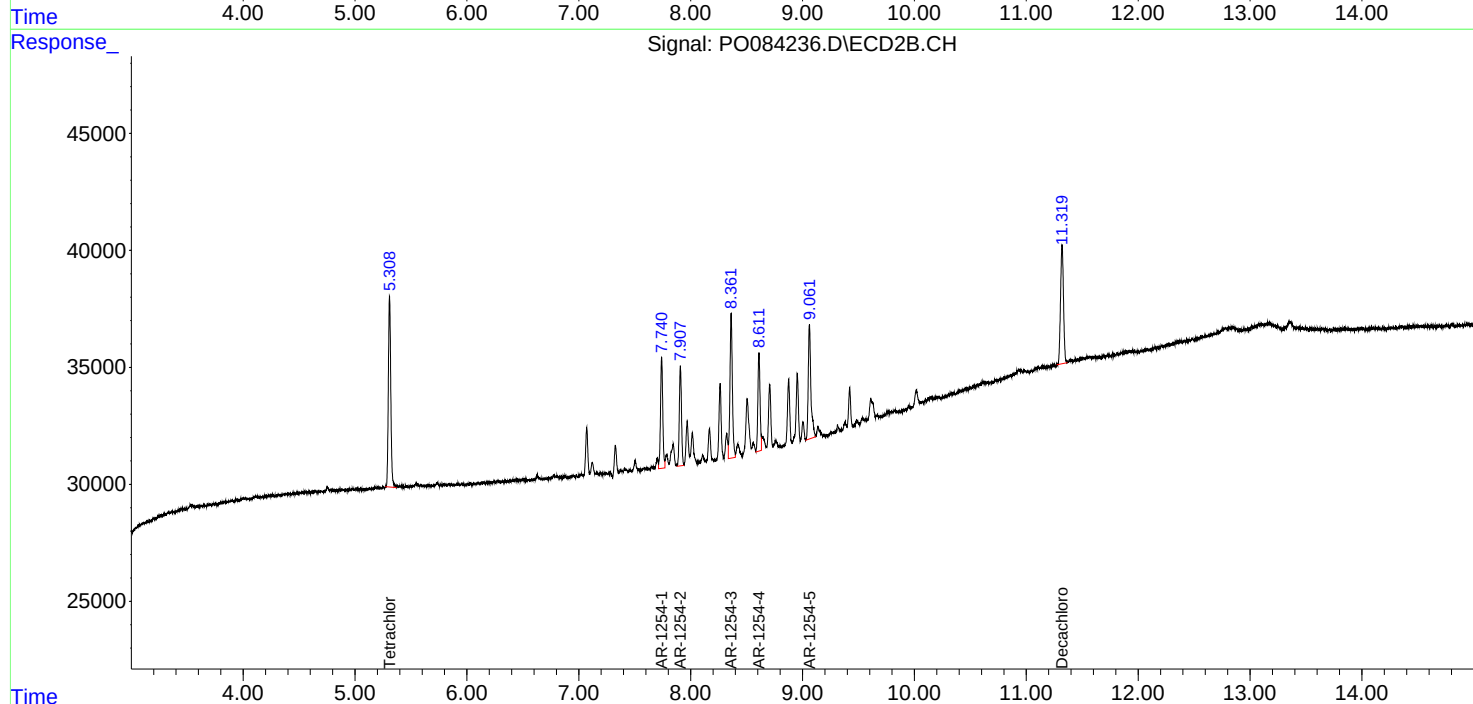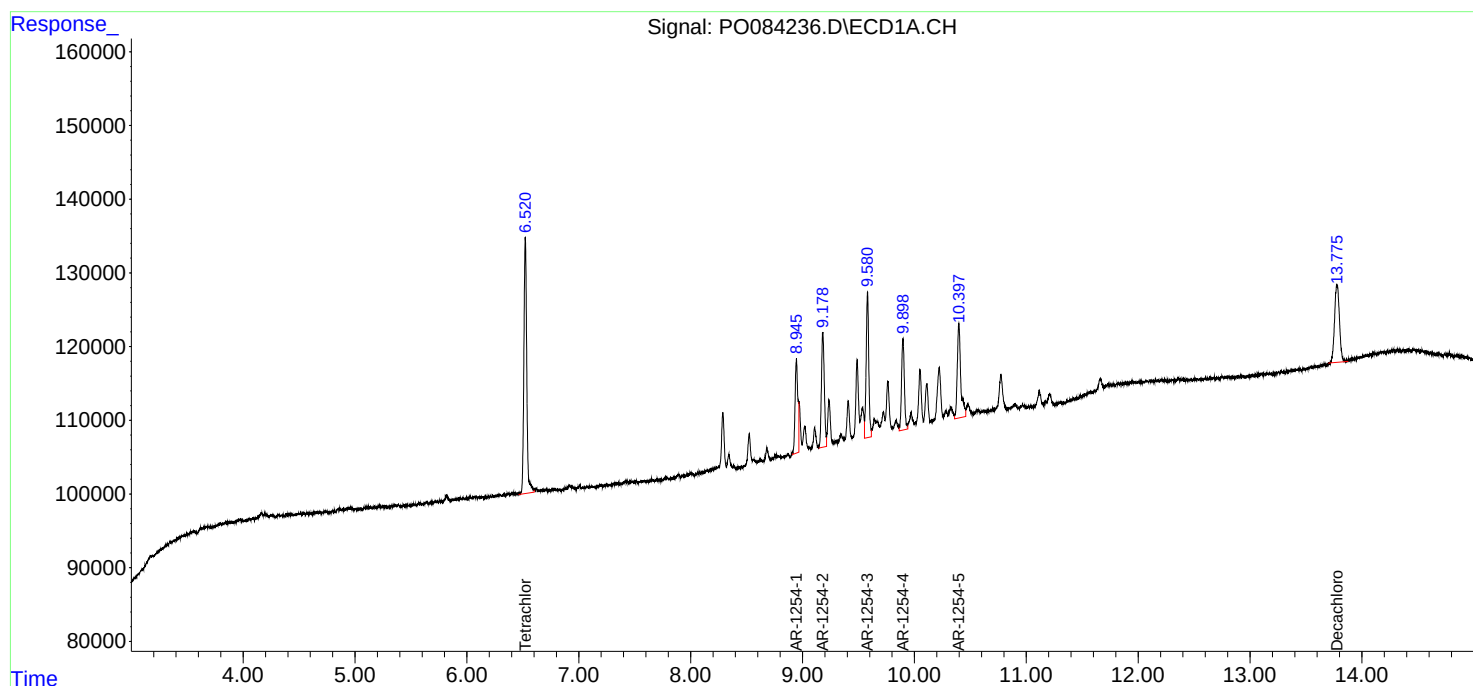

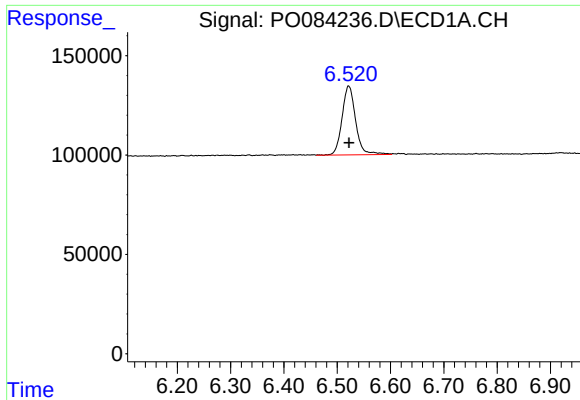


#1 Tetrachloro-m-xylene

R.T.: 6.522 min
Delta R.T.: 0.000 min
Response: 615122
Conc: 6.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/14/2022
Supervised By :mohammad ahmed 01/14/2022

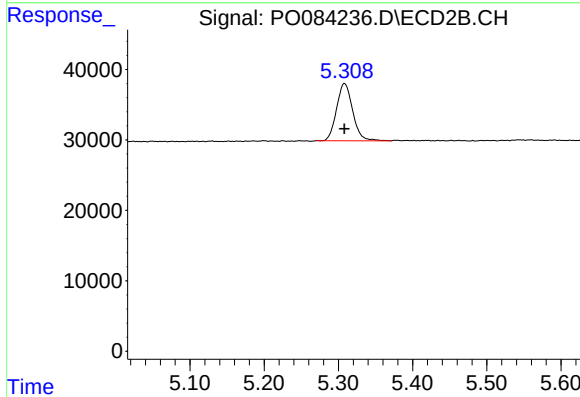


#1 Tetrachloro-m-xylene

R.T.: 5.308 min
Delta R.T.: 0.000 min
Response: 122688
Conc: 5.28 ng/ml

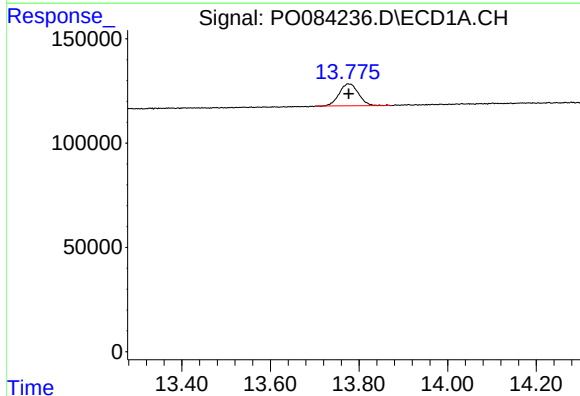


#2 Decachlorobiphenyl

R.T.: 13.777 min
Delta R.T.: 0.000 min
Response: 320547
Conc: 5.32 ng/ml

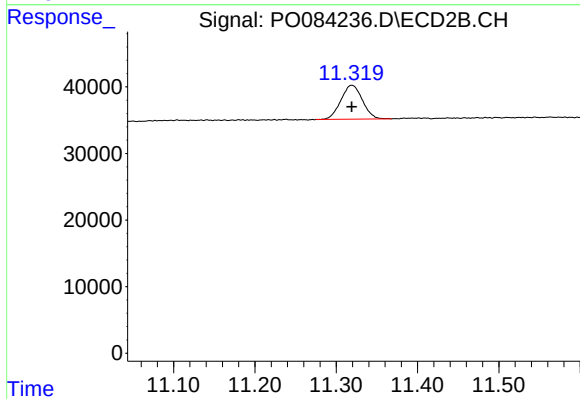

#2 Decachlorobiphenyl

R.T.: 11.319 min
Delta R.T.: 0.000 min
Response: 93416
Conc: 5.02 ng/ml

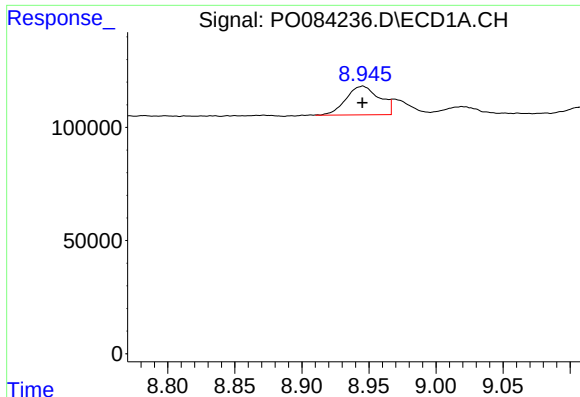


#26 AR-1254-1

R.T.: 8.945 min
Delta R.T.: 0.000 min
Response: 218293
Conc: 63.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/14/2022
Supervised By :mohammad ahmed 01/14/2022

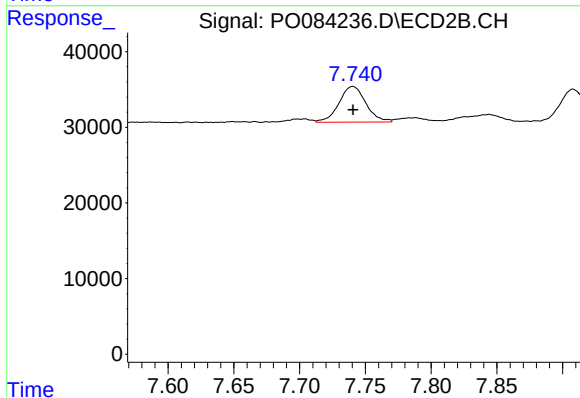


#26 AR-1254-1

R.T.: 7.741 min
Delta R.T.: 0.000 min
Response: 67388
Conc: 58.24 ng/ml

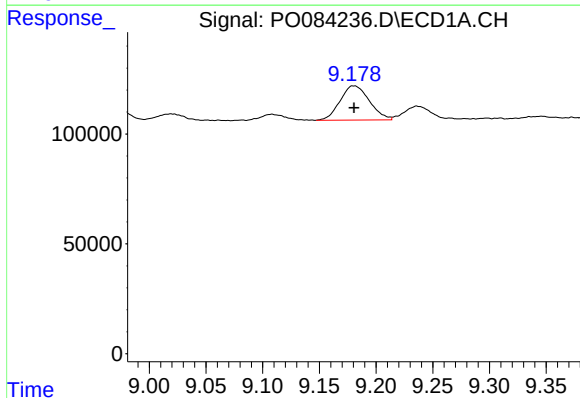


#27 AR-1254-2

R.T.: 9.181 min
Delta R.T.: 0.000 min
Response: 281185
Conc: 61.25 ng/ml

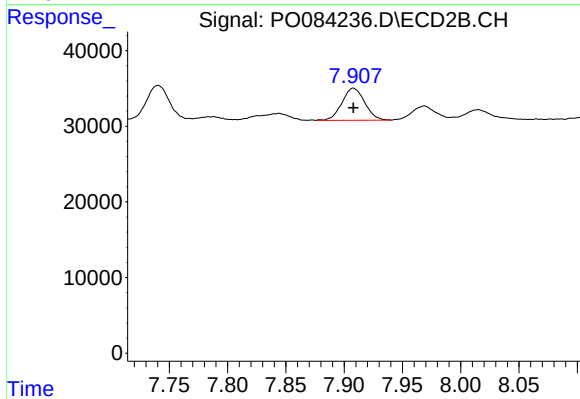

#27 AR-1254-2

R.T.: 7.908 min
Delta R.T.: 0.000 min
Response: 57804
Conc: 58.22 ng/ml

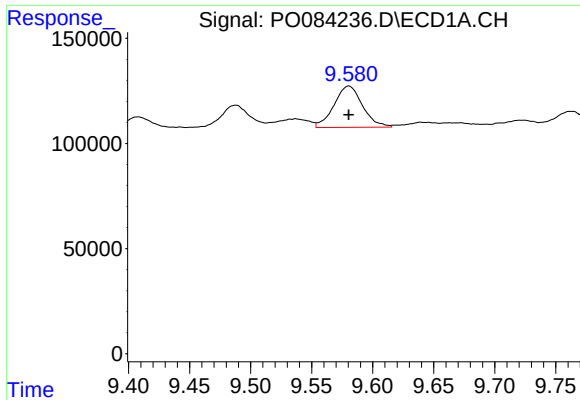


#28 AR-1254-3

R.T.: 9.580 min
Delta R.T.: 0.000 min
Response: 320873
Conc: 66.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/14/2022
Supervised By :mohammad ahmed 01/14/2022

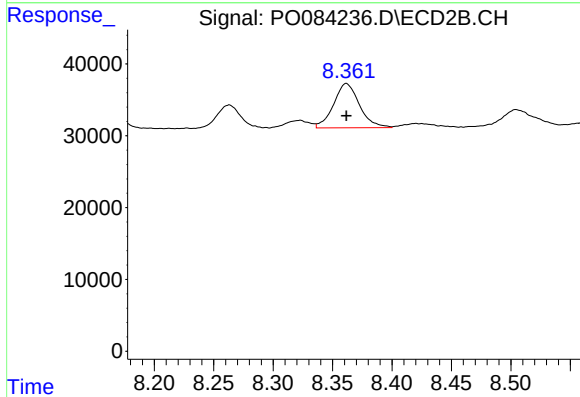


#28 AR-1254-3

R.T.: 8.362 min
Delta R.T.: 0.000 min
Response: 93092
Conc: 58.04 ng/ml

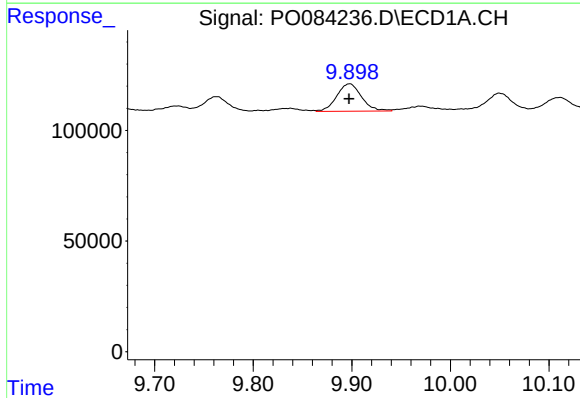


#29 AR-1254-4

R.T.: 9.897 min
Delta R.T.: 0.000 min
Response: 217450
Conc: 63.73 ng/ml

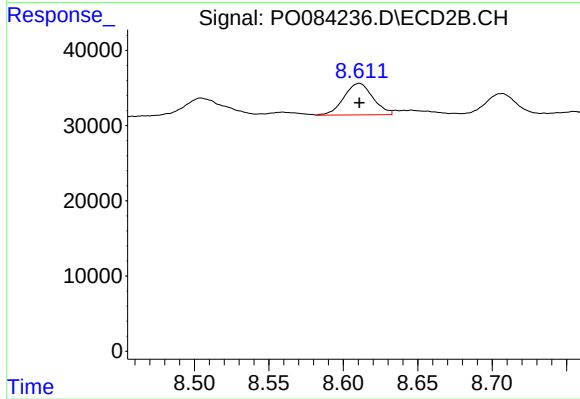

#29 AR-1254-4

R.T.: 8.611 min
Delta R.T.: 0.000 min
Response: 56874
Conc: 56.35 ng/ml

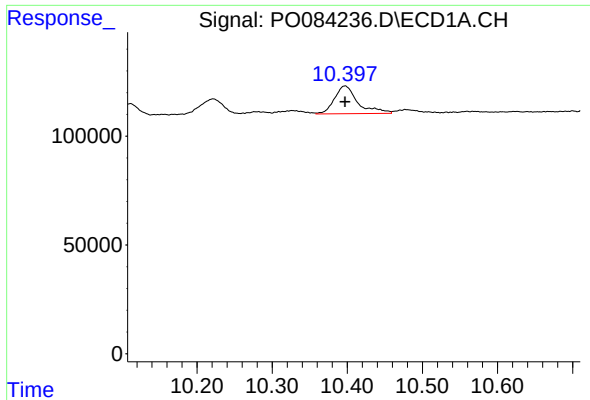


#30 AR-1254-5

R.T.: 10.397 min
Delta R.T.: 0.000 min
Response: 277045
Conc: 64.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/14/2022
Supervised By :mohammad ahmed 01/14/2022

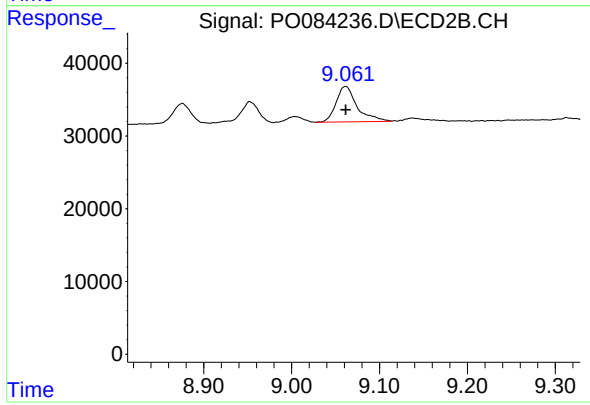

#30 AR-1254-5

R.T.: 9.062 min
Delta R.T.: 0.000 min
Response: 81251
Conc: 59.10 ng/ml