

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011323\
 Data File : P0092015.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jan 2023 09:56
 Operator : YP/AJ
 Sample : 01102-08 10X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC226467-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/16/2023
 Supervised By :Ankita Jodhani 01/16/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 10:51:28 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 11 04:41:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.445	3.648	4803544	2682200	1.722m	1.932
2) SA Decachlor...	10.361	8.704	4831562	2633344	2.468m	2.970

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011323\
Data File : PO092015.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jan 2023 09:56
Operator : YP/AJ
Sample : 01102-08 10X
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BC226467-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/16/2023
Supervised By :Ankita Jodhani 01/16/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 10:51:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011023.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 11 04:41:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

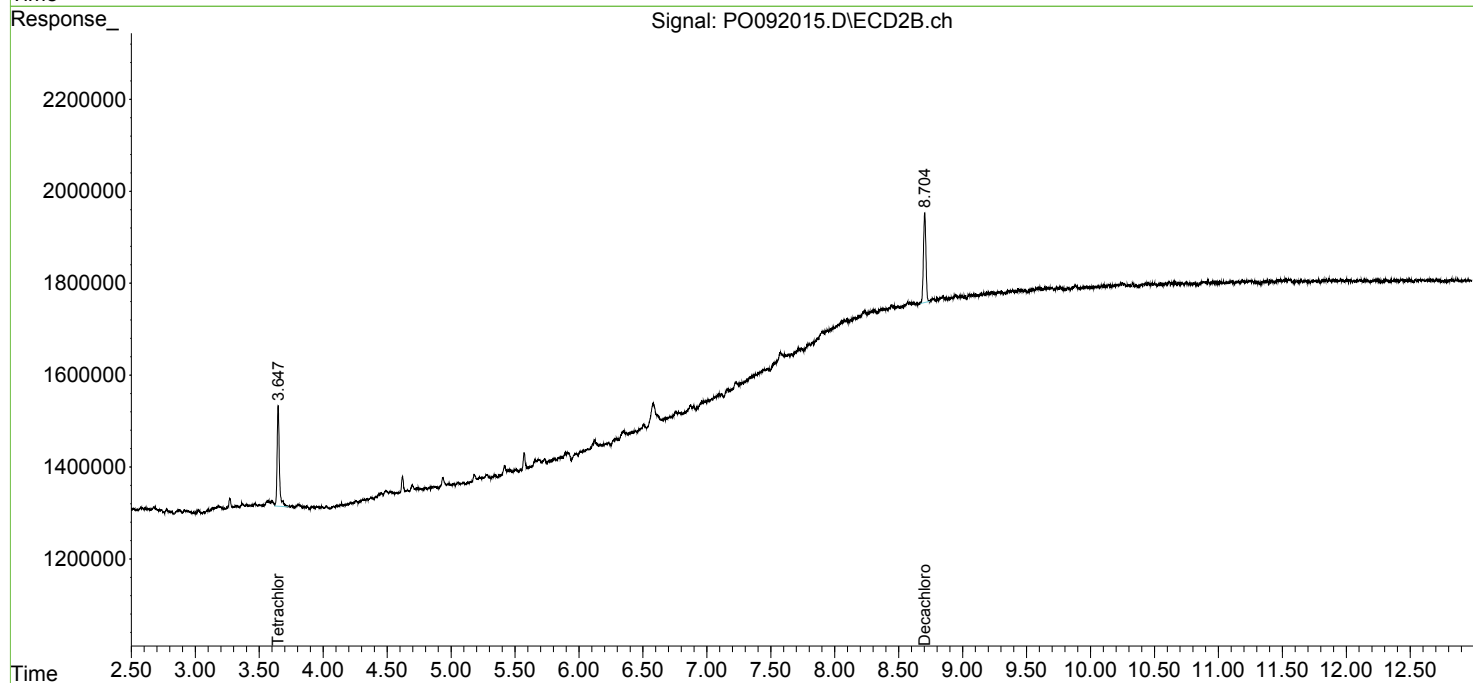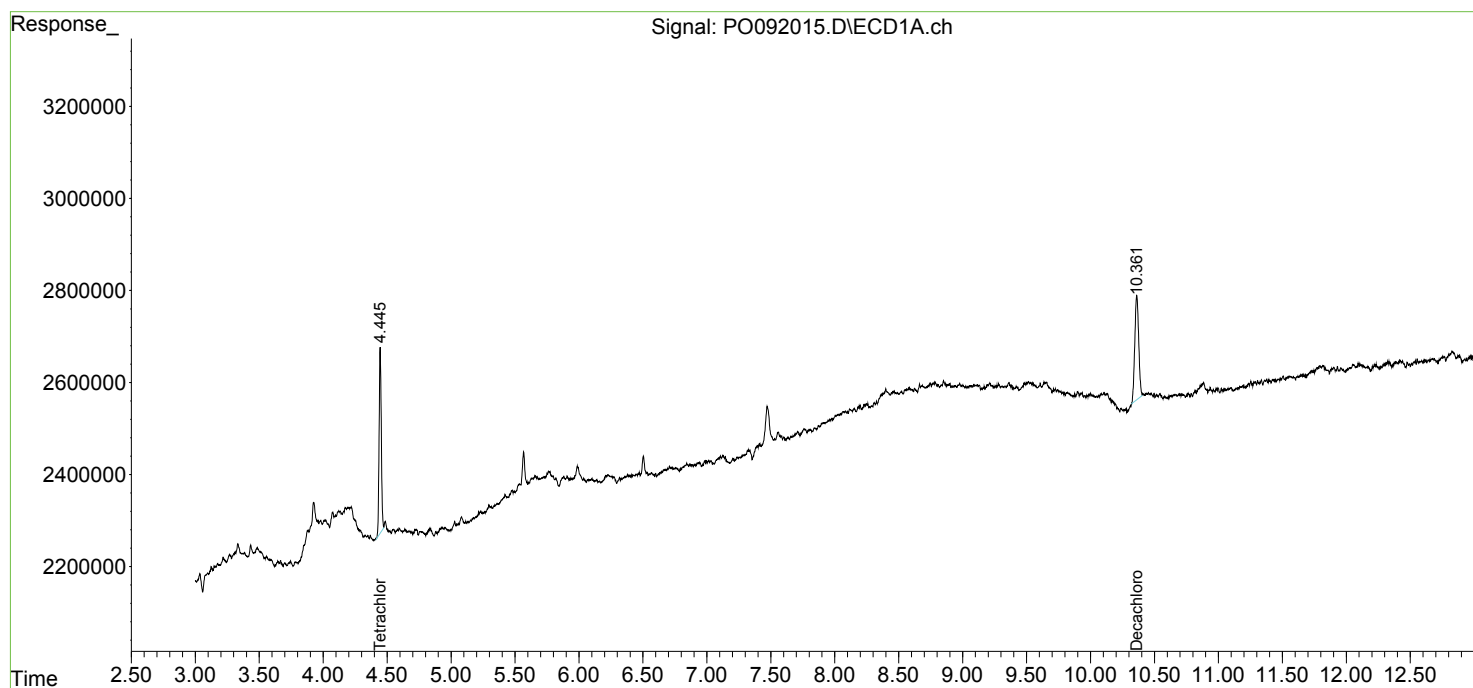

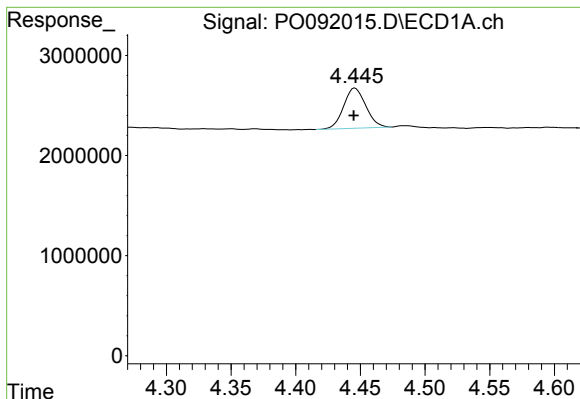


#1 Tetrachloro-m-xylene

R.T.: 4.445 min
Delta R.T.: 0.000 min
Response: 4803544
Conc: 1.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC226467-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/16/2023
Supervised By :Ankita Jodhani 01/16/2023

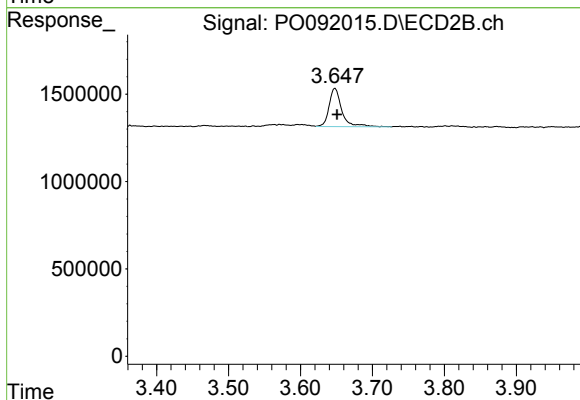


#1 Tetrachloro-m-xylene

R.T.: 3.648 min
Delta R.T.: -0.003 min
Response: 2682200
Conc: 1.93 ng/ml

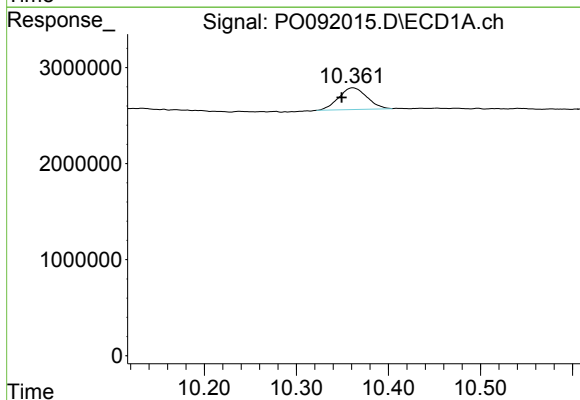

#2 Decachlorobiphenyl

R.T.: 10.361 min
Delta R.T.: 0.011 min
Response: 4831562
Conc: 2.47 ng/ml m

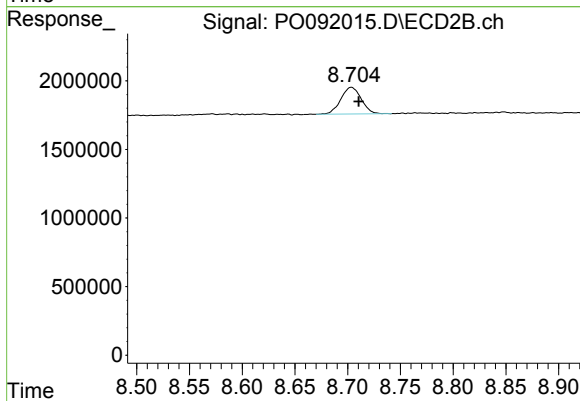

#2 Decachlorobiphenyl

R.T.: 8.704 min
Delta R.T.: -0.007 min
Response: 2633344
Conc: 2.97 ng/ml