

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011323\
 Data File : P0092017.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jan 2023 10:30
 Operator : YP/AJ
 Sample : 01102-10 10X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC248186-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/16/2023
 Supervised By :Ankita Jodhani 01/16/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 10:51:59 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 11 04:41:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.447	3.648	5811783	2698812	2.084	1.944m
2) SA Decachlor...	10.362	8.705	5285618	1893982	2.700m	2.136m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011323\
Data File : PO092017.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jan 2023 10:30
Operator : YP/AJ
Sample : 01102-10 10X
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BC248186-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/16/2023
Supervised By :Ankita Jodhani 01/16/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 10:51:59 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011023.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 11 04:41:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

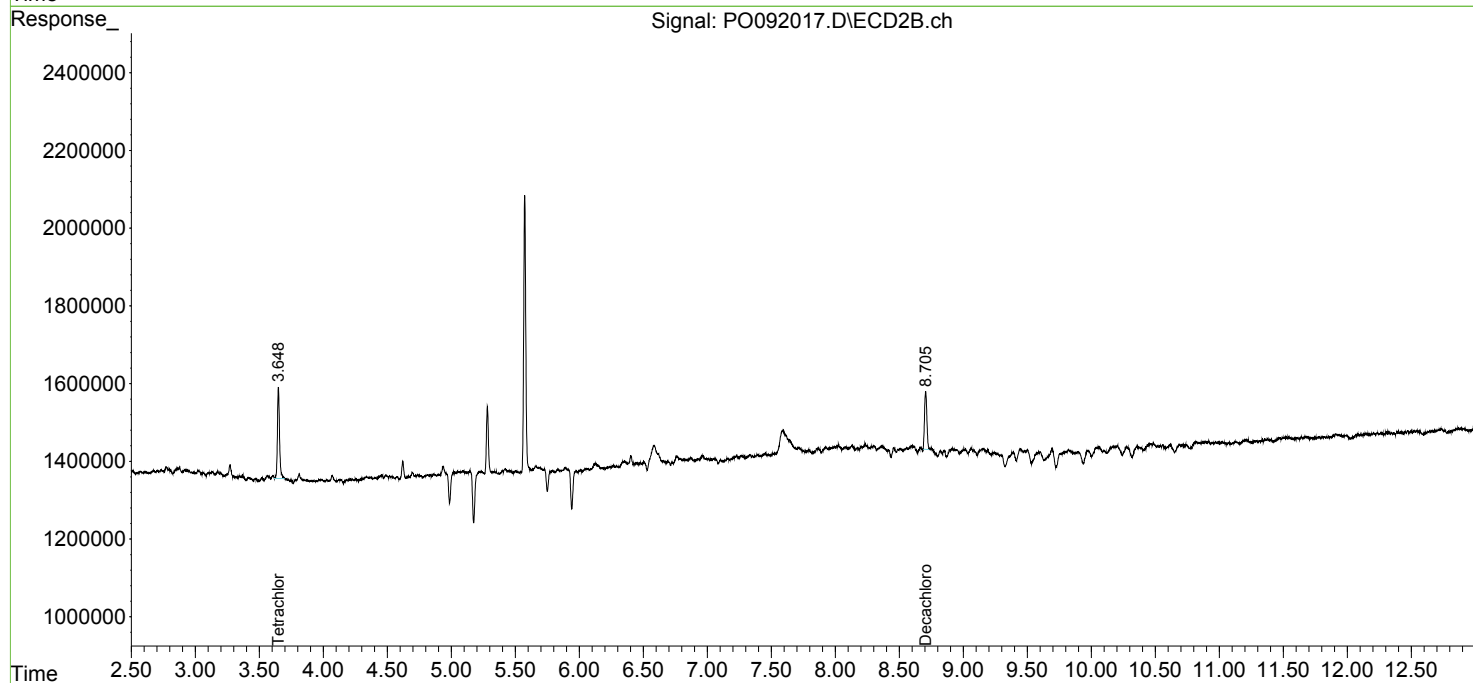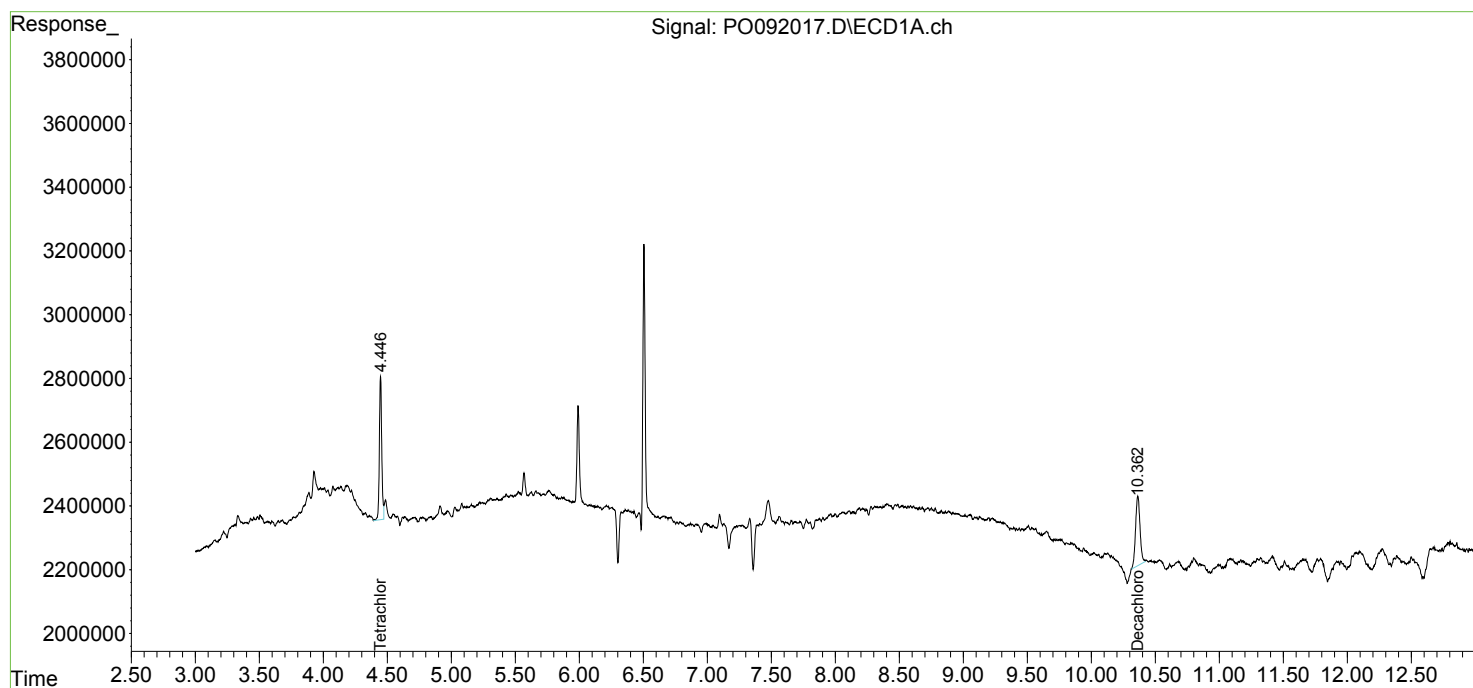

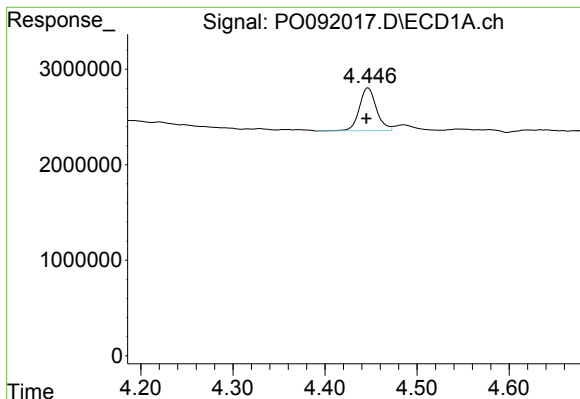


#1 Tetrachloro-m-xylene

R.T.: 4.447 min
Delta R.T.: 0.002 min
Response: 5811783
Conc: 2.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC248186-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/16/2023
Supervised By :Ankita Jodhani 01/16/2023

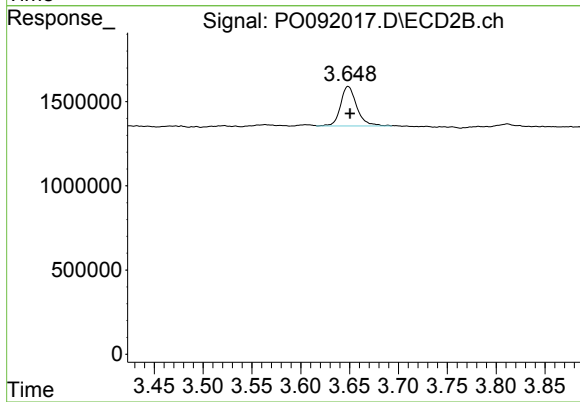


#1 Tetrachloro-m-xylene

R.T.: 3.648 min
Delta R.T.: -0.003 min
Response: 2698812
Conc: 1.94 ng/ml m

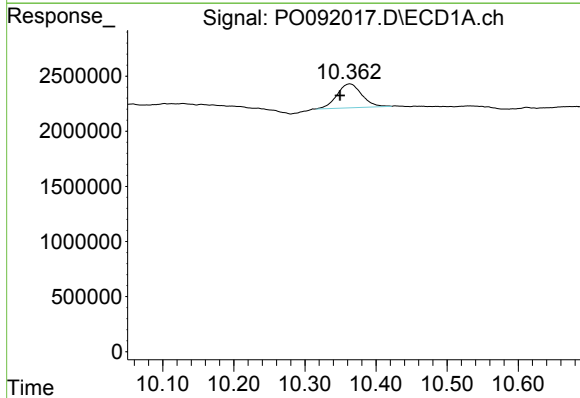

#2 Decachlorobiphenyl

R.T.: 10.362 min
Delta R.T.: 0.013 min
Response: 5285618
Conc: 2.70 ng/ml m

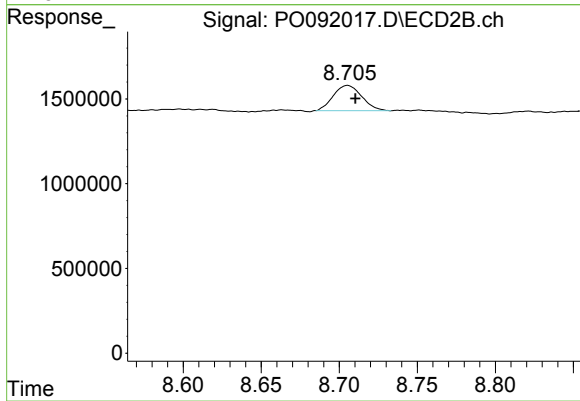

#2 Decachlorobiphenyl

R.T.: 8.705 min
Delta R.T.: -0.005 min
Response: 1893982
Conc: 2.14 ng/ml m