

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011323\
 Data File : P0092022.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jan 2023 11:56
 Operator : YP/AJ
 Sample : 01102-15 10X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KZA4310-3-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/16/2023
 Supervised By :Ankita Jodhani 01/16/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 12:11:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 11 04:41:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.446	3.649	4388353	2372416	1.573m	1.709
2) SA Decachlor...	10.361	8.704	4314479	2342229	2.204m	2.642

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011323\
Data File : PO092022.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jan 2023 11:56
Operator : YP/AJ
Sample : 01102-15 10X
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
KZA4310-3-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/16/2023
Supervised By :Ankita Jodhani 01/16/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 12:11:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011023.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 11 04:41:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

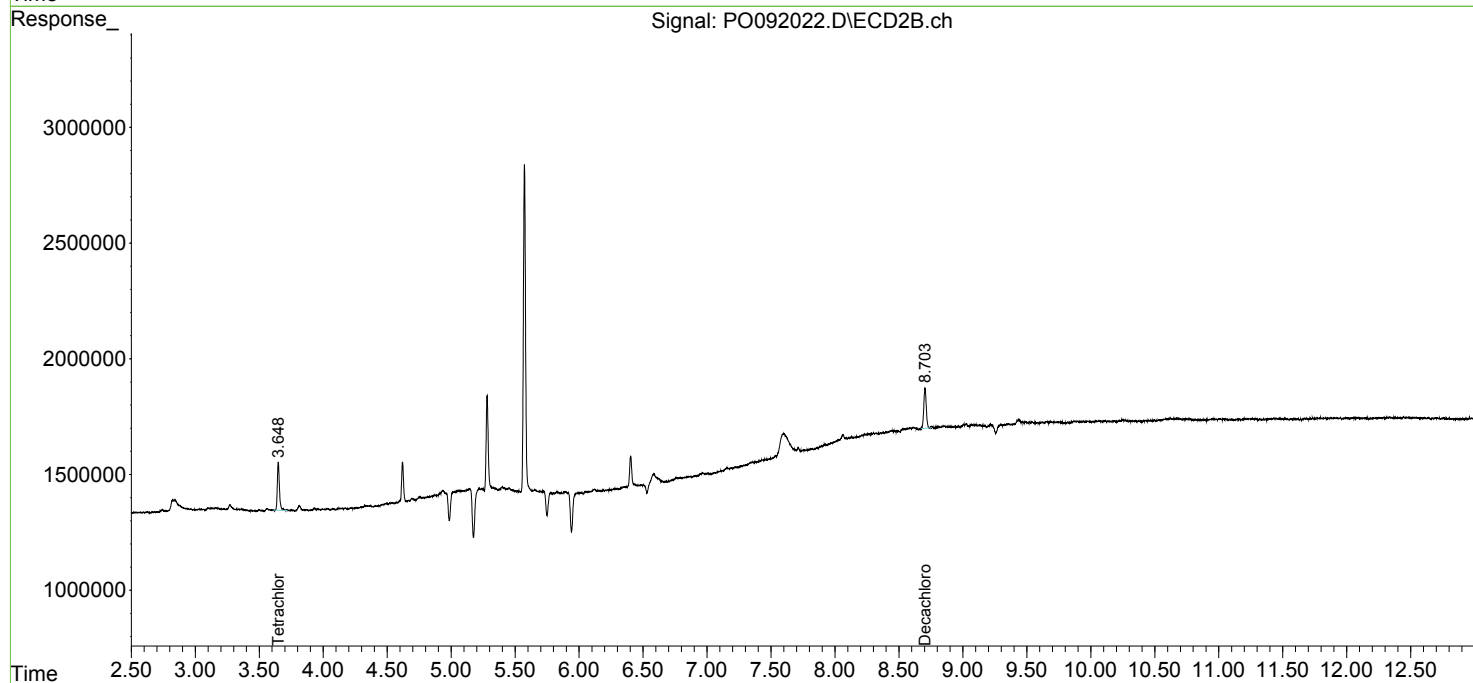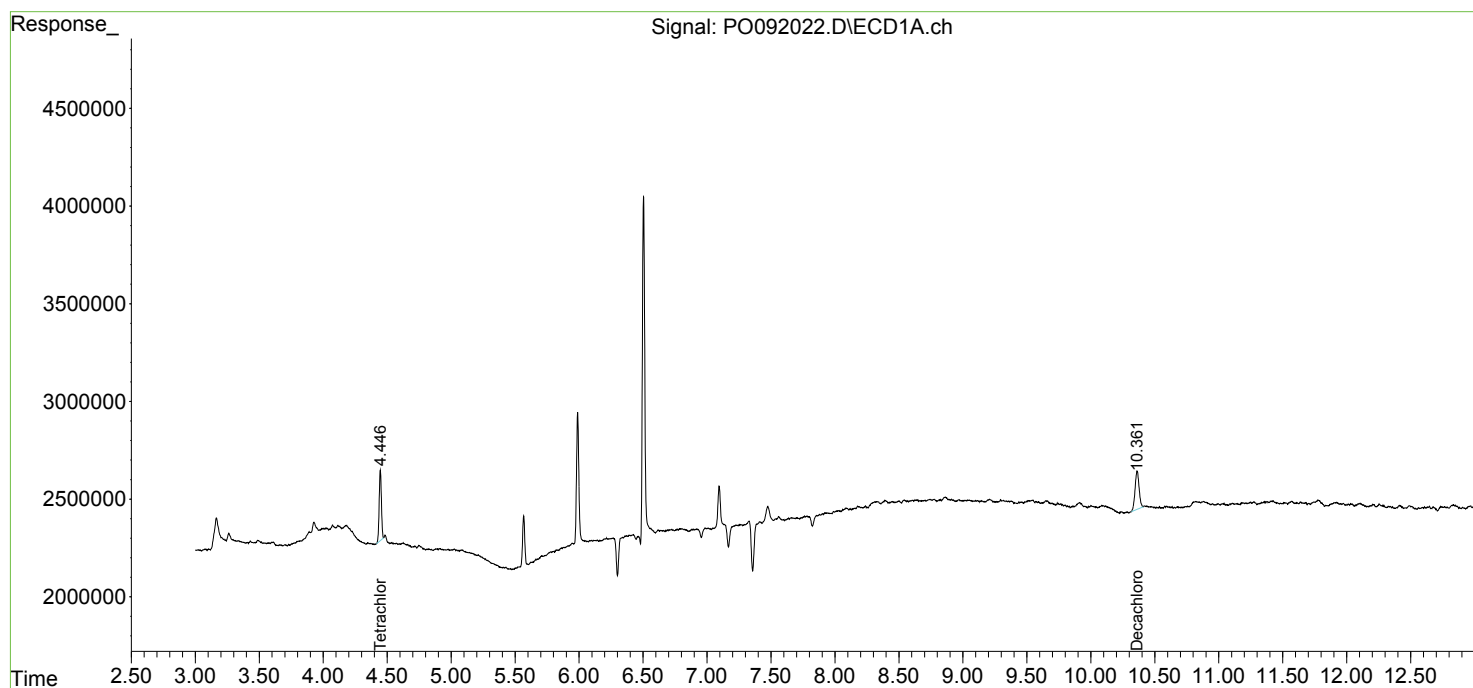

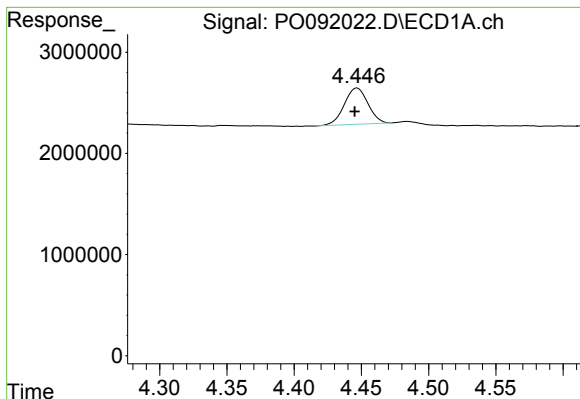

#1 Tetrachloro-m-xylene

R.T.: 4.446 min
Delta R.T.: 0.001 min
Response: 4388353
Conc: 1.57 ng/ml

Instrument :

ECD_O


ClientSampleId :

KZA4310-3-1

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 01/16/2023
Supervised By :Ankita Jodhani 01/16/2023

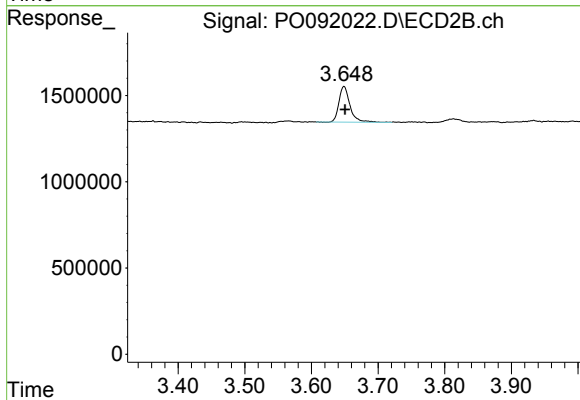


#1 Tetrachloro-m-xylene

R.T.: 3.649 min
Delta R.T.: -0.002 min
Response: 2372416
Conc: 1.71 ng/ml

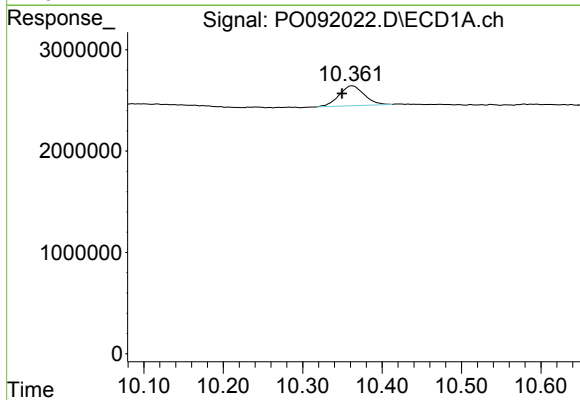

#2 Decachlorobiphenyl

R.T.: 10.361 min
Delta R.T.: 0.012 min
Response: 4314479
Conc: 2.20 ng/ml m

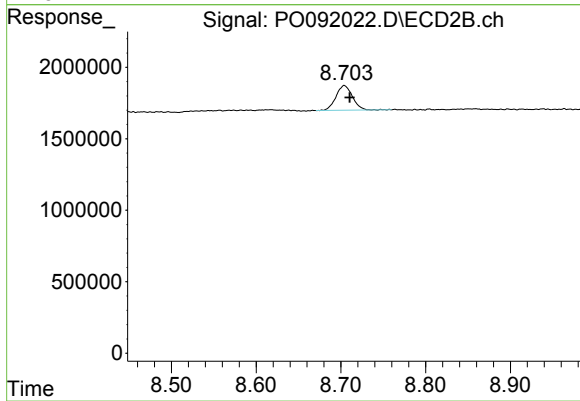

#2 Decachlorobiphenyl

R.T.: 8.704 min
Delta R.T.: -0.006 min
Response: 2342229
Conc: 2.64 ng/ml