

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\P0011323\  
 Data File : P0092023.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 13 Jan 2023 12:13  
 Operator : YP/AJ  
 Sample : 01102-16 10X  
 Misc :  
 ALS Vial : 35 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 KZA4310-3-2

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jan 13 12:28:00 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\P0011023.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Jan 11 04:41:00 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound        | RT#1   | RT#2  | Resp#1  | Resp#2  | ng/ml | ng/ml |
|-----------------------------|-----------------|--------|-------|---------|---------|-------|-------|
| -----                       |                 |        |       |         |         |       |       |
| System Monitoring Compounds |                 |        |       |         |         |       |       |
| 1)                          | SA Tetrachlo... | 4.447  | 3.649 | 4848453 | 2304385 | 1.738 | 1.660 |
| 2)                          | SA Decachlor... | 10.361 | 8.704 | 4879923 | 2509009 | 2.493 | 2.830 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\PO011323\  
Data File : PO092023.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 13 Jan 2023 12:13  
Operator : YP/AJ  
Sample : 01102-16 10X  
Misc :  
ALS Vial : 35 Sample Multiplier: 1

Instrument :  
ECD\_O  
ClientSampleId :  
KZA4310-3-2

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jan 13 12:28:00 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\PO011023.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Wed Jan 11 04:41:00 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

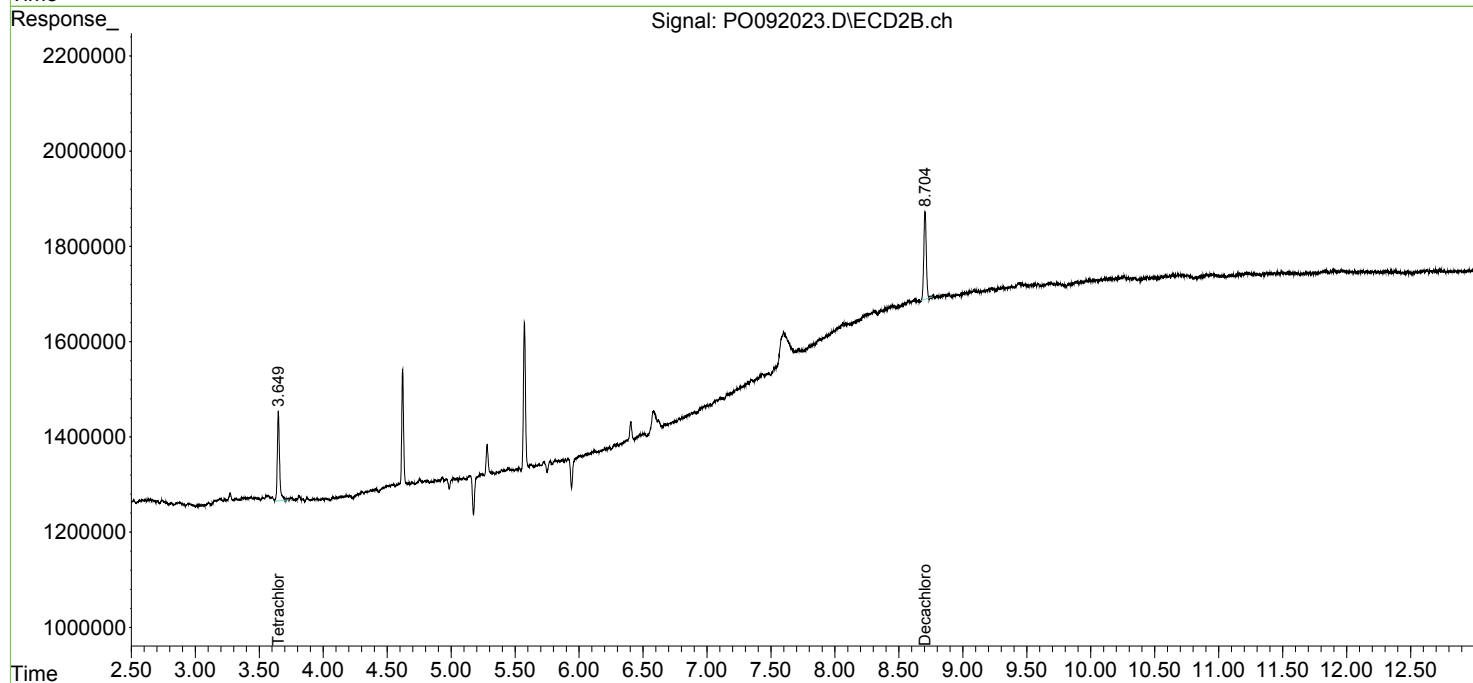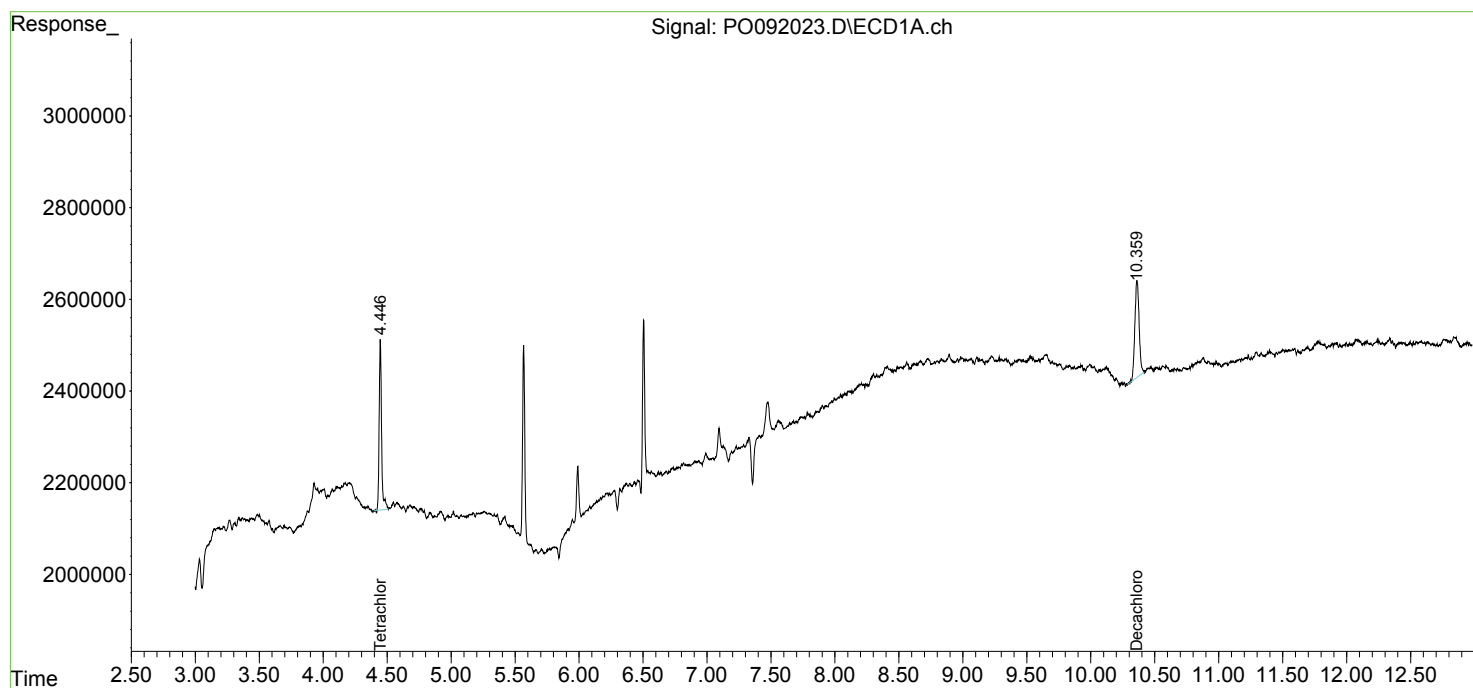


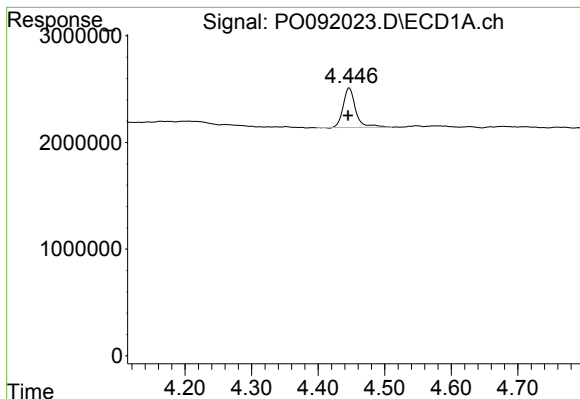

#1 Tetrachloro-m-xylene


R.T.: 4.447 min  
Delta R.T.: 0.002 min  
Response: 4848453  
Conc: 1.74 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
KZA4310-3-2

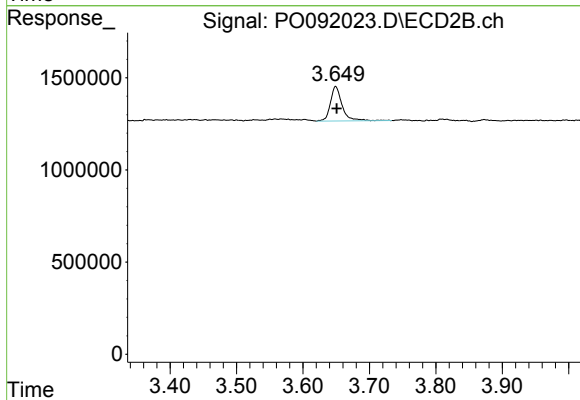


#1 Tetrachloro-m-xylene

R.T.: 3.649 min  
Delta R.T.: -0.001 min  
Response: 2304385  
Conc: 1.66 ng/ml

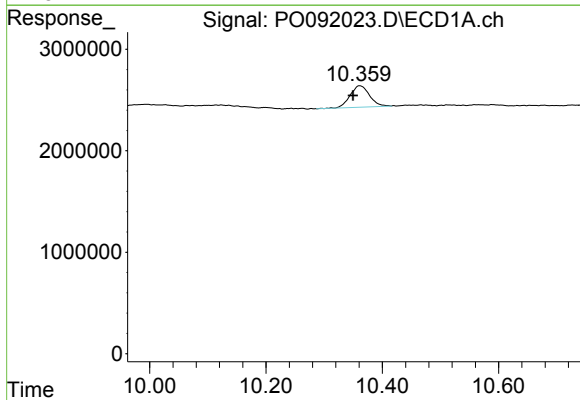

#2 Decachlorobiphenyl

R.T.: 10.361 min  
Delta R.T.: 0.012 min  
Response: 4879923  
Conc: 2.49 ng/ml

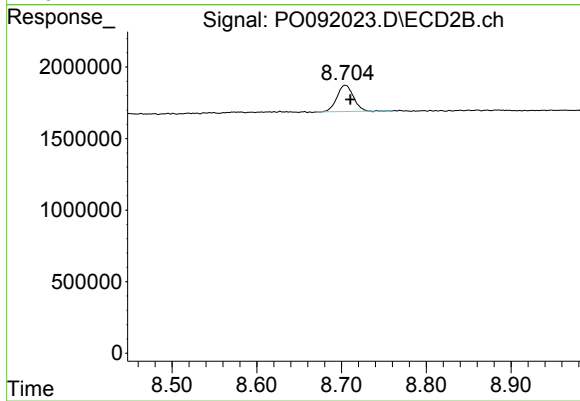

#2 Decachlorobiphenyl

R.T.: 8.704 min  
Delta R.T.: -0.006 min  
Response: 2509009  
Conc: 2.83 ng/ml