

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011421\
 Data File : P0074703.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Jan 2021 23:12
 Operator : AJ/MA
 Sample : M1134-02 10X
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SN1055023320

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 15 03:50:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.931	4.005	189313	90977	1.794	1.617
2)	SA Decachlor...	10.949	9.256	218529	132647	2.153	2.416
Target Compounds							
6)	L1 AR-1016-4	6.468f	0.000	48624	0	17.101	N.D. #
14)	L3 AR-1232-4	6.468f	0.000	48624	0	40.455	N.D. #
19)	L4 AR-1242-4	6.468f	0.000	48624	0	21.427	N.D. #
26)	L6 AR-1254-1	7.138f	0.000	67563	0	15.362	N.D. #
31)	L7 AR-1260-1	7.974f	0.000	94179	0	18.878	N.D. #
35)	L7 AR-1260-5	9.133	0.000	71223	0	5.700	N.D. #
37)	L8 AR-1262-2	9.133	0.000	71223	0	4.652	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011421\
Data File : P0074703.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jan 2021 23:12
Operator : AJ/MA
Sample : M1134-02 10X
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SN1055023320

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 15 03:50:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

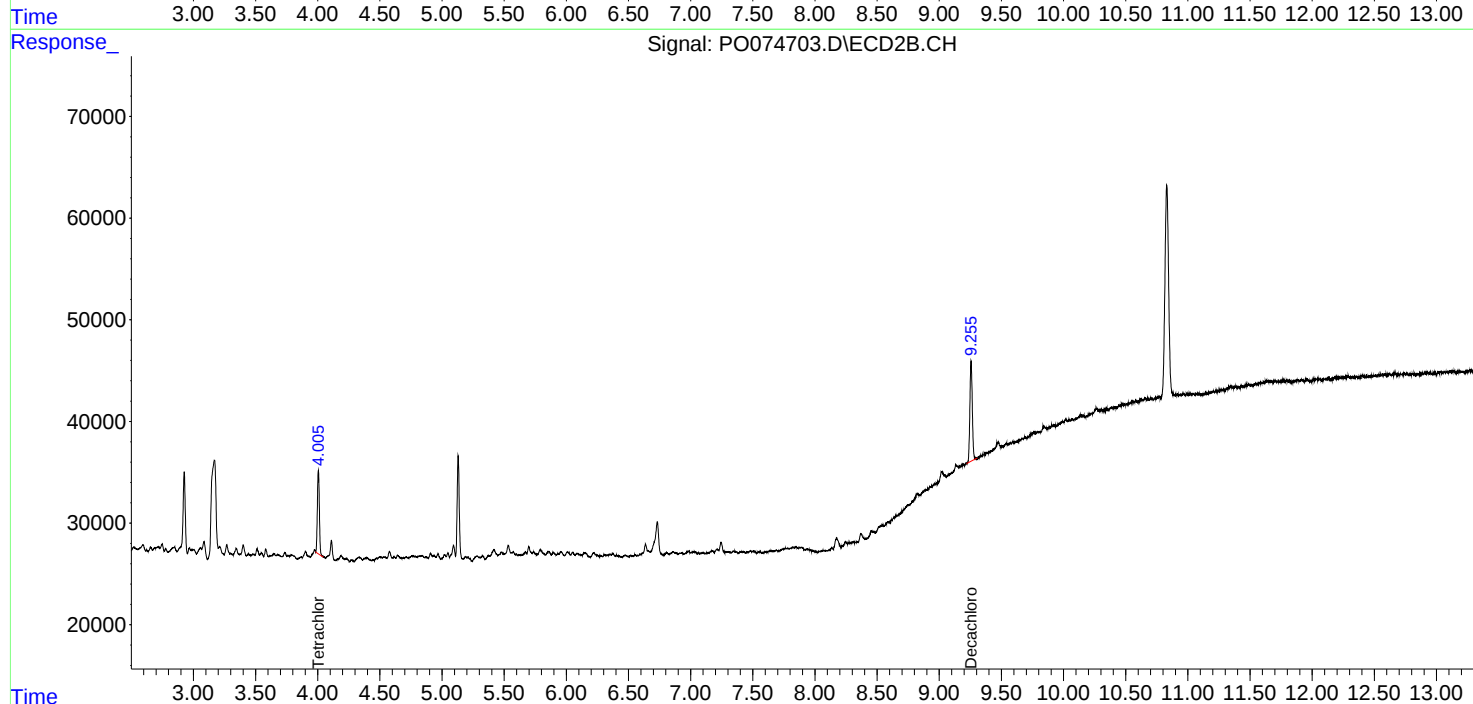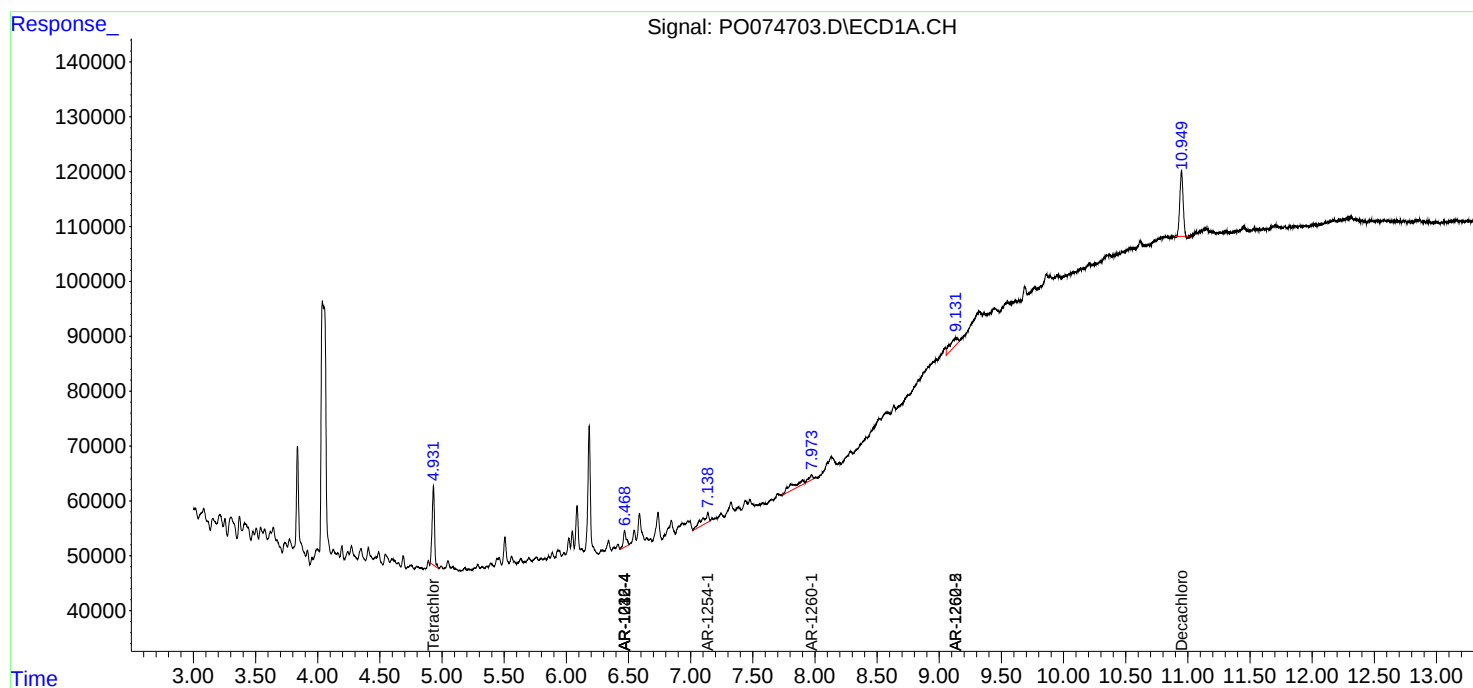


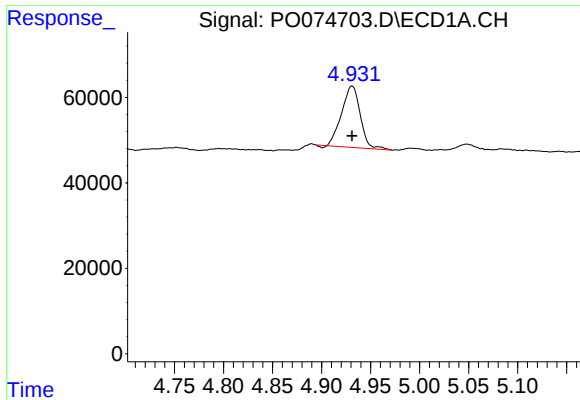

#1 Tetrachloro-m-xylene


R.T.: 4.931 min
Delta R.T.: 0.000 min
Response: 189313
Conc: 1.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
SN1055023320

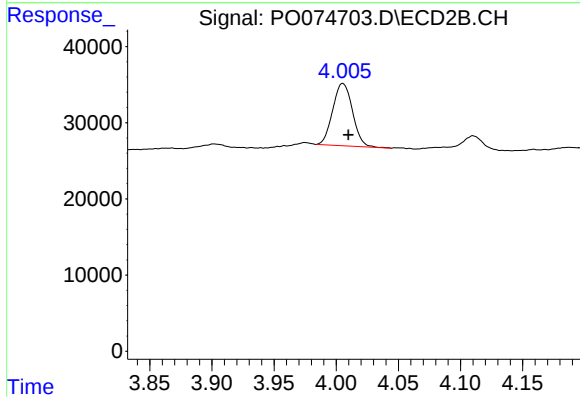


#1 Tetrachloro-m-xylene

R.T.: 4.005 min
Delta R.T.: -0.004 min
Response: 90977
Conc: 1.62 ng/ml

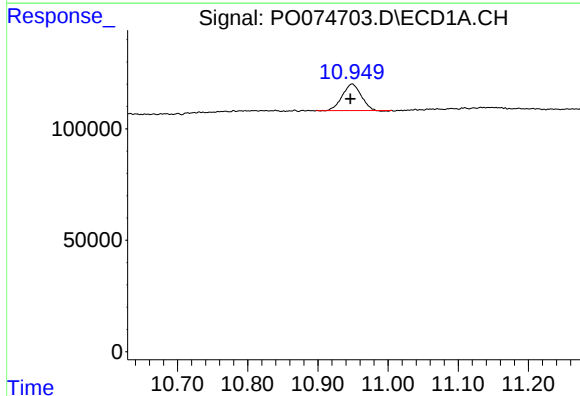


#2 Decachlorobiphenyl

R.T.: 10.949 min
Delta R.T.: 0.002 min
Response: 218529
Conc: 2.15 ng/ml

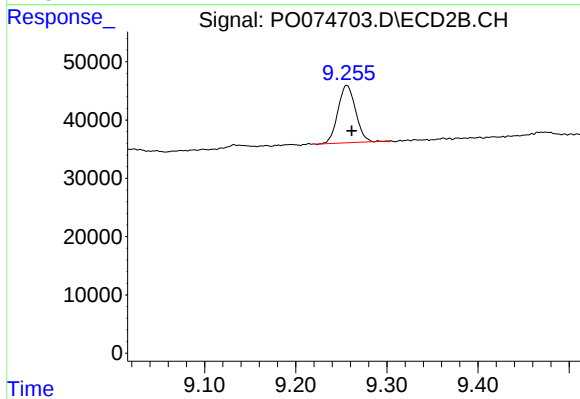

#2 Decachlorobiphenyl


R.T.: 9.256 min
Delta R.T.: -0.005 min
Response: 132647
Conc: 2.42 ng/ml

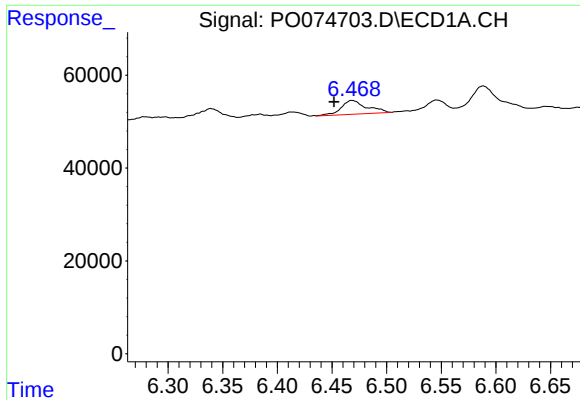

#6 AR-1016-4


R.T.: 6.468 min
Delta R.T.: 0.016 min
Response: 48624
Conc: 17.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
SN1055023320

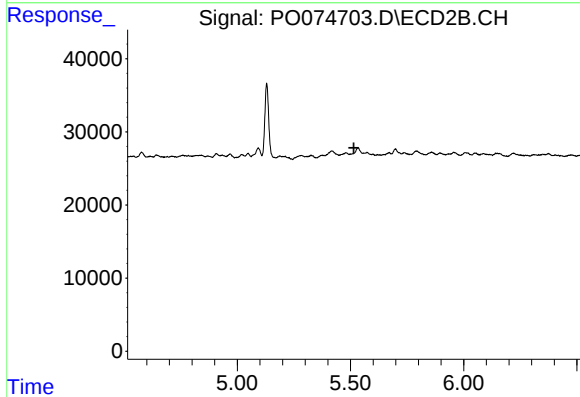


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T. : 5.515 min
Response: 0
Conc: N.D.

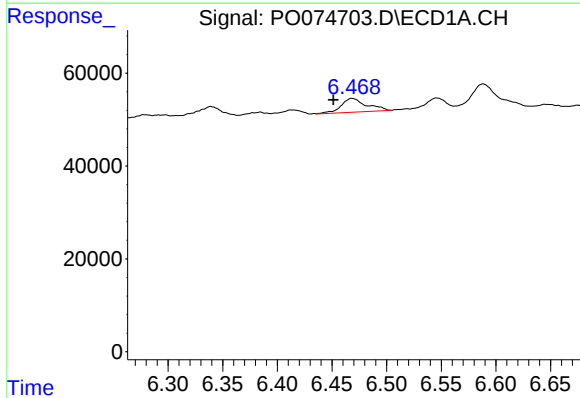


#14 AR-1232-4

R.T.: 6.468 min
Delta R.T.: 0.017 min
Response: 48624
Conc: 40.46 ng/ml

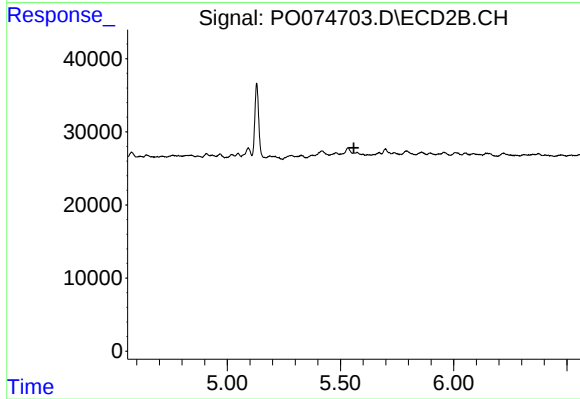

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T. : 5.559 min
Response: 0
Conc: N.D.

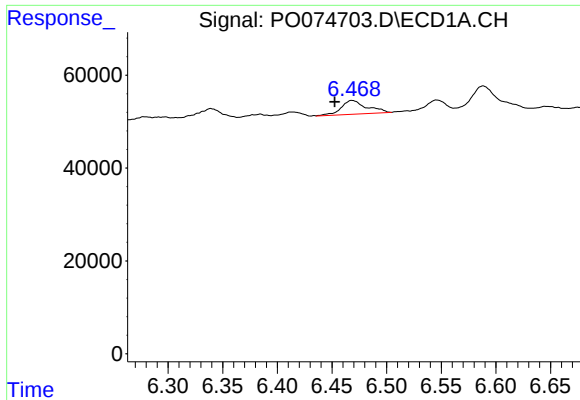

#19 AR-1242-4


R.T.: 6.468 min
Delta R.T.: 0.016 min
Response: 48624
Conc: 21.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
SN1055023320

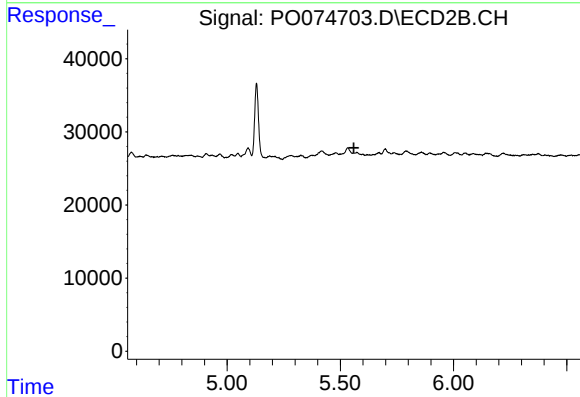


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T. : 5.560 min
Response: 0
Conc: N.D.

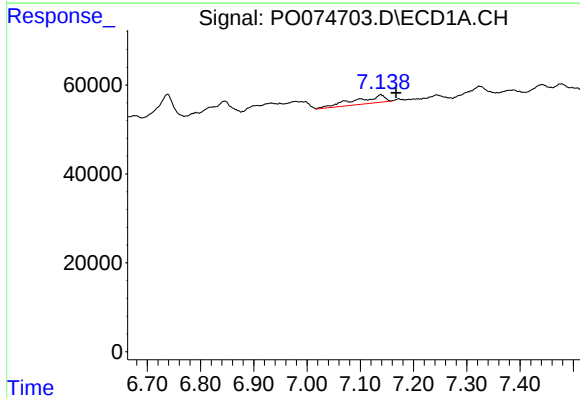


#26 AR-1254-1

R.T.: 7.138 min
Delta R.T.: -0.029 min
Response: 67563
Conc: 15.36 ng/ml

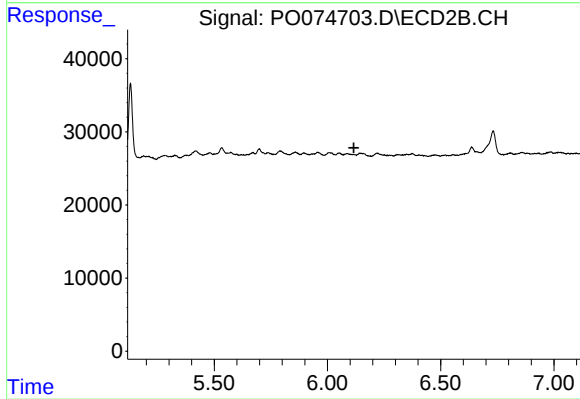

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.117 min
Response: 0
Conc: N.D.

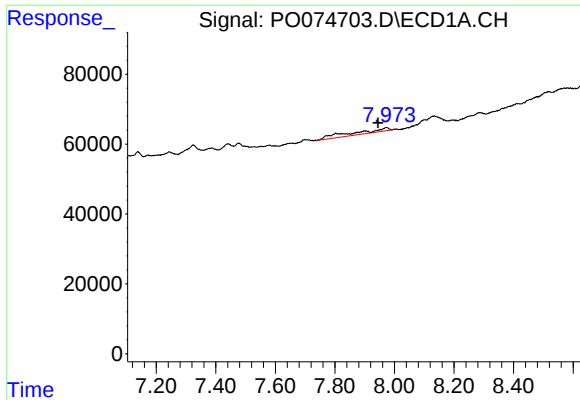

#31 AR-1260-1


R.T.: 7.974 min
Delta R.T.: 0.028 min
Response: 94179
Conc: 18.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
SN1055023320

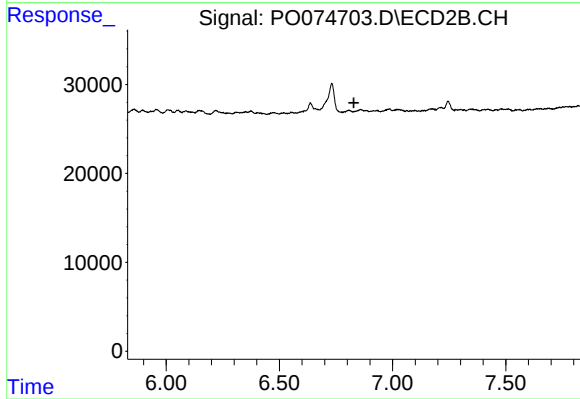


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 6.829 min
Response: 0
Conc: N.D.

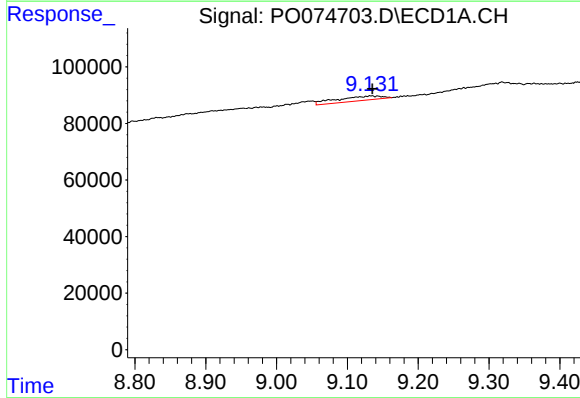


#35 AR-1260-5

R.T.: 9.133 min
Delta R.T.: -0.002 min
Response: 71223
Conc: 5.70 ng/ml

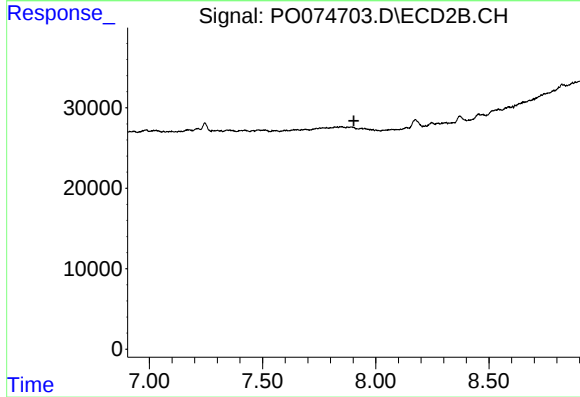

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 7.903 min
Response: 0
Conc: N.D.

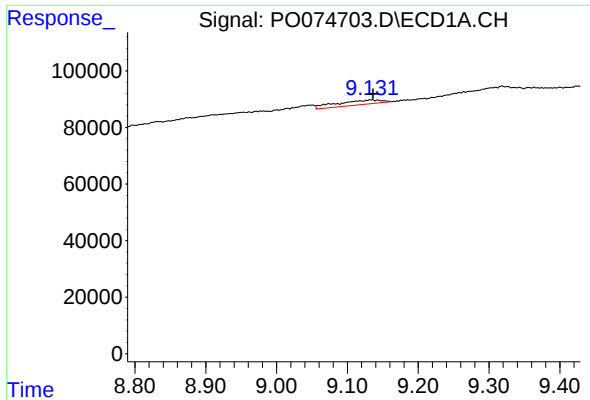

#37 AR-1262-2

R.T.: 9.133 min
Delta R.T.: -0.003 min
Response: 71223
Conc: 4.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
SN1055023320

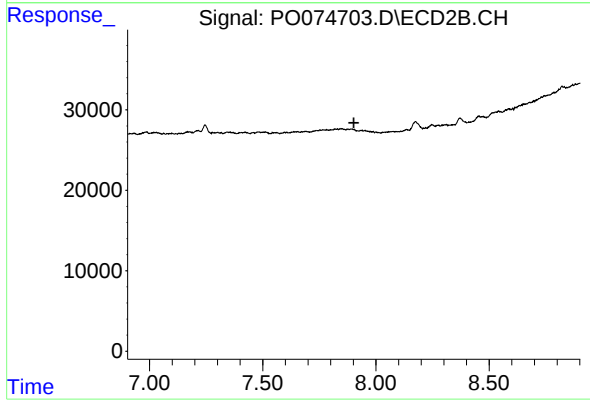

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.902 min
Response: 0
Conc: N.D.