

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011421\
 Data File : P0074660.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Jan 2021 10:05
 Operator : AJ/MA
 Sample : M1123-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 VW-SP

Manual Integrations
 APPROVED

Ankita
 1/15/2021 12:31:22 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 14 17:35:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.931	4.004	1619562	888034	15.349	15.787
2) SA Decachlor...	10.949	9.257	1513418	802801	14.912	14.622
Target Compounds						
31) L7 AR-1260-1	7.947	6.823	236812	209122	47.469m	65.550m#
32) L7 AR-1260-2	8.214	7.020	439109	275689	64.555m	64.852m
33) L7 AR-1260-3	8.580	7.171	246176	191573	42.950m	53.163m
34) L7 AR-1260-4	8.807	7.653	321095	126182	58.687m	40.297 #
35) L7 AR-1260-5	9.138	7.898	360940	272183	28.887	34.243

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011421\
Data File : PO074660.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jan 2021 10:05
Operator : AJ/MA
Sample : M1123-03
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampled :
VW-SP


Manual Integrations
APPROVED

Ankita
1/15/2021 12:31:22 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 14 17:35:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

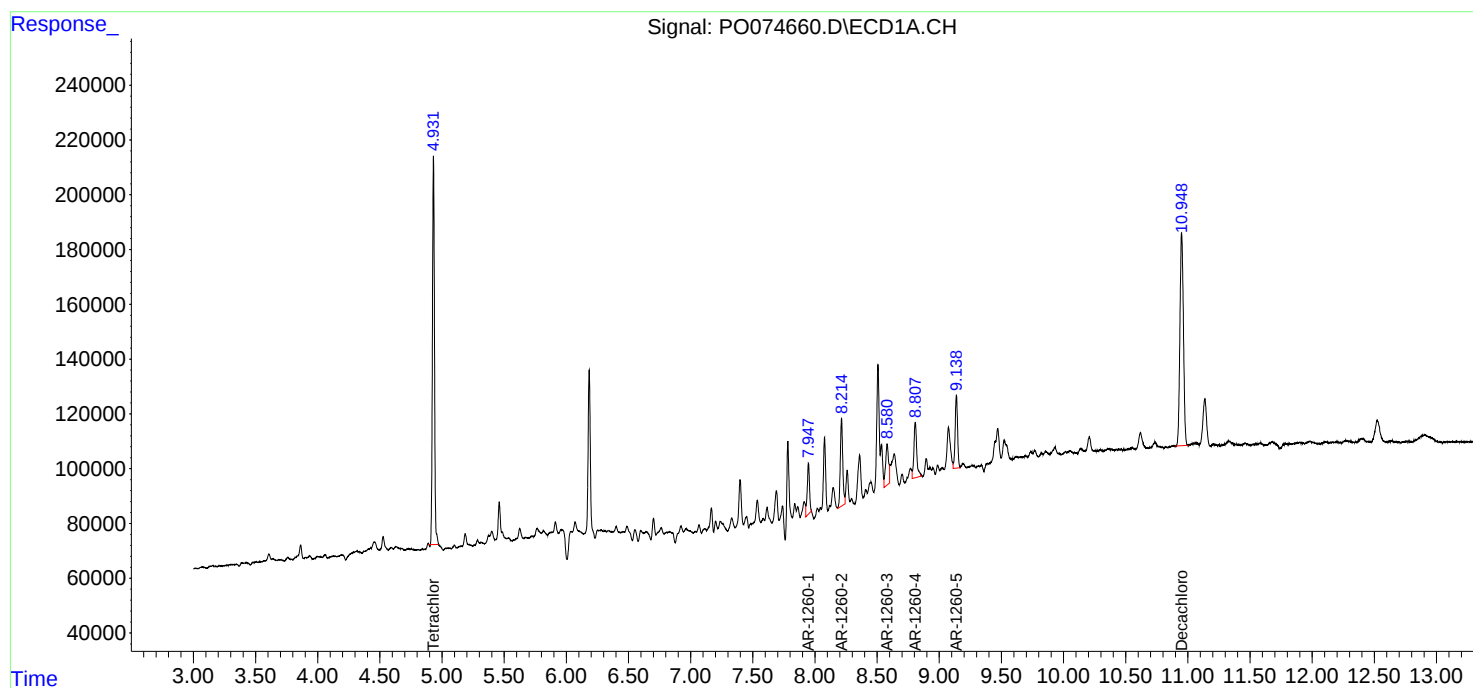

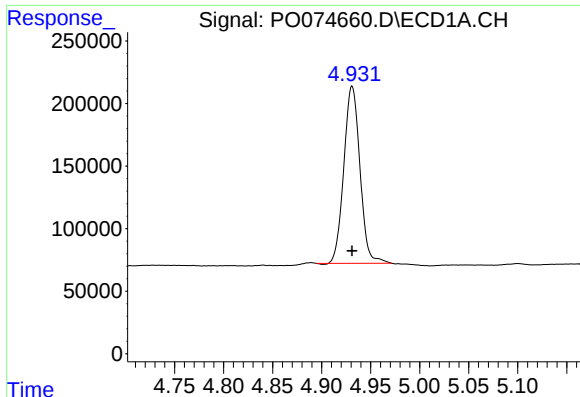


#1 Tetrachloro-m-xylene

R.T.: 4.931 min
Delta R.T.: 0.000 min
Response: 1619562
Conc: 15.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
VW-SP


Manual Integrations
APPROVED

Ankita
1/15/2021 12:31:22 PM

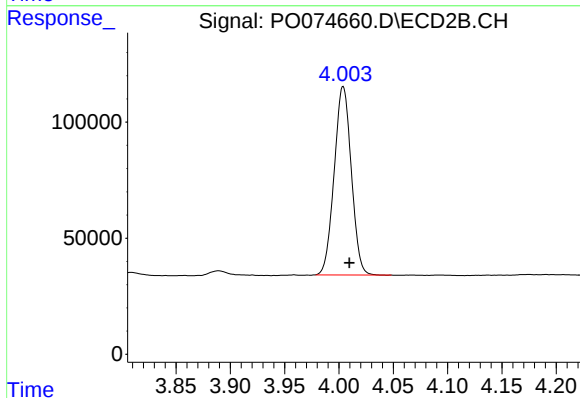


#1 Tetrachloro-m-xylene

R.T.: 4.004 min
Delta R.T.: -0.006 min
Response: 888034
Conc: 15.79 ng/ml

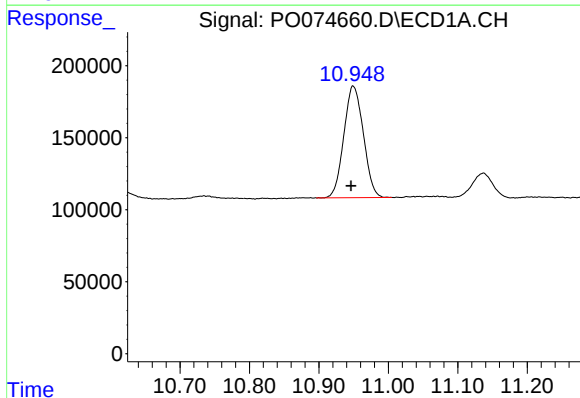


#2 Decachlorobiphenyl

R.T.: 10.949 min
Delta R.T.: 0.003 min
Response: 1513418
Conc: 14.91 ng/ml

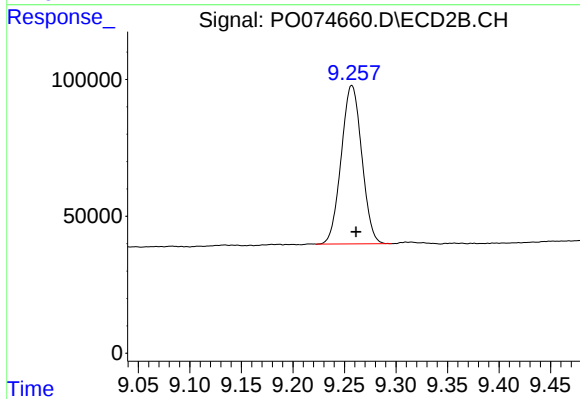

#2 Decachlorobiphenyl

R.T.: 9.257 min
Delta R.T.: -0.004 min
Response: 802801
Conc: 14.62 ng/ml

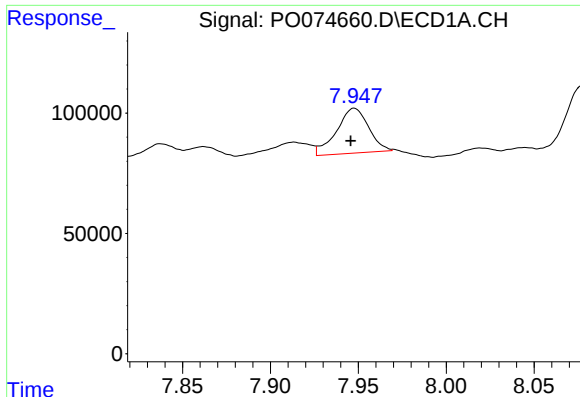


#31 AR-1260-1

R.T.: 7.947 min
Delta R.T.: 0.001 min
Response: 236812
Conc: 47.47 ng/ml m

Instrument :
ECD_O
ClientSampleId :
VW-SP


Manual Integrations
APPROVED

Ankita
1/15/2021 12:31:22 PM

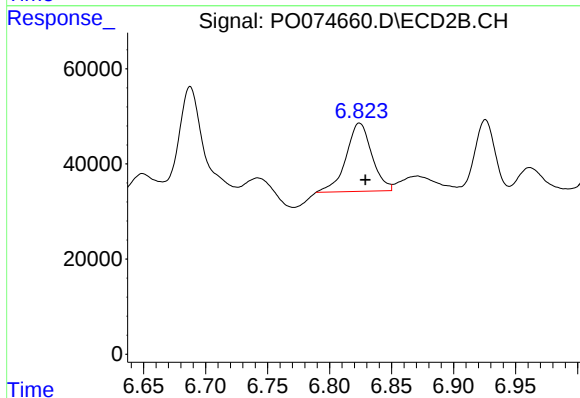


#31 AR-1260-1

R.T.: 6.823 min
Delta R.T.: -0.005 min
Response: 209122
Conc: 65.55 ng/ml m

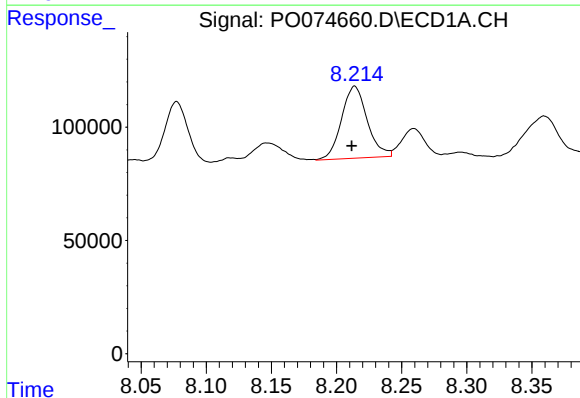


#32 AR-1260-2

R.T.: 8.214 min
Delta R.T.: 0.002 min
Response: 439109
Conc: 64.55 ng/ml m

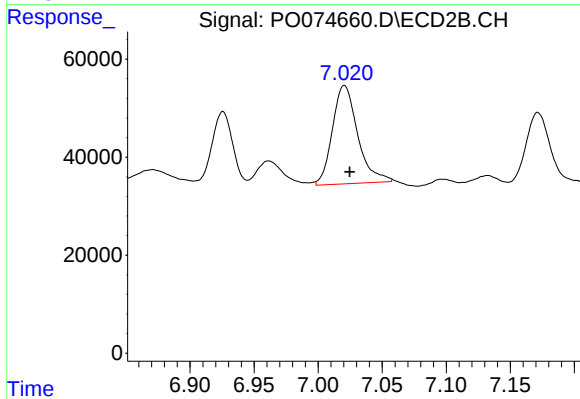

#32 AR-1260-2

R.T.: 7.020 min
Delta R.T.: -0.005 min
Response: 275689
Conc: 64.85 ng/ml m

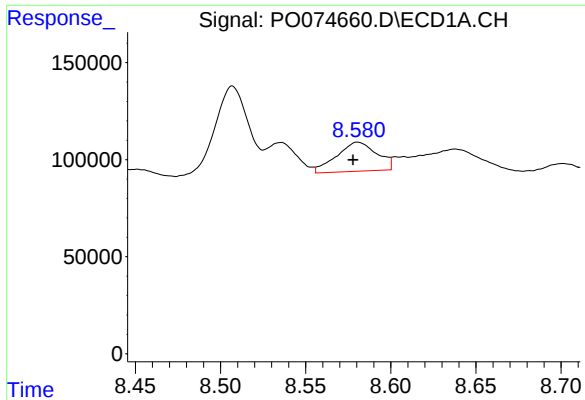


#33 AR-1260-3

R.T.: 8.580 min
Delta R.T.: 0.002 min
Response: 246176
Conc: 42.95 ng/ml m

Instrument :
ECD_O
ClientSampleId :
VW-SP


Manual Integrations
APPROVED

Ankita
1/15/2021 12:31:22 PM

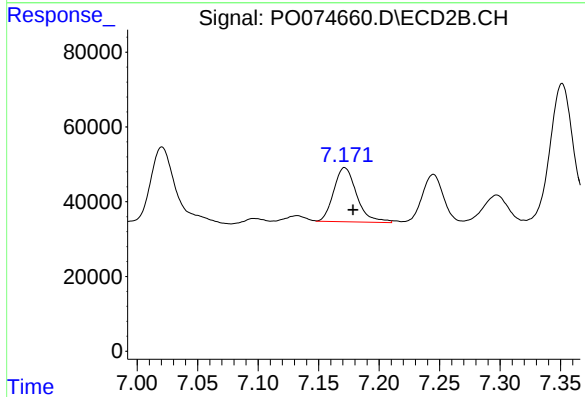


#33 AR-1260-3

R.T.: 7.171 min
Delta R.T.: -0.008 min
Response: 191573
Conc: 53.16 ng/ml m

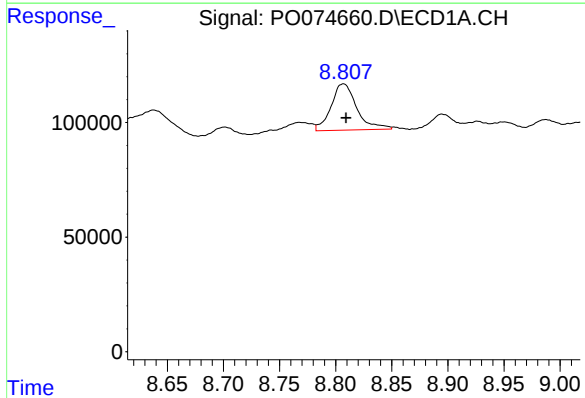


#34 AR-1260-4

R.T.: 8.807 min
Delta R.T.: -0.003 min
Response: 321095
Conc: 58.69 ng/ml m

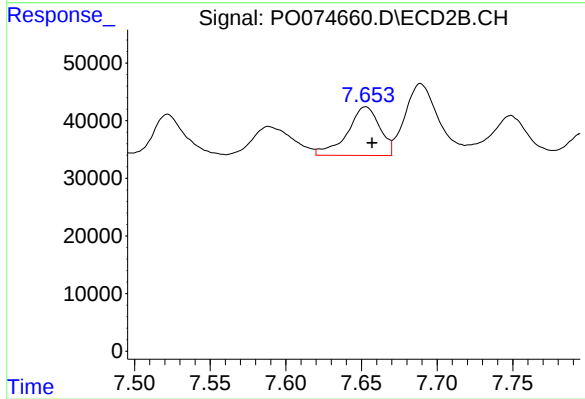

#34 AR-1260-4

R.T.: 7.653 min
Delta R.T.: -0.004 min
Response: 126182
Conc: 40.30 ng/ml

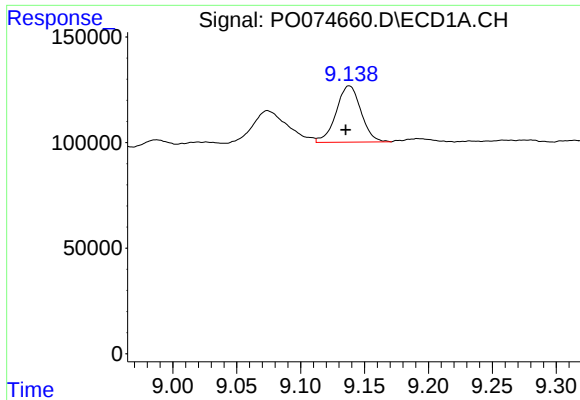


#35 AR-1260-5

R.T.: 9.138 min
Delta R.T.: 0.003 min
Response: 360940
Conc: 28.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
VW-SP

Manual Integrations
APPROVED

Ankita
1/15/2021 12:31:22 PM

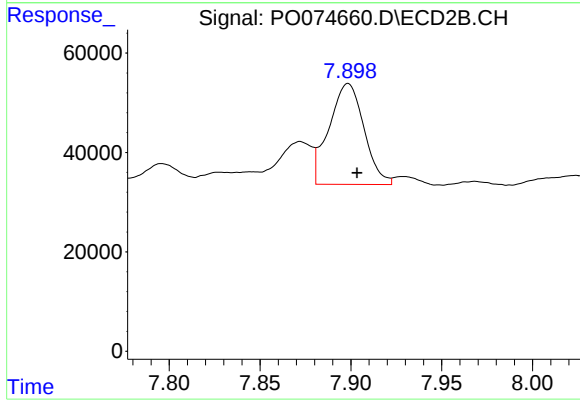

#35 AR-1260-5

R.T.: 7.898 min
Delta R.T.: -0.005 min
Response: 272183
Conc: 34.24 ng/ml