

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011421\
 Data File : P0074666.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Jan 2021 12:07
 Operator : AJ/MA
 Sample : M1112-02DL 20X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S21-03-BDL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 14 22:47:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
26)	L6	AR-1254-1	7.167	6.112	176715	41.206
27)	L6	AR-1254-2	7.396	6.271	430010	74.343
28)	L6	AR-1254-3	7.779	6.688	552634	87.036
29)	L6	AR-1254-4	8.076	6.926	612868	103.777
30)	L6	AR-1254-5	8.506	7.352	1099254	148.188
41)	L9	AR-1268-1	9.447	8.184	11244950	544.702
42)	L9	AR-1268-2	9.543	8.249	7203018	429.748
43)	L9	AR-1268-3	9.768	8.454	8695516	569.685
44)	L9	AR-1268-4	10.207	8.741	1939930	304.971
45)	L9	AR-1268-5	10.617	9.019	23829805	531.500



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011421\
Data File : PO074666.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jan 2021 12:07
Operator : AJ/MA
Sample : M1112-02DL 20X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
S21-03-BDL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 14 22:47:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

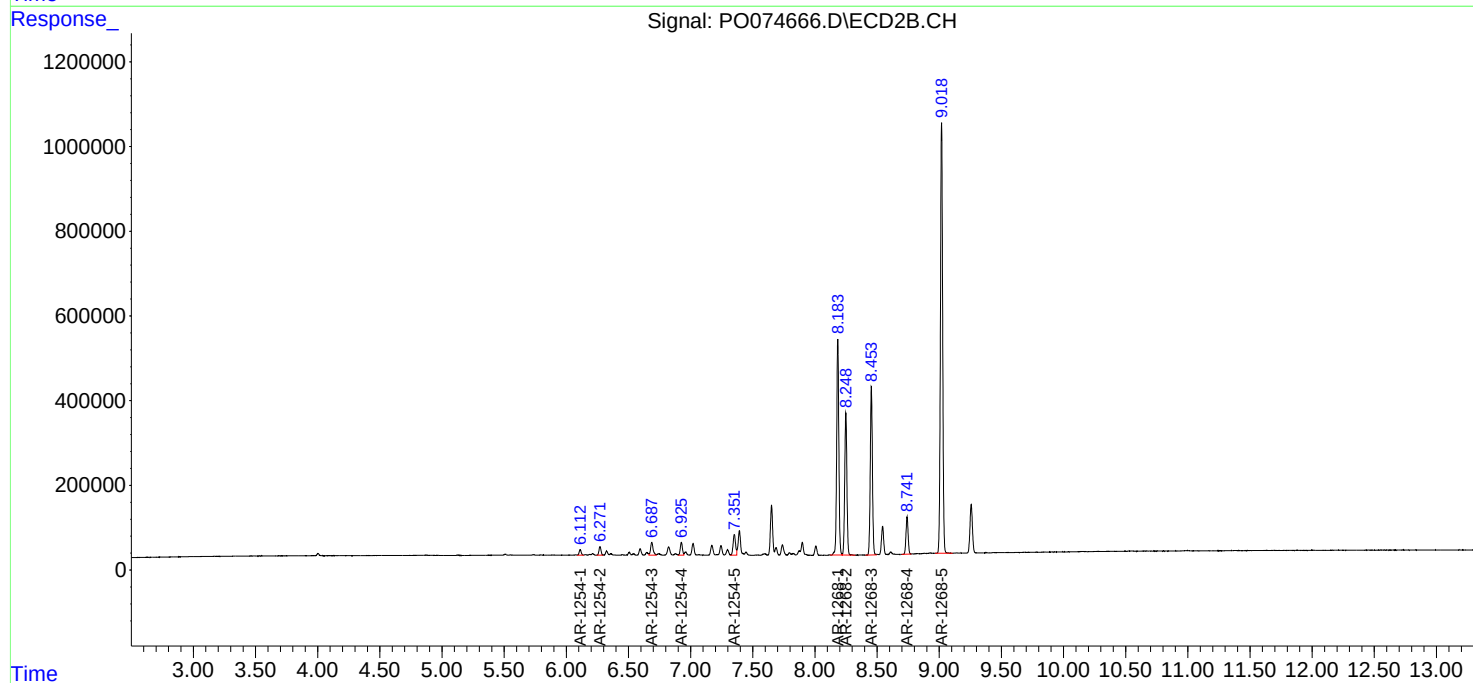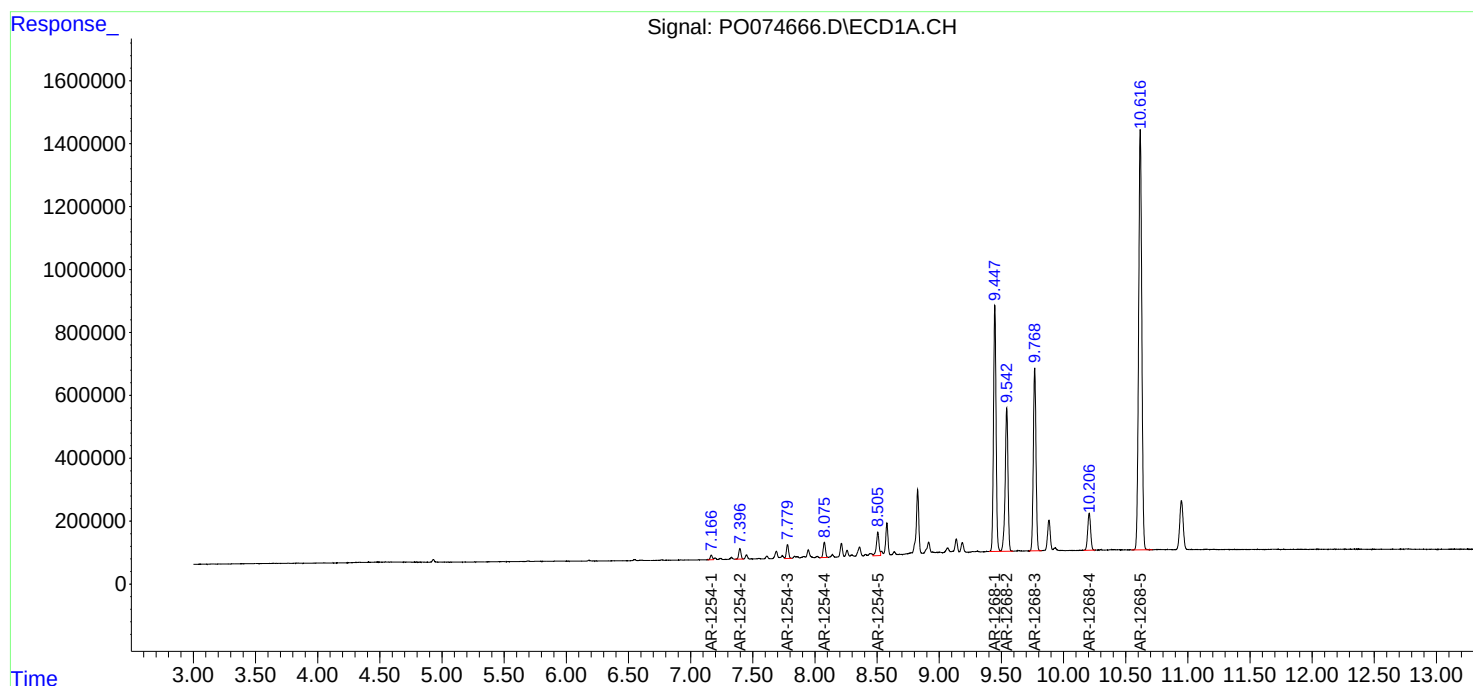


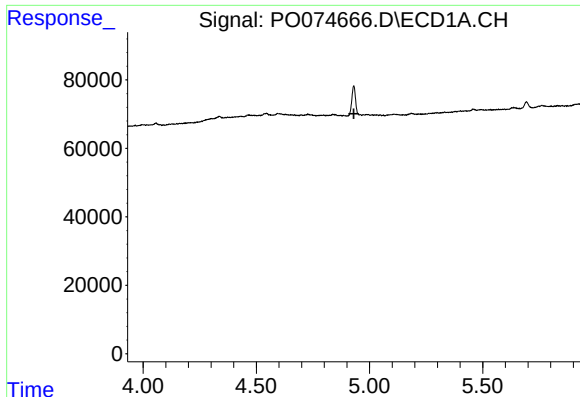

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.931 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
S21-03-BDL

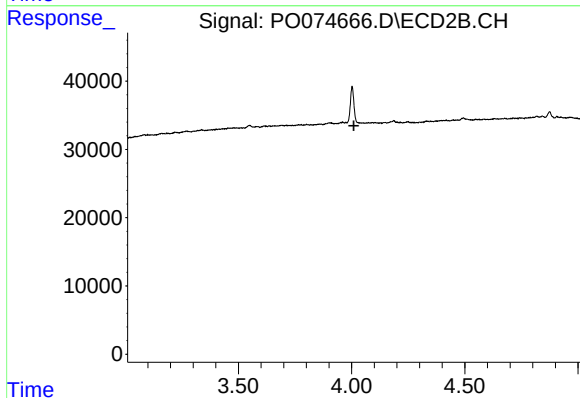


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.010 min
Response: 0
Conc: N.D.

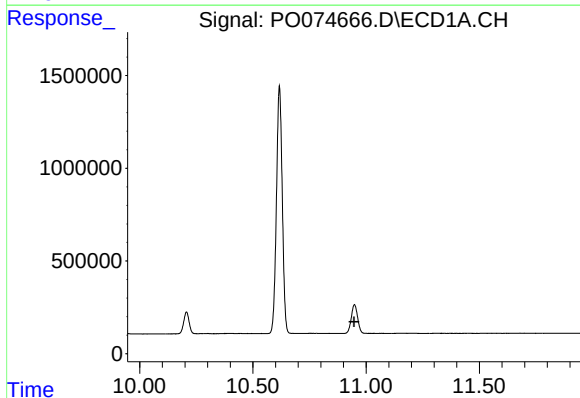


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.946 min
Response: 0
Conc: N.D.

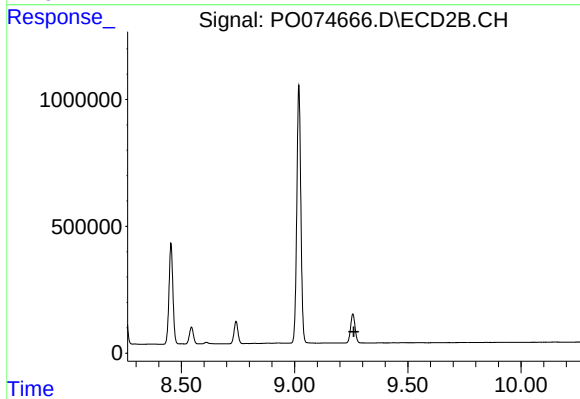

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 9.261 min
Response: 0
Conc: N.D.

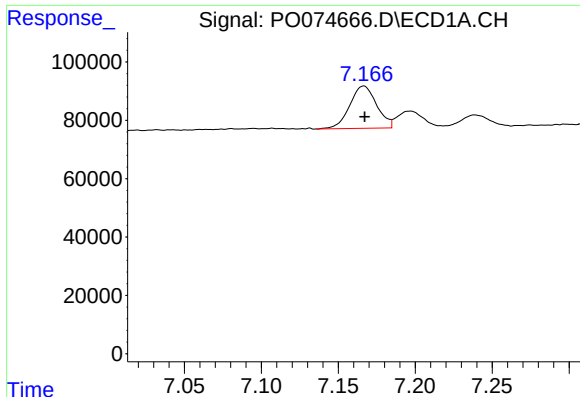

#26 AR-1254-1


R.T.: 7.167 min
Delta R.T.: 0.000 min
Response: 176715
Conc: 40.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
S21-03-BDL

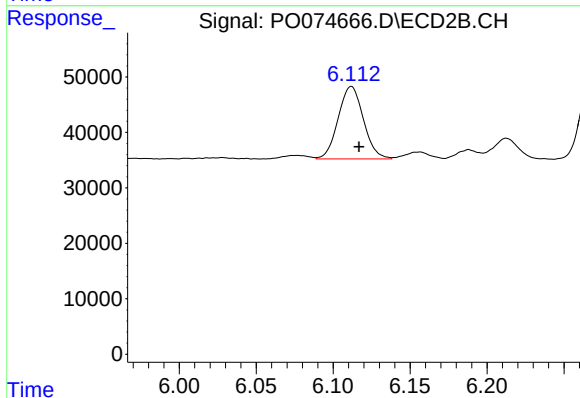


#26 AR-1254-1

R.T.: 6.112 min
Delta R.T.: -0.005 min
Response: 148836
Conc: 41.21 ng/ml

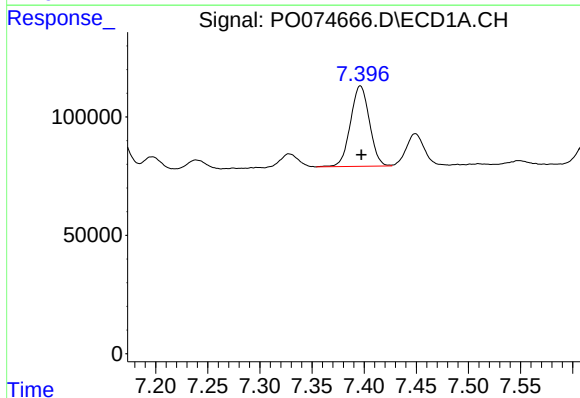


#27 AR-1254-2

R.T.: 7.396 min
Delta R.T.: -0.001 min
Response: 430010
Conc: 63.14 ng/ml

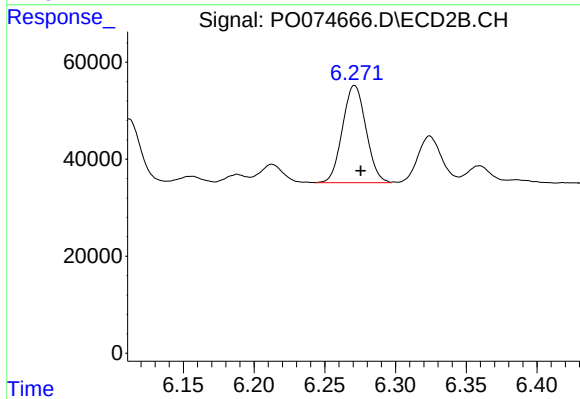

#27 AR-1254-2


R.T.: 6.271 min
Delta R.T.: -0.004 min
Response: 231694
Conc: 74.34 ng/ml

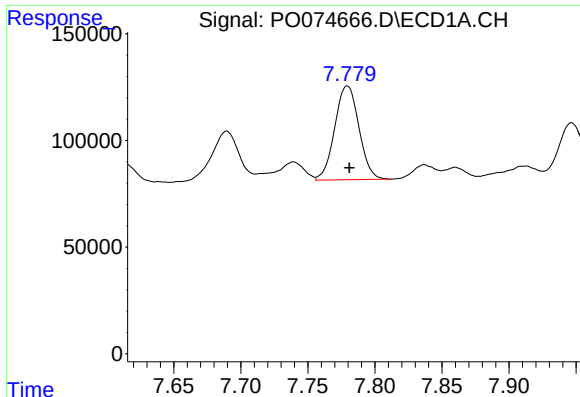

#28 AR-1254-3


R.T.: 7.779 min
Delta R.T.: -0.001 min
Response: 552634
Conc: 78.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
S21-03-BDL

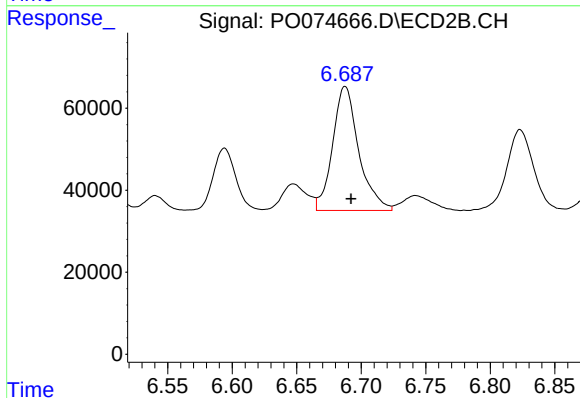


#28 AR-1254-3

R.T.: 6.688 min
Delta R.T.: -0.005 min
Response: 426818
Conc: 87.04 ng/ml

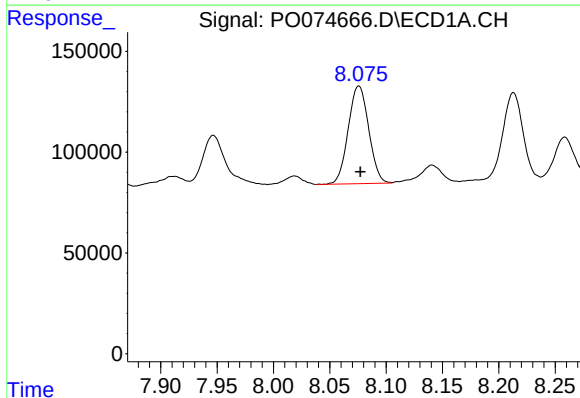


#29 AR-1254-4

R.T.: 8.076 min
Delta R.T.: -0.001 min
Response: 612868
Conc: 101.06 ng/ml

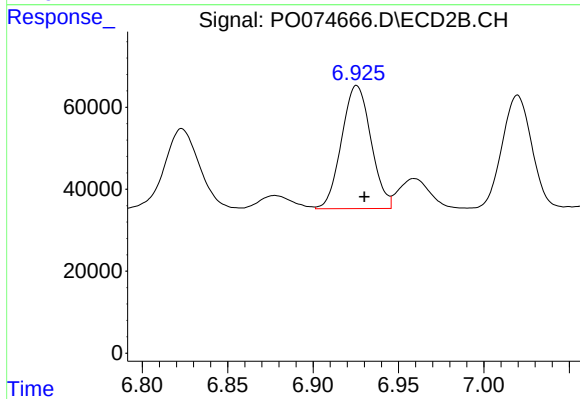

#29 AR-1254-4


R.T.: 6.926 min
Delta R.T.: -0.004 min
Response: 359876
Conc: 103.78 ng/ml

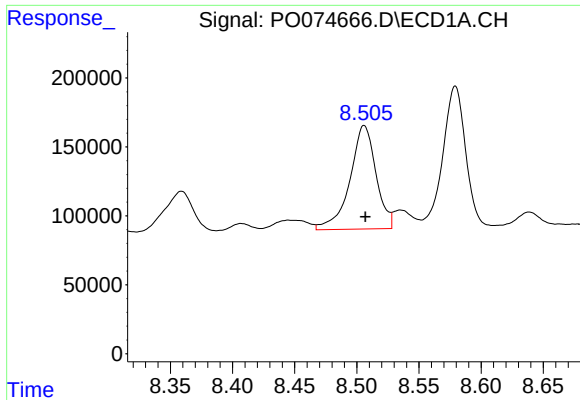

#30 AR-1254-5


R.T.: 8.506 min
Delta R.T.: -0.001 min
Response: 1099254
Conc: 189.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
S21-03-BDL

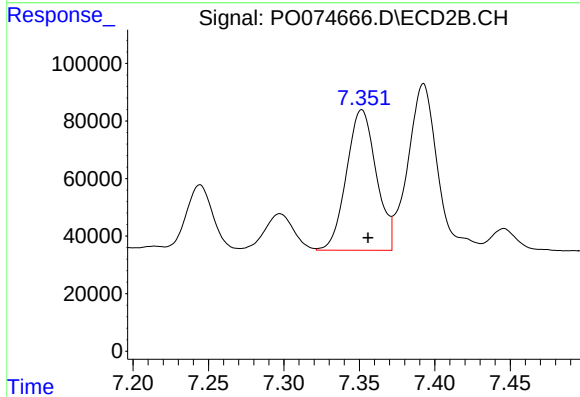


#30 AR-1254-5

R.T.: 7.352 min
Delta R.T.: -0.004 min
Response: 670692
Conc: 148.19 ng/ml

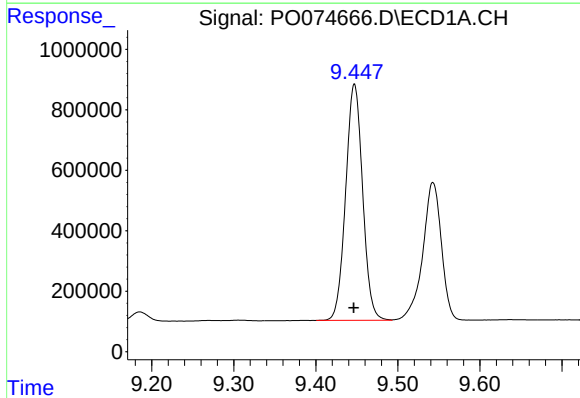


#41 AR-1268-1

R.T.: 9.447 min
Delta R.T.: 0.000 min
Response: 11244950
Conc: 601.87 ng/ml

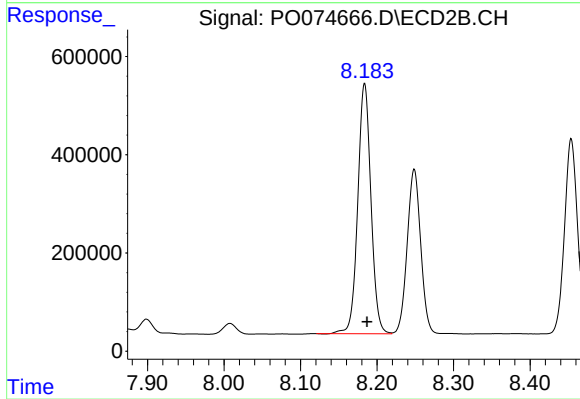

#41 AR-1268-1


R.T.: 8.184 min
Delta R.T.: -0.003 min
Response: 6097797
Conc: 544.70 ng/ml

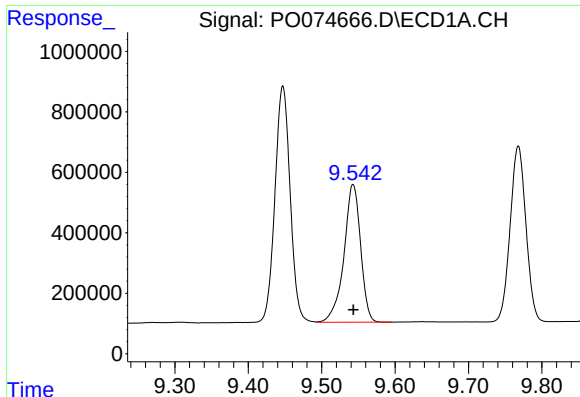

#42 AR-1268-2


R.T.: 9.543 min
Delta R.T.: 0.000 min
Response: 7203018
Conc: 451.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
S21-03-BDL

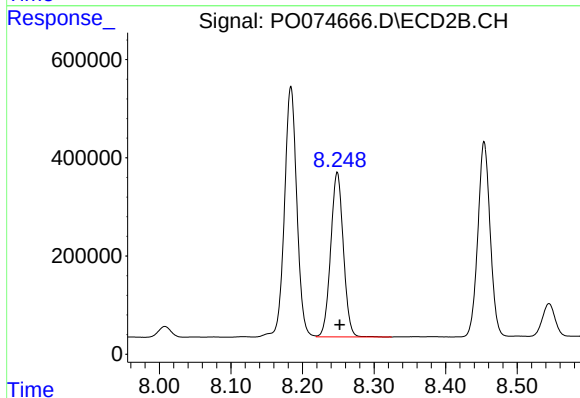


#42 AR-1268-2

R.T.: 8.249 min
Delta R.T.: -0.003 min
Response: 4111494
Conc: 429.75 ng/ml

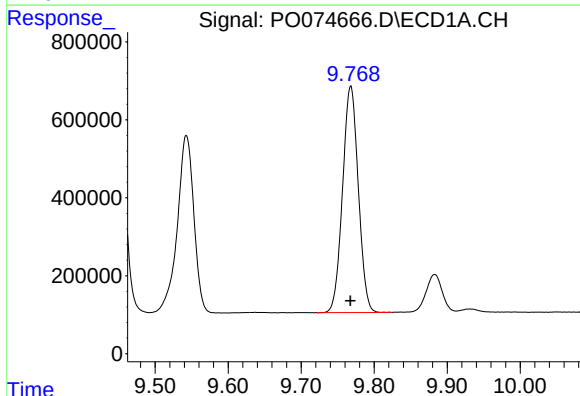


#43 AR-1268-3

R.T.: 9.768 min
Delta R.T.: 0.000 min
Response: 8695516
Conc: 612.27 ng/ml

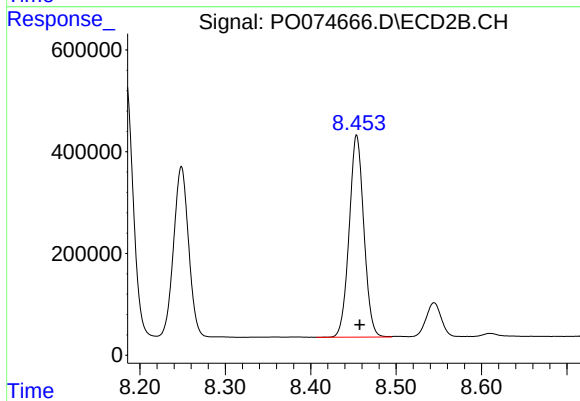

#43 AR-1268-3


R.T.: 8.454 min
Delta R.T.: -0.003 min
Response: 4733434
Conc: 569.69 ng/ml

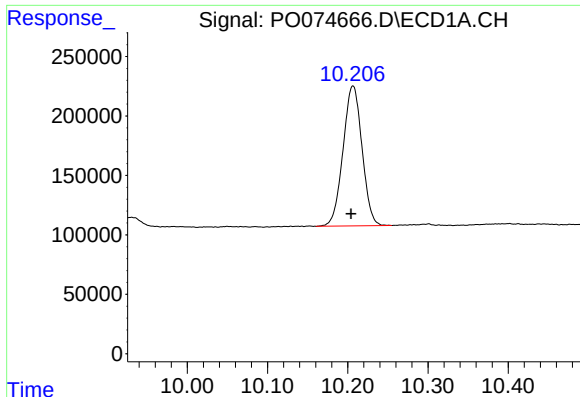

#44 AR-1268-4


R.T.: 10.207 min
Delta R.T.: 0.002 min
Response: 1939930
Conc: 331.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
S21-03-BDL

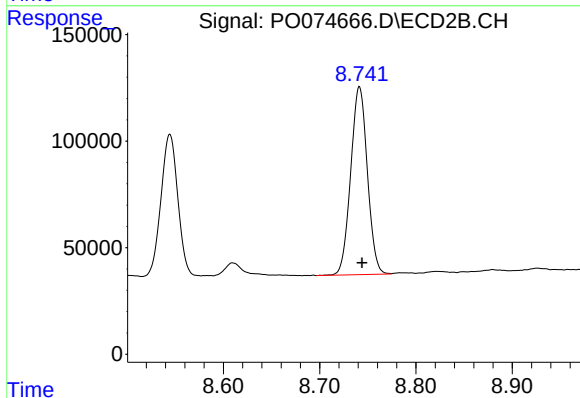


#44 AR-1268-4

R.T.: 8.741 min
Delta R.T.: -0.003 min
Response: 1057991
Conc: 304.97 ng/ml

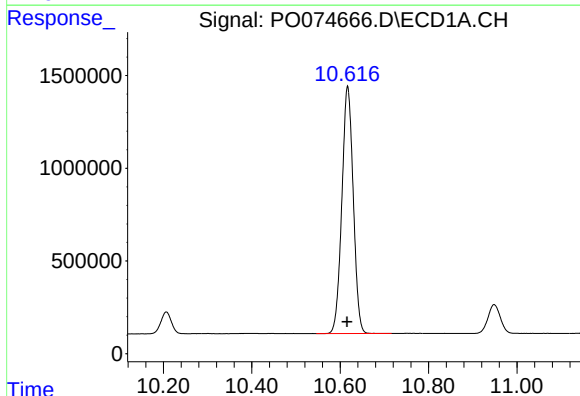

#45 AR-1268-5

R.T.: 10.617 min
Delta R.T.: 0.001 min
Response: 23829805
Conc: 570.25 ng/ml

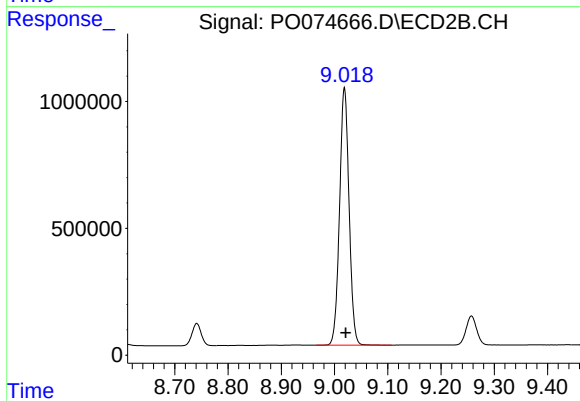

#45 AR-1268-5

R.T.: 9.019 min
Delta R.T.: -0.003 min
Response: 12585310
Conc: 531.50 ng/ml