

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011421\
 Data File : P0074671.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Jan 2021 13:47
 Operator : AJ/MA
 Sample : M1106-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S6-02-B

Manual Integrations
 APPROVED

Ankita
 1/15/2021 12:31:31 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 14 22:49:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.932	4.003	1969141	1060283	18.662	18.849
2) SA Decachlor...	10.953	9.257	1278584	658331	12.598	11.990
Target Compounds						
41) L9 AR-1268-1	9.450	8.184	443533	278687	23.739	24.894
42) L9 AR-1268-2	9.545	8.249	351974	202598	22.060	21.176
43) L9 AR-1268-3	9.771	8.454	341638	224480	24.056	27.017m
44) L9 AR-1268-4	10.209	8.740	57508	38506	9.816m	11.100
45) L9 AR-1268-5	10.619	9.018	1024739	519464	24.522	21.938

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO011421\
Data File : PO074671.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jan 2021 13:47
Operator : AJ/MA
Sample : M1106-02
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S6-02-B


Manual Integrations
APPROVED

Ankita
1/15/2021 12:31:31 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 14 22:49:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

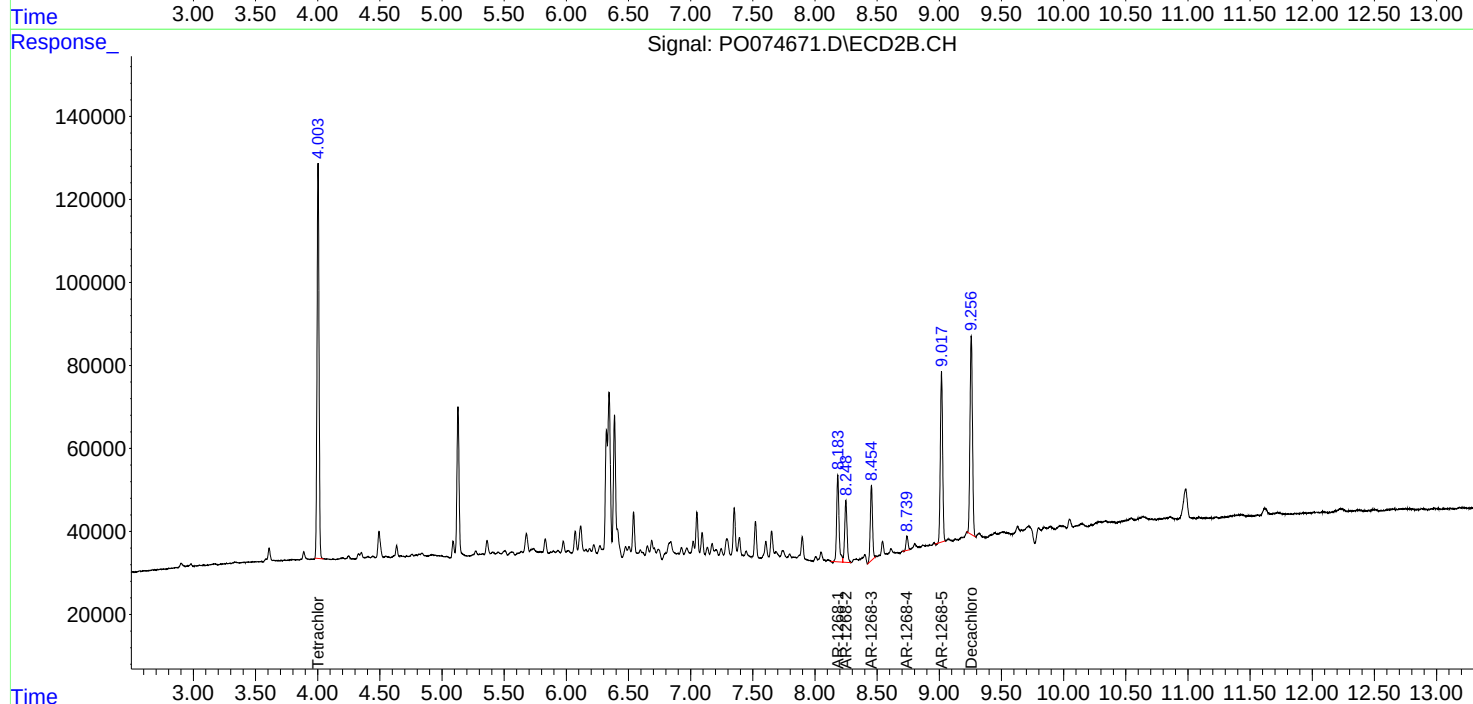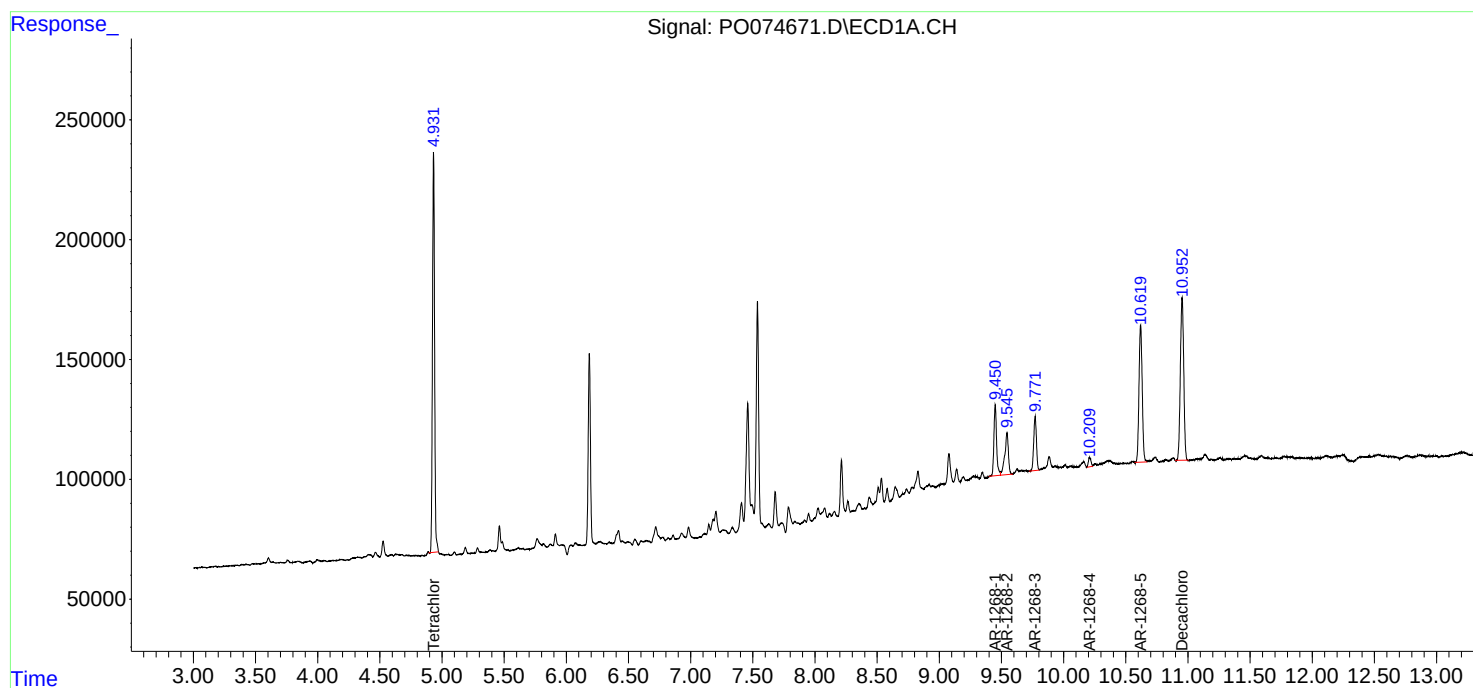

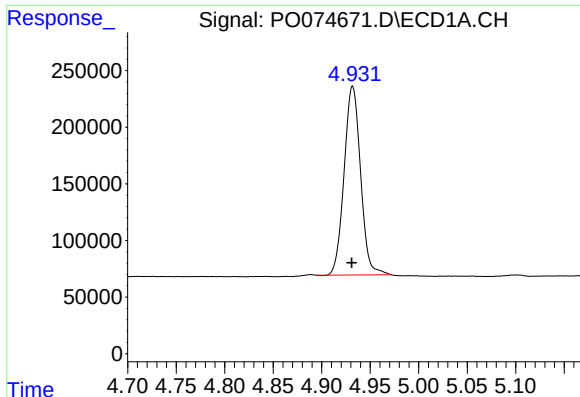


#1 Tetrachloro-m-xylene

R.T.: 4.932 min
Delta R.T.: 0.000 min
Response: 1969141
Conc: 18.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
S6-02-B


Manual Integrations
APPROVED

Ankita
1/15/2021 12:31:31 PM

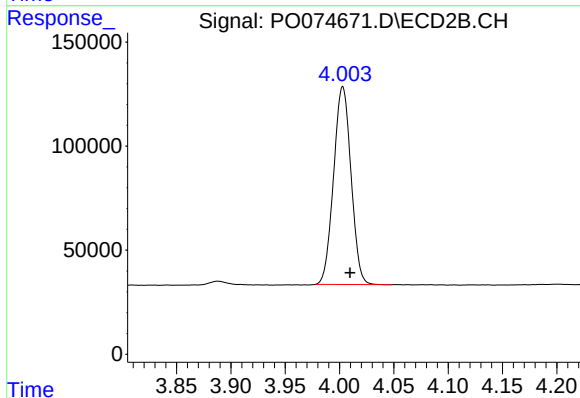


#1 Tetrachloro-m-xylene

R.T.: 4.003 min
Delta R.T.: -0.007 min
Response: 1060283
Conc: 18.85 ng/ml

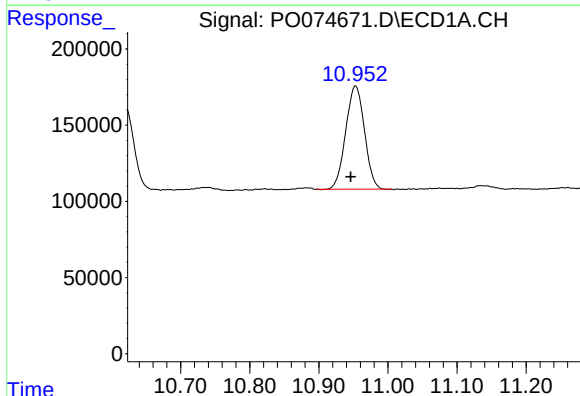


#2 Decachlorobiphenyl

R.T.: 10.953 min
Delta R.T.: 0.007 min
Response: 1278584
Conc: 12.60 ng/ml

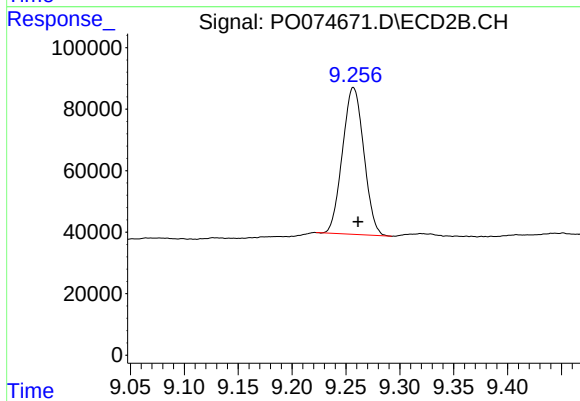

#2 Decachlorobiphenyl

R.T.: 9.257 min
Delta R.T.: -0.004 min
Response: 658331
Conc: 11.99 ng/ml

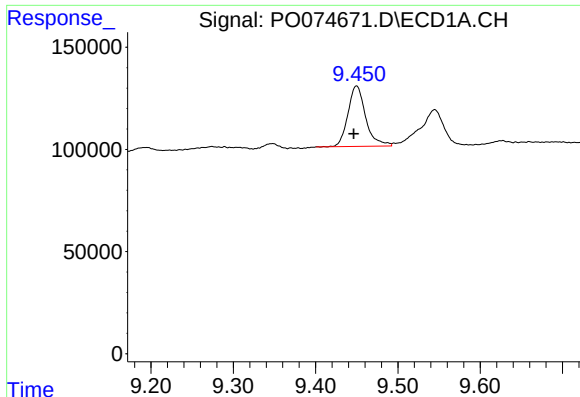


#41 AR-1268-1

R.T.: 9.450 min
Delta R.T.: 0.003 min
Response: 443533
Conc: 23.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
S6-02-B


Manual Integrations
APPROVED

Ankita
1/15/2021 12:31:31 PM

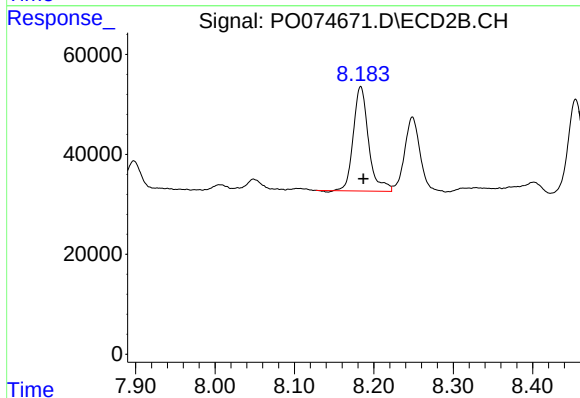


#41 AR-1268-1

R.T.: 8.184 min
Delta R.T.: -0.003 min
Response: 278687
Conc: 24.89 ng/ml

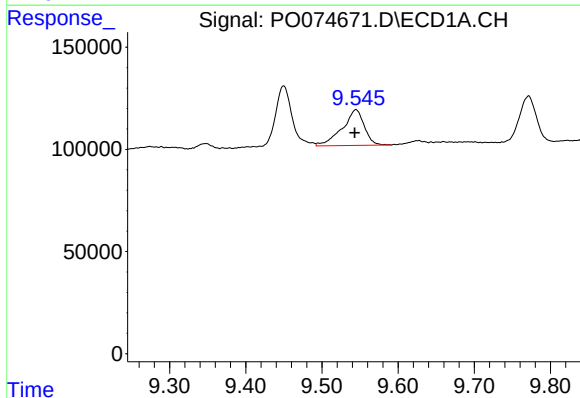


#42 AR-1268-2

R.T.: 9.545 min
Delta R.T.: 0.001 min
Response: 351974
Conc: 22.06 ng/ml

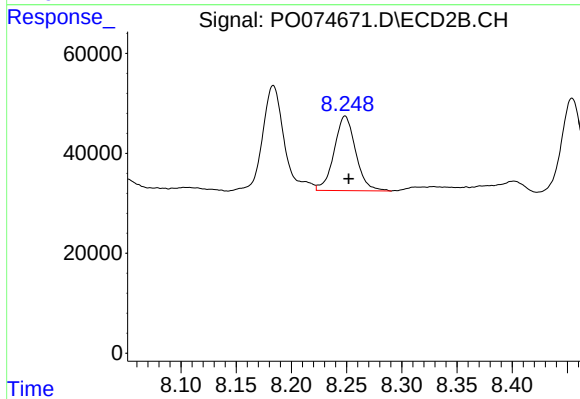

#42 AR-1268-2

R.T.: 8.249 min
Delta R.T.: -0.003 min
Response: 202598
Conc: 21.18 ng/ml

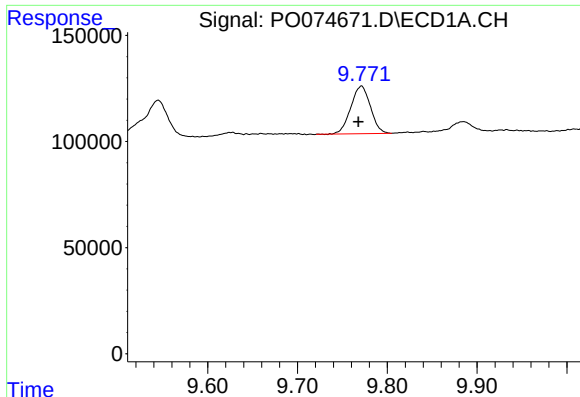


#43 AR-1268-3

R.T.: 9.771 min
Delta R.T.: 0.004 min
Response: 341638
Conc: 24.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
S6-02-B


Manual Integrations
APPROVED

Ankita
1/15/2021 12:31:31 PM

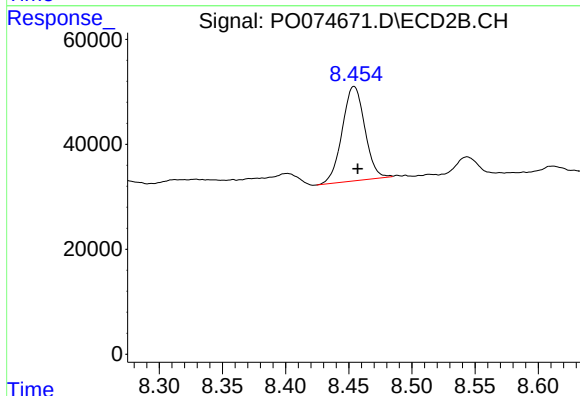


#43 AR-1268-3

R.T.: 8.454 min
Delta R.T.: -0.004 min
Response: 224480
Conc: 27.02 ng/ml m

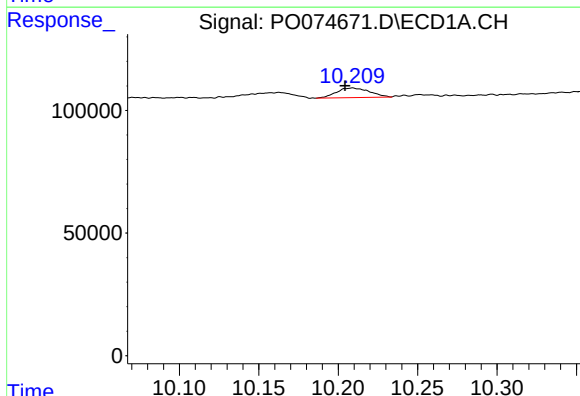


#44 AR-1268-4

R.T.: 10.209 min
Delta R.T.: 0.005 min
Response: 57508
Conc: 9.82 ng/ml m

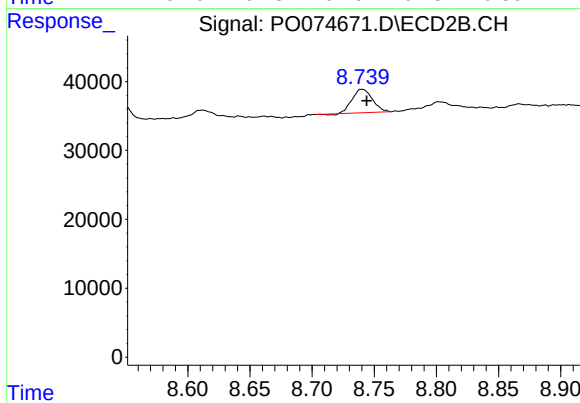

#44 AR-1268-4

R.T.: 8.740 min
Delta R.T.: -0.004 min
Response: 38506
Conc: 11.10 ng/ml

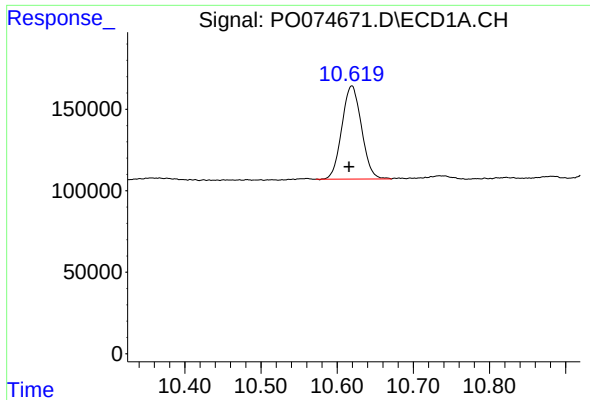


#45 AR-1268-5

R.T.: 10.619 min
Delta R.T.: 0.004 min
Response: 1024739
Conc: 24.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
S6-02-B

Manual Integrations
APPROVED

Ankita
1/15/2021 12:31:31 PM

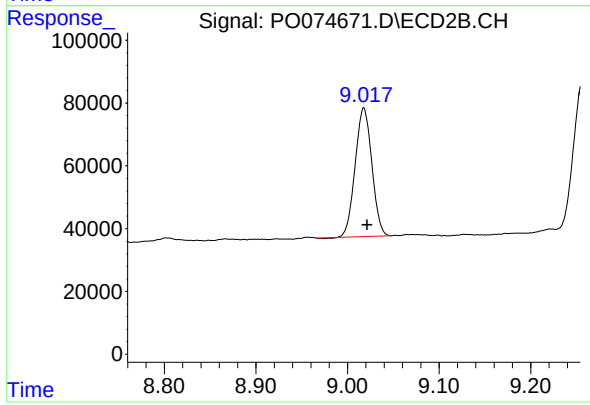

#45 AR-1268-5

R.T.: 9.018 min
Delta R.T.: -0.003 min
Response: 519464
Conc: 21.94 ng/ml