

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011421\
 Data File : P0074689.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Jan 2021 18:55
 Operator : AJ/MA
 Sample : M1097-02
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 263K-37A

Manual Integrations
 APPROVED

Ankita
 1/15/2021 1:21:31 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 15 08:57:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.931	4.004	1722602	940663	16.325	16.722
2) SA Decachlor...	10.951	9.256	1054080	609930	10.386	11.109
Target Compounds						
26) L6 AR-1254-1	7.168	6.113	155523	219828	35.361	60.860 #
27) L6 AR-1254-2	7.399	6.272	550414	235050	80.815	75.420
28) L6 AR-1254-3	7.782	6.688	980999	753813	139.856	153.716
29) L6 AR-1254-4	8.076	6.926	560812	270528	92.472	78.012
30) L6 AR-1254-5	8.513	7.352	1506883	7210875	259.408m	1593.232 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011421\
Data File : PO074689.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jan 2021 18:55
Operator : AJ/MA
Sample : M1097-02
Misc :
ALS Vial : 53 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
263K-37A


Manual Integrations
APPROVED

Ankita
1/15/2021 1:21:31 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 15 08:57:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

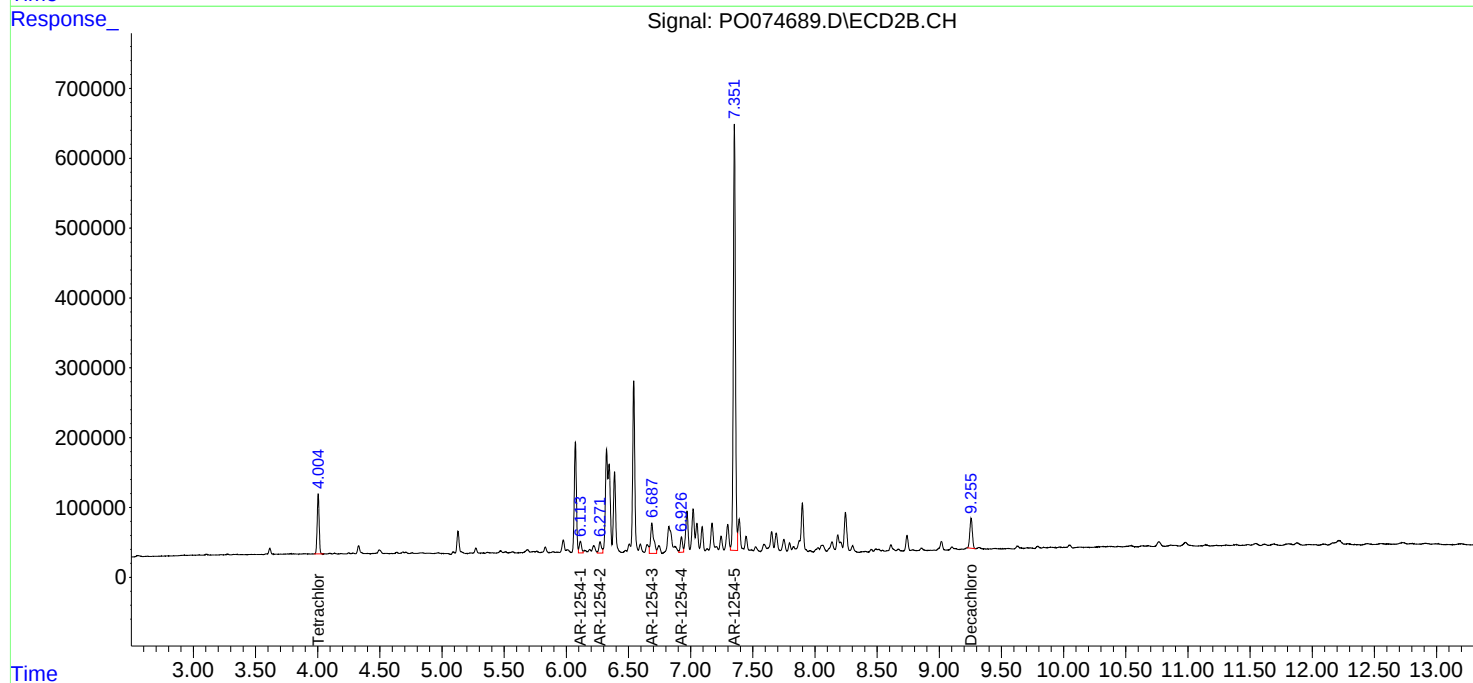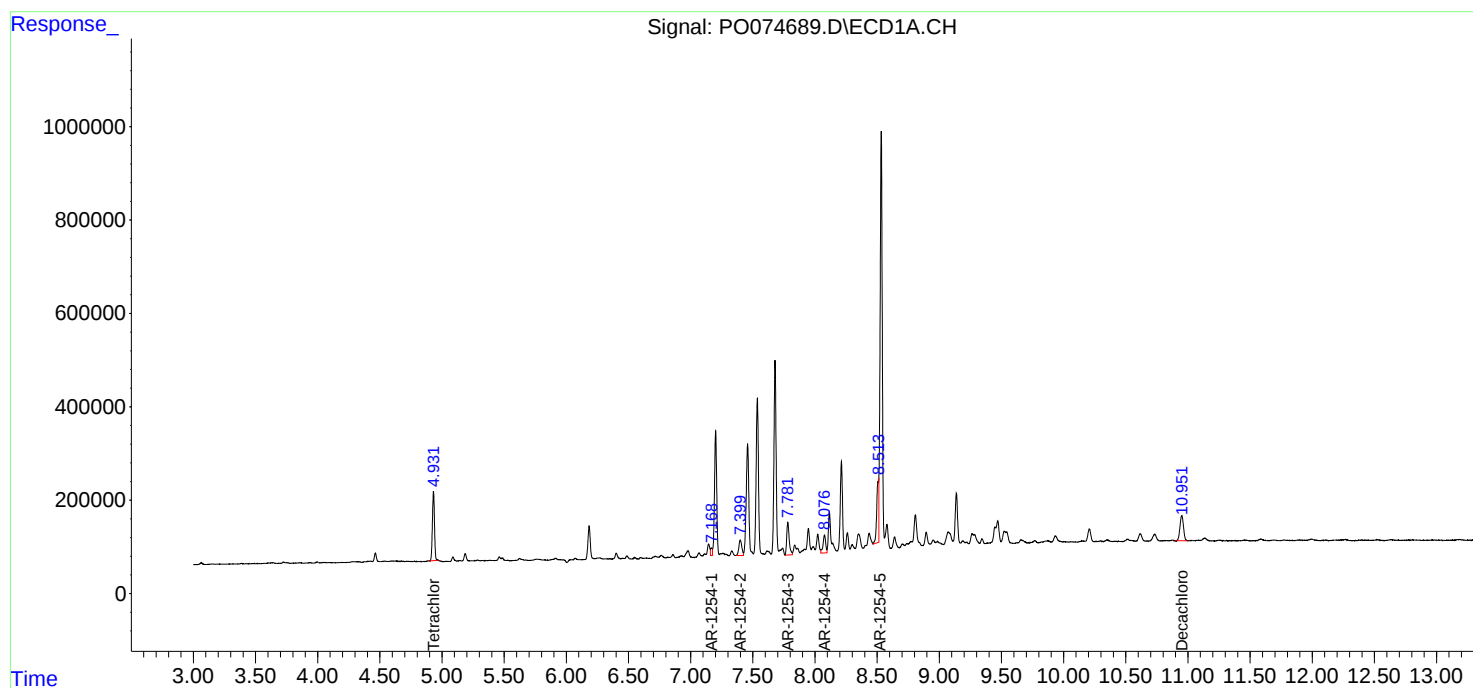

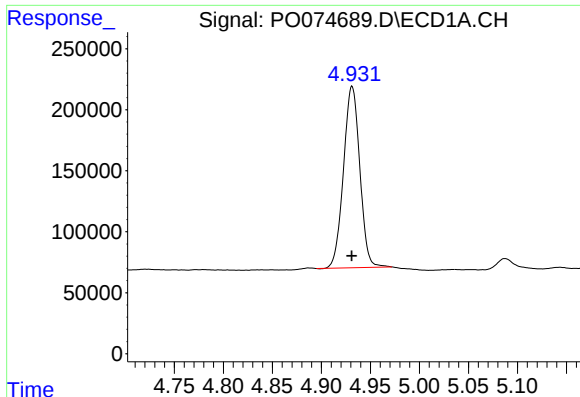


#1 Tetrachloro-m-xylene

R.T.: 4.931 min
Delta R.T.: 0.000 min
Response: 1722602
Conc: 16.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-37A


Manual Integrations
APPROVED

Ankita
1/15/2021 1:21:31 PM

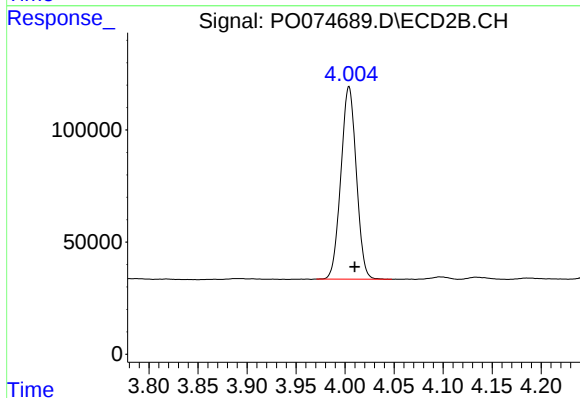


#1 Tetrachloro-m-xylene

R.T.: 4.004 min
Delta R.T.: -0.006 min
Response: 940663
Conc: 16.72 ng/ml

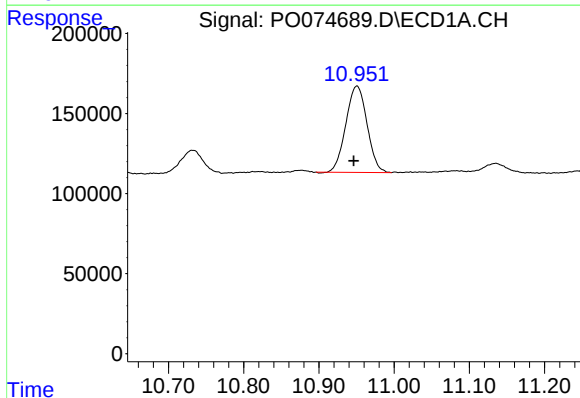


#2 Decachlorobiphenyl

R.T.: 10.951 min
Delta R.T.: 0.004 min
Response: 1054080
Conc: 10.39 ng/ml

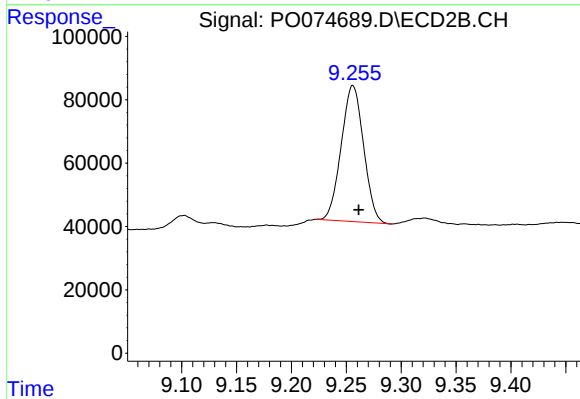

#2 Decachlorobiphenyl

R.T.: 9.256 min
Delta R.T.: -0.005 min
Response: 609930
Conc: 11.11 ng/ml

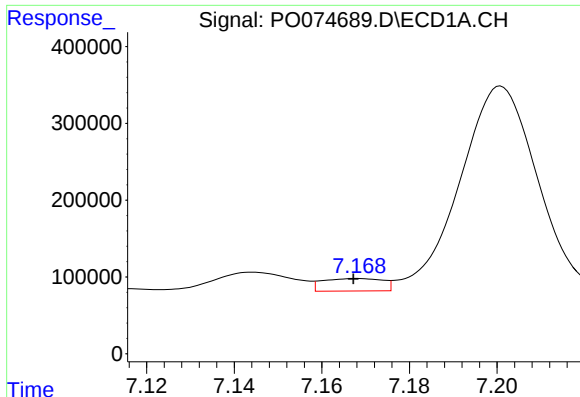


#26 AR-1254-1

R.T.: 7.168 min
Delta R.T.: 0.001 min
Response: 155523
Conc: 35.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-37A


Manual Integrations
APPROVED

Ankita
1/15/2021 1:21:31 PM

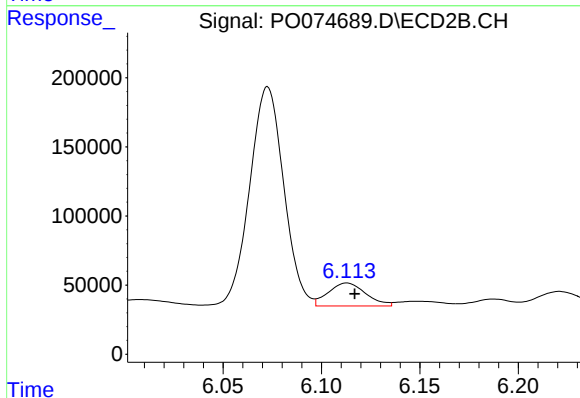


#26 AR-1254-1

R.T.: 6.113 min
Delta R.T.: -0.004 min
Response: 219828
Conc: 60.86 ng/ml

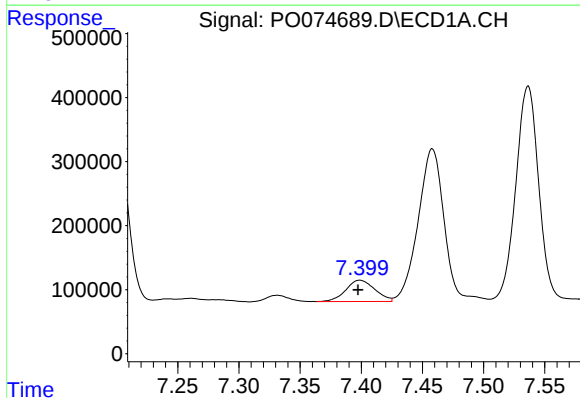


#27 AR-1254-2

R.T.: 7.399 min
Delta R.T.: 0.001 min
Response: 550414
Conc: 80.82 ng/ml

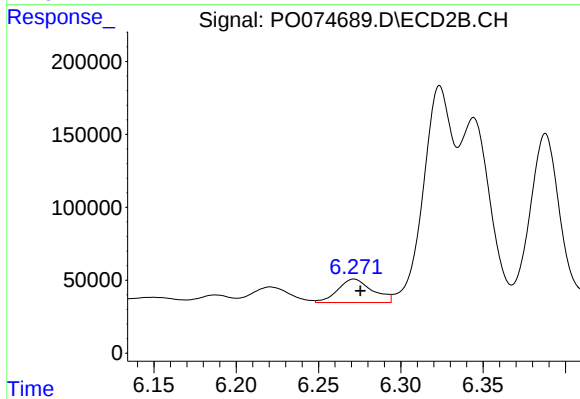

#27 AR-1254-2

R.T.: 6.272 min
Delta R.T.: -0.004 min
Response: 235050
Conc: 75.42 ng/ml

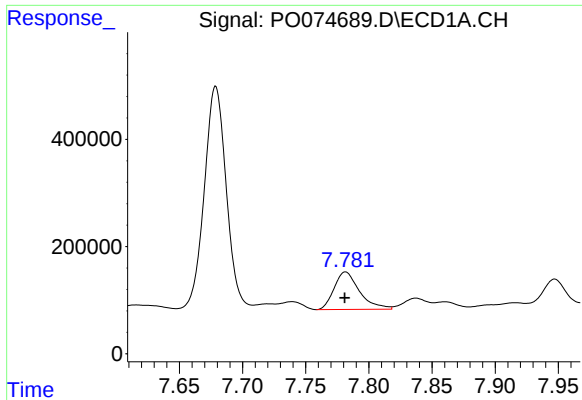


#28 AR-1254-3

R.T.: 7.782 min
Delta R.T.: 0.000 min
Response: 980999
Conc: 139.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-37A


Manual Integrations
APPROVED

Ankita
1/15/2021 1:21:31 PM

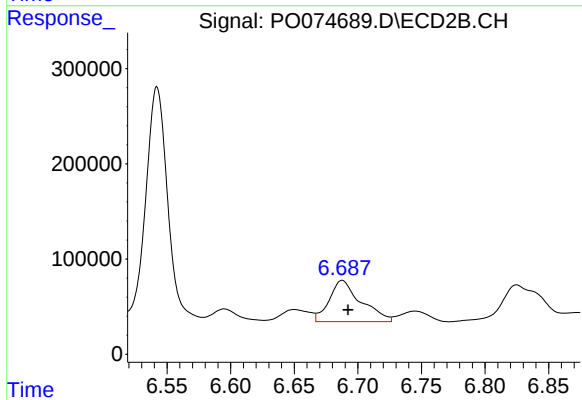


#28 AR-1254-3

R.T.: 6.688 min
Delta R.T.: -0.004 min
Response: 753813
Conc: 153.72 ng/ml

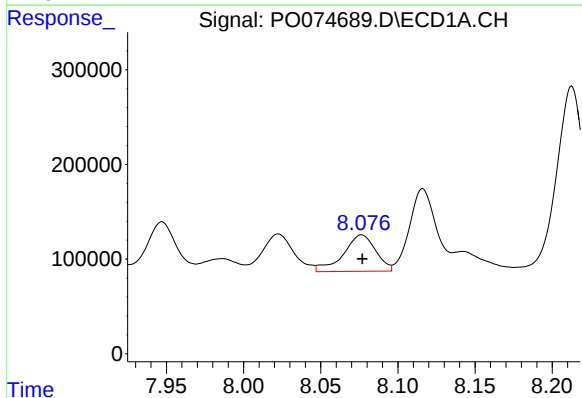


#29 AR-1254-4

R.T.: 8.076 min
Delta R.T.: 0.000 min
Response: 560812
Conc: 92.47 ng/ml

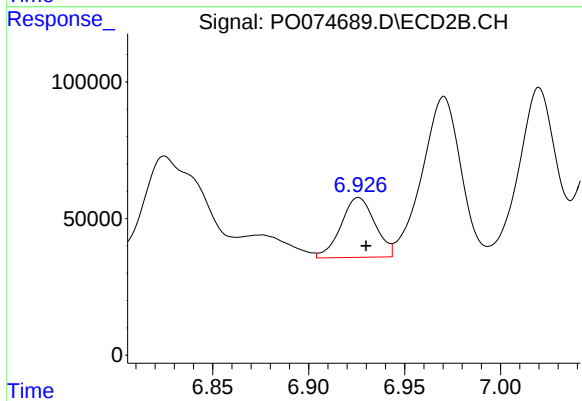

#29 AR-1254-4

R.T.: 6.926 min
Delta R.T.: -0.004 min
Response: 270528
Conc: 78.01 ng/ml

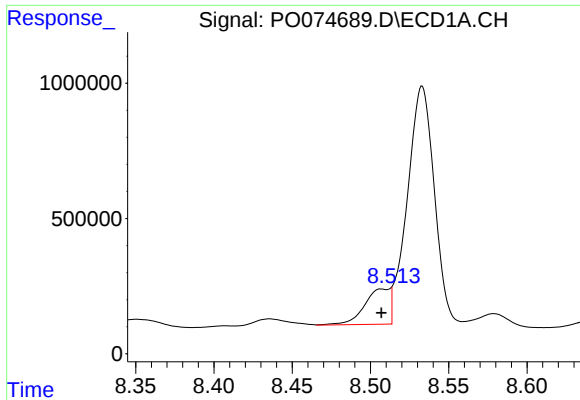


#30 AR-1254-5

R.T.: 8.513 min
Delta R.T.: 0.006 min
Response: 1506883
Conc: 259.41 ng/ml m

Instrument :
ECD_O
ClientSampleId :
263K-37A

Manual Integrations
APPROVED

Ankita
1/15/2021 1:21:31 PM

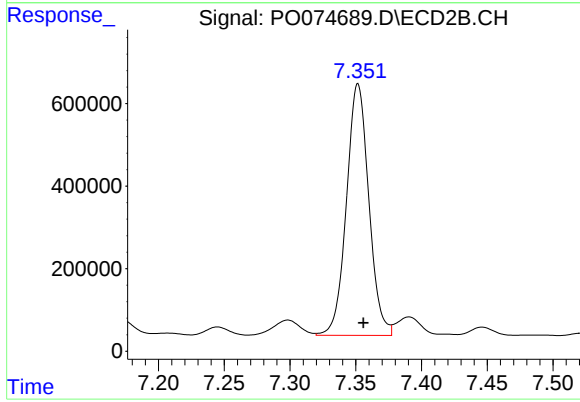

#30 AR-1254-5

R.T.: 7.352 min
Delta R.T.: -0.004 min
Response: 7210875
Conc: 1593.23 ng/ml