

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011421\
 Data File : P0074690.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Jan 2021 19:12
 Operator : AJ/MA
 Sample : M1097-05
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 263K-38A

Manual Integrations
 APPROVED

Ankita
 1/15/2021 1:21:32 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 15 09:00:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.932	4.005	1960020	1111837	18.575	19.765
2) SA Decachlor...	10.952	9.258	1270200	760971	12.515	13.860
Target Compounds						
26) L6 AR-1254-1	7.177	6.115	131196	228026	29.830m	63.130 #
27) L6 AR-1254-2	7.404	6.272	539535	135439	79.218	43.458 #
28) L6 AR-1254-3	7.783	6.689	859560	611558	122.543	124.708
29) L6 AR-1254-4	8.077	6.928	485785	186106	80.101	53.667 #
30) L6 AR-1254-5	8.514	7.353	1381212	5614539	237.774m	1240.524 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011421\
Data File : PO074690.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jan 2021 19:12
Operator : AJ/MA
Sample : M1097-05
Misc :
ALS Vial : 54 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
263K-38A


Manual Integrations
APPROVED

Ankita
1/15/2021 1:21:32 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 15 09:00:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

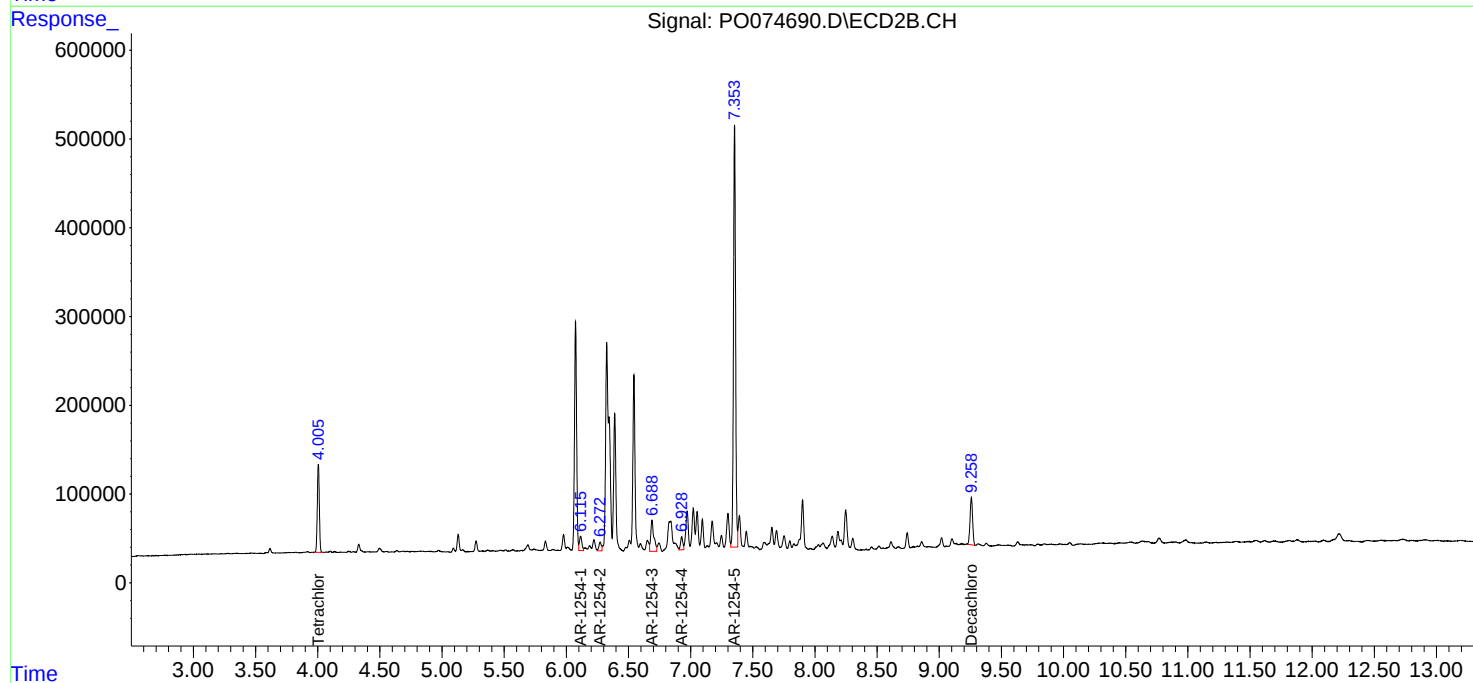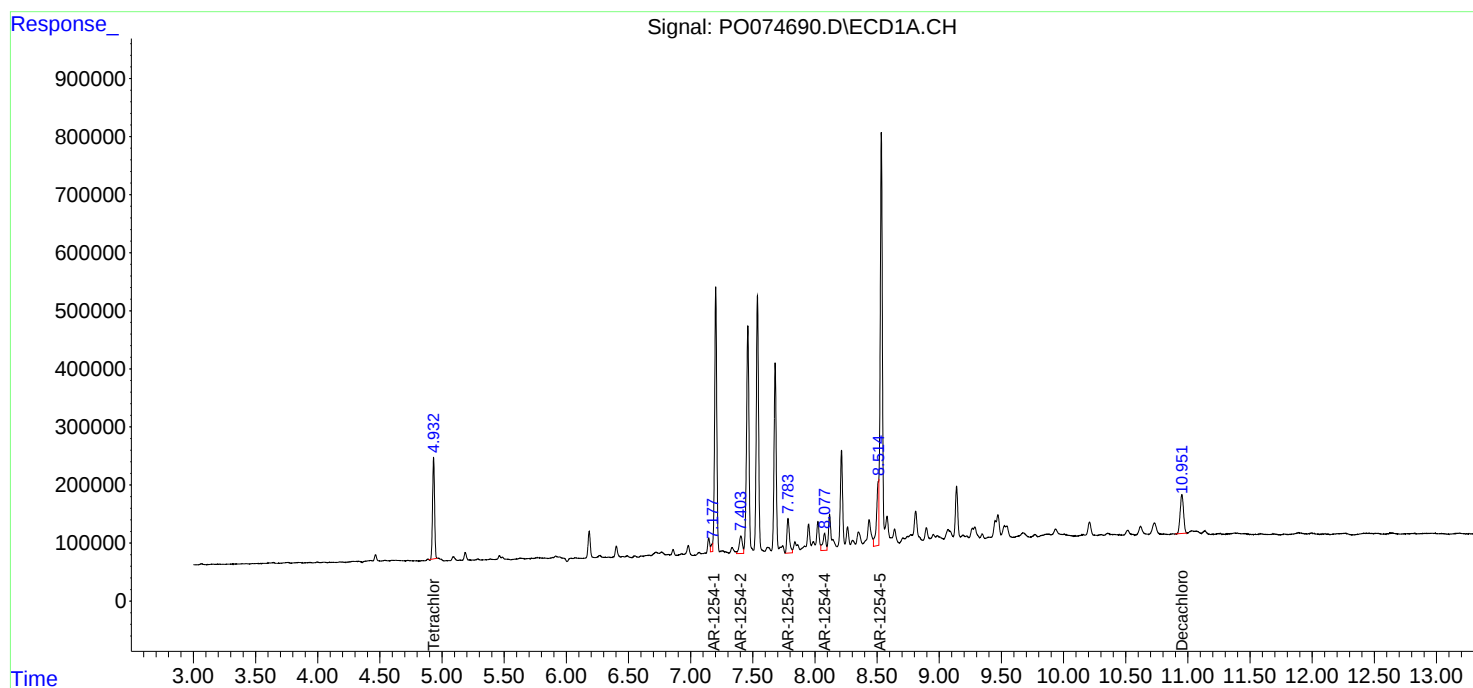

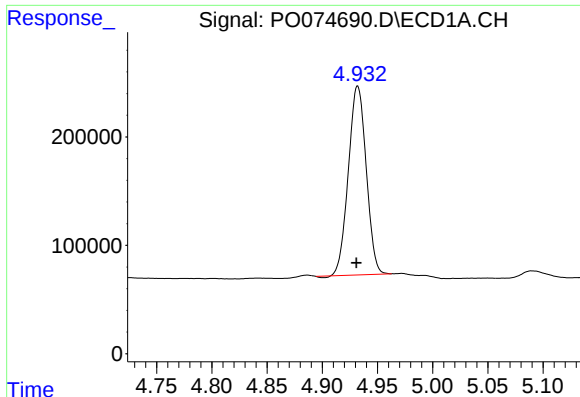


#1 Tetrachloro-m-xylene

R.T.: 4.932 min
Delta R.T.: 0.001 min
Response: 1960020
Conc: 18.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-38A


Manual Integrations
APPROVED

Ankita
1/15/2021 1:21:32 PM

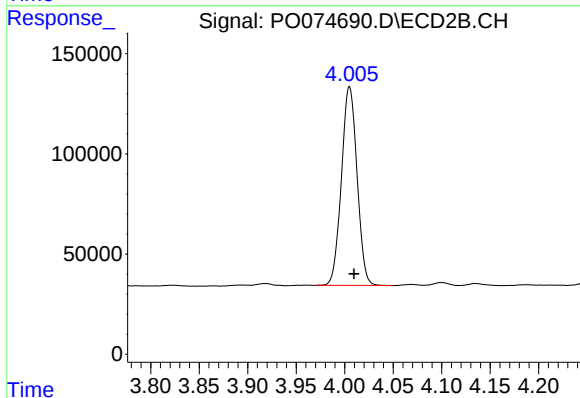


#1 Tetrachloro-m-xylene

R.T.: 4.005 min
Delta R.T.: -0.005 min
Response: 1111837
Conc: 19.77 ng/ml

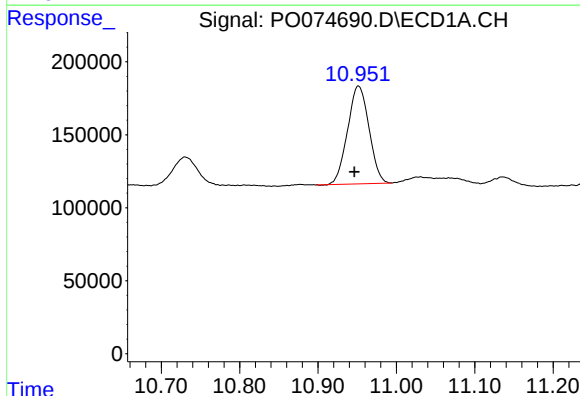


#2 Decachlorobiphenyl

R.T.: 10.952 min
Delta R.T.: 0.005 min
Response: 1270200
Conc: 12.52 ng/ml

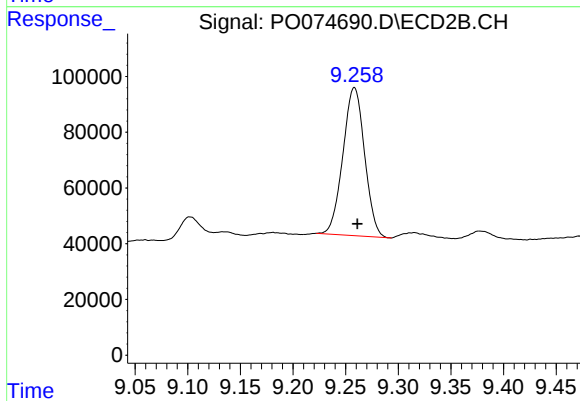

#2 Decachlorobiphenyl

R.T.: 9.258 min
Delta R.T.: -0.003 min
Response: 760971
Conc: 13.86 ng/ml

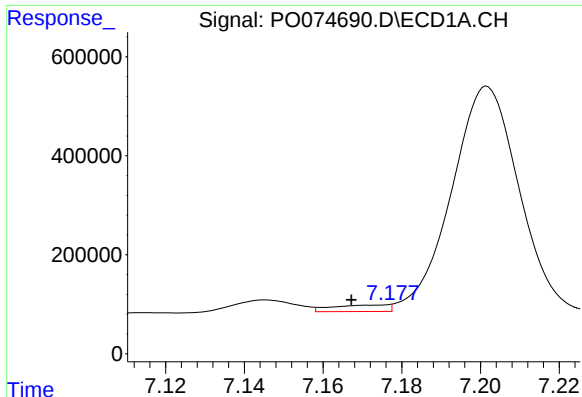


#26 AR-1254-1

R.T.: 7.177 min
Delta R.T.: 0.010 min
Response: 131196
Conc: 29.83 ng/ml m

Instrument :
ECD_O
ClientSampleId :
263K-38A


Manual Integrations
APPROVED

Ankita
1/15/2021 1:21:32 PM

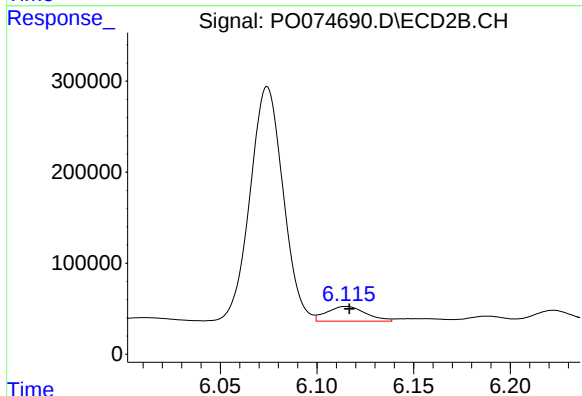


#26 AR-1254-1

R.T.: 6.115 min
Delta R.T.: -0.002 min
Response: 228026
Conc: 63.13 ng/ml

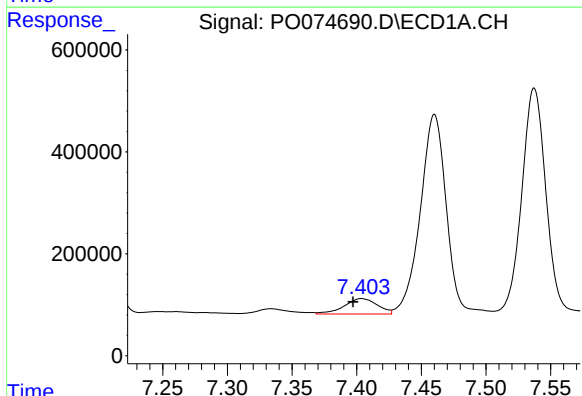


#27 AR-1254-2

R.T.: 7.404 min
Delta R.T.: 0.006 min
Response: 539535
Conc: 79.22 ng/ml

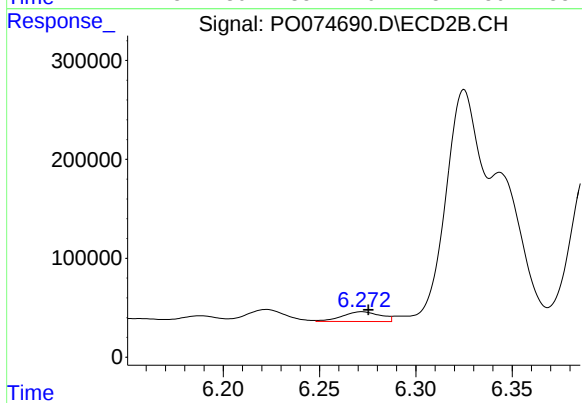

#27 AR-1254-2

R.T.: 6.272 min
Delta R.T.: -0.003 min
Response: 135439
Conc: 43.46 ng/ml

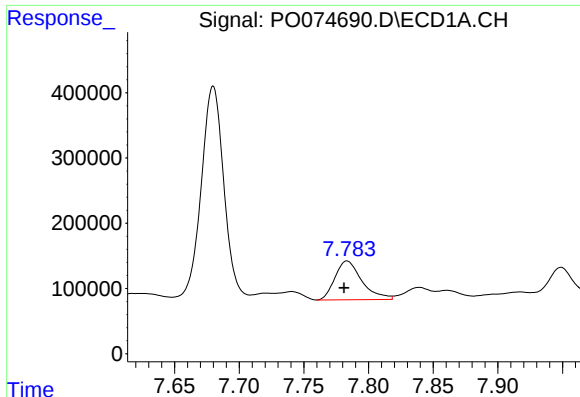


#28 AR-1254-3

R.T.: 7.783 min
Delta R.T.: 0.002 min
Response: 859560
Conc: 122.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-38A


Manual Integrations
APPROVED

Ankita
1/15/2021 1:21:32 PM

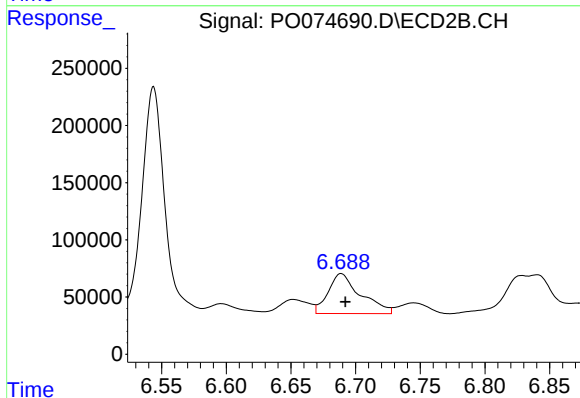


#28 AR-1254-3

R.T.: 6.689 min
Delta R.T.: -0.003 min
Response: 611558
Conc: 124.71 ng/ml

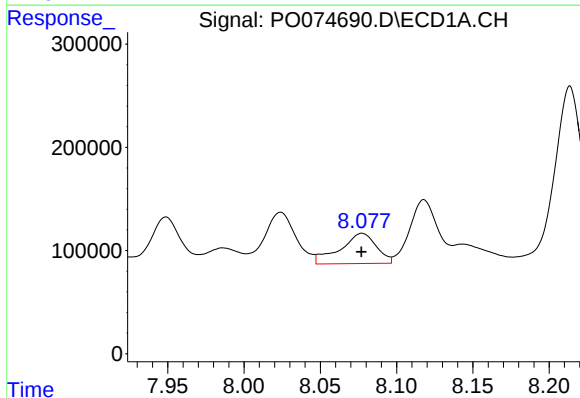


#29 AR-1254-4

R.T.: 8.077 min
Delta R.T.: 0.000 min
Response: 485785
Conc: 80.10 ng/ml

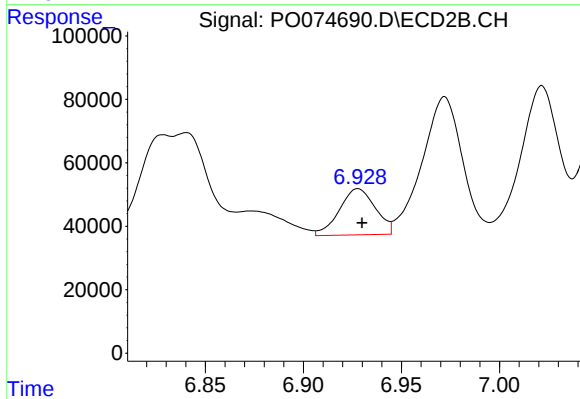

#29 AR-1254-4

R.T.: 6.928 min
Delta R.T.: -0.002 min
Response: 186106
Conc: 53.67 ng/ml

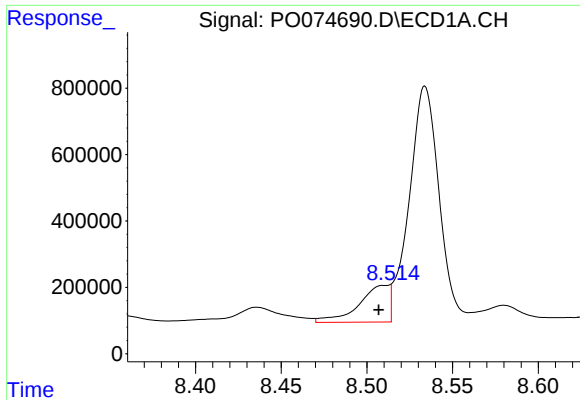


#30 AR-1254-5

R.T.: 8.514 min
Delta R.T.: 0.007 min
Response: 1381212
Conc: 237.77 ng/ml m

Instrument :
ECD_O
ClientSampleId :
263K-38A

Manual Integrations
APPROVED

Ankita
1/15/2021 1:21:32 PM

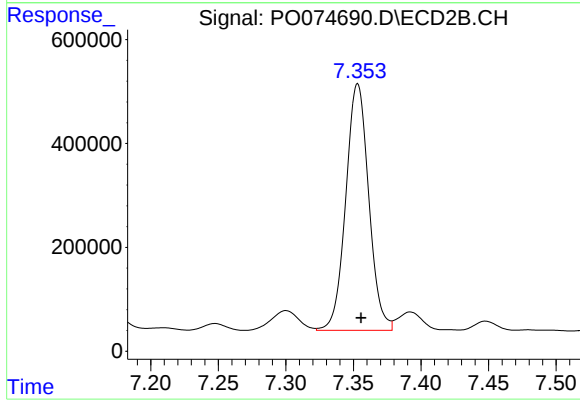

#30 AR-1254-5

R.T.: 7.353 min
Delta R.T.: -0.003 min
Response: 5614539
Conc: 1240.52 ng/ml