

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011421\
 Data File : P0074694.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Jan 2021 20:20
 Operator : AJ/MA
 Sample : M1097-11
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 263K-40A

Manual Integrations
 APPROVED

Ankita
 1/15/2021 1:21:36 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 15 09:03:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.930	4.003	1316900	679695	12.480	12.083
2) SA Decachlor...	10.948	9.256	815319	468086	8.033	8.525
Target Compounds						
26) L6 AR-1254-1	7.171	6.112	78570	161161	17.864m	44.618 #
27) L6 AR-1254-2	7.400	6.270	423422	146760	62.169	47.091
28) L6 AR-1254-3	7.782	6.686	710468	320472	101.288	65.350m#
29) L6 AR-1254-4	8.076	6.925	450321	167734	74.253	48.369 #
30) L6 AR-1254-5	8.506	7.351	1628003	3934540	280.258	869.331 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011421\
Data File : PO074694.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jan 2021 20:20
Operator : AJ/MA
Sample : M1097-11
Misc :
ALS Vial : 58 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
263K-40A


Manual Integrations
APPROVED

Ankita
1/15/2021 1:21:36 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 15 09:03:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

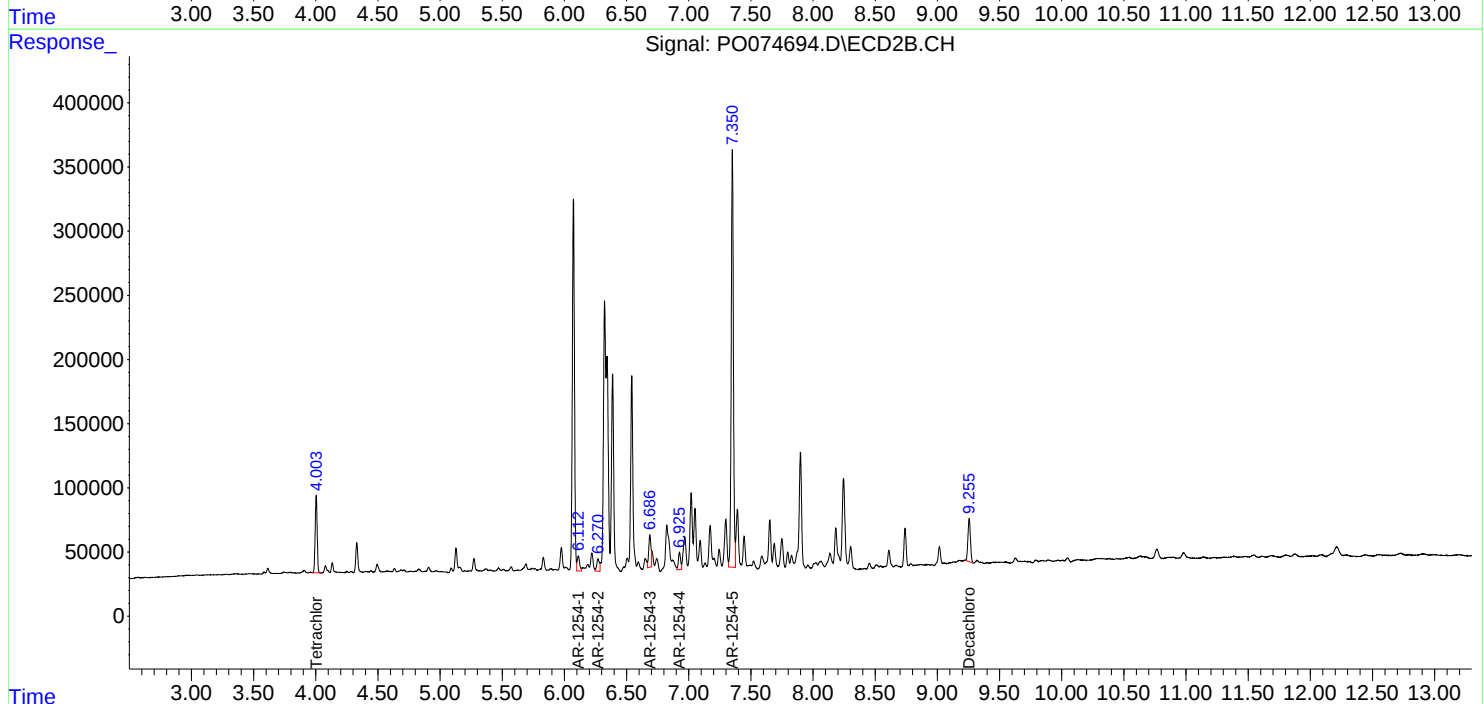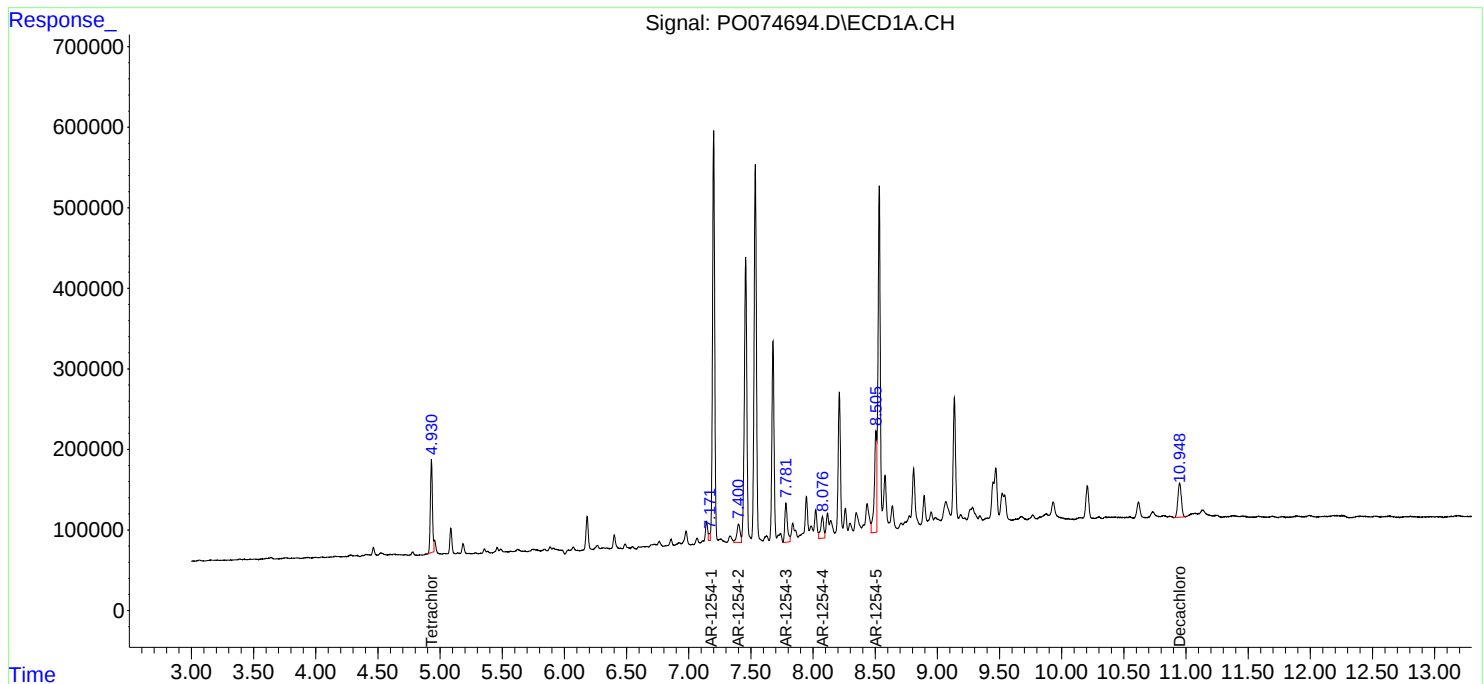

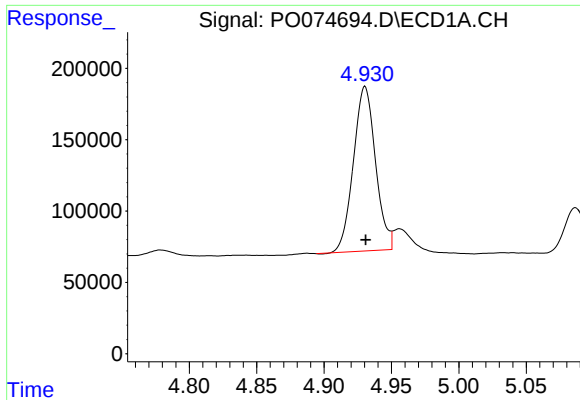


#1 Tetrachloro-m-xylene

R.T.: 4.930 min
Delta R.T.: 0.000 min
Response: 1316900
Conc: 12.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-40A


Manual Integrations
APPROVED

Ankita
1/15/2021 1:21:36 PM

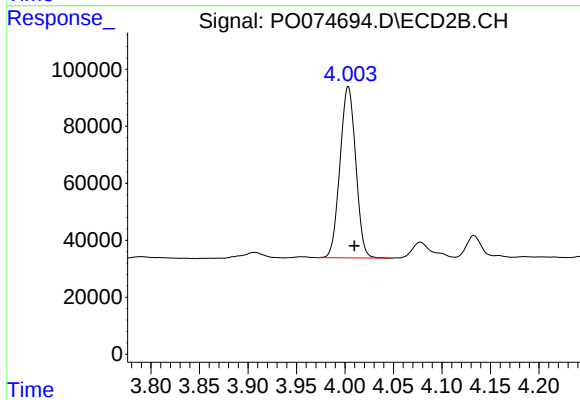


#1 Tetrachloro-m-xylene

R.T.: 4.003 min
Delta R.T.: -0.006 min
Response: 679695
Conc: 12.08 ng/ml

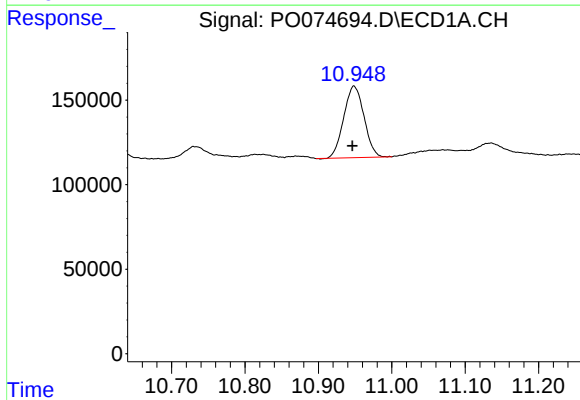


#2 Decachlorobiphenyl

R.T.: 10.948 min
Delta R.T.: 0.002 min
Response: 815319
Conc: 8.03 ng/ml

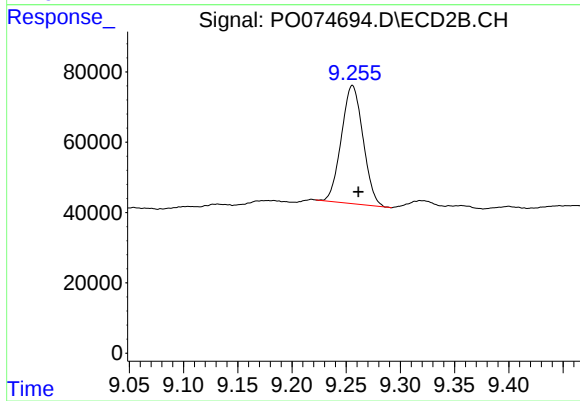

#2 Decachlorobiphenyl

R.T.: 9.256 min
Delta R.T.: -0.006 min
Response: 468086
Conc: 8.53 ng/ml

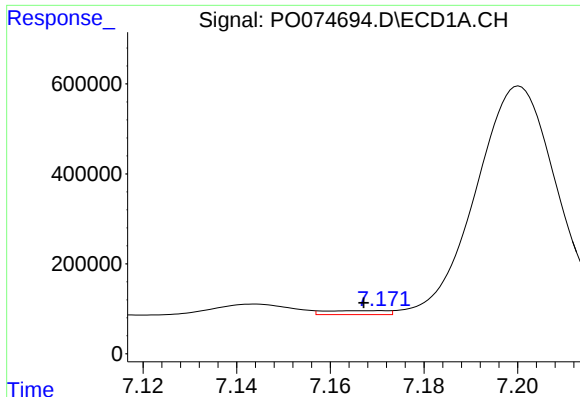


#26 AR-1254-1

R.T.: 7.171 min
Delta R.T.: 0.004 min
Response: 78570
Conc: 17.86 ng/ml m

Instrument :
ECD_O
ClientSampleId :
263K-40A


Manual Integrations
APPROVED

Ankita
1/15/2021 1:21:36 PM

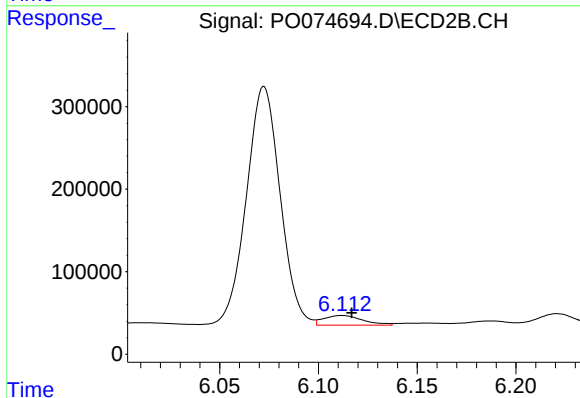


#26 AR-1254-1

R.T.: 6.112 min
Delta R.T.: -0.005 min
Response: 161161
Conc: 44.62 ng/ml

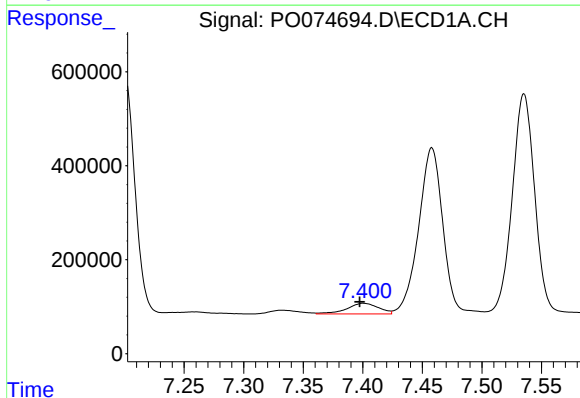


#27 AR-1254-2

R.T.: 7.400 min
Delta R.T.: 0.003 min
Response: 423422
Conc: 62.17 ng/ml

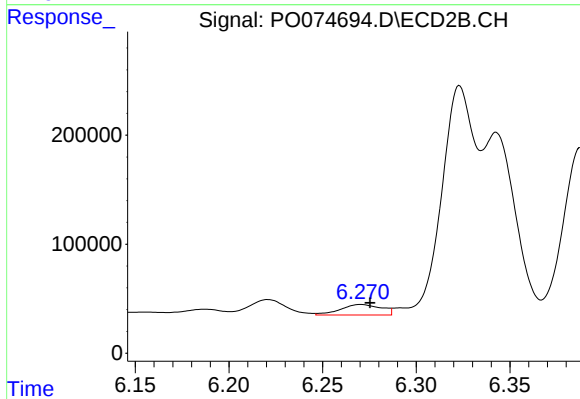

#27 AR-1254-2

R.T.: 6.270 min
Delta R.T.: -0.005 min
Response: 146760
Conc: 47.09 ng/ml

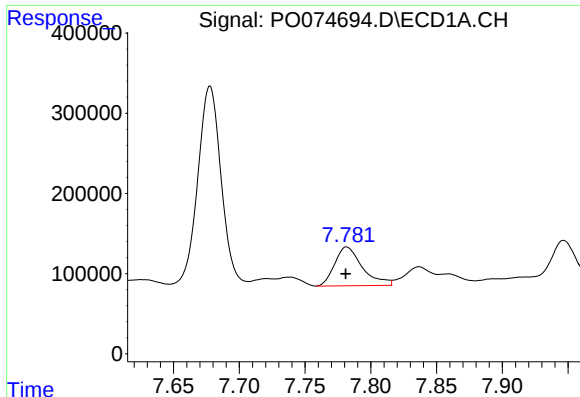


#28 AR-1254-3

R.T.: 7.782 min
Delta R.T.: 0.000 min
Response: 710468
Conc: 101.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-40A


Manual Integrations
APPROVED

Ankita
1/15/2021 1:21:36 PM

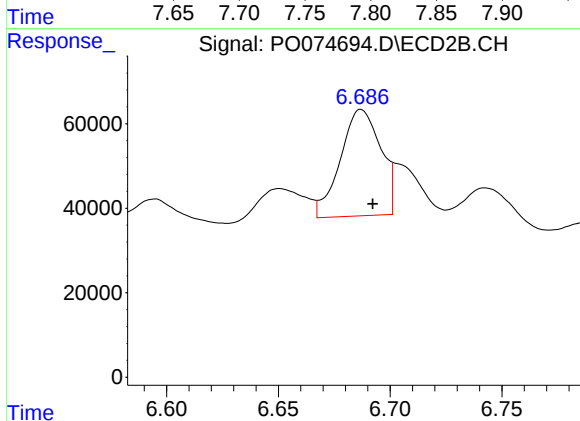


#28 AR-1254-3

R.T.: 6.686 min
Delta R.T.: -0.006 min
Response: 320472
Conc: 65.35 ng/ml m

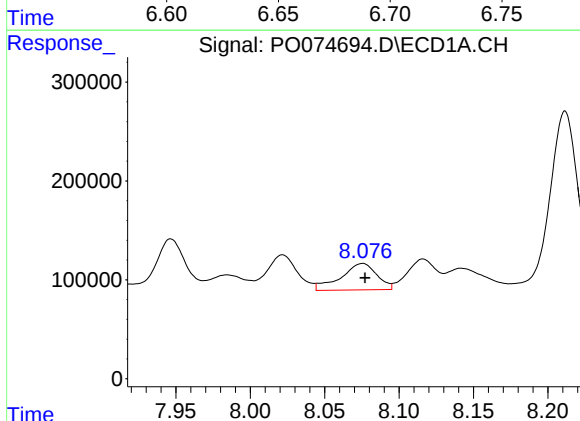


#29 AR-1254-4

R.T.: 8.076 min
Delta R.T.: -0.001 min
Response: 450321
Conc: 74.25 ng/ml

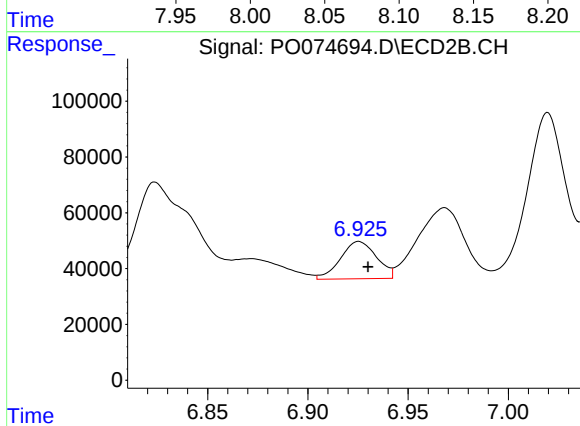

#29 AR-1254-4

R.T.: 6.925 min
Delta R.T.: -0.005 min
Response: 167734
Conc: 48.37 ng/ml

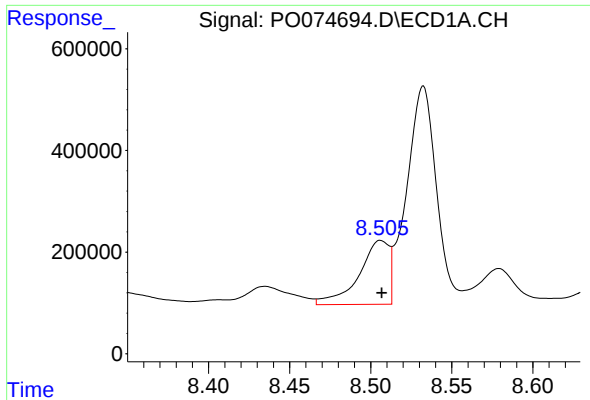


#30 AR-1254-5

R.T.: 8.506 min
Delta R.T.: 0.000 min
Response: 1628003
Conc: 280.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-40A

Manual Integrations
APPROVED

Ankita
1/15/2021 1:21:36 PM

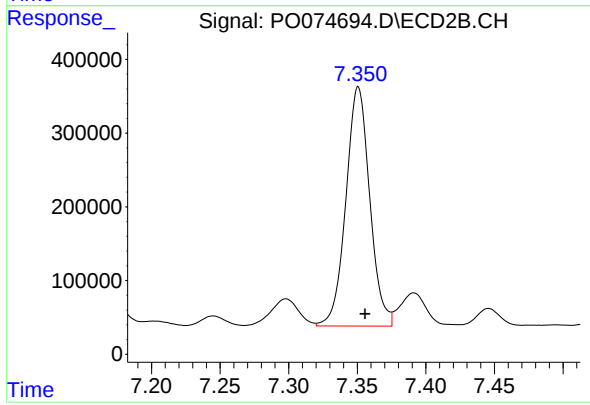

#30 AR-1254-5

R.T.: 7.351 min
Delta R.T.: -0.005 min
Response: 3934540
Conc: 869.33 ng/ml