

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011421\
 Data File : P0074695.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Jan 2021 20:37
 Operator : AJ/MA
 Sample : M1097-14
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 263K-41A

Manual Integrations
 APPROVED

Ankita
 1/15/2021 1:21:38 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 15 09:05:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.931	4.003	1819891	1015031	17.247	18.044
2)	SA Decachlor...	10.948	9.257	1200590	680278	11.829	12.390
Target Compounds							
26)	L6 AR-1254-1	7.166	6.112	144603	141063	32.878	39.054
27)	L6 AR-1254-2	7.398	6.271	506547	142348	74.374	45.675 #
28)	L6 AR-1254-3	7.780	6.687	1003843	465732	143.113	94.971m#
29)	L6 AR-1254-4	8.075	6.926	497533	205414	82.038	59.235 #
30)	L6 AR-1254-5	8.506	7.351	2215996	7216763	381.480	1594.533 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011421\
Data File : PO074695.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jan 2021 20:37
Operator : AJ/MA
Sample : M1097-14
Misc :
ALS Vial : 59 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
263K-41A


Manual Integrations
APPROVED

Ankita
1/15/2021 1:21:38 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 15 09:05:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

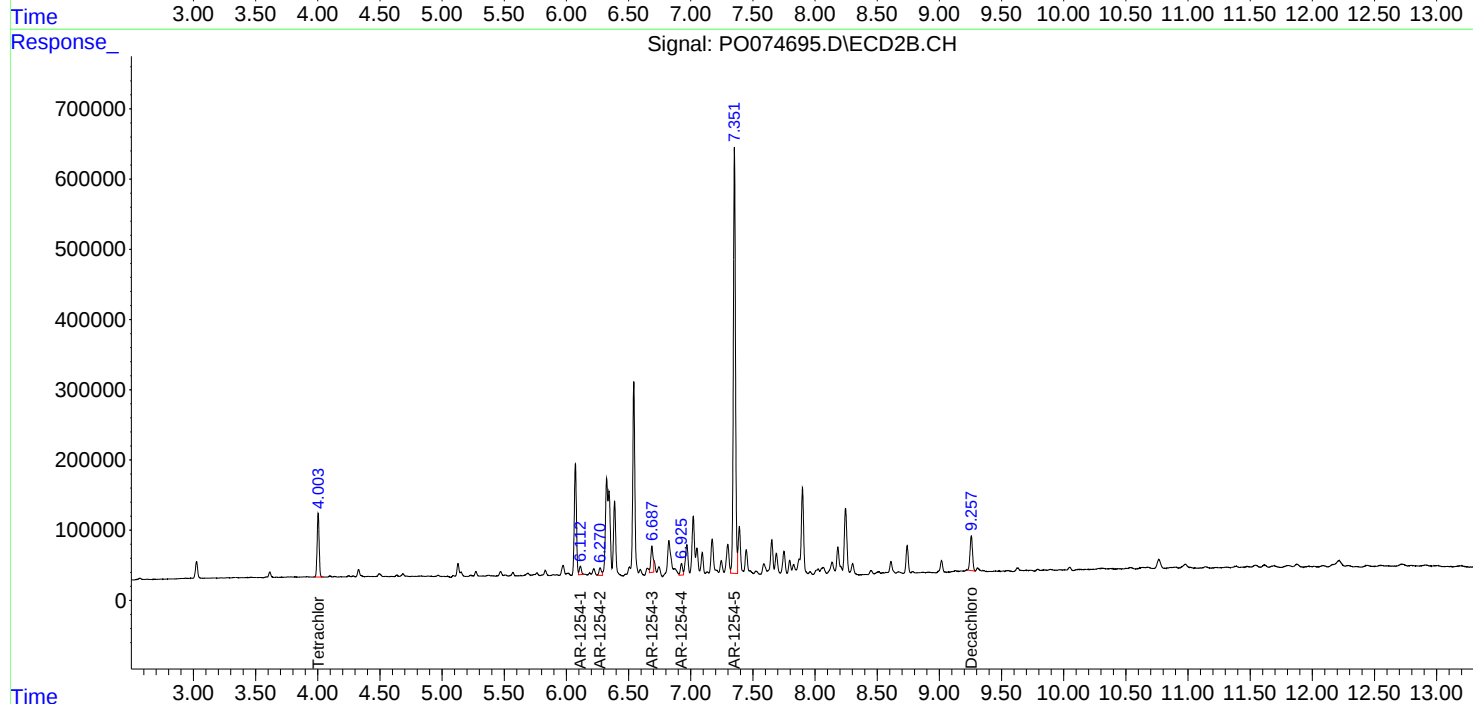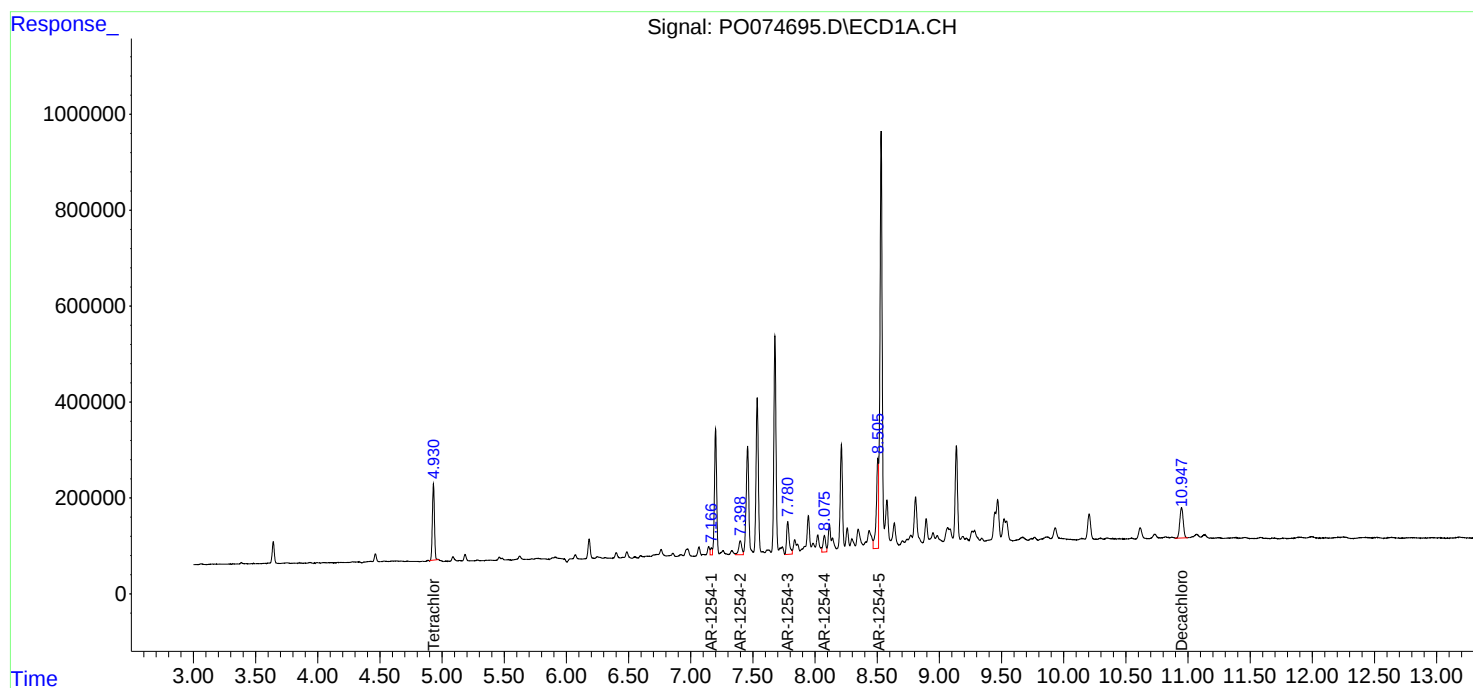

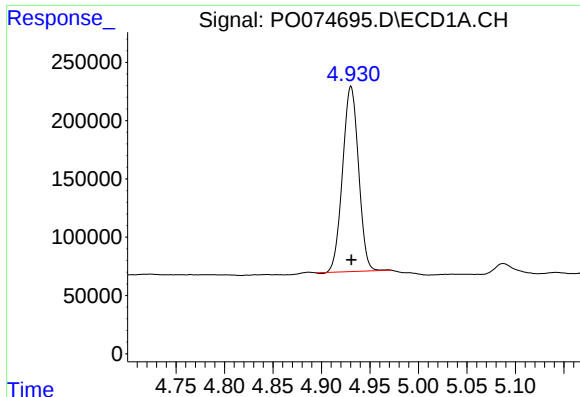


#1 Tetrachloro-m-xylene

R.T.: 4.931 min
Delta R.T.: 0.000 min
Response: 1819891
Conc: 17.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-41A


Manual Integrations
APPROVED

Ankita
1/15/2021 1:21:38 PM

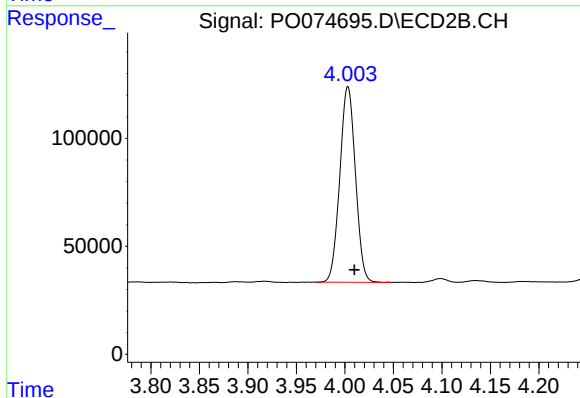


#1 Tetrachloro-m-xylene

R.T.: 4.003 min
Delta R.T.: -0.007 min
Response: 1015031
Conc: 18.04 ng/ml

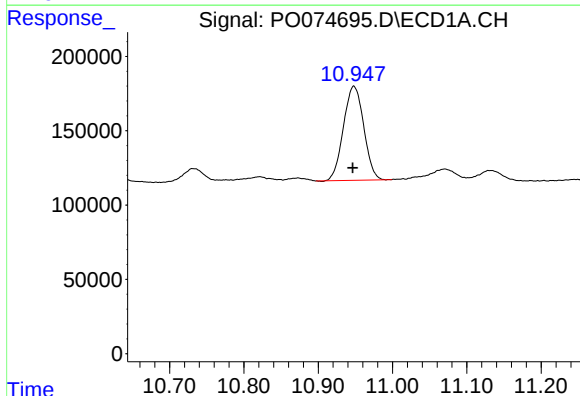


#2 Decachlorobiphenyl

R.T.: 10.948 min
Delta R.T.: 0.002 min
Response: 1200590
Conc: 11.83 ng/ml

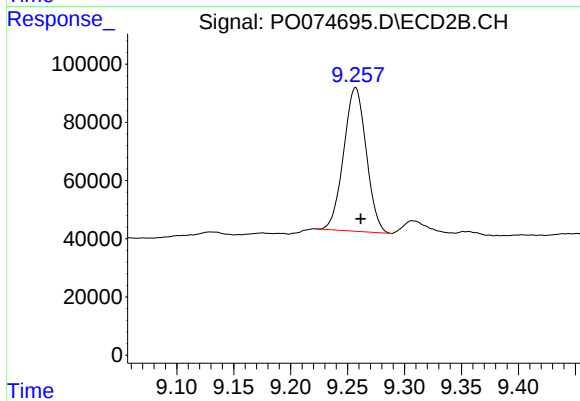

#2 Decachlorobiphenyl

R.T.: 9.257 min
Delta R.T.: -0.004 min
Response: 680278
Conc: 12.39 ng/ml

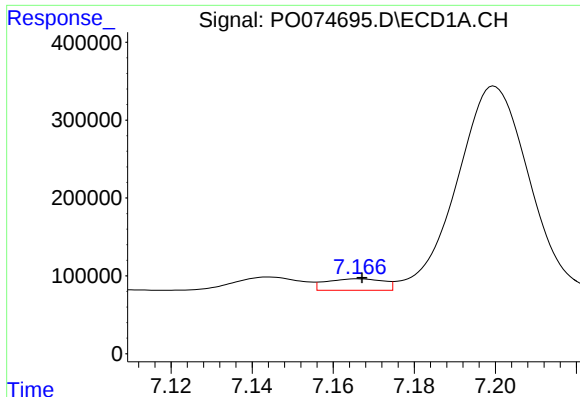


#26 AR-1254-1

R.T.: 7.166 min
Delta R.T.: 0.000 min
Response: 144603
Conc: 32.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-41A


Manual Integrations
APPROVED

Ankita
1/15/2021 1:21:38 PM

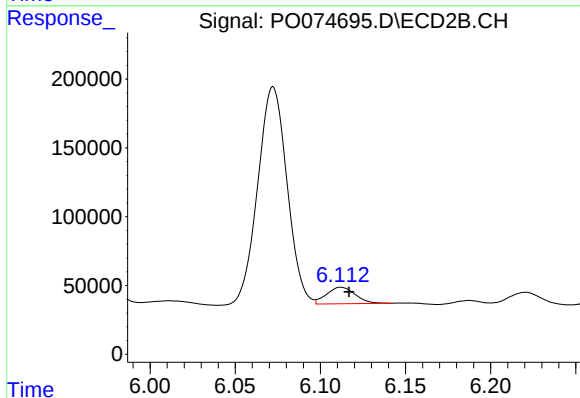


#26 AR-1254-1

R.T.: 6.112 min
Delta R.T.: -0.005 min
Response: 141063
Conc: 39.05 ng/ml

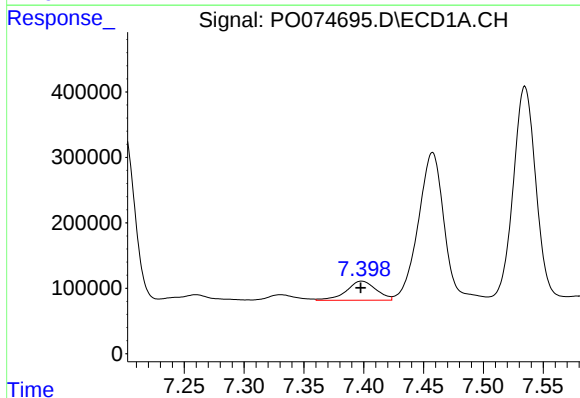


#27 AR-1254-2

R.T.: 7.398 min
Delta R.T.: 0.000 min
Response: 506547
Conc: 74.37 ng/ml

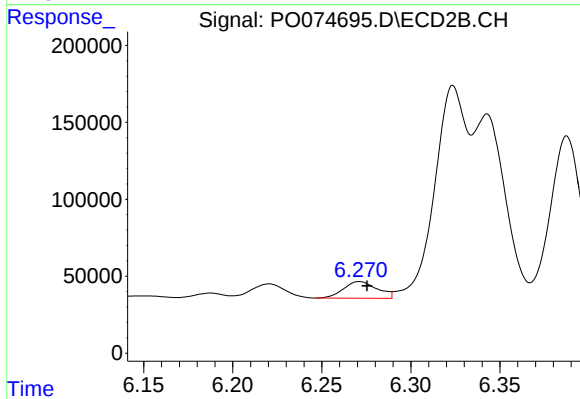

#27 AR-1254-2

R.T.: 6.271 min
Delta R.T.: -0.004 min
Response: 142348
Conc: 45.67 ng/ml

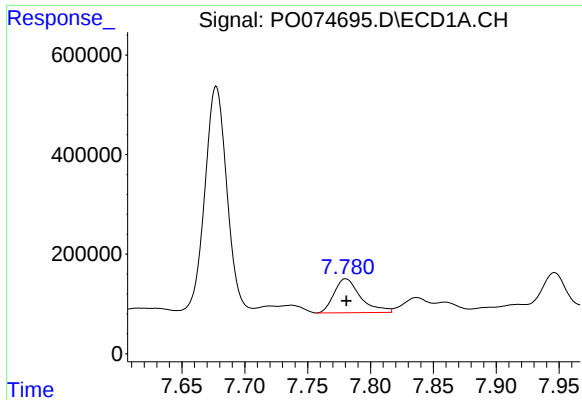


#28 AR-1254-3

R.T.: 7.780 min
Delta R.T.: 0.000 min
Response: 1003843
Conc: 143.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-41A


Manual Integrations
APPROVED

Ankita
1/15/2021 1:21:38 PM

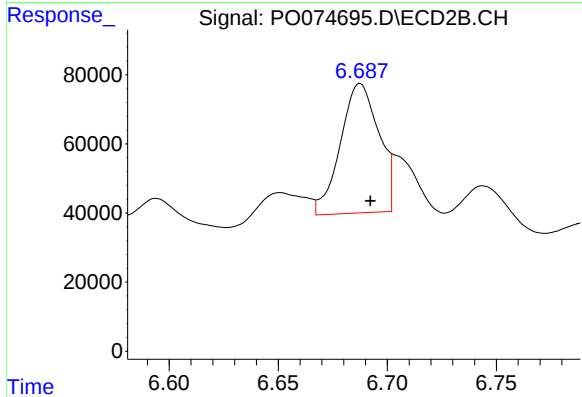


#28 AR-1254-3

R.T.: 6.687 min
Delta R.T.: -0.005 min
Response: 465732
Conc: 94.97 ng/ml m

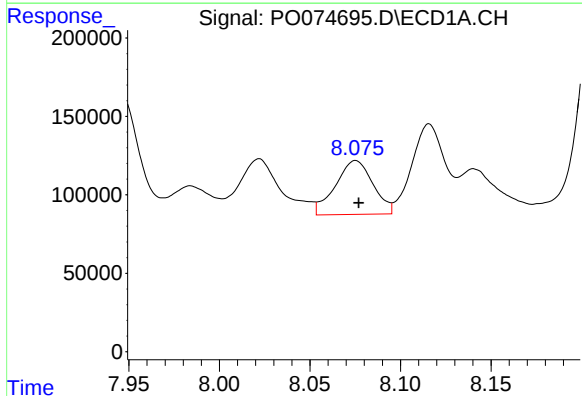


#29 AR-1254-4

R.T.: 8.075 min
Delta R.T.: -0.002 min
Response: 497533
Conc: 82.04 ng/ml

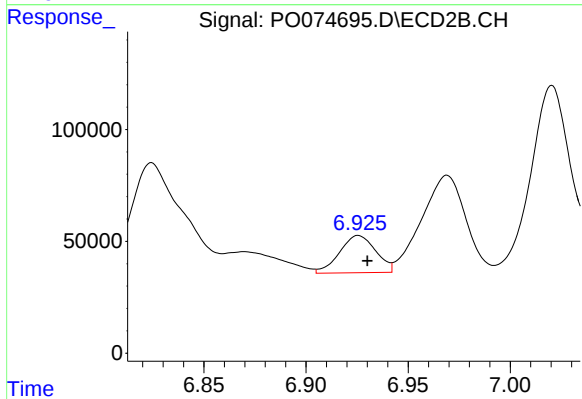

#29 AR-1254-4

R.T.: 6.926 min
Delta R.T.: -0.004 min
Response: 205414
Conc: 59.24 ng/ml

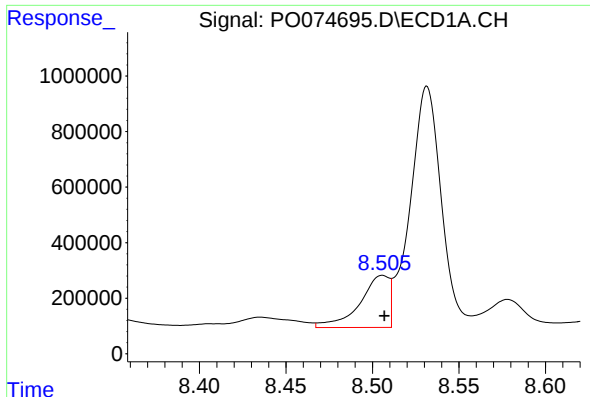


#30 AR-1254-5

R.T.: 8.506 min
Delta R.T.: -0.001 min
Response: 2215996
Conc: 381.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-41A

Manual Integrations
APPROVED

Ankita
1/15/2021 1:21:38 PM

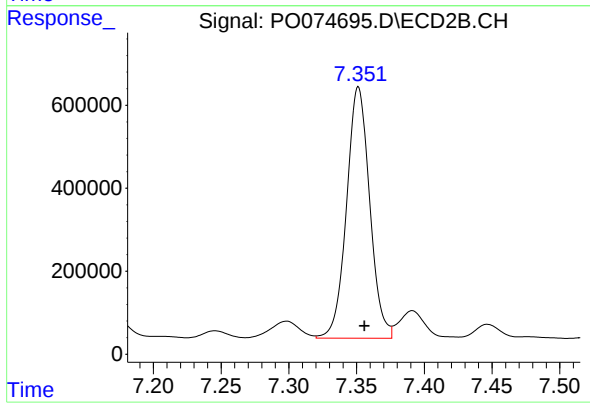

#30 AR-1254-5

R.T.: 7.351 min
Delta R.T.: -0.004 min
Response: 7216763
Conc: 1594.53 ng/ml