

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011421\
 Data File : P0074696.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Jan 2021 20:54
 Operator : AJ/MA
 Sample : M1097-17
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 263K-42A

Manual Integrations
 APPROVED

Ankita
 1/15/2021 1:21:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 15 09:07:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.931	4.004	2166824	1171050	20.535	20.818
2) SA Decachlor...	10.948	9.257	1332475	750358	13.129	13.667
Target Compounds						
26) L6 AR-1254-1	7.168	6.113	201302	208973	45.770	57.855 #
27) L6 AR-1254-2	7.400	6.271	724145	203958	106.323	65.444 #
28) L6 AR-1254-3	7.781	6.688	910280	380554	129.774	77.602m#
29) L6 AR-1254-4	8.075	6.926	449458	199742	74.111	57.599
30) L6 AR-1254-5	8.506	7.352	1847911	5541463	318.115	1224.378 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011421\
Data File : PO074696.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jan 2021 20:54
Operator : AJ/MA
Sample : M1097-17
Misc :
ALS Vial : 60 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
263K-42A


Manual Integrations
APPROVED

Ankita
1/15/2021 1:21:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 15 09:07:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

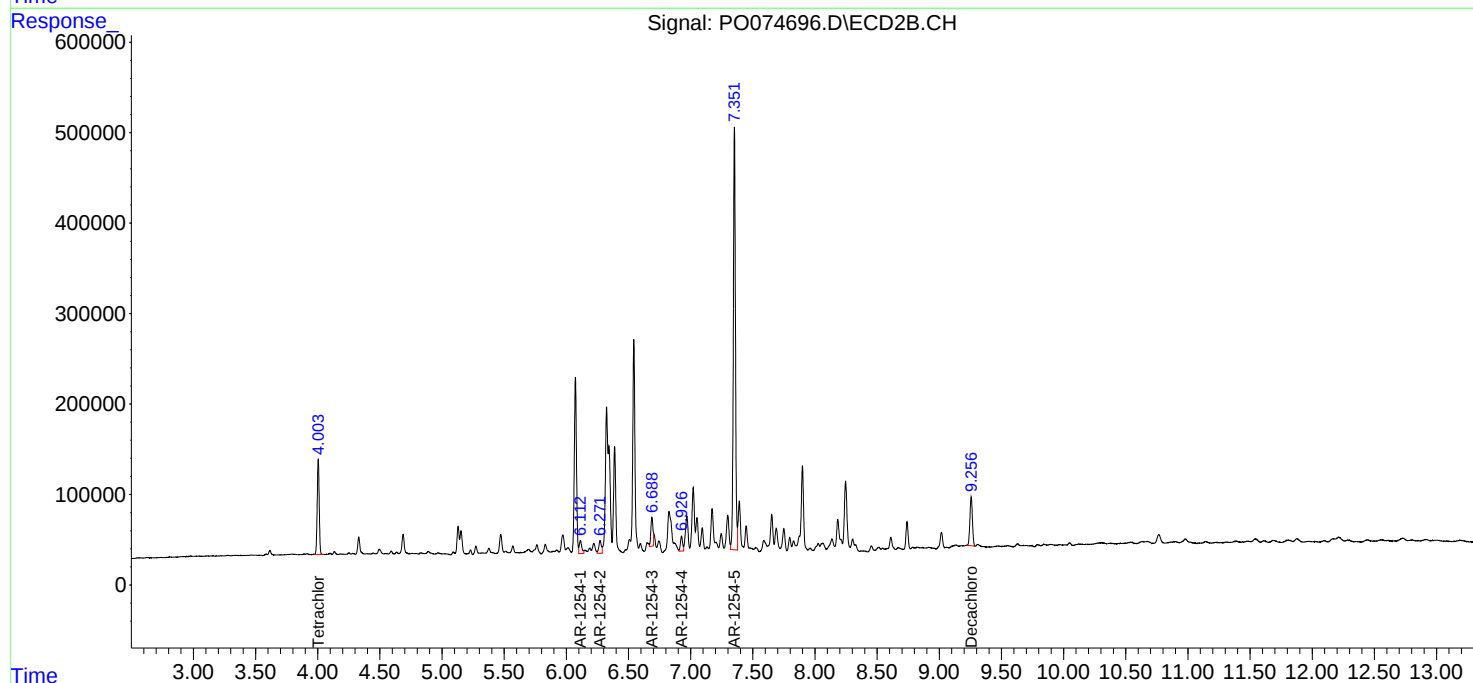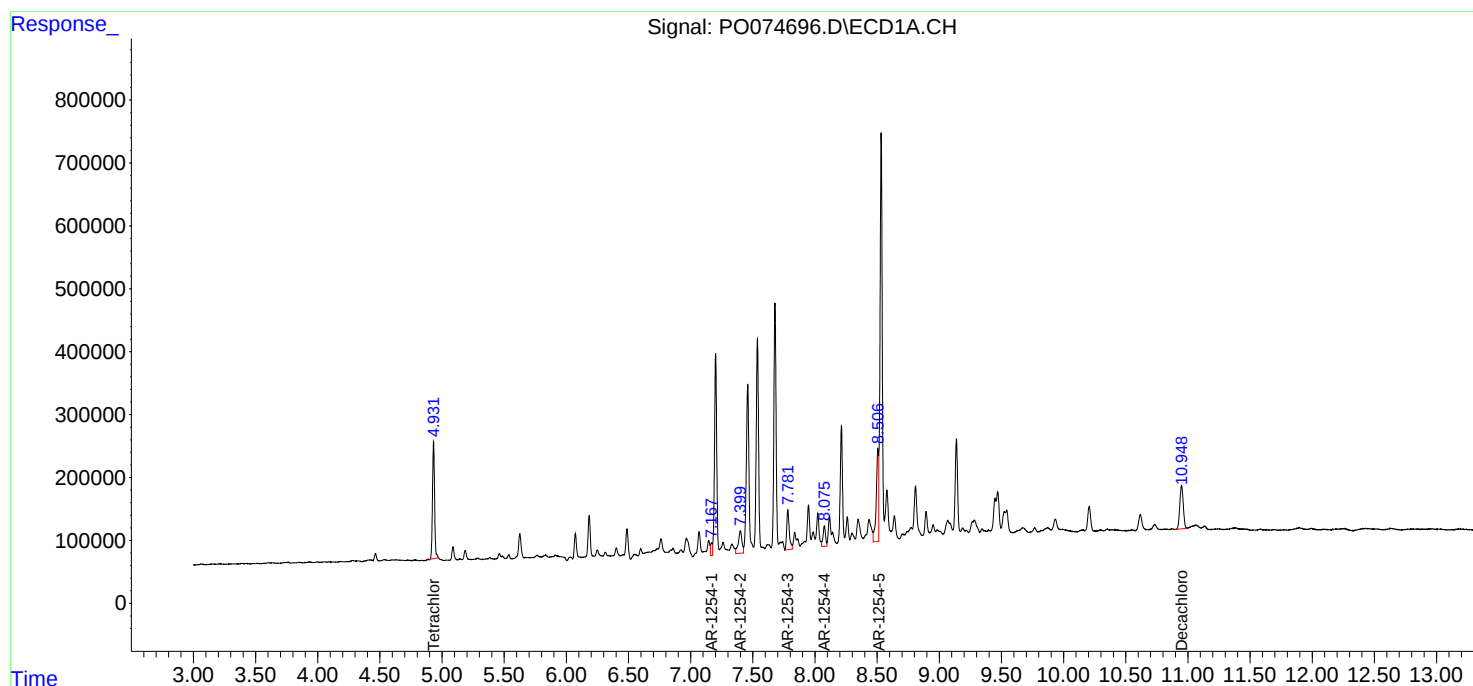

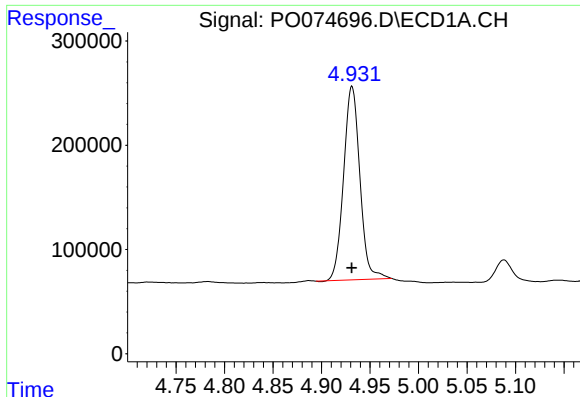


#1 Tetrachloro-m-xylene

R.T.: 4.931 min
Delta R.T.: 0.000 min
Response: 2166824
Conc: 20.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-42A


Manual Integrations
APPROVED

Ankita
1/15/2021 1:21:40 PM

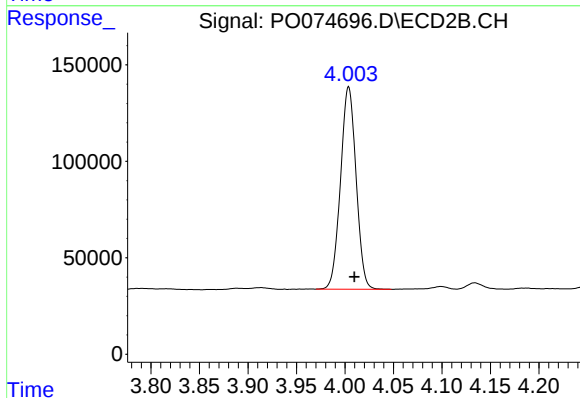


#1 Tetrachloro-m-xylene

R.T.: 4.004 min
Delta R.T.: -0.006 min
Response: 1171050
Conc: 20.82 ng/ml

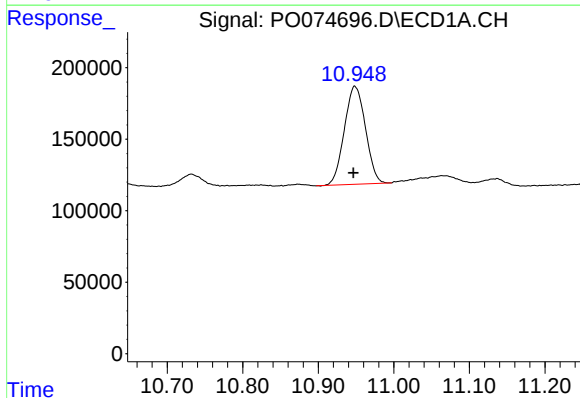


#2 Decachlorobiphenyl

R.T.: 10.948 min
Delta R.T.: 0.002 min
Response: 1332475
Conc: 13.13 ng/ml

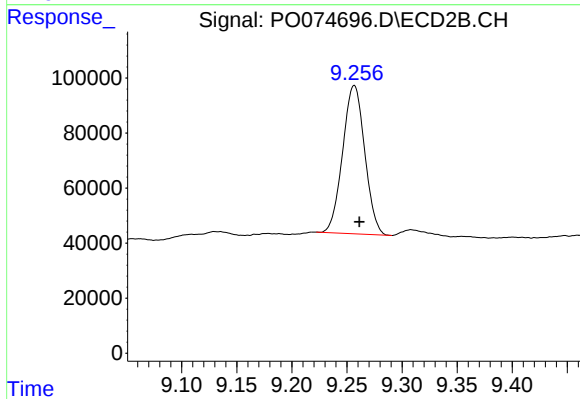

#2 Decachlorobiphenyl

R.T.: 9.257 min
Delta R.T.: -0.005 min
Response: 750358
Conc: 13.67 ng/ml

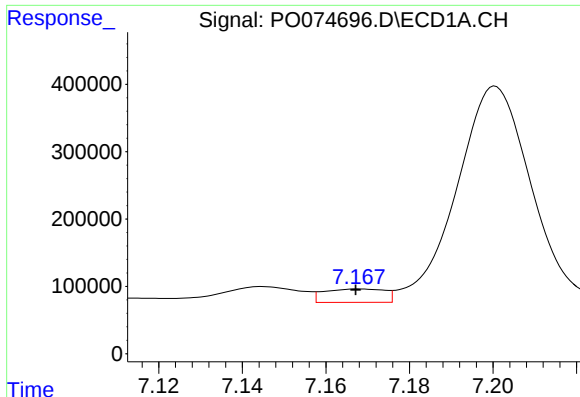


#26 AR-1254-1

R.T.: 7.168 min
Delta R.T.: 0.000 min
Response: 201302
Conc: 45.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-42A


Manual Integrations
APPROVED

Ankita
1/15/2021 1:21:40 PM

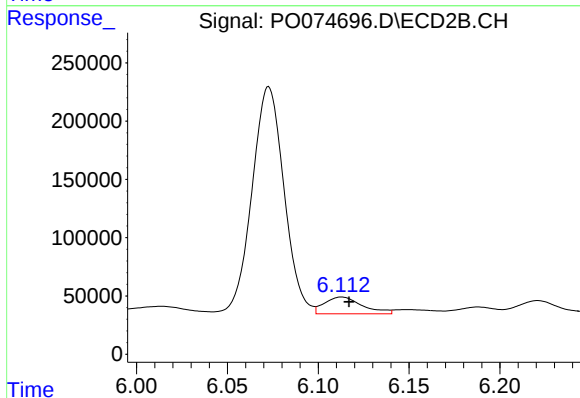


#26 AR-1254-1

R.T.: 6.113 min
Delta R.T.: -0.004 min
Response: 208973
Conc: 57.86 ng/ml

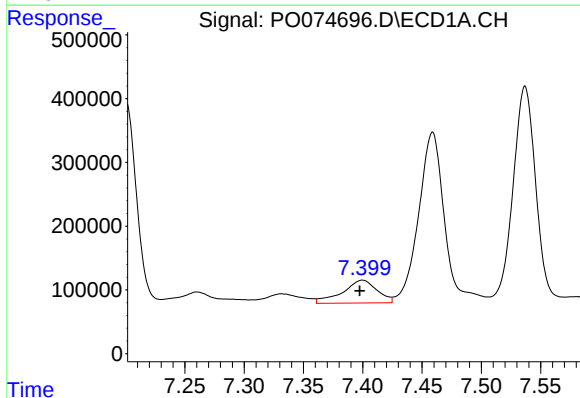


#27 AR-1254-2

R.T.: 7.400 min
Delta R.T.: 0.002 min
Response: 724145
Conc: 106.32 ng/ml

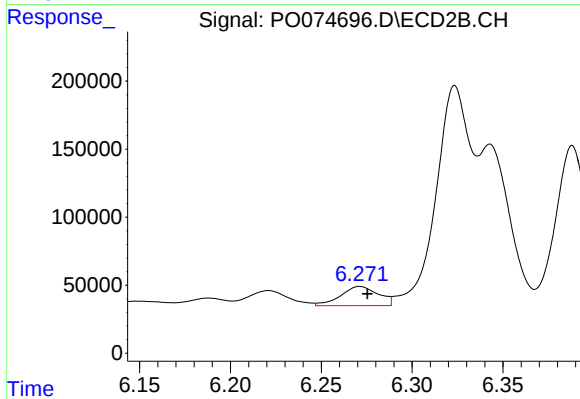

#27 AR-1254-2

R.T.: 6.271 min
Delta R.T.: -0.004 min
Response: 203958
Conc: 65.44 ng/ml

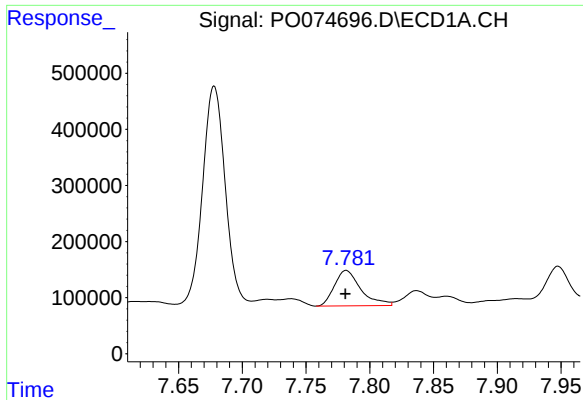


#28 AR-1254-3

R.T.: 7.781 min
Delta R.T.: 0.000 min
Response: 910280
Conc: 129.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-42A


Manual Integrations
APPROVED

Ankita
1/15/2021 1:21:40 PM

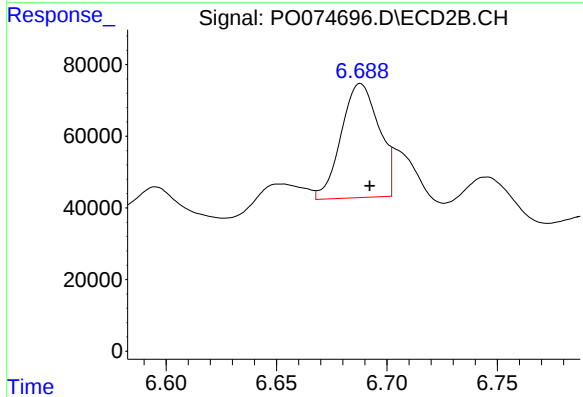


#28 AR-1254-3

R.T.: 6.688 min
Delta R.T.: -0.005 min
Response: 380554
Conc: 77.60 ng/ml m

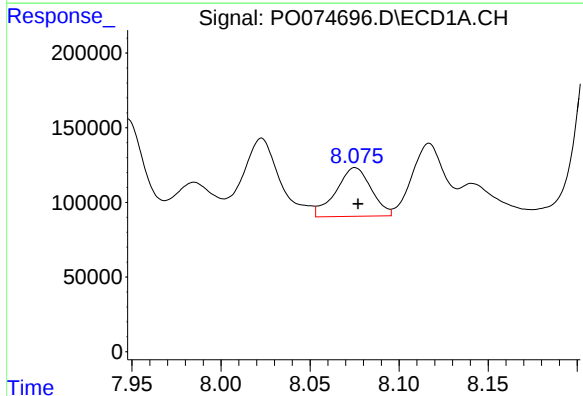


#29 AR-1254-4

R.T.: 8.075 min
Delta R.T.: -0.002 min
Response: 449458
Conc: 74.11 ng/ml

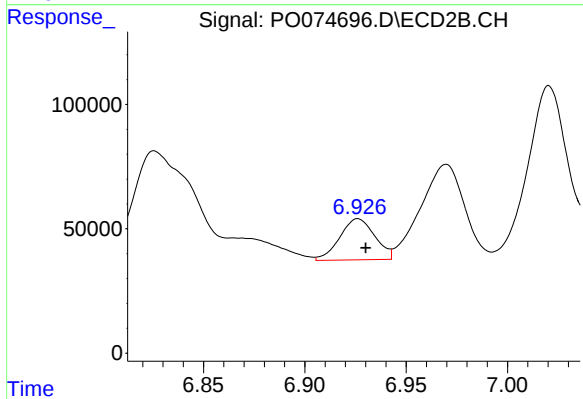

#29 AR-1254-4

R.T.: 6.926 min
Delta R.T.: -0.004 min
Response: 199742
Conc: 57.60 ng/ml

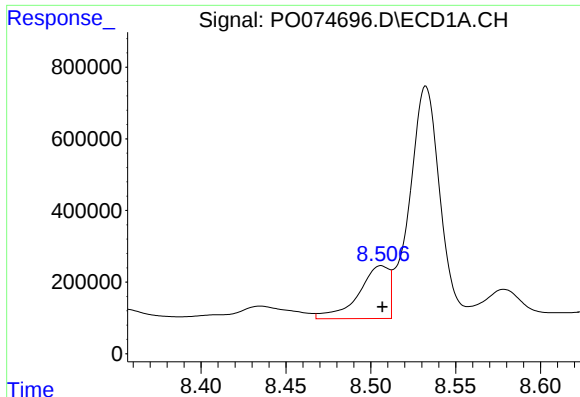


#30 AR-1254-5

R.T.: 8.506 min
Delta R.T.: 0.000 min
Response: 1847911
Conc: 318.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-42A

Manual Integrations
APPROVED

Ankita
1/15/2021 1:21:40 PM

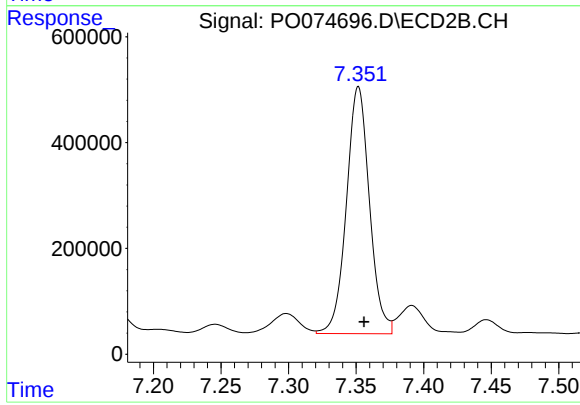

#30 AR-1254-5

R.T.: 7.352 min
Delta R.T.: -0.004 min
Response: 5541463
Conc: 1224.38 ng/ml