

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011421\
 Data File : P0074697.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Jan 2021 21:12
 Operator : AJ/MA
 Sample : M1097-20
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 263K-43A

Manual Integrations
 APPROVED

Ankita
 1/15/2021 1:21:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 15 09:08:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.931	4.003	2090284	1132155	19.810	20.126
2) SA Decachlor...	10.950	9.255	1225919	778150	12.079	14.173
Target Compounds						
26) L6 AR-1254-1	7.166	6.113	487503	414683	110.843	114.807
27) L6 AR-1254-2	7.397	6.272	1115982	469948	163.855	150.792
28) L6 AR-1254-3	7.780	6.688	1995760	1452437	284.526	296.179
29) L6 AR-1254-4	8.076	6.926	1228975	590053	202.645	170.153
30) L6 AR-1254-5	8.513	7.351	2846831	15630723	490.078m	3453.585 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011421\
Data File : PO074697.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jan 2021 21:12
Operator : AJ/MA
Sample : M1097-20
Misc :
ALS Vial : 61 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
263K-43A


Manual Integrations
APPROVED

Ankita
1/15/2021 1:21:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 15 09:08:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

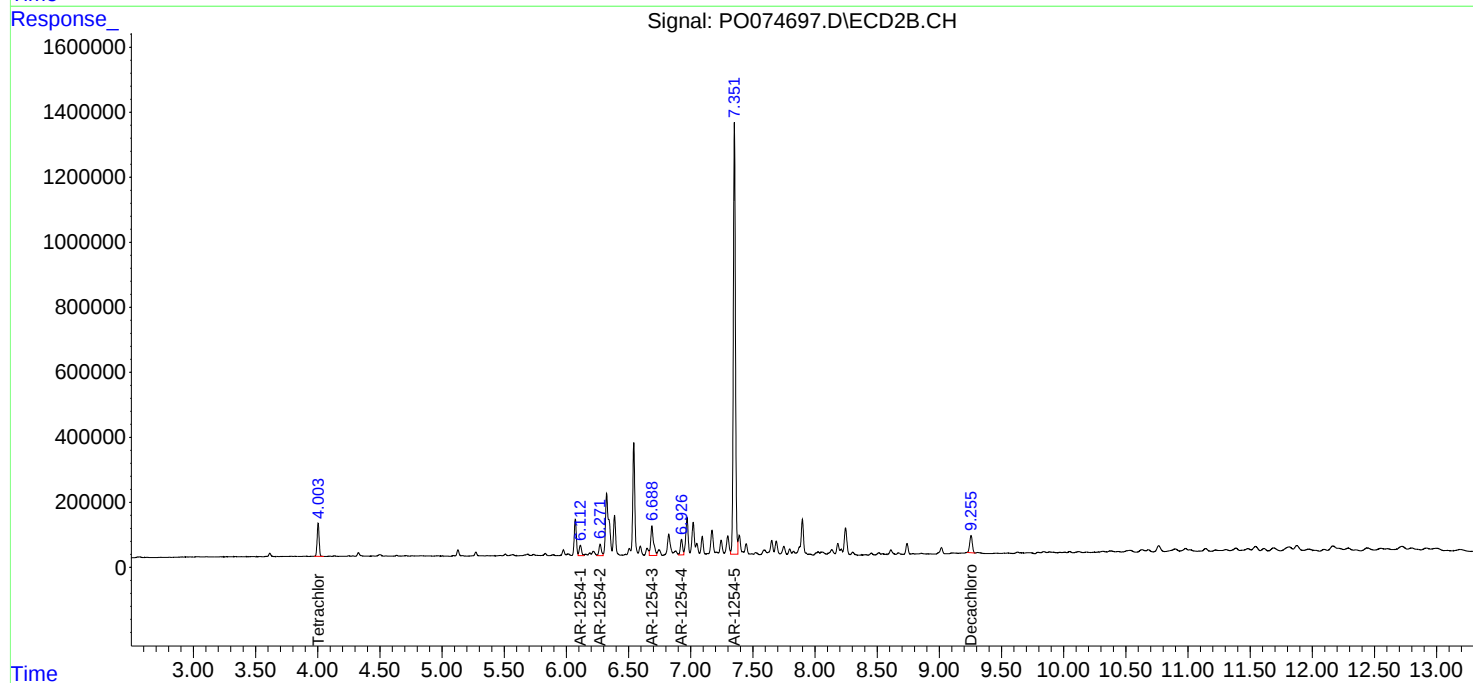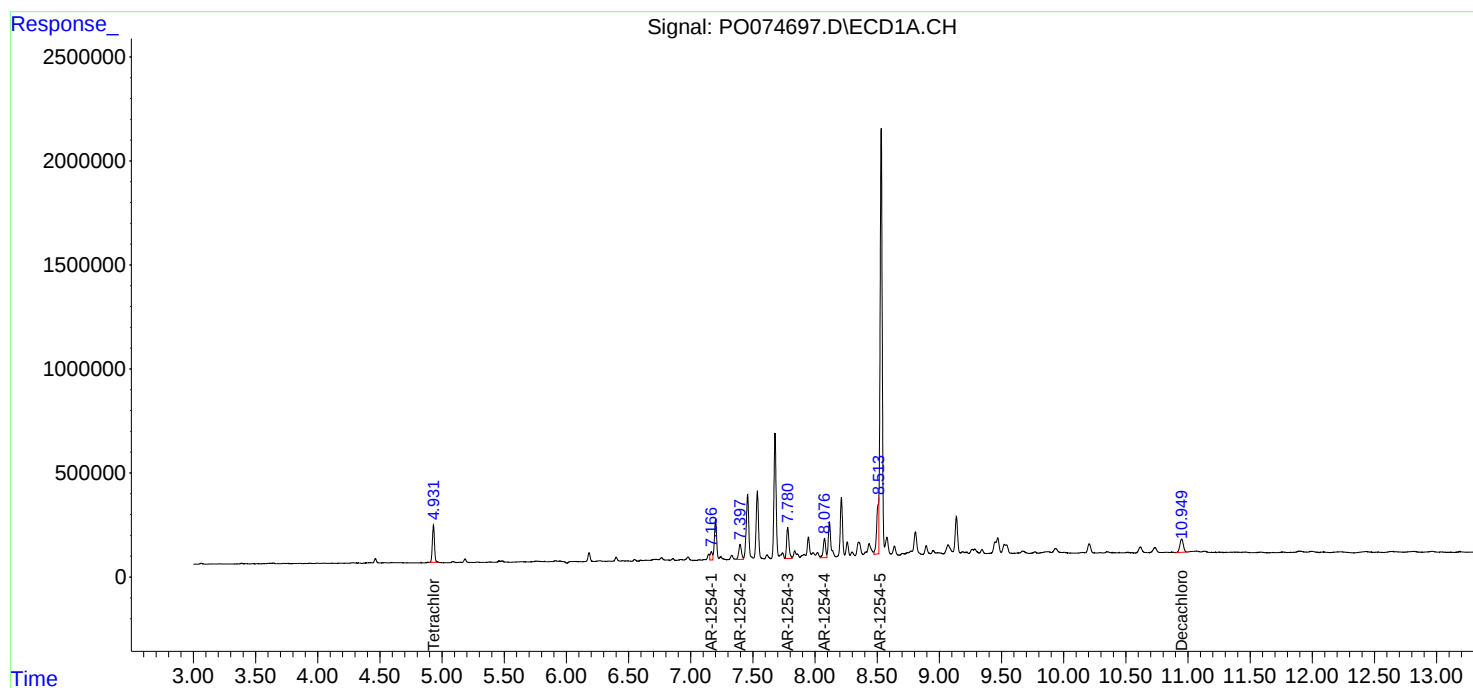

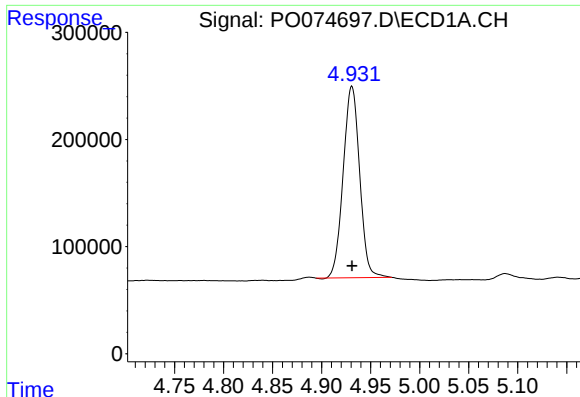


#1 Tetrachloro-m-xylene

R.T.: 4.931 min
Delta R.T.: 0.000 min
Response: 2090284
Conc: 19.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-43A


Manual Integrations
APPROVED

Ankita
1/15/2021 1:21:42 PM

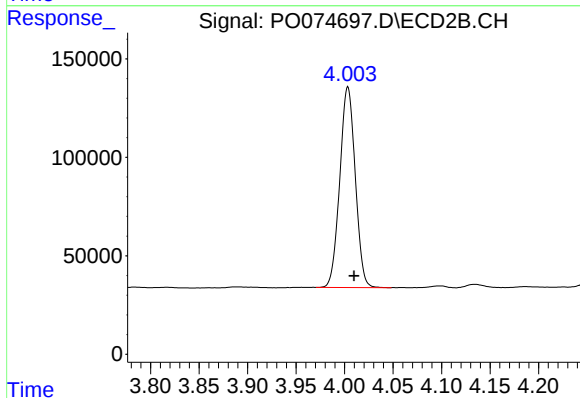


#1 Tetrachloro-m-xylene

R.T.: 4.003 min
Delta R.T.: -0.006 min
Response: 1132155
Conc: 20.13 ng/ml

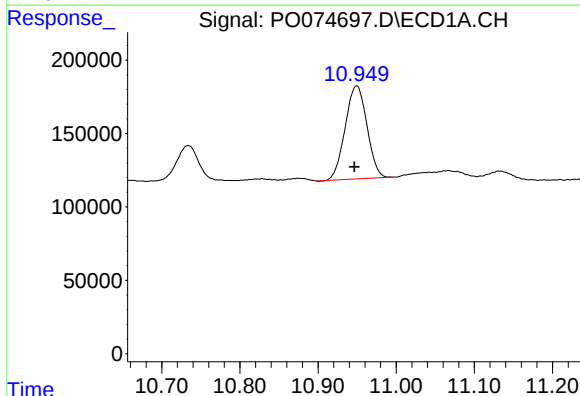


#2 Decachlorobiphenyl

R.T.: 10.950 min
Delta R.T.: 0.003 min
Response: 1225919
Conc: 12.08 ng/ml

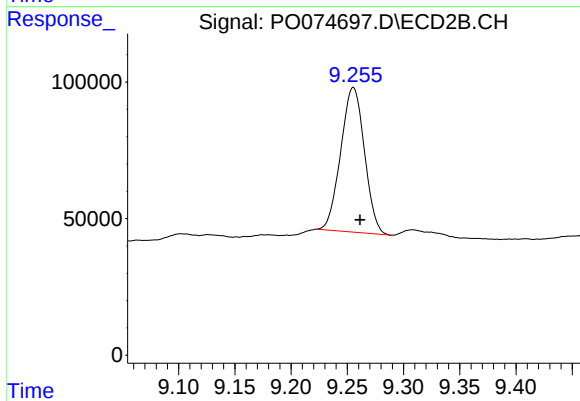

#2 Decachlorobiphenyl

R.T.: 9.255 min
Delta R.T.: -0.006 min
Response: 778150
Conc: 14.17 ng/ml

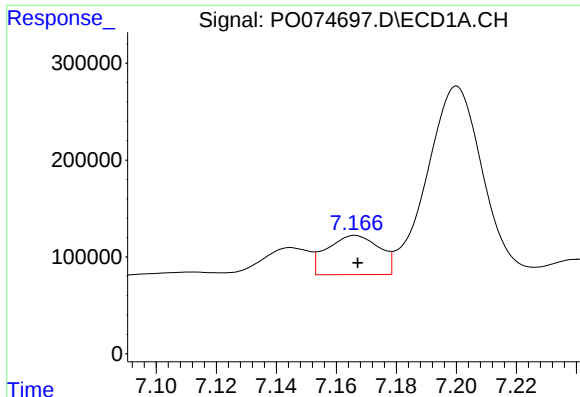


#26 AR-1254-1

R.T.: 7.166 min
Delta R.T.: 0.000 min
Response: 487503
Conc: 110.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-43A


Manual Integrations
APPROVED

Ankita
1/15/2021 1:21:42 PM

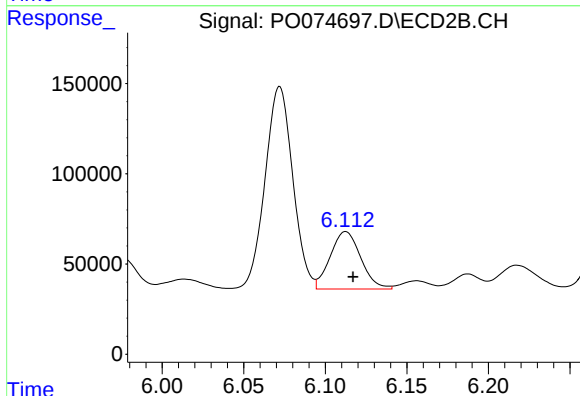


#26 AR-1254-1

R.T.: 6.113 min
Delta R.T.: -0.004 min
Response: 414683
Conc: 114.81 ng/ml

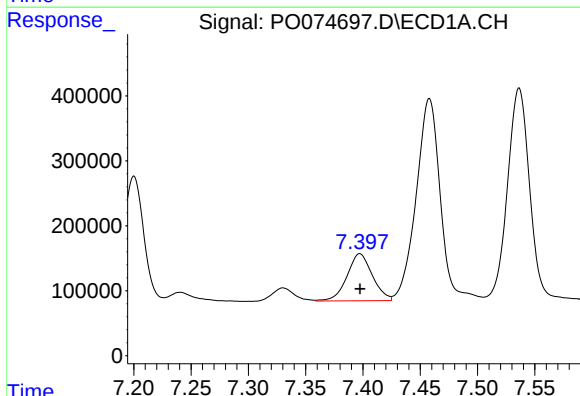


#27 AR-1254-2

R.T.: 7.397 min
Delta R.T.: 0.000 min
Response: 1115982
Conc: 163.86 ng/ml

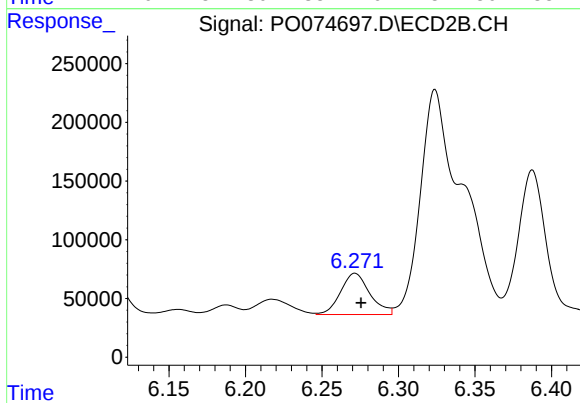

#27 AR-1254-2

R.T.: 6.272 min
Delta R.T.: -0.004 min
Response: 469948
Conc: 150.79 ng/ml

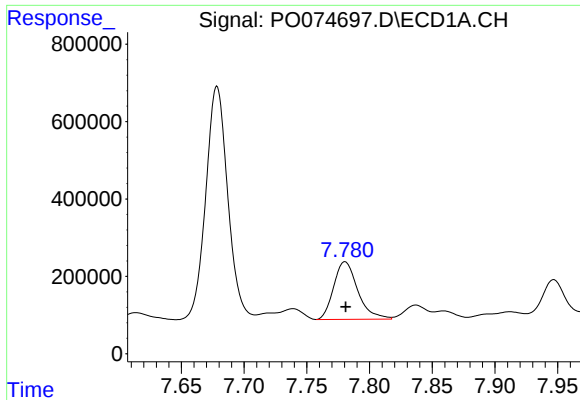


#28 AR-1254-3

R.T.: 7.780 min
Delta R.T.: 0.000 min
Response: 1995760
Conc: 284.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-43A


Manual Integrations
APPROVED

Ankita
1/15/2021 1:21:42 PM

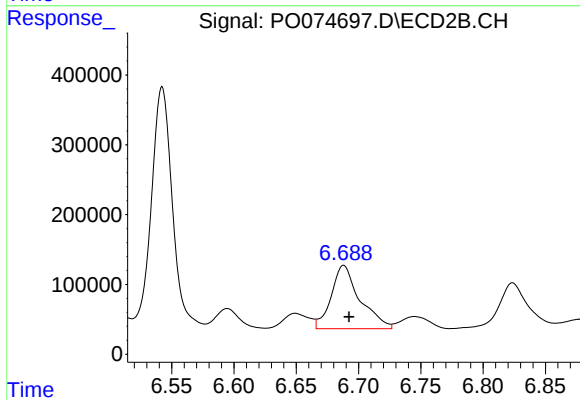


#28 AR-1254-3

R.T.: 6.688 min
Delta R.T.: -0.004 min
Response: 1452437
Conc: 296.18 ng/ml

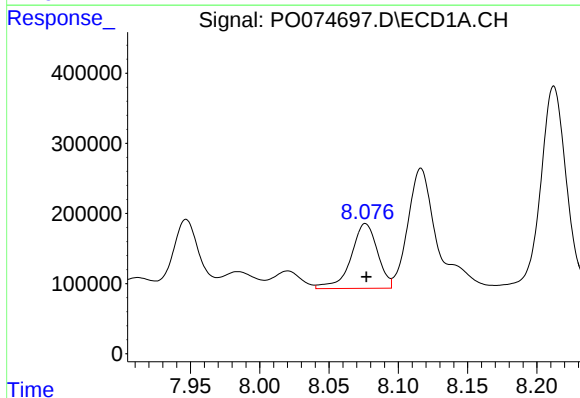


#29 AR-1254-4

R.T.: 8.076 min
Delta R.T.: 0.000 min
Response: 1228975
Conc: 202.64 ng/ml

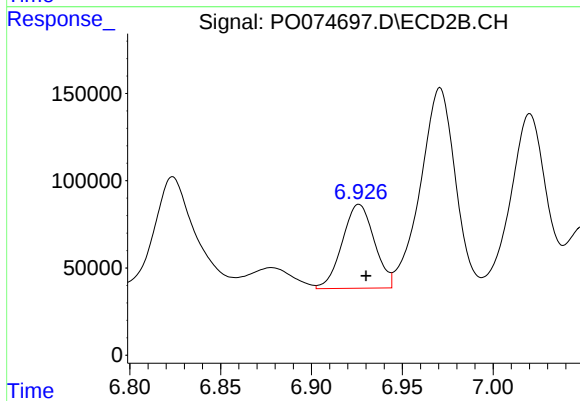

#29 AR-1254-4

R.T.: 6.926 min
Delta R.T.: -0.004 min
Response: 590053
Conc: 170.15 ng/ml

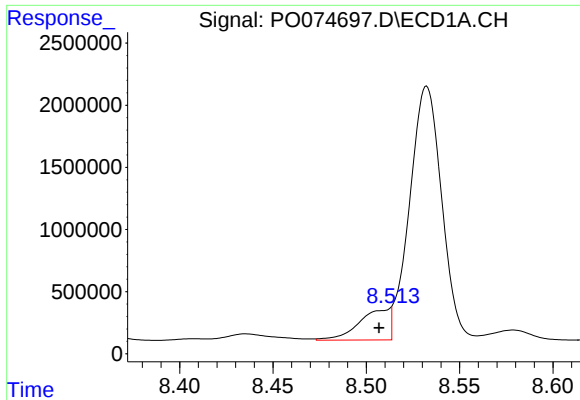


#30 AR-1254-5

R.T.: 8.513 min
Delta R.T.: 0.006 min
Response: 2846831
Conc: 490.08 ng/ml m

Instrument :
ECD_O
ClientSampleId :
263K-43A

Manual Integrations
APPROVED

Ankita
1/15/2021 1:21:42 PM

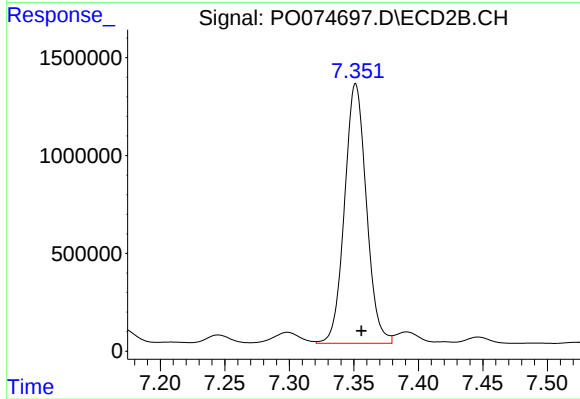

#30 AR-1254-5

R.T.: 7.351 min
Delta R.T.: -0.004 min
Response: 15630723
Conc: 3453.59 ng/ml