

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011422\
 Data File : P0084249.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Jan 2022 12:37
 Operator : AJ\MA
 Sample : N1125-07 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 IRV-2022-28A

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/17/2022
 Supervised By :mohammad ahmed 01/17/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 14 23:52:49 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011322.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 14 22:49:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	6.524	5.308	189905	32454	2.103m	1.569m#
2) SA Decachlor...	13.788	11.322	105488	31075	1.887m	1.757m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011422\
Data File : P0084249.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jan 2022 12:37
Operator : AJ\MA
Sample : N1125-07 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
IRV-2022-28A


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/17/2022
Supervised By :mohammad ahmed 01/17/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 14 23:52:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011322.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 14 22:49:17 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

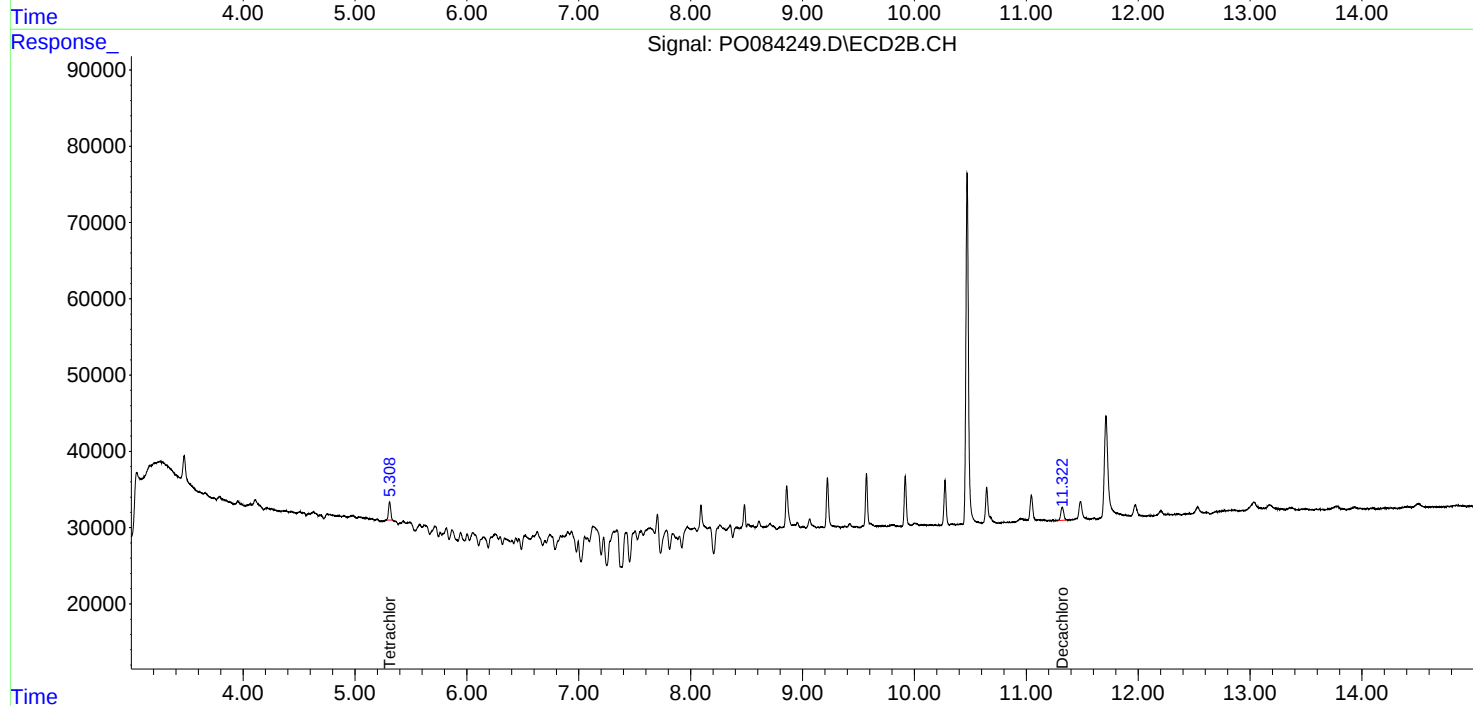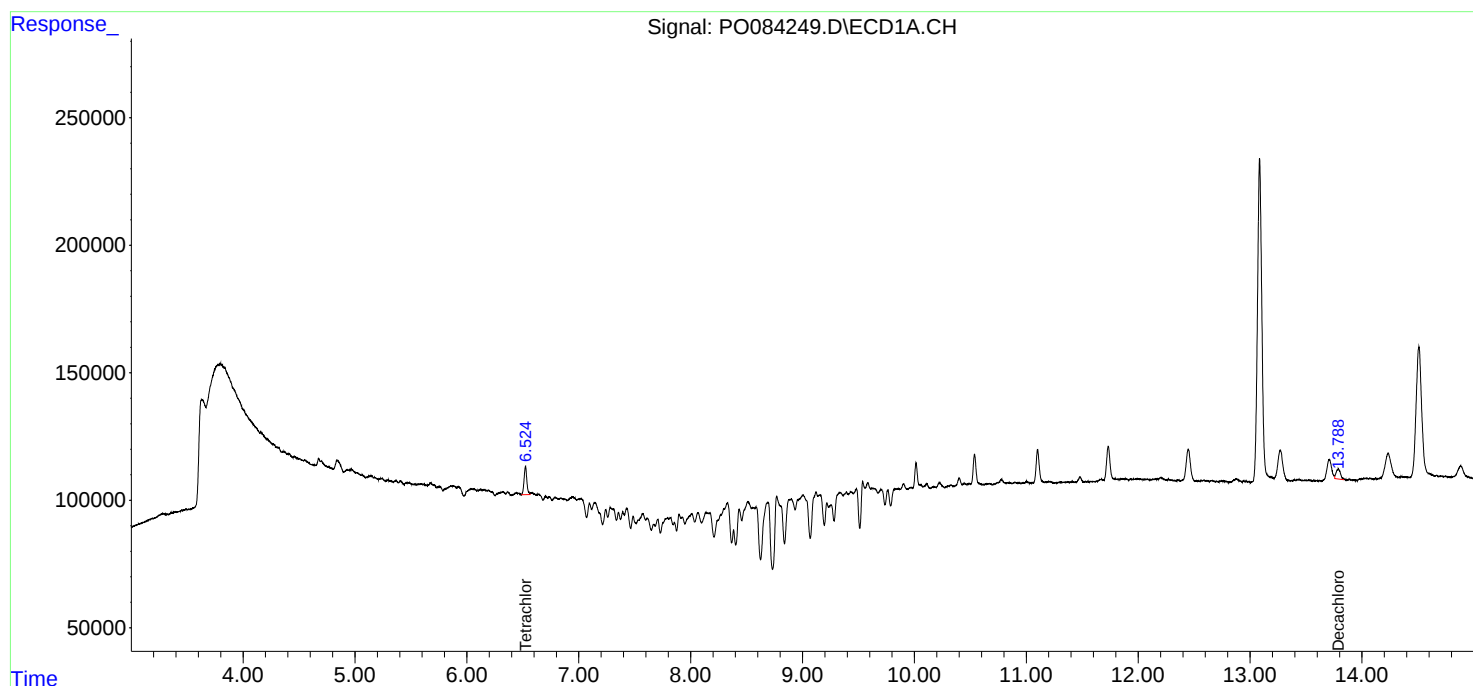

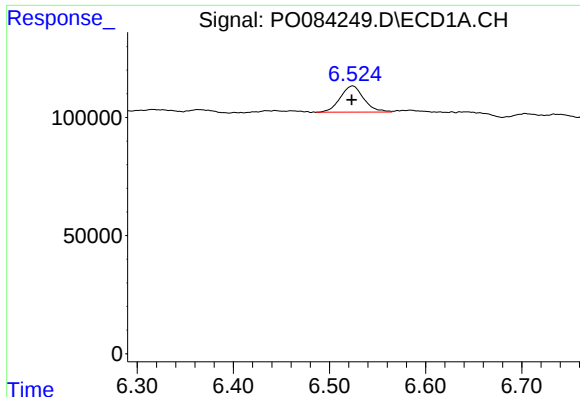


#1 Tetrachloro-m-xylene

R.T.: 6.524 min
Delta R.T.: 0.000 min
Response: 189905
Conc: 2.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-28A


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/17/2022
Supervised By :mohammad ahmed 01/17/2022

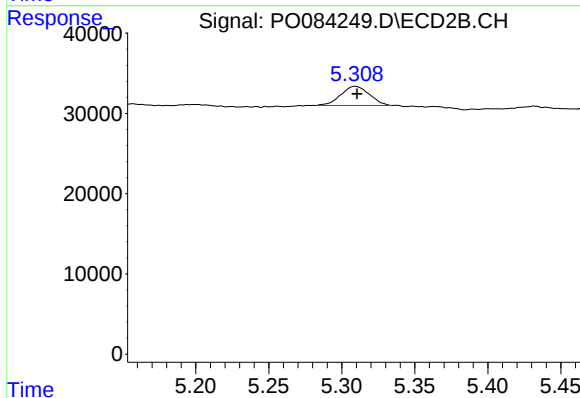


#1 Tetrachloro-m-xylene

R.T.: 5.308 min
Delta R.T.: -0.002 min
Response: 32454
Conc: 1.57 ng/ml m

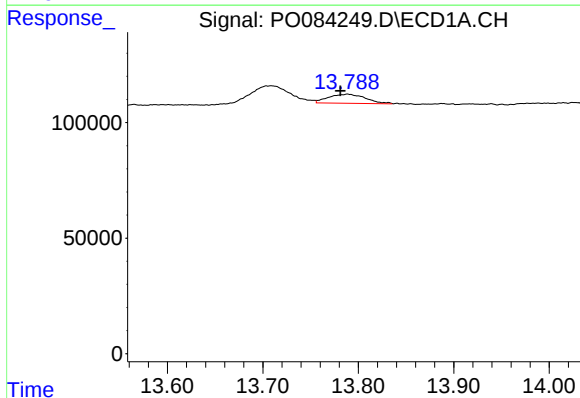

#2 Decachlorobiphenyl

R.T.: 13.788 min
Delta R.T.: 0.007 min
Response: 105488
Conc: 1.89 ng/ml m

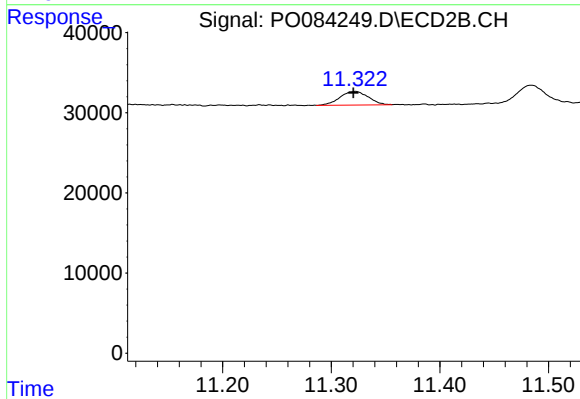

#2 Decachlorobiphenyl

R.T.: 11.322 min
Delta R.T.: 0.002 min
Response: 31075
Conc: 1.76 ng/ml m