

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011520\
 Data File : P0065508.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Jan 2020 14:20
 Operator : DD\AJ
 Sample : PB126098BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB126098BL

Manual Integrations
 APPROVED

mohammad
 1/16/2020 11:31:44 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 15 14:38:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jan 04 04:01:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.180	3.441	451343	485024	24.717m	22.049
2) SA Decachlor...	9.694	8.352	801973	931213	23.669	22.455

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011520\
Data File : P0065508.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Jan 2020 14:20
Operator : DD\AJ
Sample : PB126098BL
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB126098BL


Manual Integrations
APPROVED

mohammad
1/16/2020 11:31:44 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 15 14:38:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jan 04 04:01:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

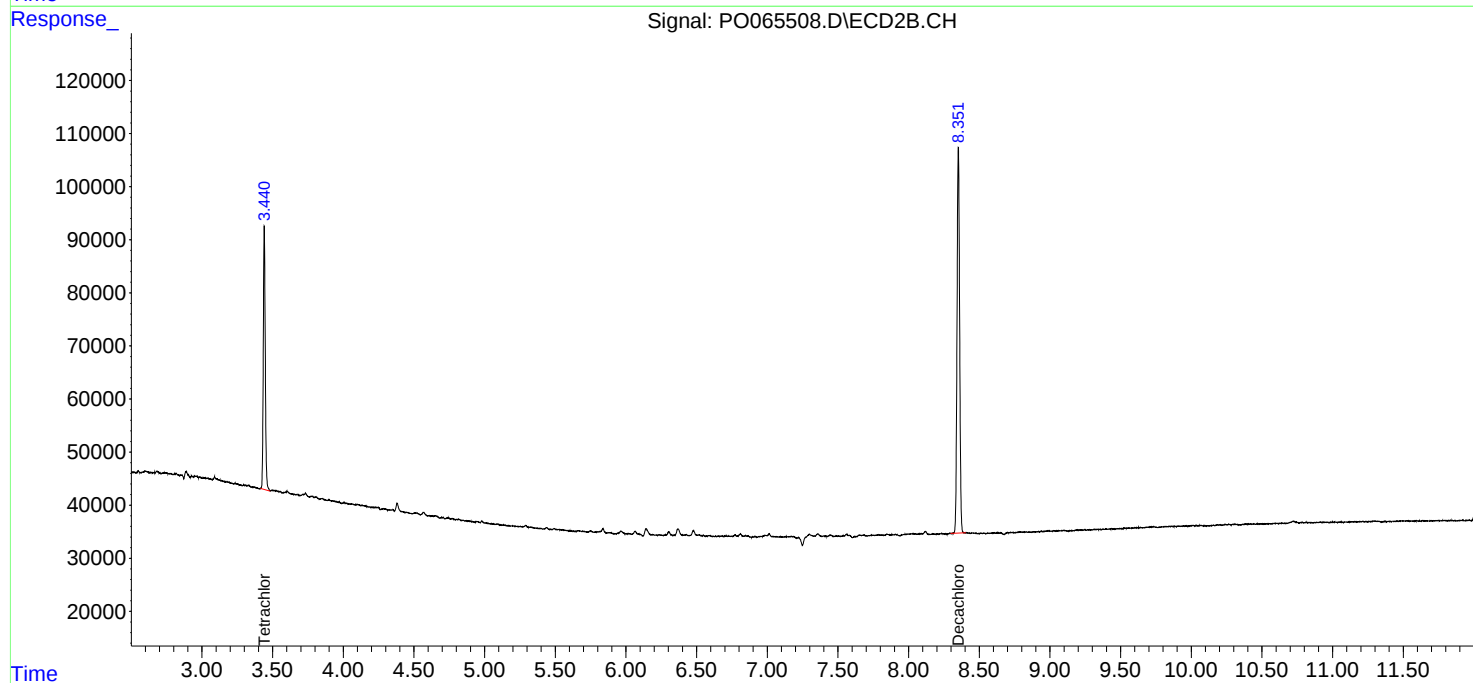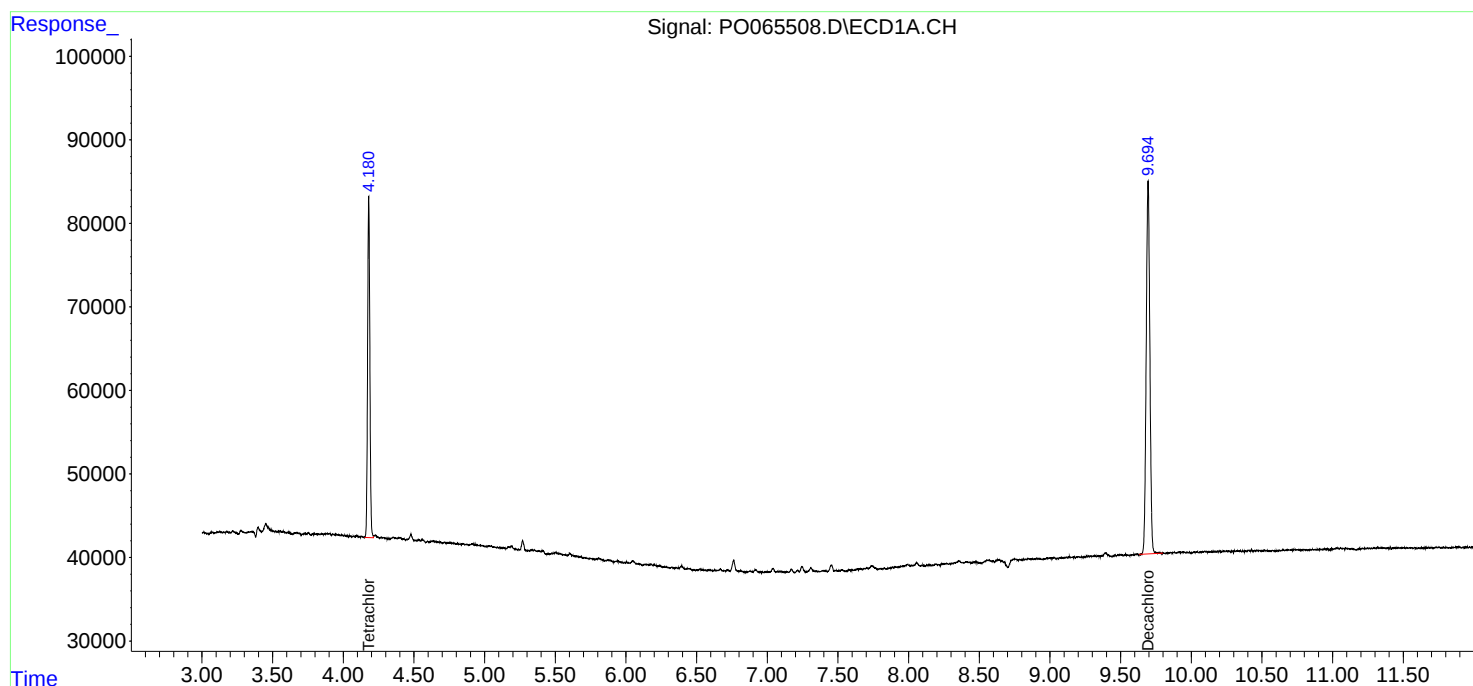

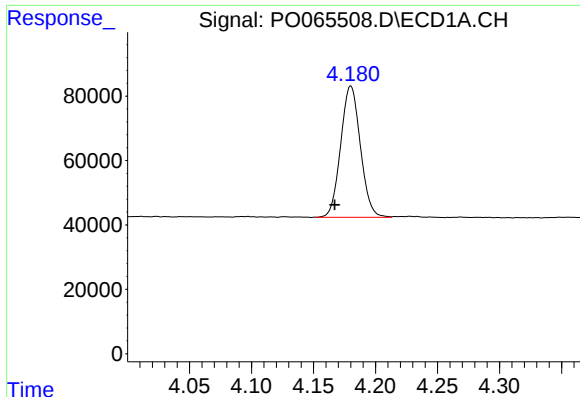


#1 Tetrachloro-m-xylene

R.T.: 4.180 min
Delta R.T.: 0.013 min
Response: 451343
Conc: 24.72 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PB126098BL


Manual Integrations
APPROVED

mohammad
1/16/2020 11:31:44 AM

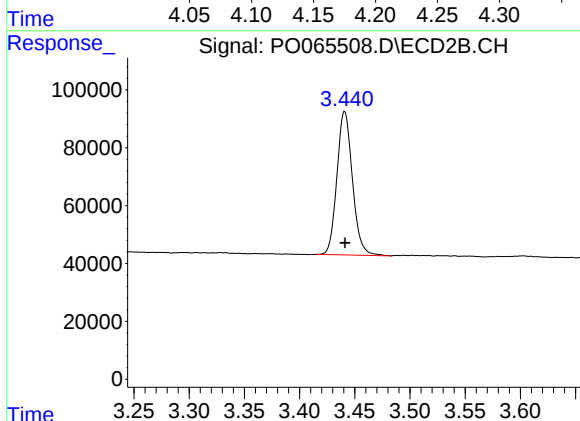


#1 Tetrachloro-m-xylene

R.T.: 3.441 min
Delta R.T.: 0.000 min
Response: 485024
Conc: 22.05 ng/ml

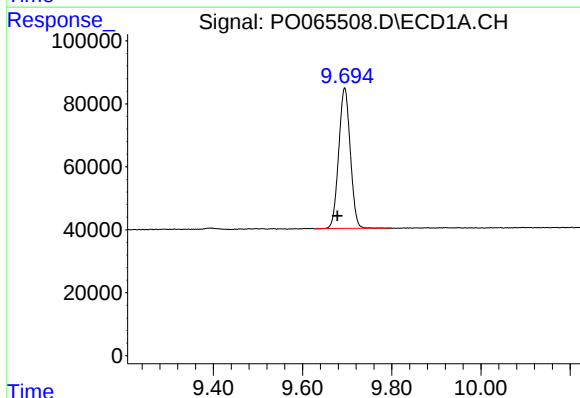

#2 Decachlorobiphenyl

R.T.: 9.694 min
Delta R.T.: 0.016 min
Response: 801973
Conc: 23.67 ng/ml

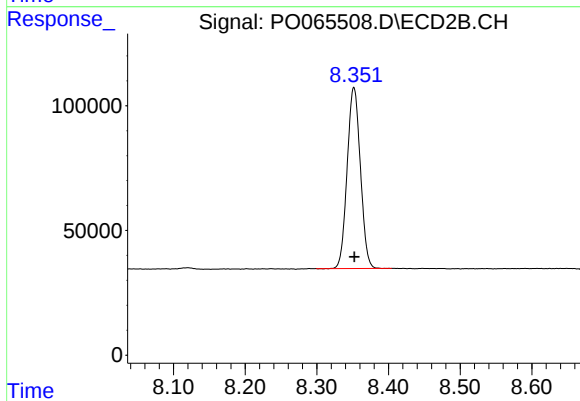

#2 Decachlorobiphenyl

R.T.: 8.352 min
Delta R.T.: 0.000 min
Response: 931213
Conc: 22.46 ng/ml