

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011520\
 Data File : P0065520.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Jan 2020 17:41
 Operator : DD\AJ
 Sample : L1125-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FESB-28-(1.5-2)

Manual Integrations
 APPROVED

mohammad
 1/16/2020 11:31:58 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 16 00:40:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jan 04 04:01:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.165	3.439	489210	540459	26.791	24.569
2) SA Decachlor...	9.670	8.343	683914	803743	20.185	19.381

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011520\
Data File : P0065520.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Jan 2020 17:41
Operator : DD\AJ
Sample : L1125-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FESB-28-(1.5-2)


Manual Integrations
APPROVED

mohammad
1/16/2020 11:31:58 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 16 00:40:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jan 04 04:01:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

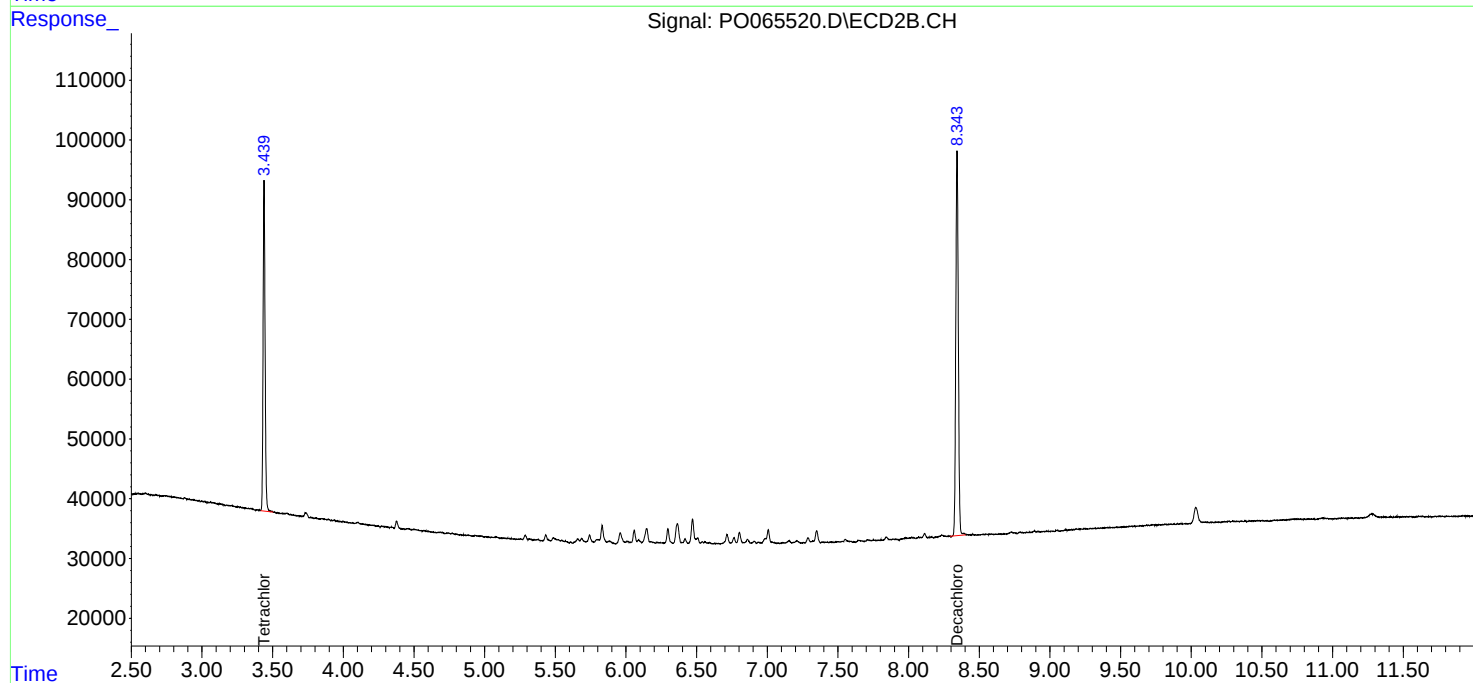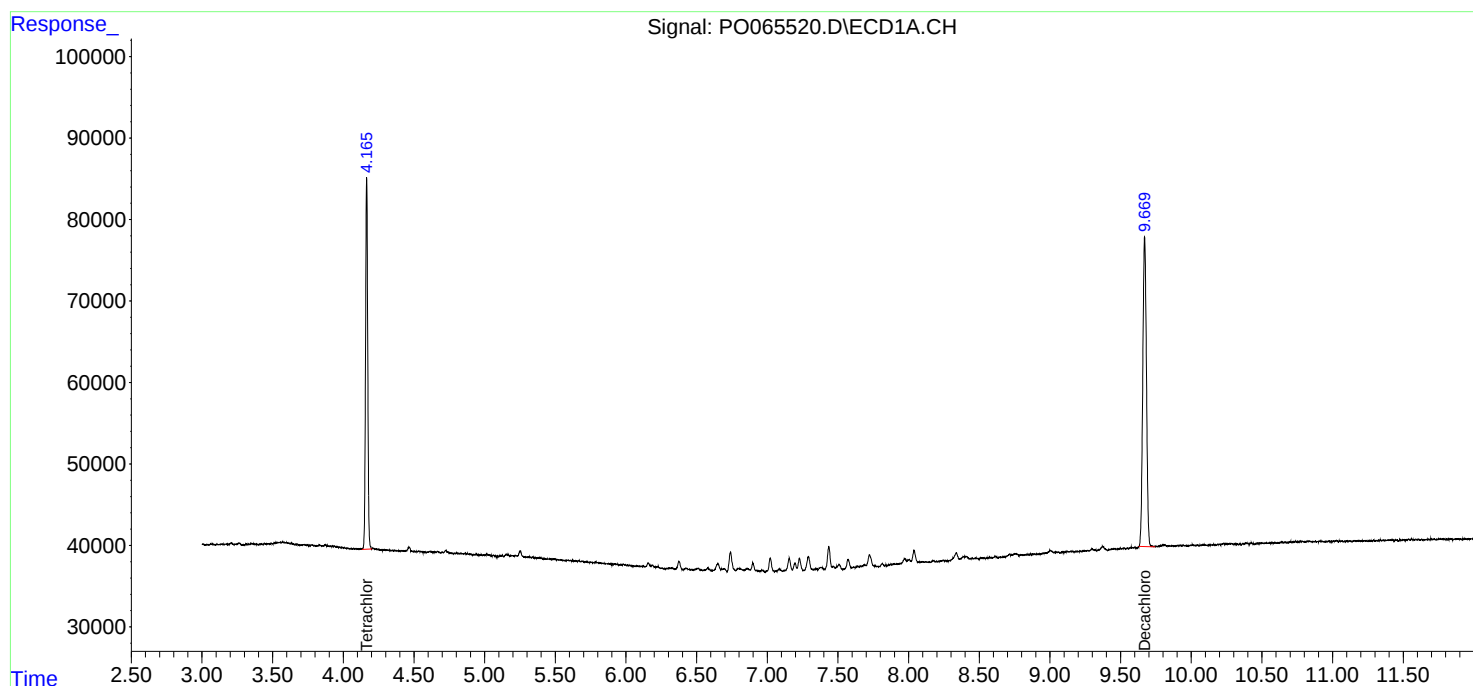

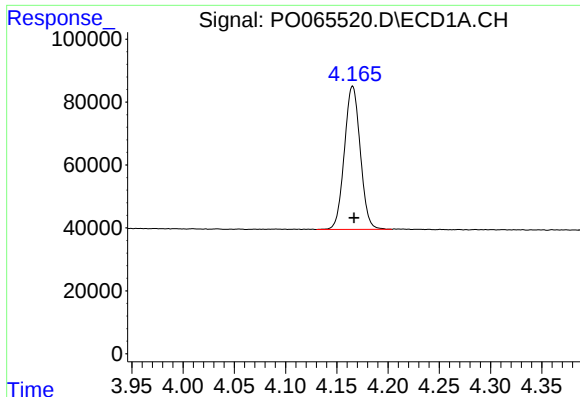


#1 Tetrachloro-m-xylene

R.T.: 4.165 min
Delta R.T.: -0.002 min
Response: 489210
Conc: 26.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
FESB-28-(1.5-2)


Manual Integrations
APPROVED

mohammad
1/16/2020 11:31:58 AM

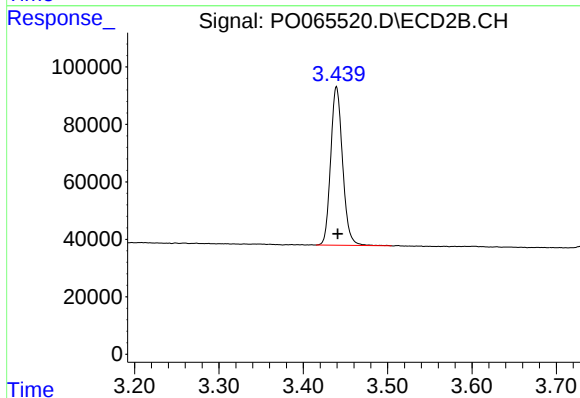


#1 Tetrachloro-m-xylene

R.T.: 3.439 min
Delta R.T.: -0.002 min
Response: 540459
Conc: 24.57 ng/ml

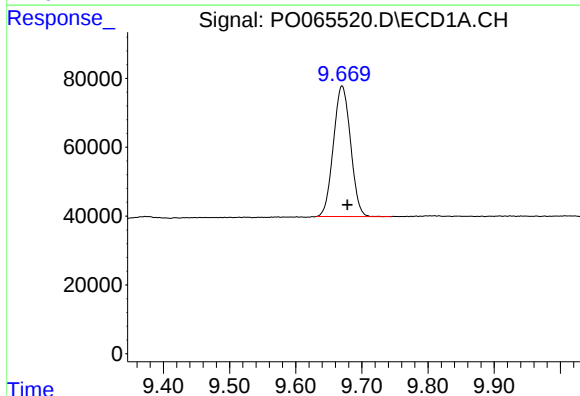

#2 Decachlorobiphenyl

R.T.: 9.670 min
Delta R.T.: -0.008 min
Response: 683914
Conc: 20.18 ng/ml

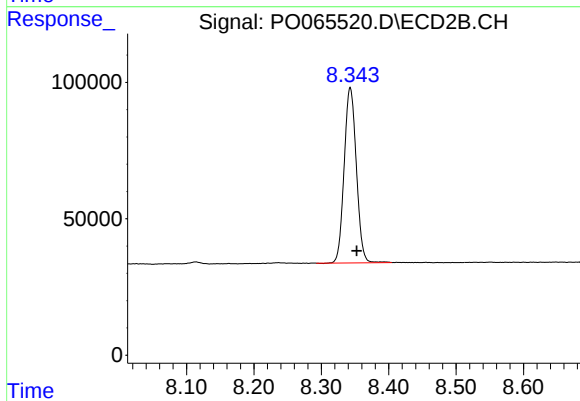

#2 Decachlorobiphenyl

R.T.: 8.343 min
Delta R.T.: -0.010 min
Response: 803743
Conc: 19.38 ng/ml