

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011521\
 Data File : P0074788.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Jan 2021 2:22
 Operator : AJ/MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 16 04:23:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.932	4.004	2254101	1190166	21.362	21.158
2)	SA Decachlor...	10.952	9.258	2087632	1090387	20.569	19.860
Target Compounds							
20)	L4 AR-1242-5	0.000	6.137f	0	72652	N.D.	41.496 #
24)	L5 AR-1248-4	7.174f	0.000	187183	0	41.974	N.D. #
25)	L5 AR-1248-5	0.000	6.137f	0	72652	N.D.	30.903 #
26)	L6 AR-1254-1	7.174	6.137f	187183	72652	42.560	20.114 #
28)	L6 AR-1254-3	7.803f	0.000	54614	0	7.786	N.D. #
34)	L7 AR-1260-4	8.815	0.000	13305	0	2.432	N.D. #
45)	L9 AR-1268-5	0.000	9.018	0	22738	N.D.	0.960 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011521\
Data File : P0074788.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Jan 2021 2:22
Operator : AJ/MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 16 04:23:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

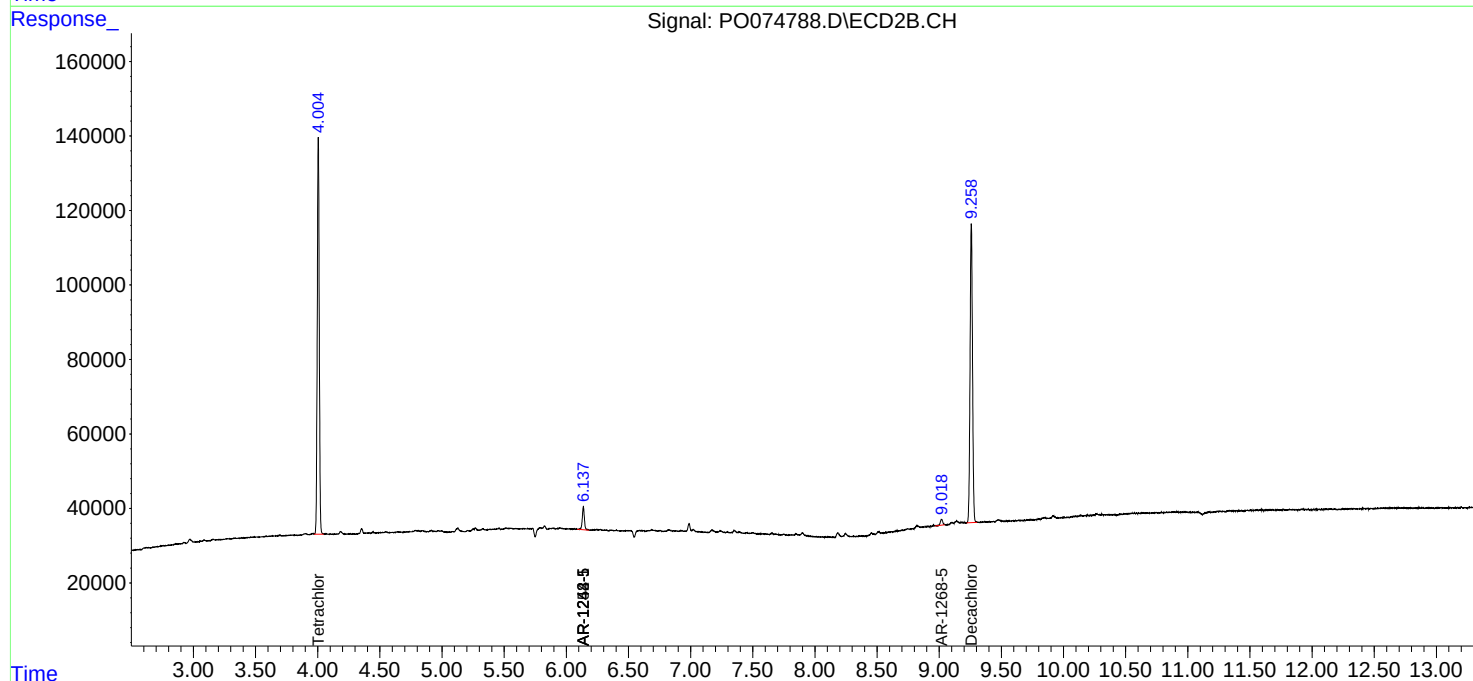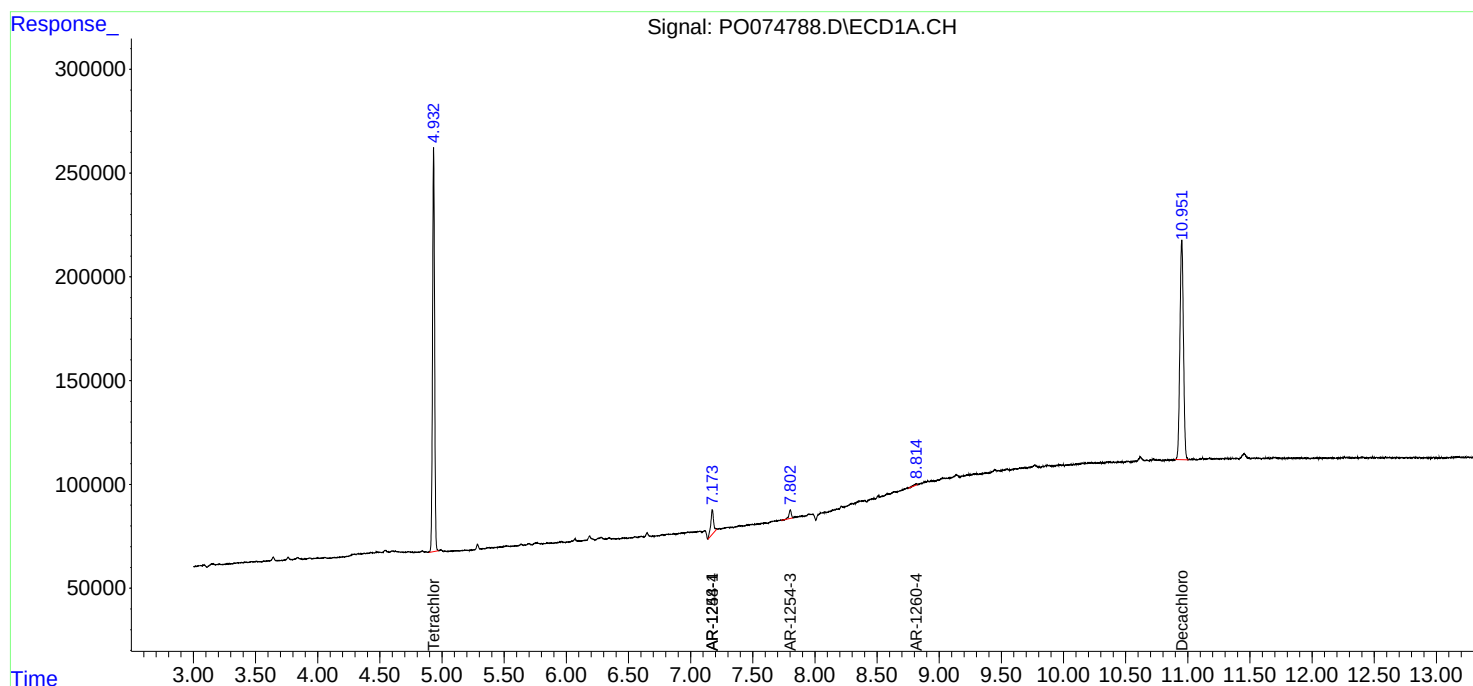


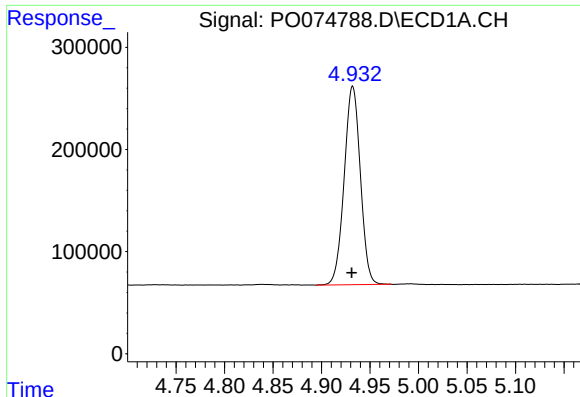

#1 Tetrachloro-m-xylene


R.T.: 4.932 min
Delta R.T.: 0.001 min
Response: 2254101
Conc: 21.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

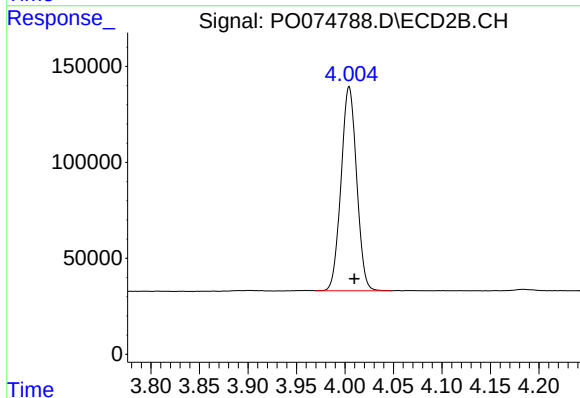


#1 Tetrachloro-m-xylene

R.T.: 4.004 min
Delta R.T.: -0.005 min
Response: 1190166
Conc: 21.16 ng/ml

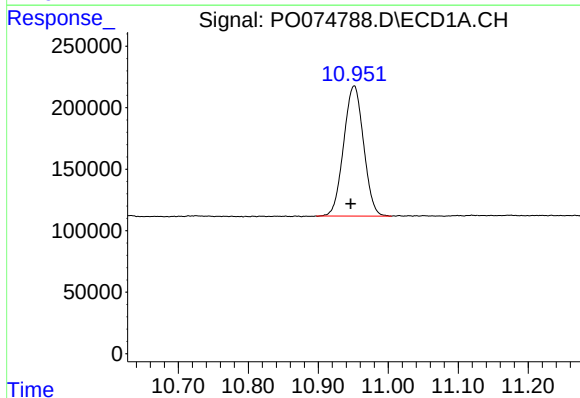


#2 Decachlorobiphenyl

R.T.: 10.952 min
Delta R.T.: 0.005 min
Response: 2087632
Conc: 20.57 ng/ml

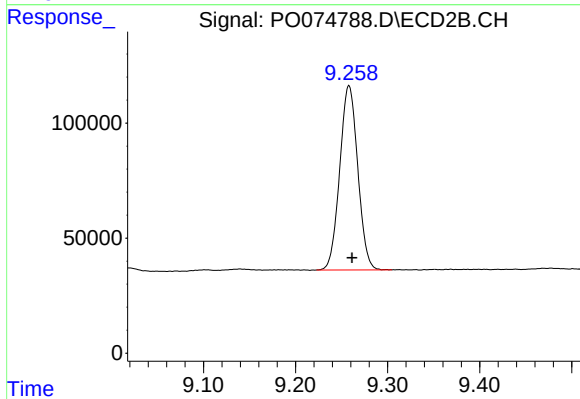

#2 Decachlorobiphenyl


R.T.: 9.258 min
Delta R.T.: -0.003 min
Response: 1090387
Conc: 19.86 ng/ml

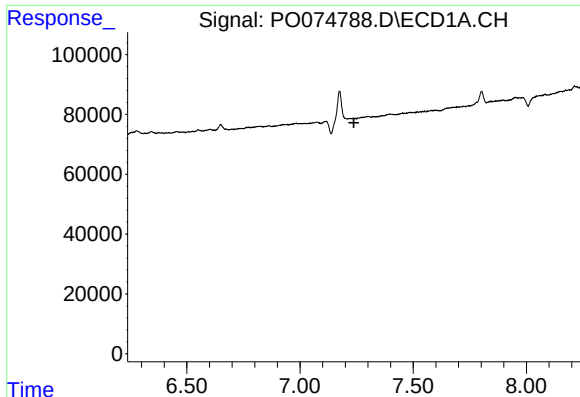

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 7.238 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

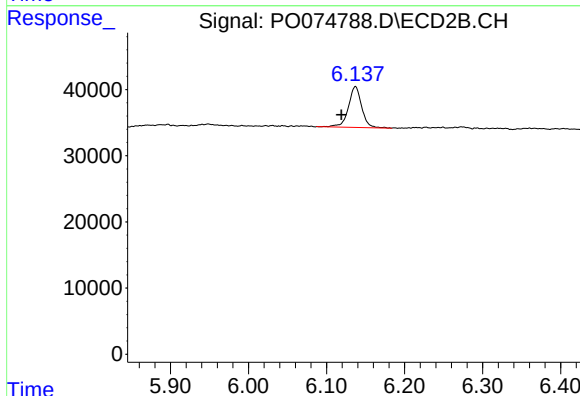


#20 AR-1242-5

R.T.: 6.137 min
Delta R.T.: 0.018 min
Response: 72652
Conc: 41.50 ng/ml

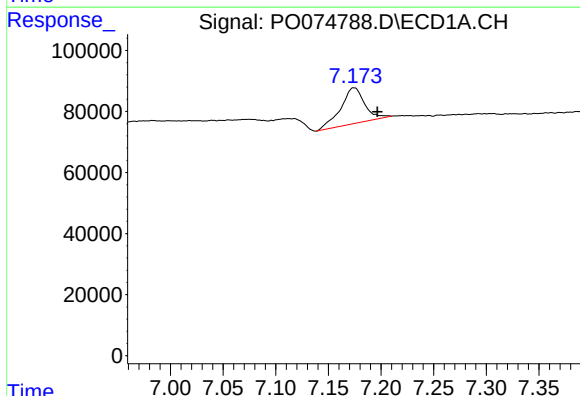


#24 AR-1248-4

R.T.: 7.174 min
Delta R.T.: -0.022 min
Response: 187183
Conc: 41.97 ng/ml

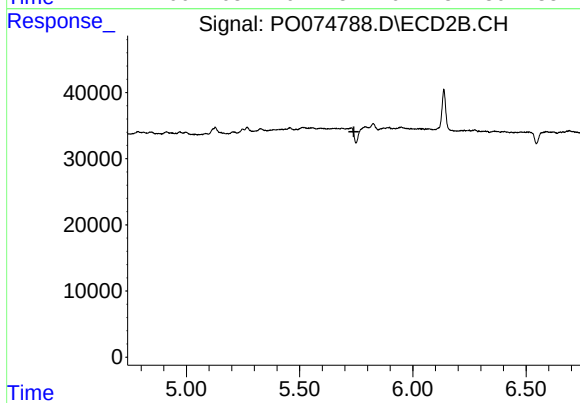

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.740 min
Response: 0
Conc: N.D.

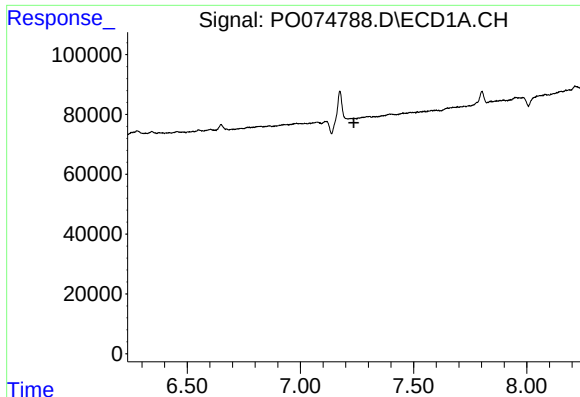

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 7.236 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

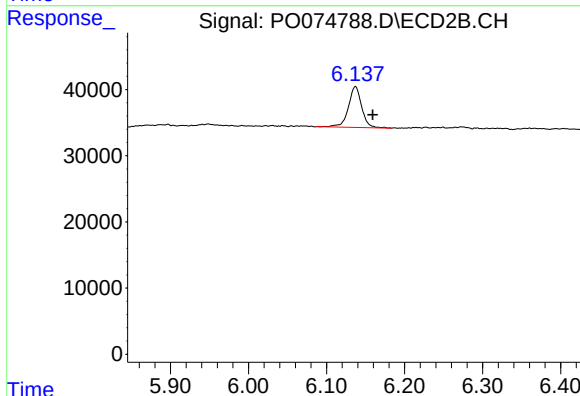


#25 AR-1248-5

R.T.: 6.137 min
Delta R.T.: -0.022 min
Response: 72652
Conc: 30.90 ng/ml

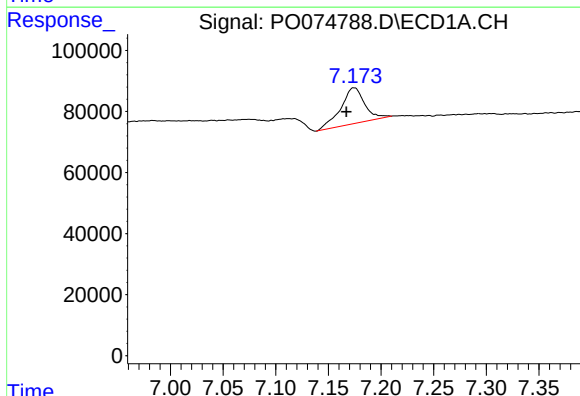


#26 AR-1254-1

R.T.: 7.174 min
Delta R.T.: 0.007 min
Response: 187183
Conc: 42.56 ng/ml

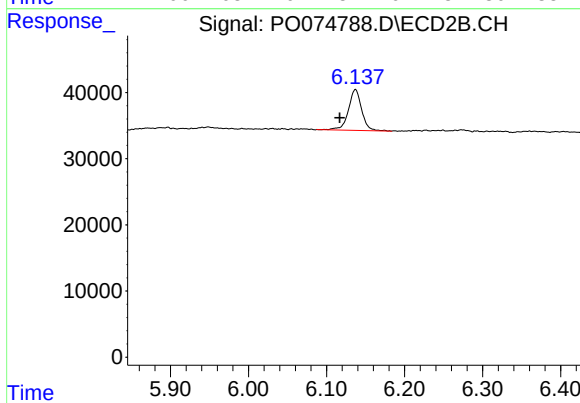

#26 AR-1254-1


R.T.: 6.137 min
Delta R.T.: 0.020 min
Response: 72652
Conc: 20.11 ng/ml

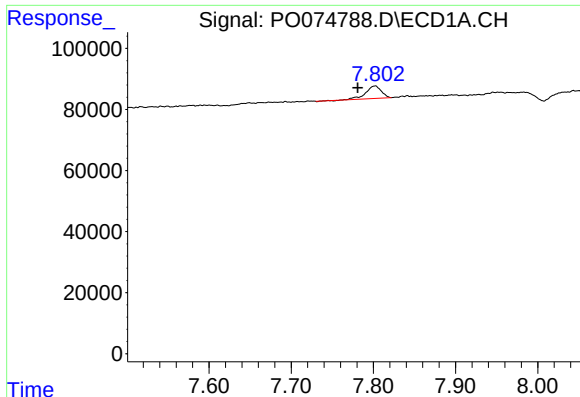

#28 AR-1254-3


R.T.: 7.803 min
Delta R.T.: 0.022 min
Response: 54614
Conc: 7.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

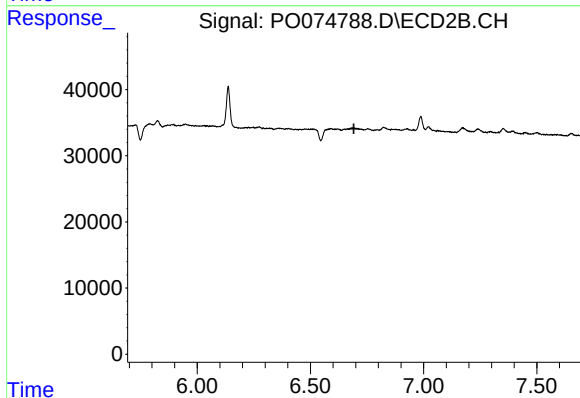


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.692 min
Response: 0
Conc: N.D.

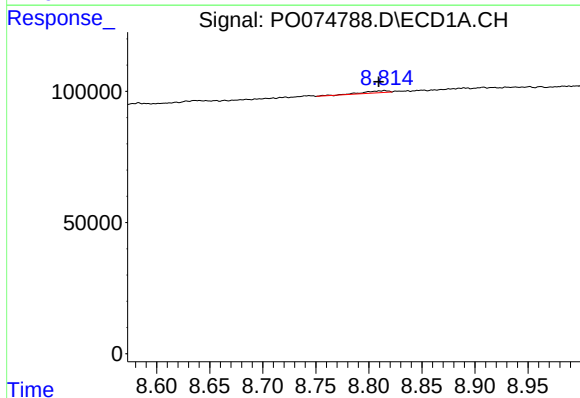


#34 AR-1260-4

R.T.: 8.815 min
Delta R.T.: 0.006 min
Response: 13305
Conc: 2.43 ng/ml

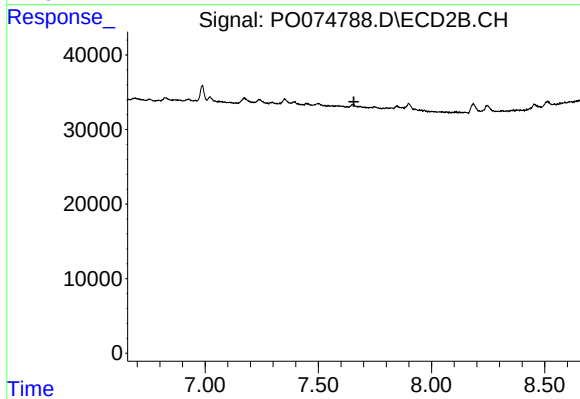

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.657 min
Response: 0
Conc: N.D.

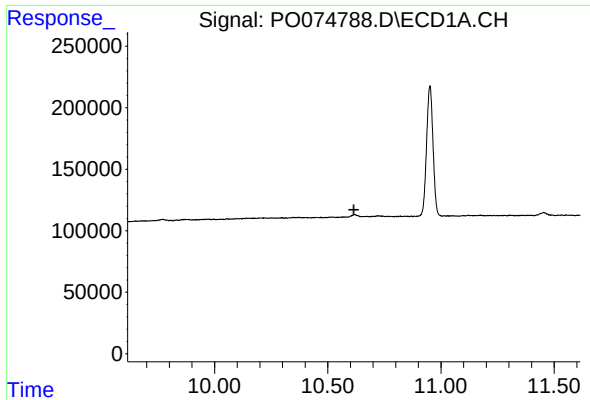

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.616 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

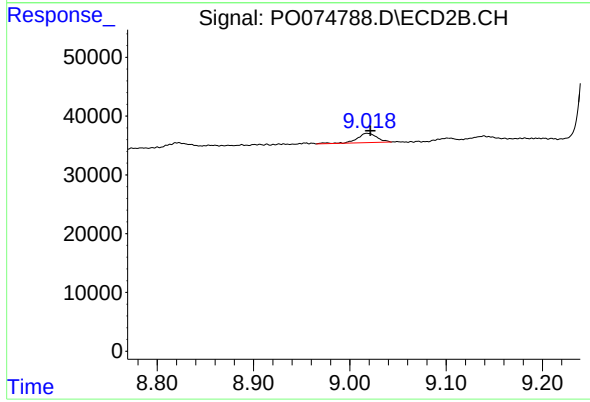

#45 AR-1268-5

R.T.: 9.018 min
Delta R.T.: -0.003 min
Response: 22738
Conc: 0.96 ng/ml