

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011521\
 Data File : P0074801.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Jan 2021 6:22
 Operator : AJ/MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 00:22:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.931	4.003	2275312	1205545	21.563	21.431
2)	SA Decachlor...	10.953	9.258	2119253	1143392	20.881	20.825
Target Compounds							
20)	L4 AR-1242-5	0.000	6.135f	0	86330	N.D.	49.308 #
24)	L5 AR-1248-4	7.173f	0.000	239979	0	53.813	N.D. #
25)	L5 AR-1248-5	0.000	6.135f	0	86330	N.D.	36.720 #
26)	L6 AR-1254-1	7.173	6.135f	239979	86330	54.564	23.901 #
28)	L6 AR-1254-3	7.801f	6.688	62497	5623	8.910	1.147 #
29)	L6 AR-1254-4	8.078	0.000	96930	0	15.983	N.D. #
32)	L7 AR-1260-2	8.213	0.000	14649	0	2.154	N.D. #
45)	L9 AR-1268-5	0.000	9.017	0	25731	N.D.	1.087 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011521\
Data File : P0074801.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Jan 2021 6:22
Operator : AJ/MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 00:22:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

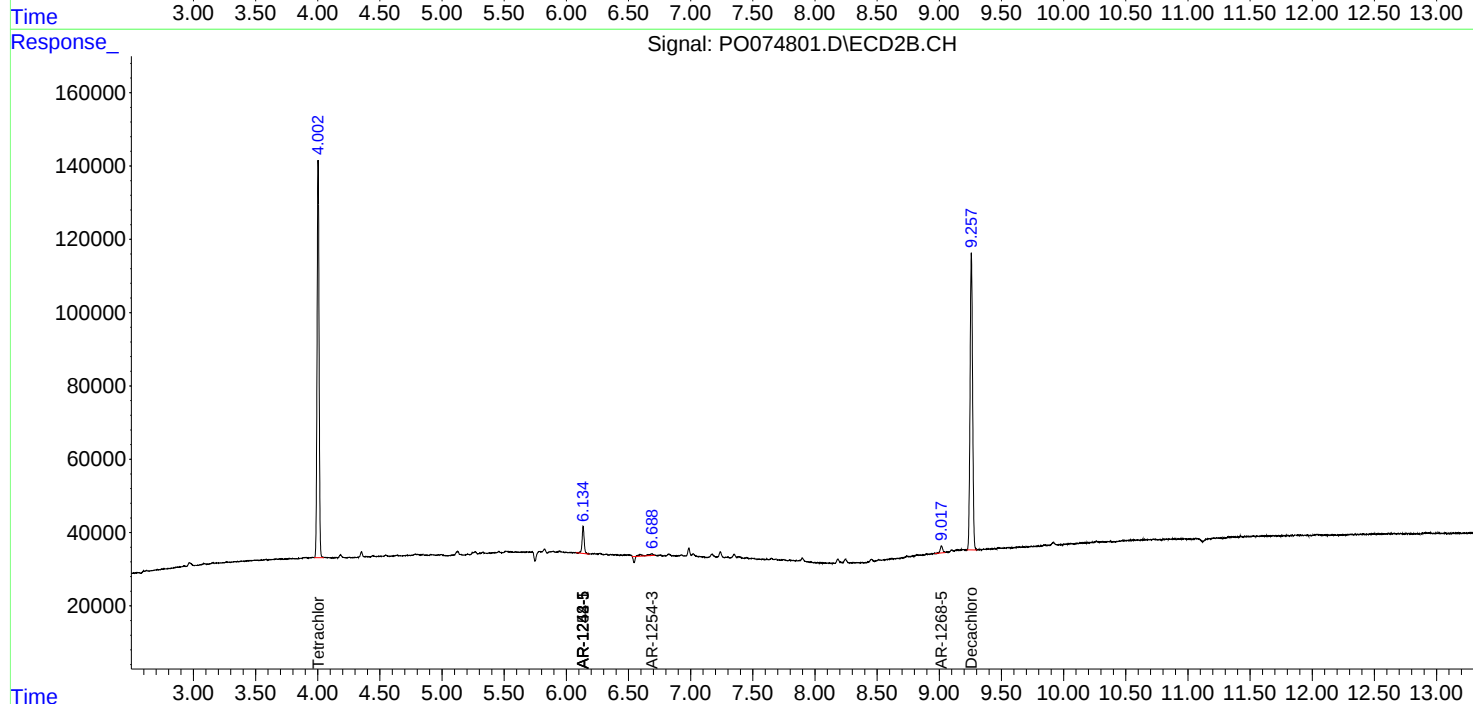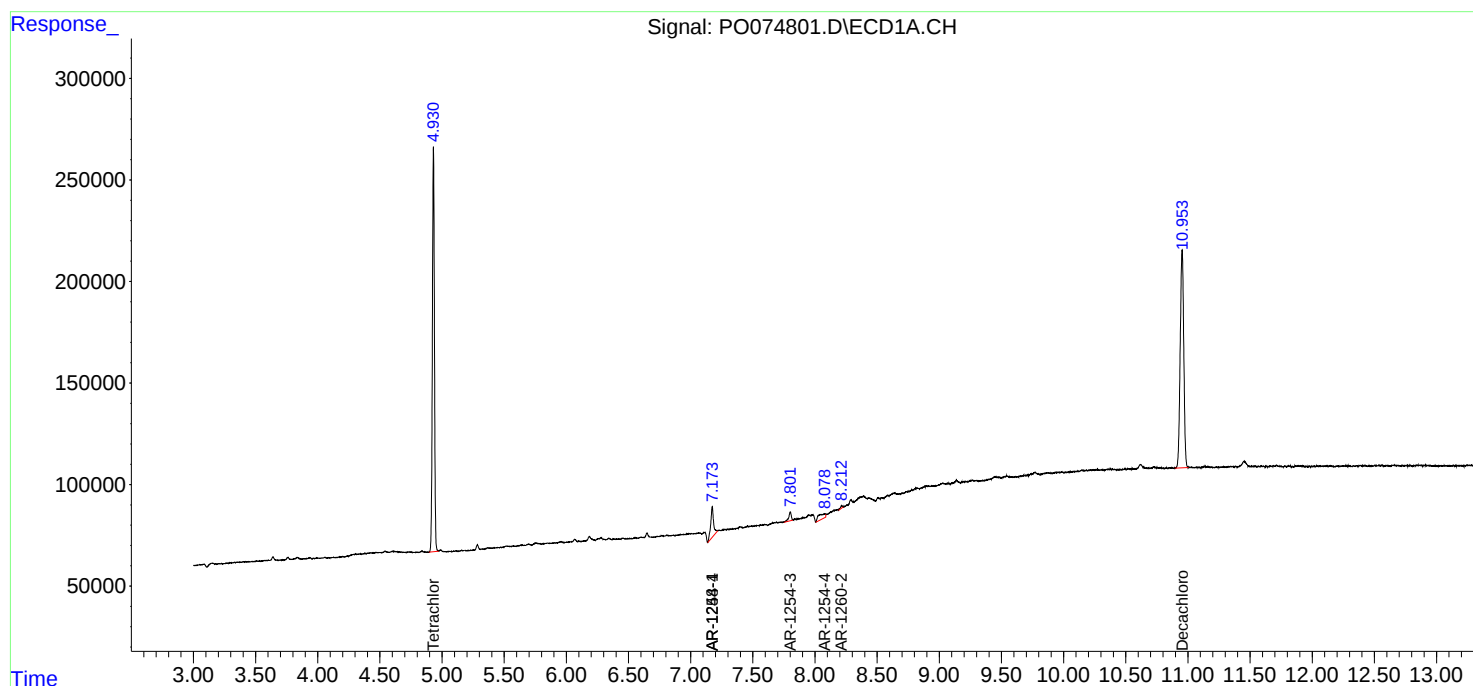


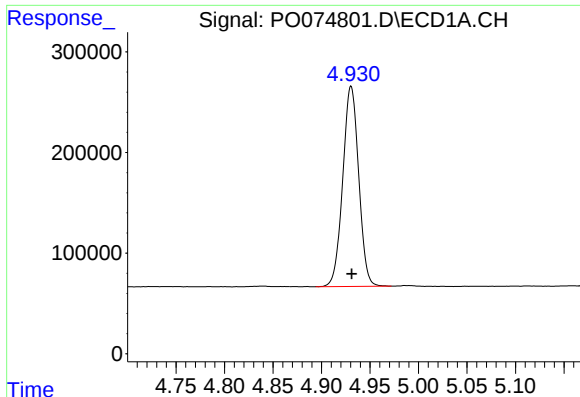

#1 Tetrachloro-m-xylene


R.T.: 4.931 min
Delta R.T.: 0.000 min
Response: 2275312
Conc: 21.56 ng/ml

Instrument :
ECD_O
ClientSampleId :

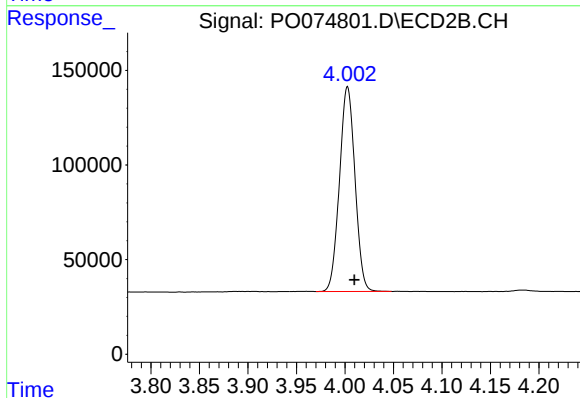


#1 Tetrachloro-m-xylene

R.T.: 4.003 min
Delta R.T.: -0.007 min
Response: 1205545
Conc: 21.43 ng/ml

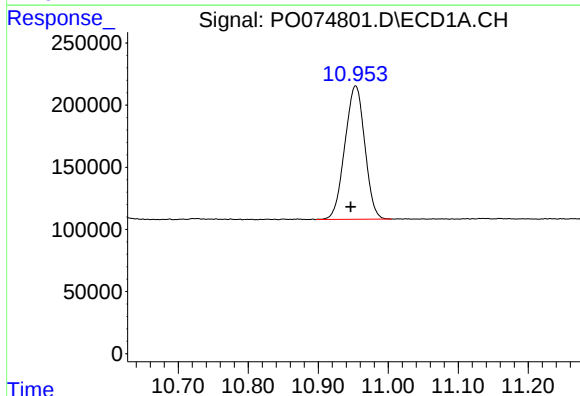


#2 Decachlorobiphenyl

R.T.: 10.953 min
Delta R.T.: 0.007 min
Response: 2119253
Conc: 20.88 ng/ml

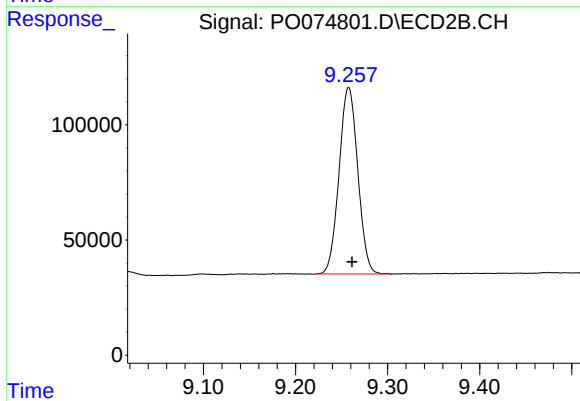

#2 Decachlorobiphenyl


R.T.: 9.258 min
Delta R.T.: -0.004 min
Response: 1143392
Conc: 20.83 ng/ml

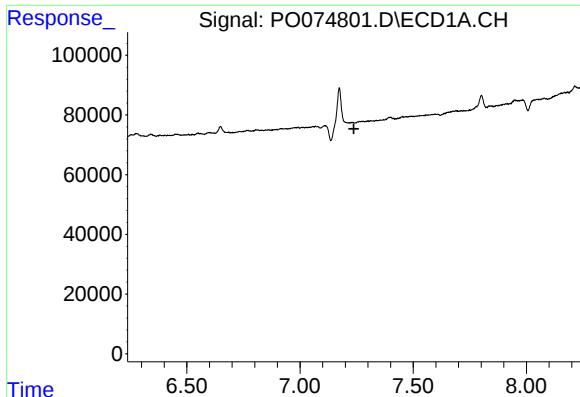

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 7.238 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

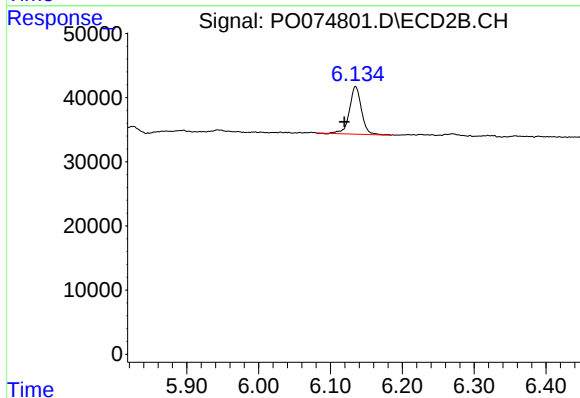


#20 AR-1242-5

R.T.: 6.135 min
Delta R.T.: 0.016 min
Response: 86330
Conc: 49.31 ng/ml

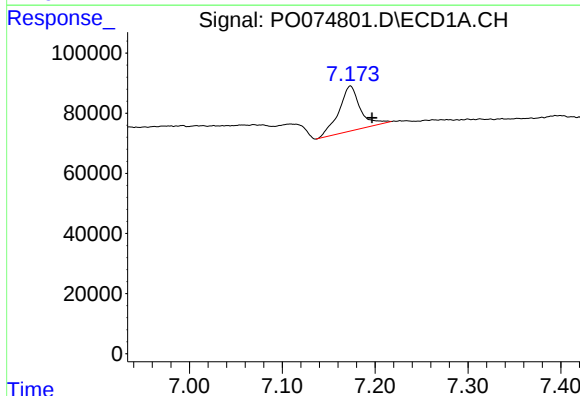


#24 AR-1248-4

R.T.: 7.173 min
Delta R.T.: -0.023 min
Response: 239979
Conc: 53.81 ng/ml

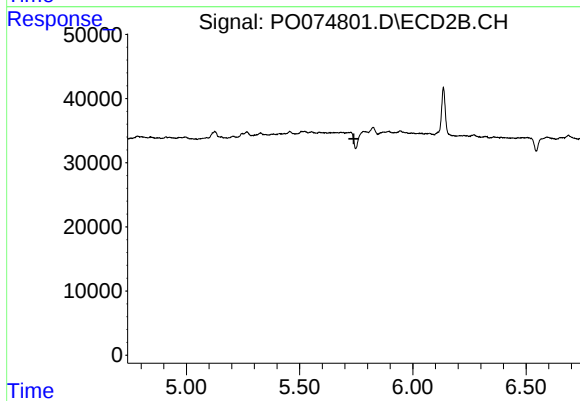

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.740 min
Response: 0
Conc: N.D.

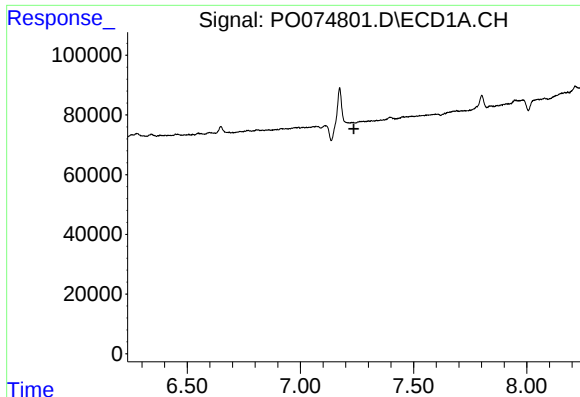

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 7.236 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

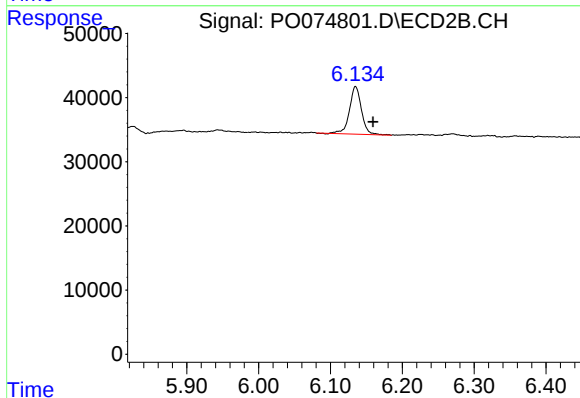


#25 AR-1248-5

R.T.: 6.135 min
Delta R.T.: -0.024 min
Response: 86330
Conc: 36.72 ng/ml

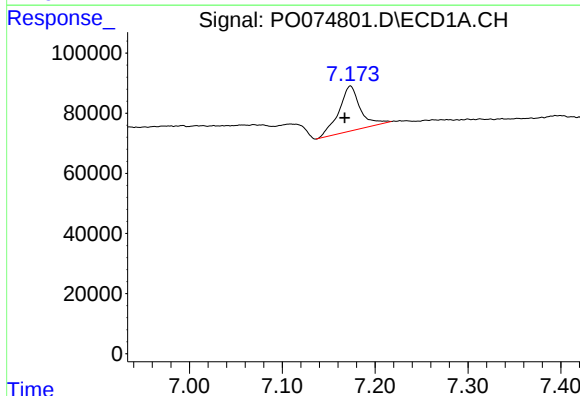


#26 AR-1254-1

R.T.: 7.173 min
Delta R.T.: 0.006 min
Response: 239979
Conc: 54.56 ng/ml

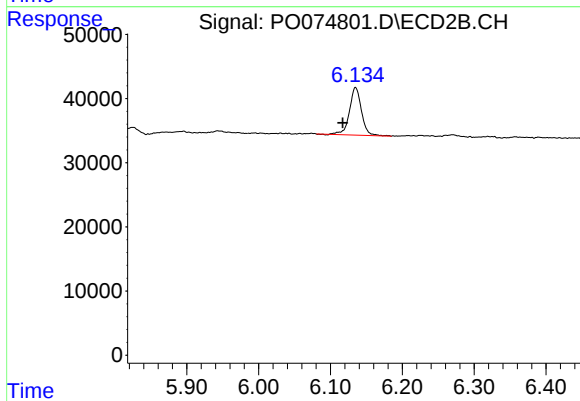

#26 AR-1254-1


R.T.: 6.135 min
Delta R.T.: 0.018 min
Response: 86330
Conc: 23.90 ng/ml

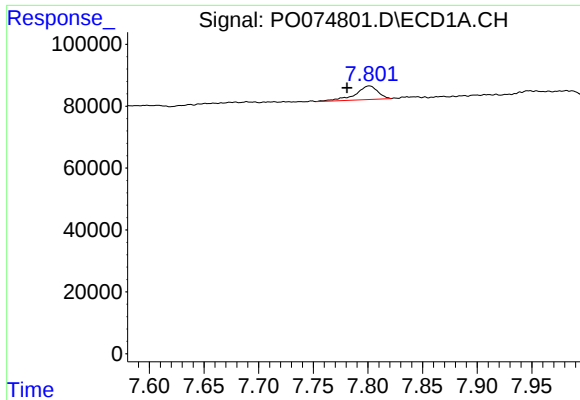

#28 AR-1254-3


R.T.: 7.801 min
Delta R.T.: 0.020 min
Response: 62497
Conc: 8.91 ng/ml

Instrument :
ECD_O
ClientSampleId :

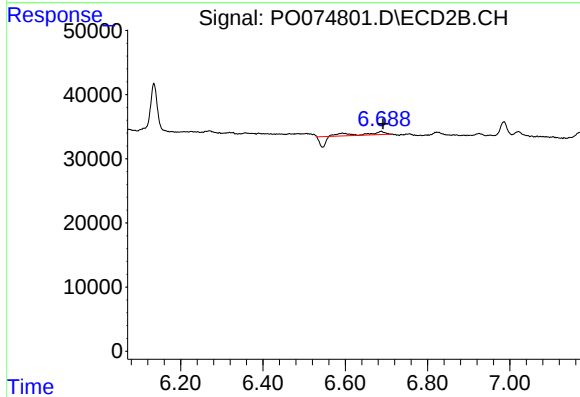


#28 AR-1254-3

R.T.: 6.688 min
Delta R.T.: -0.004 min
Response: 5623
Conc: 1.15 ng/ml

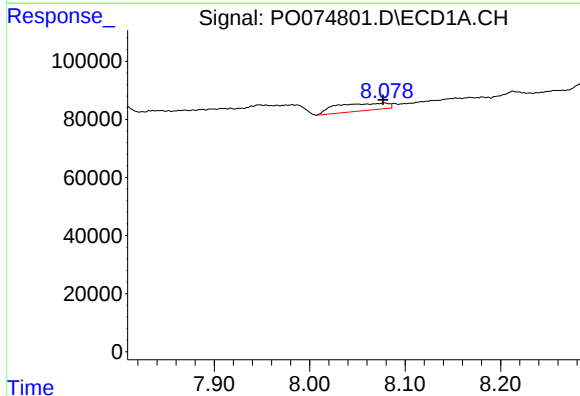


#29 AR-1254-4

R.T.: 8.078 min
Delta R.T.: 0.001 min
Response: 96930
Conc: 15.98 ng/ml

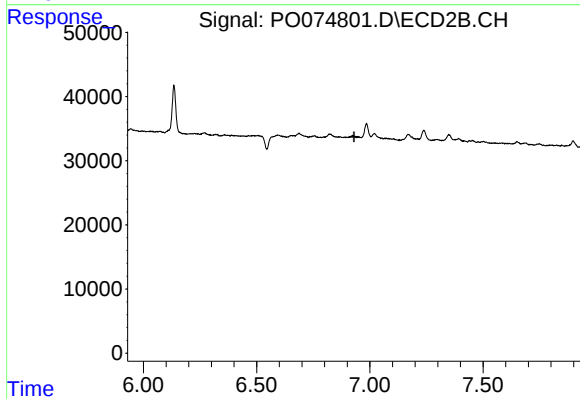

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 6.930 min
Response: 0
Conc: N.D.

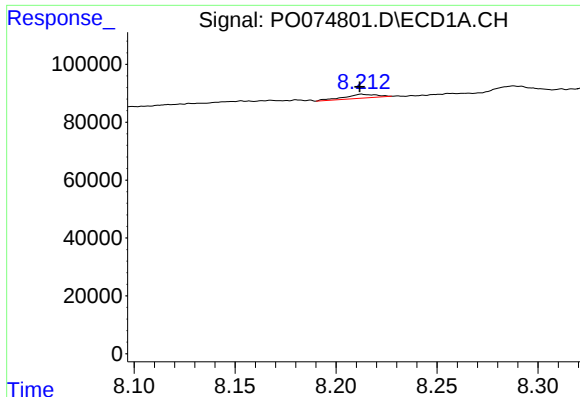

#32 AR-1260-2


R.T.: 8.213 min
Delta R.T.: 0.001 min
Response: 14649
Conc: 2.15 ng/ml

Instrument :
ECD_O
ClientSampleId :

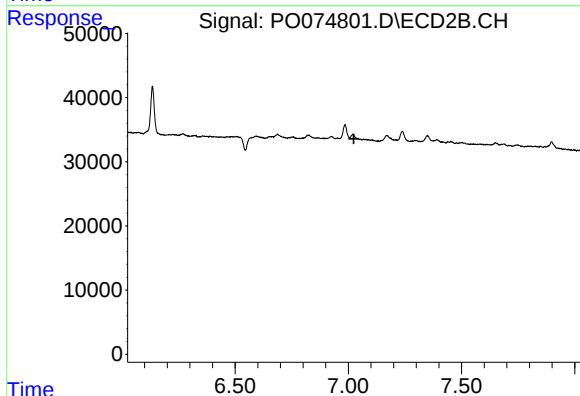


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.025 min
Response: 0
Conc: N.D.

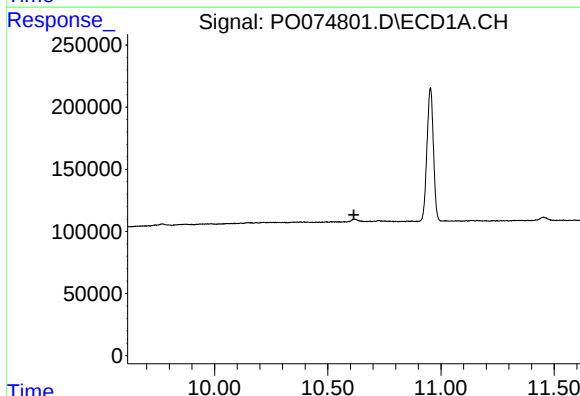

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 10.616 min
Response: 0
Conc: N.D.

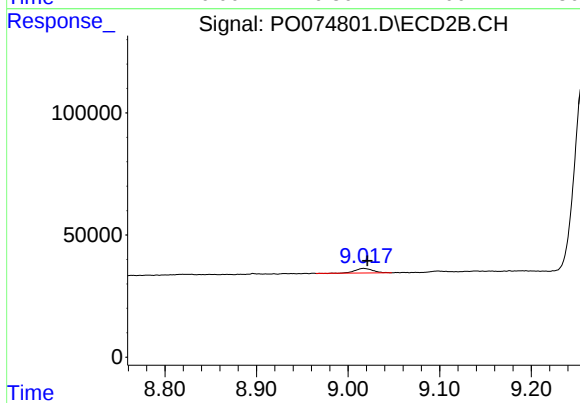

#45 AR-1268-5

R.T.: 9.017 min
Delta R.T.: -0.004 min
Response: 25731
Conc: 1.09 ng/ml