

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011521\
 Data File : P0074840.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Jan 2021 18:21
 Operator : AJ/MA
 Sample : M1041-02 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-PS-01-068

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 00:49:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.930	4.002	2462906	1276228	23.341	22.688
2)	SA Decachlor...	10.953	9.259	1642089	861672	16.179	15.694
Target Compounds							
8)	L2 AR-1221-1	5.185	0.000	528864	0	430.566	N.D. #
27)	L6 AR-1254-2	7.407	0.000	42380	0	6.222	N.D. #
30)	L6 AR-1254-5	8.533f	7.351	89109	41039	15.340	9.067 #
32)	L7 AR-1260-2	8.213	7.050f	56813	32882	8.352	7.735
35)	L7 AR-1260-5	9.136	0.000	36605	0	2.930	N.D. #
36)	L8 AR-1262-1	0.000	7.351	0	41039	N.D.	16.128 #
37)	L8 AR-1262-2	9.136	0.000	36605	0	2.391	N.D. #
45)	L9 AR-1268-5	0.000	9.019	0	22870	N.D.	0.966 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011521\
Data File : PO074840.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Jan 2021 18:21
Operator : AJ/MA
Sample : M1041-02 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
FK-PS-01-068

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 00:49:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

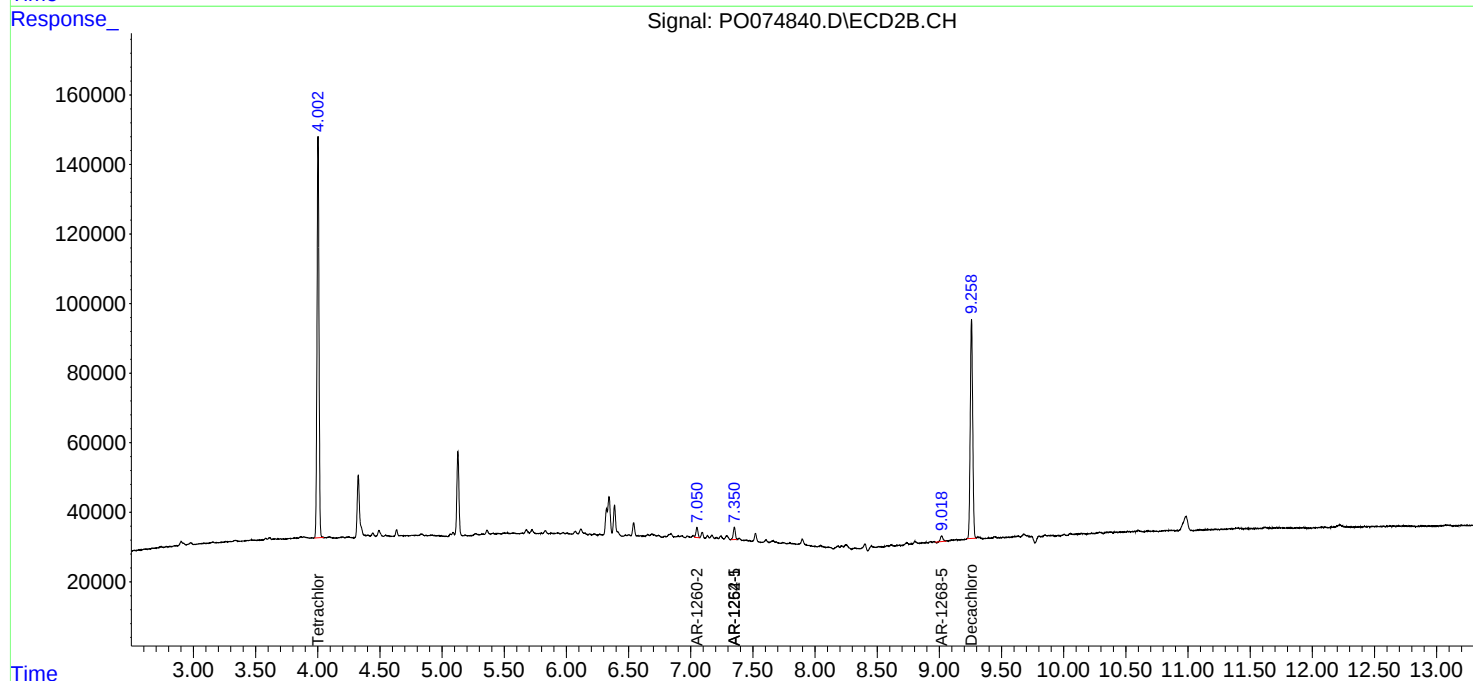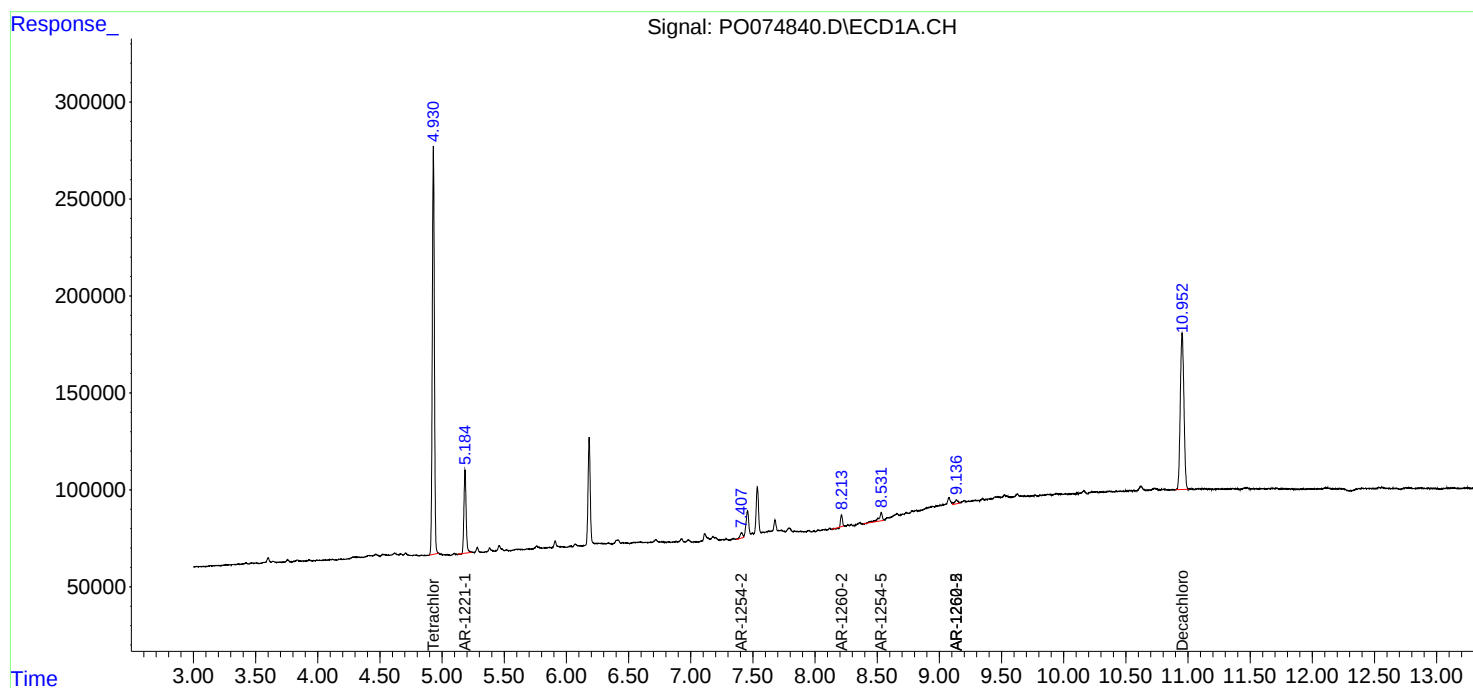


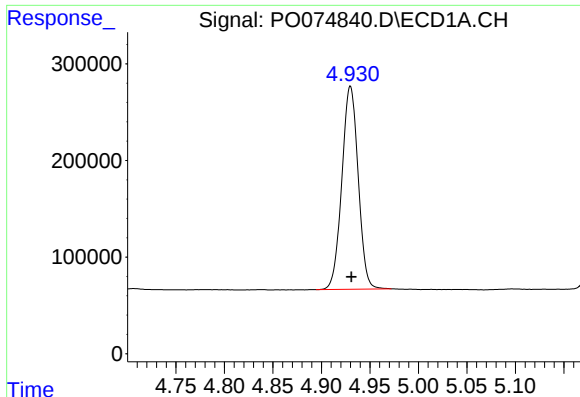

#1 Tetrachloro-m-xylene


R.T.: 4.930 min
Delta R.T.: -0.001 min
Response: 2462906
Conc: 23.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-068

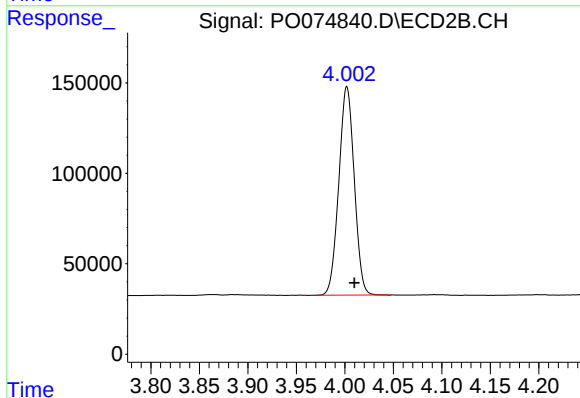


#1 Tetrachloro-m-xylene

R.T.: 4.002 min
Delta R.T.: -0.008 min
Response: 1276228
Conc: 22.69 ng/ml

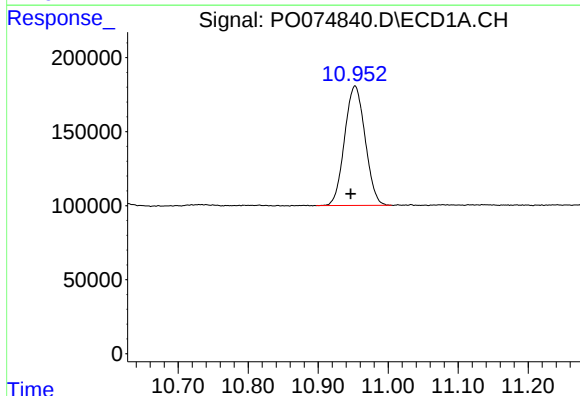


#2 Decachlorobiphenyl

R.T.: 10.953 min
Delta R.T.: 0.006 min
Response: 1642089
Conc: 16.18 ng/ml

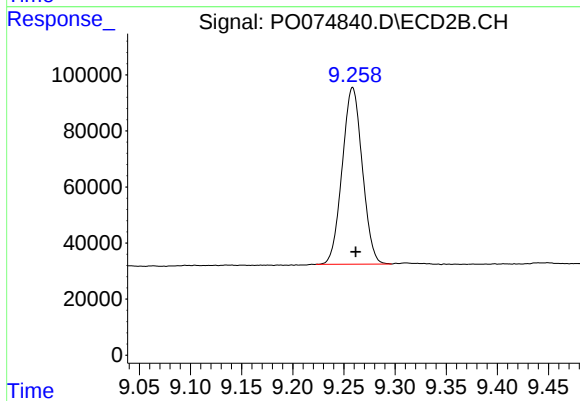

#2 Decachlorobiphenyl


R.T.: 9.259 min
Delta R.T.: -0.003 min
Response: 861672
Conc: 15.69 ng/ml

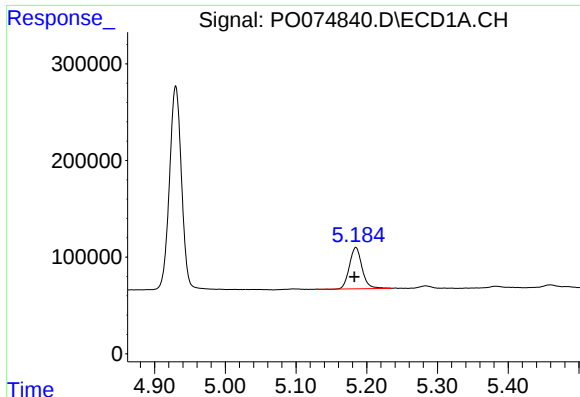

#8 AR-1221-1


R.T.: 5.185 min
Delta R.T.: 0.002 min
Response: 528864
Conc: 430.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-068

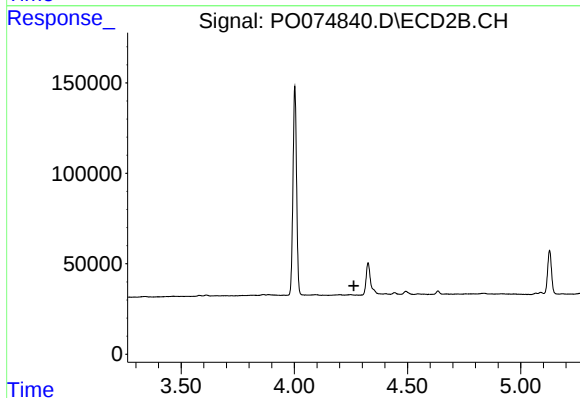


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.263 min
Response: 0
Conc: N.D.

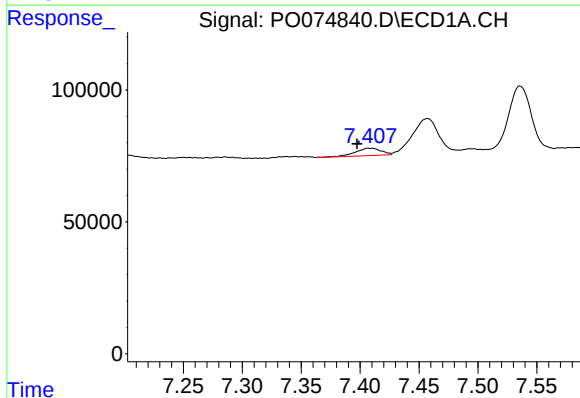


#27 AR-1254-2

R.T.: 7.407 min
Delta R.T.: 0.009 min
Response: 42380
Conc: 6.22 ng/ml

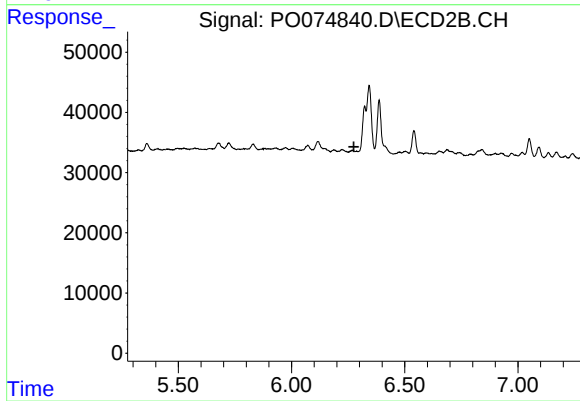

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T. : 6.275 min
Response: 0
Conc: N.D.

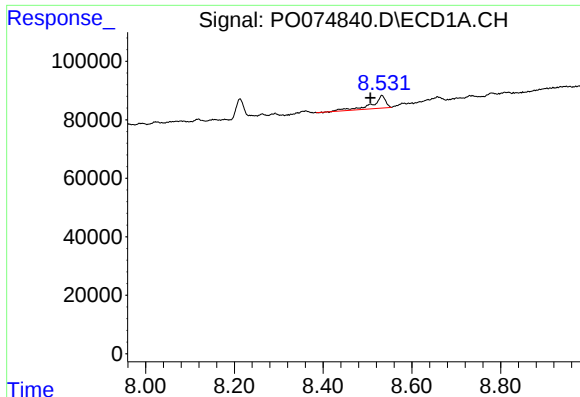

#30 AR-1254-5


R.T.: 8.533 min
Delta R.T.: 0.026 min
Response: 89109
Conc: 15.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-068

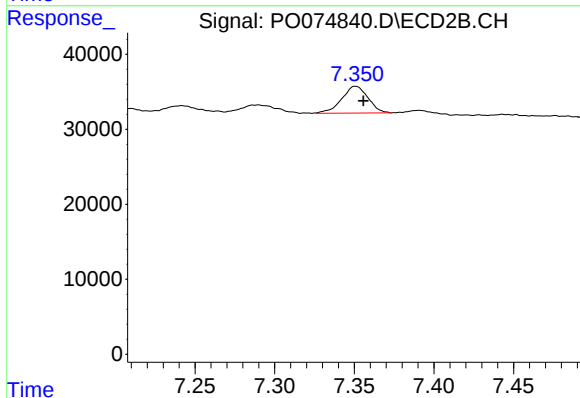


#30 AR-1254-5

R.T.: 7.351 min
Delta R.T.: -0.005 min
Response: 41039
Conc: 9.07 ng/ml

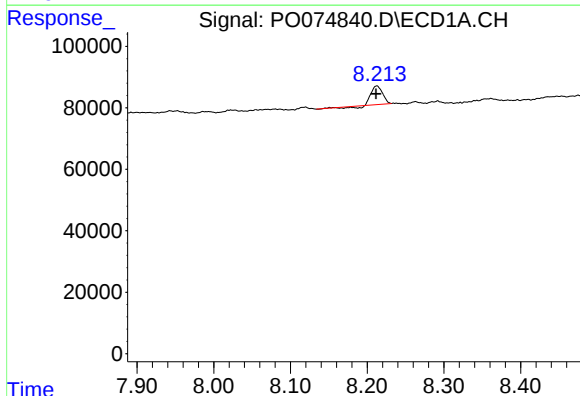


#32 AR-1260-2

R.T.: 8.213 min
Delta R.T.: 0.000 min
Response: 56813
Conc: 8.35 ng/ml

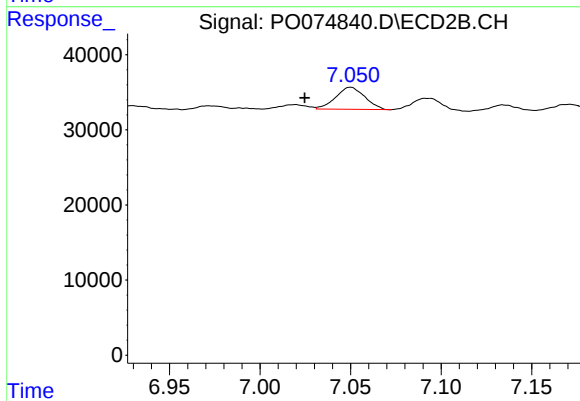

#32 AR-1260-2


R.T.: 7.050 min
Delta R.T.: 0.025 min
Response: 32882
Conc: 7.74 ng/ml

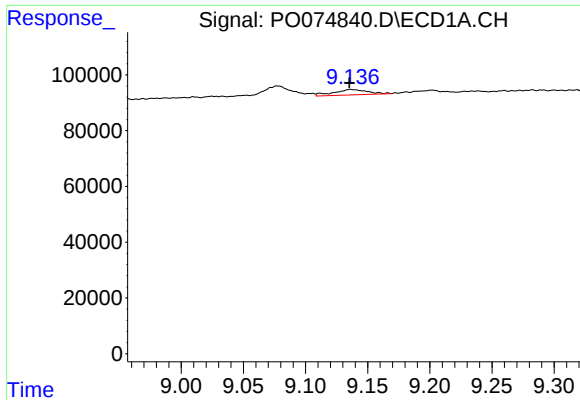

#35 AR-1260-5


R.T.: 9.136 min
Delta R.T.: 0.000 min
Response: 36605
Conc: 2.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-068

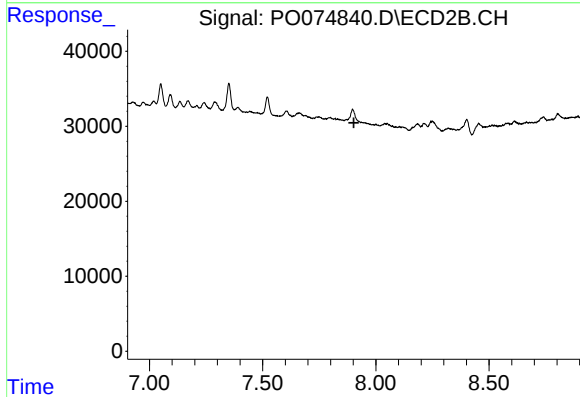


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.903 min
Response: 0
Conc: N.D.

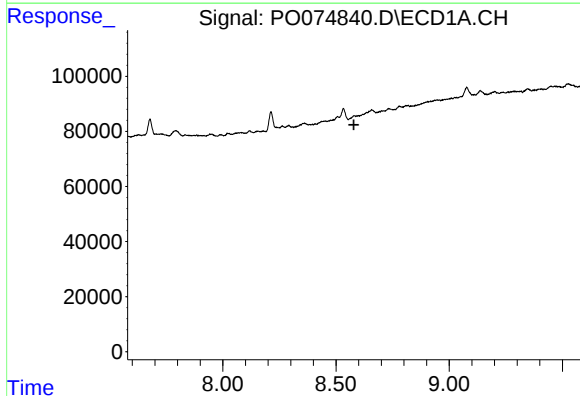


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 8.579 min
Response: 0
Conc: N.D.

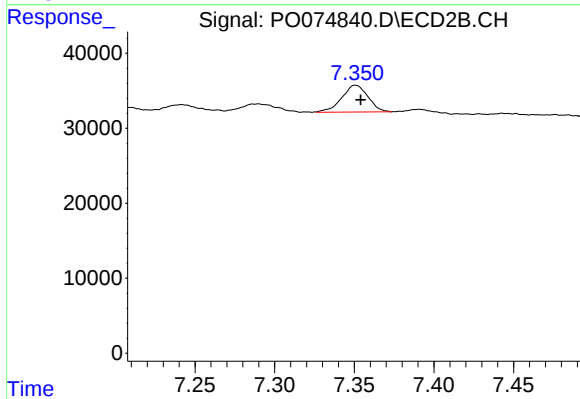

#36 AR-1262-1


R.T.: 7.351 min
Delta R.T.: -0.003 min
Response: 41039
Conc: 16.13 ng/ml

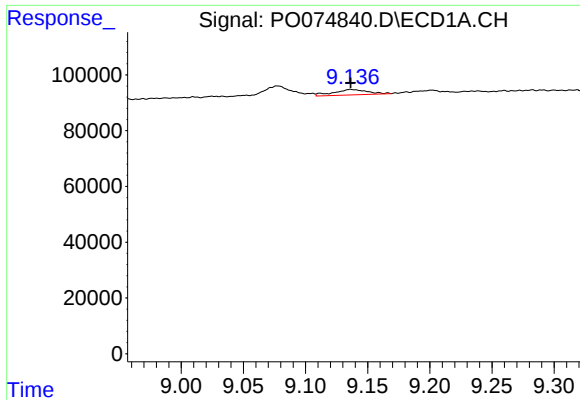

#37 AR-1262-2


R.T.: 9.136 min
Delta R.T.: 0.000 min
Response: 36605
Conc: 2.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-068

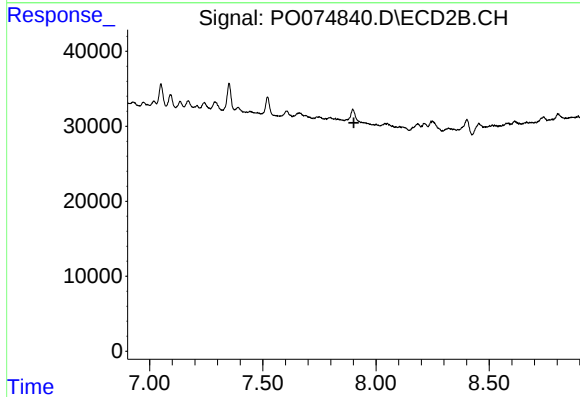


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.902 min
Response: 0
Conc: N.D.

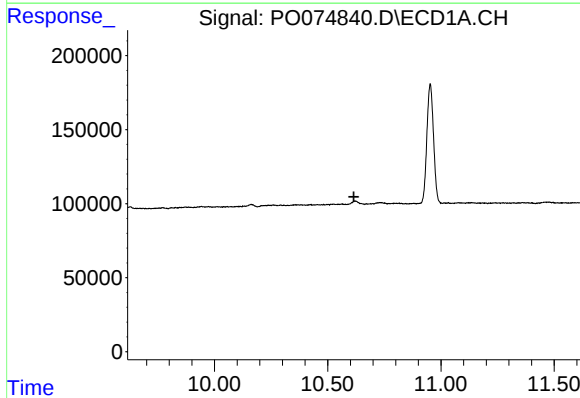

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 10.616 min
Response: 0
Conc: N.D.

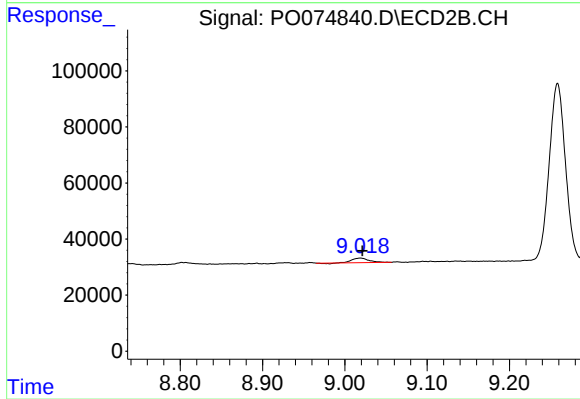

#45 AR-1268-5

R.T.: 9.019 min
Delta R.T.: -0.002 min
Response: 22870
Conc: 0.97 ng/ml