

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0011521\
 Data File : P0074730.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Jan 2021 8:27
 Operator : AJ/MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 15 16:42:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

 System Monitoring Compounds

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO011521\
 Data File : PO074730.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Jan 2021 8:27
 Operator : AJ/MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 15 16:42:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped


Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

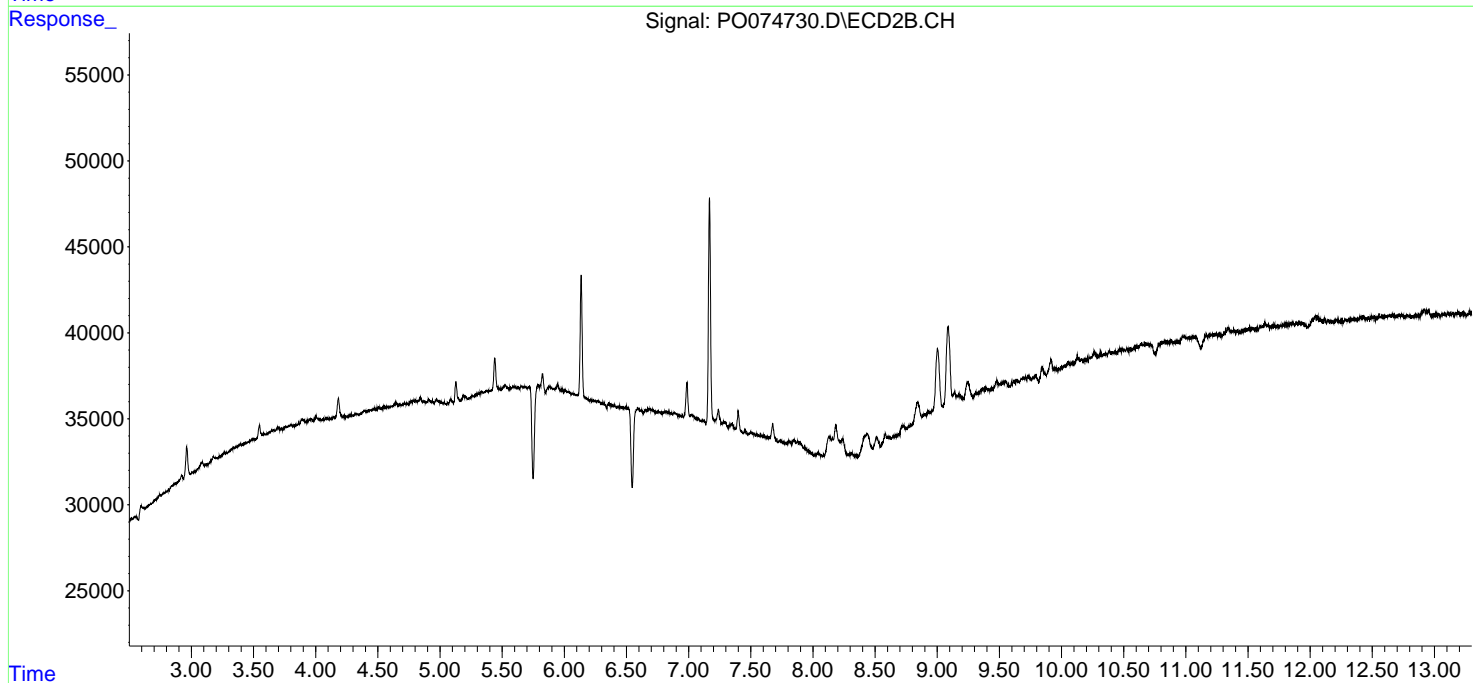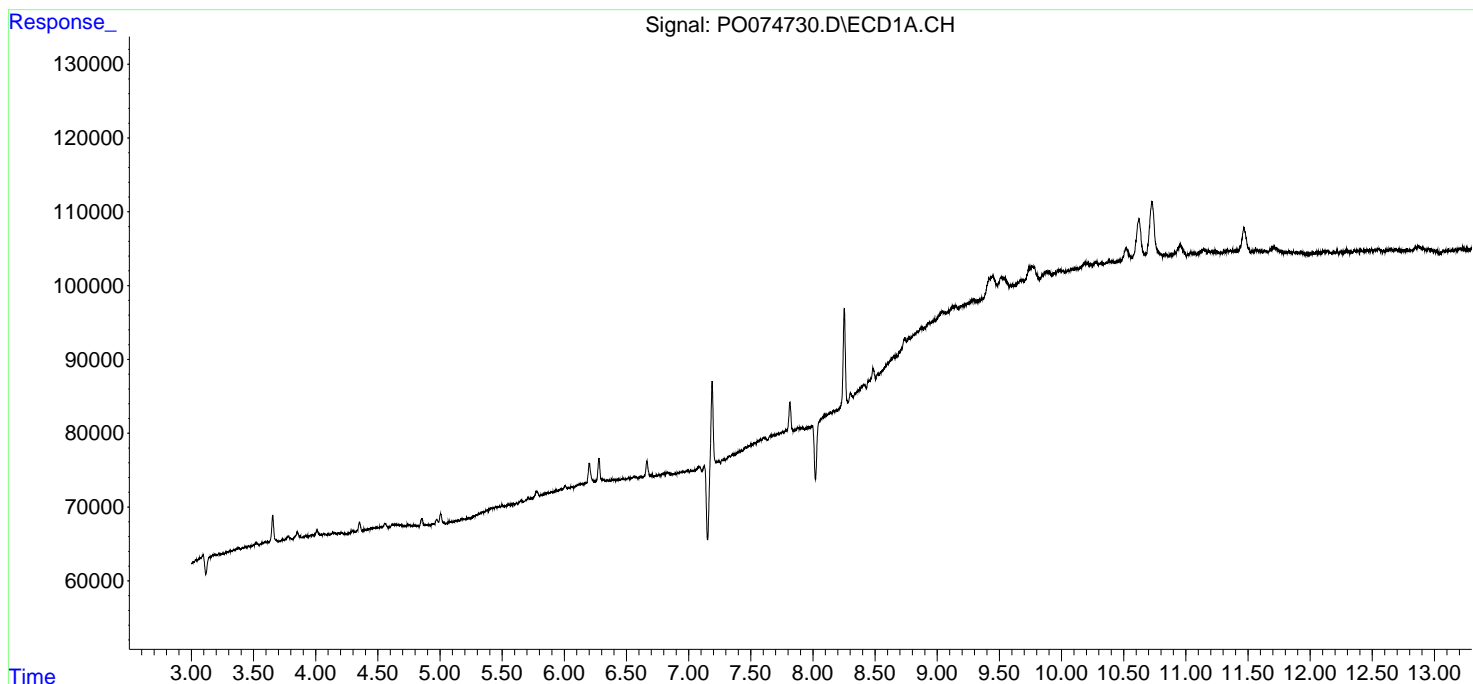

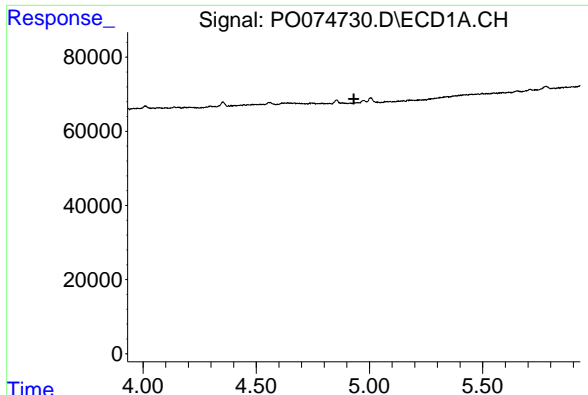


#1 Tetrachloro-m-xylene
 R.T.: 0.000 min
 Exp R.T. : 4.931 min
 Response: 0
 Conc: N.D.


Instrument :
 ECD_O
 ClientSampled :
 HEXANE

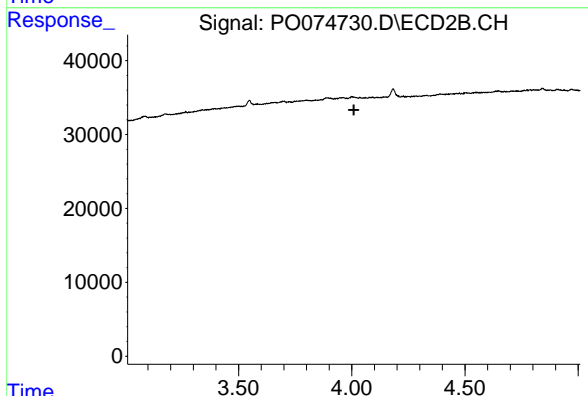

#1 Tetrachloro-m-xylene
 R.T.: 0.000 min
 Exp R.T. : 4.010 min
 Response: 0
 Conc: N.D.

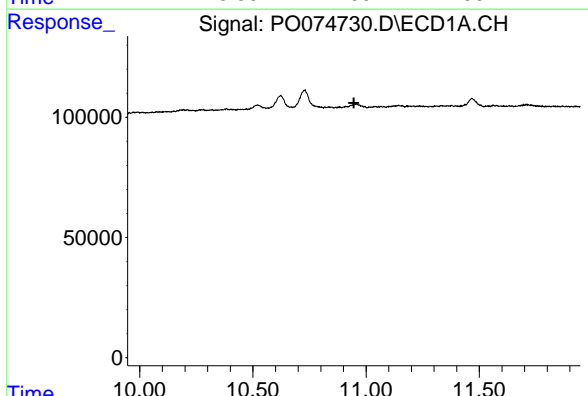

#2 Decachlorobiphenyl
 R.T.: 0.000 min
 Exp R.T. : 10.946 min
 Response: 0
 Conc: N.D.

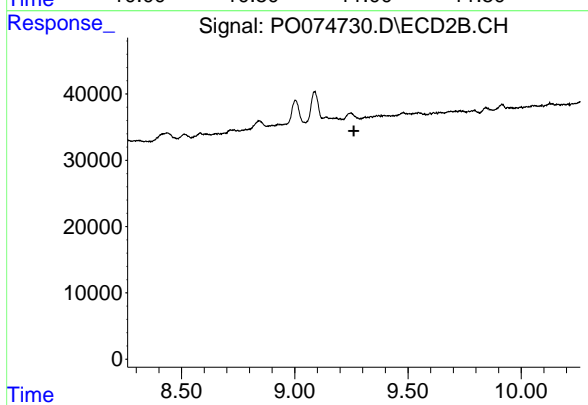

#2 Decachlorobiphenyl
 R.T.: 0.000 min
 Exp R.T. : 9.261 min
 Response: 0
 Conc: N.D.