

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011521\
 Data File : P0074741.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Jan 2021 11:53
 Operator : AJ/MA
 Sample : M1096-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 263K-31A

Manual Integrations
 APPROVED

Ankita
 1/18/2021 2:36:49 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 10:09:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.930	4.002	2390739	1286894	22.657	22.877
2)	SA Decachlor...	10.946	9.255	1710470	976898	16.853	17.793
Target Compounds							
26)	L6 AR-1254-1	7.172	6.112	162979	242894	37.056m	67.246 #
27)	L6 AR-1254-2	7.402	6.270	617163	226006	90.616	72.518
28)	L6 AR-1254-3	7.781	6.686	982566	542168	140.080	110.558
29)	L6 AR-1254-4	8.074	6.926	636435	238036	104.941	68.642 #
30)	L6 AR-1254-5	8.511	7.351	1216681	5283179	209.450m	1167.311 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011521\
Data File : PO074741.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Jan 2021 11:53
Operator : AJ/MA
Sample : M1096-06
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
263K-31A


Manual Integrations
APPROVED

Ankita
1/18/2021 2:36:49 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 10:09:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

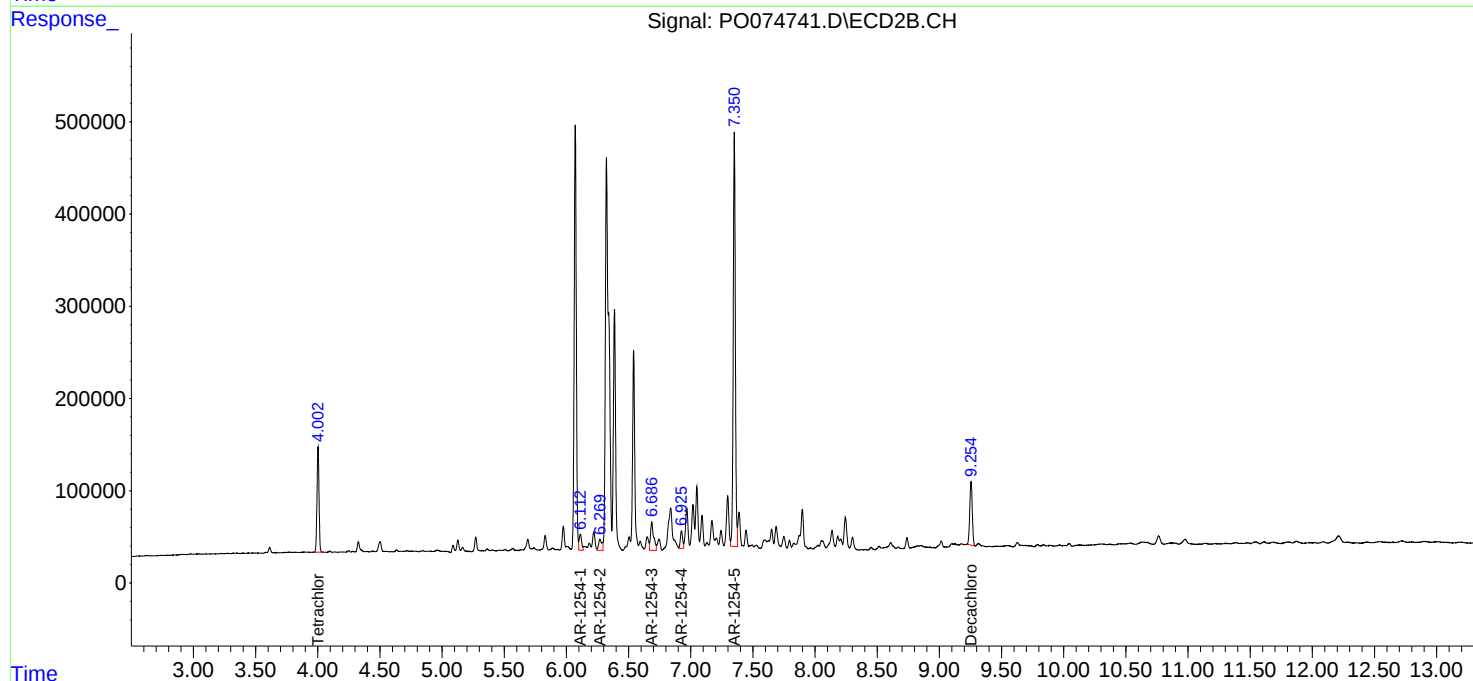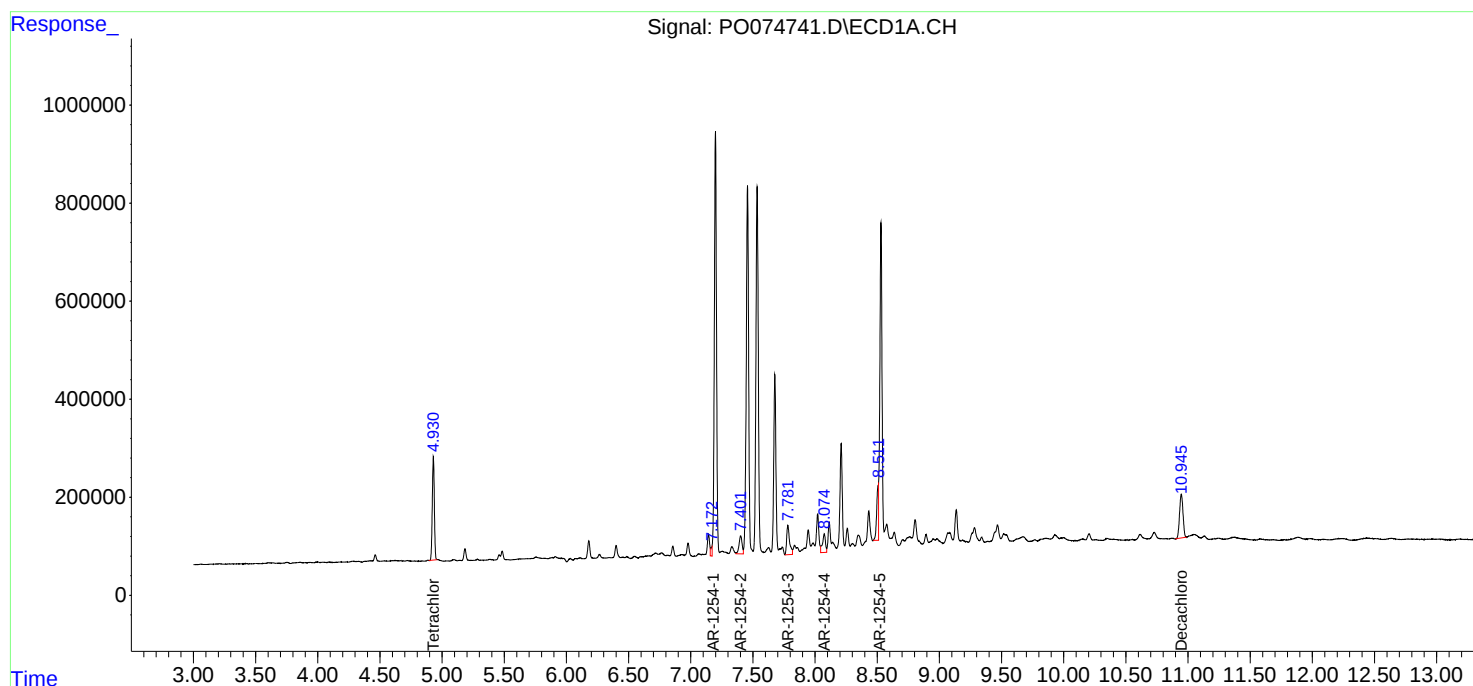

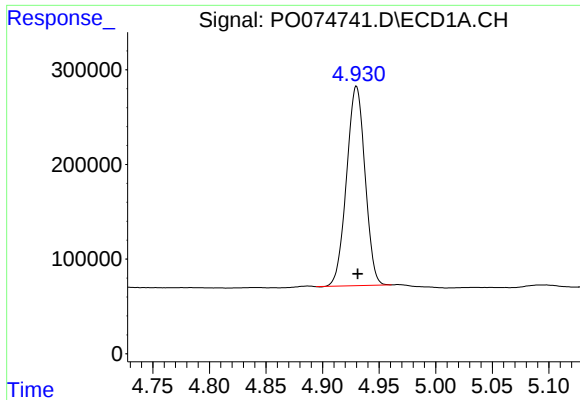


#1 Tetrachloro-m-xylene

R.T.: 4.930 min
Delta R.T.: -0.001 min
Response: 2390739
Conc: 22.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-31A


Manual Integrations
APPROVED

Ankita
1/18/2021 2:36:49 PM

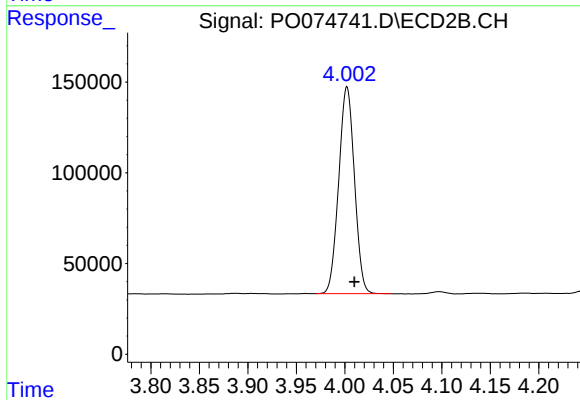


#1 Tetrachloro-m-xylene

R.T.: 4.002 min
Delta R.T.: -0.007 min
Response: 1286894
Conc: 22.88 ng/ml

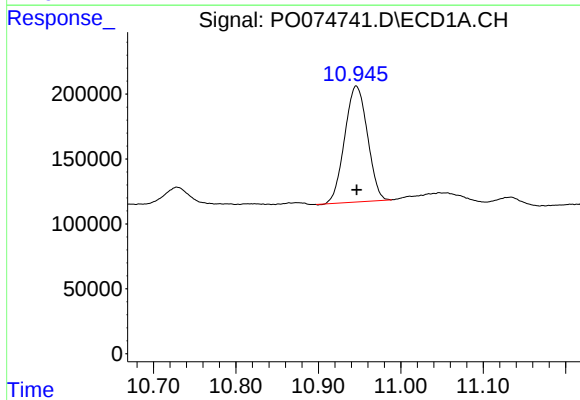


#2 Decachlorobiphenyl

R.T.: 10.946 min
Delta R.T.: 0.000 min
Response: 1710470
Conc: 16.85 ng/ml

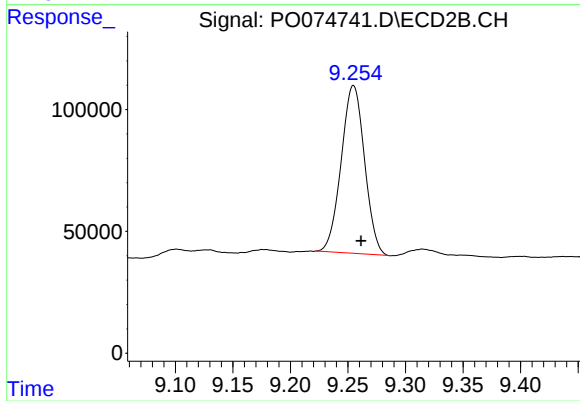

#2 Decachlorobiphenyl

R.T.: 9.255 min
Delta R.T.: -0.007 min
Response: 976898
Conc: 17.79 ng/ml

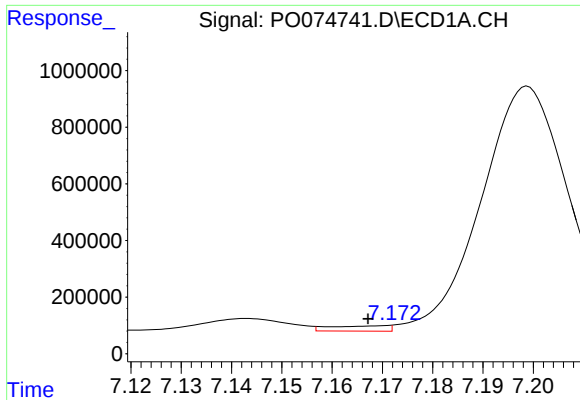


#26 AR-1254-1

R.T.: 7.172 min
Delta R.T.: 0.005 min
Response: 162979
Conc: 37.06 ng/ml m

Instrument :
ECD_O
ClientSampleId :
263K-31A


Manual Integrations
APPROVED

Ankita
1/18/2021 2:36:49 PM

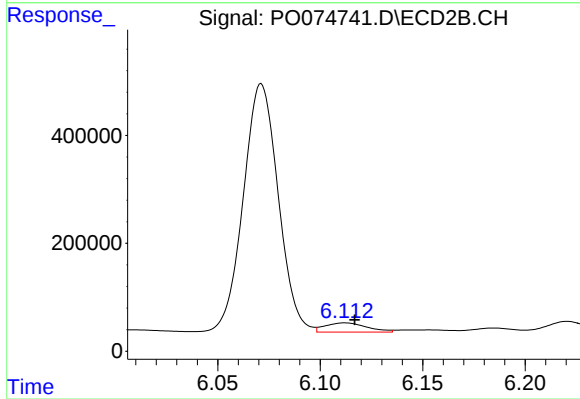


#26 AR-1254-1

R.T.: 6.112 min
Delta R.T.: -0.005 min
Response: 242894
Conc: 67.25 ng/ml

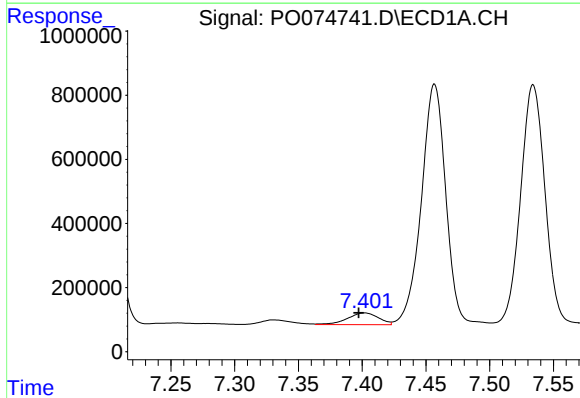


#27 AR-1254-2

R.T.: 7.402 min
Delta R.T.: 0.004 min
Response: 617163
Conc: 90.62 ng/ml

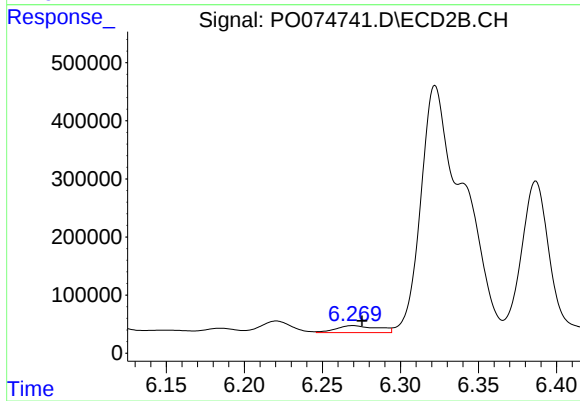

#27 AR-1254-2

R.T.: 6.270 min
Delta R.T.: -0.006 min
Response: 226006
Conc: 72.52 ng/ml

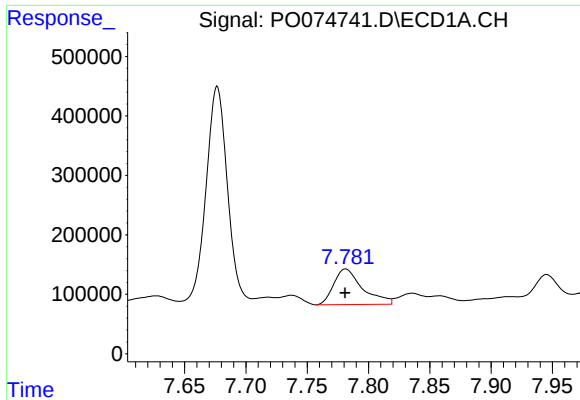


#28 AR-1254-3

R.T.: 7.781 min
Delta R.T.: 0.000 min
Response: 982566
Conc: 140.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-31A


Manual Integrations
APPROVED

Ankita
1/18/2021 2:36:49 PM

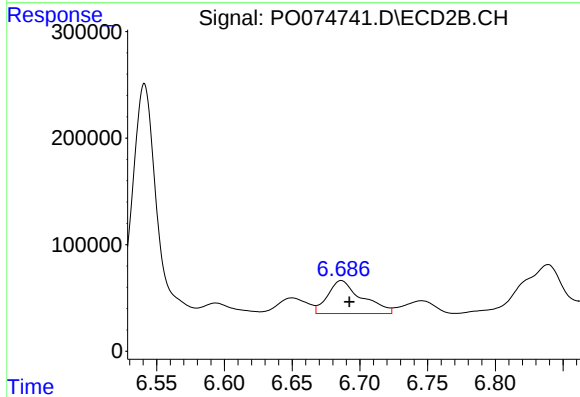


#28 AR-1254-3

R.T.: 6.686 min
Delta R.T.: -0.006 min
Response: 542168
Conc: 110.56 ng/ml

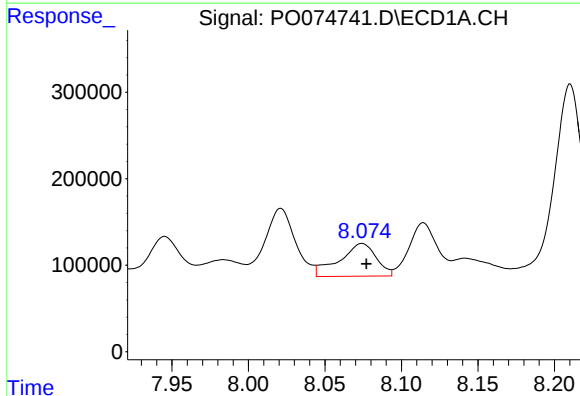


#29 AR-1254-4

R.T.: 8.074 min
Delta R.T.: -0.003 min
Response: 636435
Conc: 104.94 ng/ml

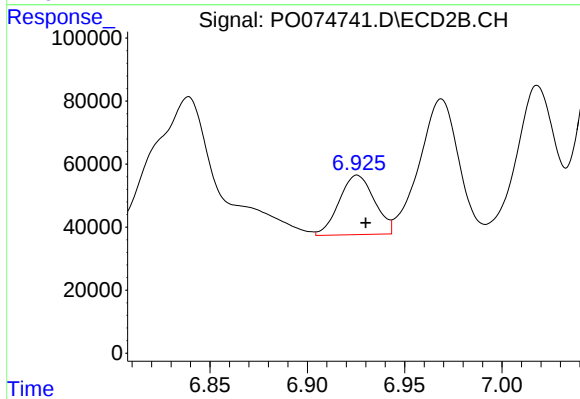

#29 AR-1254-4

R.T.: 6.926 min
Delta R.T.: -0.004 min
Response: 238036
Conc: 68.64 ng/ml

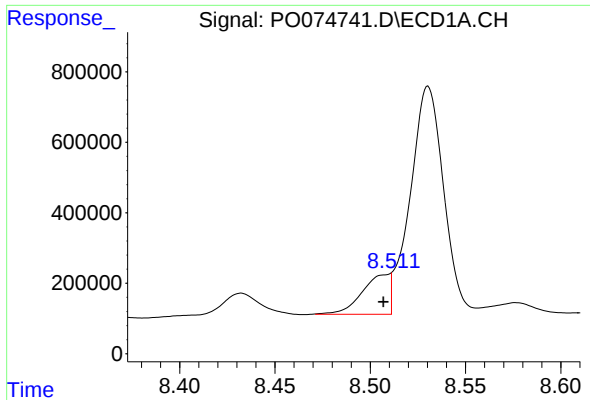


#30 AR-1254-5

R.T.: 8.511 min
Delta R.T.: 0.004 min
Response: 1216681
Conc: 209.45 ng/ml m

Instrument :
ECD_O
ClientSampleId :
263K-31A

Manual Integrations
APPROVED

Ankita
1/18/2021 2:36:49 PM

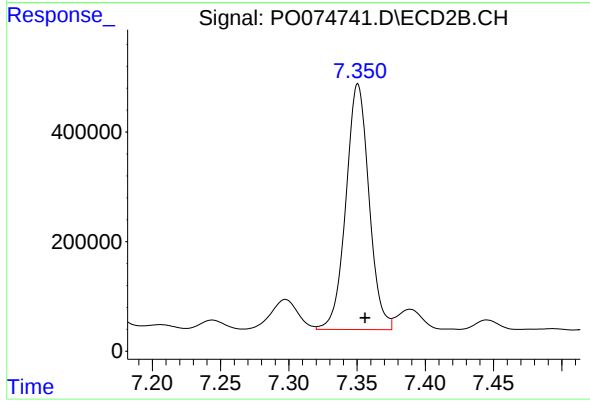

#30 AR-1254-5

R.T.: 7.351 min
Delta R.T.: -0.005 min
Response: 5283179
Conc: 1167.31 ng/ml