

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011521\
 Data File : P0074743.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Jan 2021 12:27
 Operator : AJ/MA
 Sample : M1096-09
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 263K-32A

Manual Integrations
 APPROVED

Ankita
 1/18/2021 2:36:53 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 10:11:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.930	4.002	2410726	1280606	22.847	22.765
2) SA Decachlor...	10.945	9.255	1798052	971266	17.716	17.690
Target Compounds						
26) L6 AR-1254-1	7.156	6.112	135641	193893	30.841m	53.680 #
27) L6 AR-1254-2	7.399	6.269	466009	137235	68.422	44.035 #
28) L6 AR-1254-3	7.780	6.686	560368	293498	79.889	59.850 #
29) L6 AR-1254-4	8.074	6.925	346739	153951	57.174	44.395
30) L6 AR-1254-5	8.511	7.350	854073	6776994	147.027m	1497.367 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011521\
Data File : PO074743.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Jan 2021 12:27
Operator : AJ/MA
Sample : M1096-09
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
263K-32A


Manual Integrations
APPROVED

Ankita
1/18/2021 2:36:53 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 10:11:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

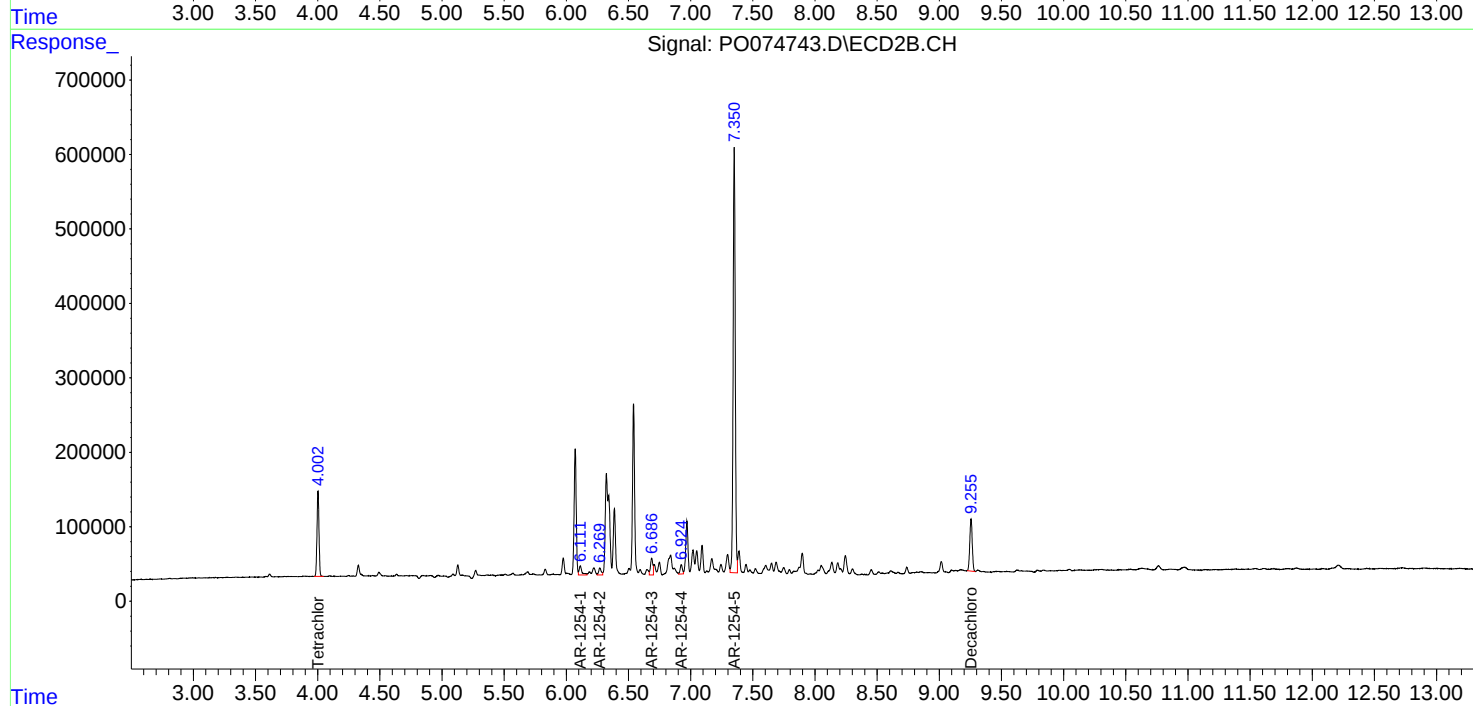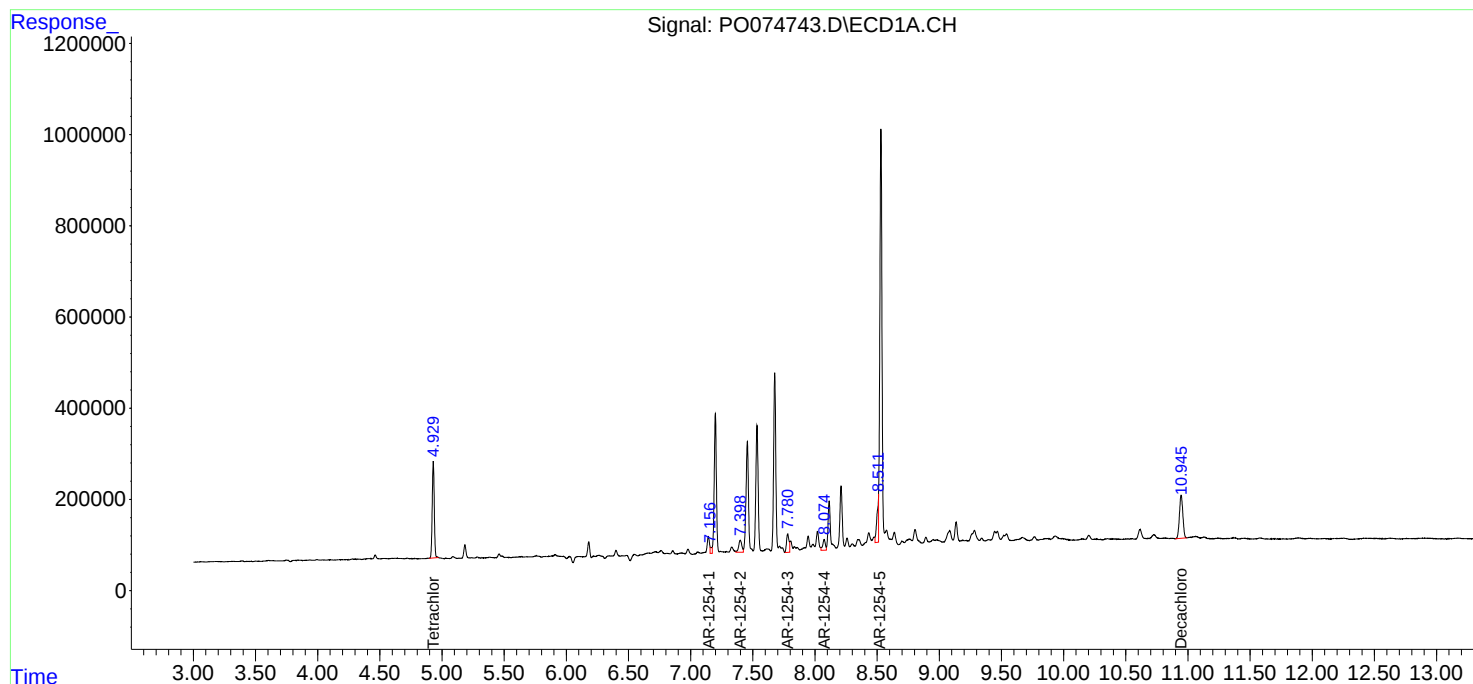

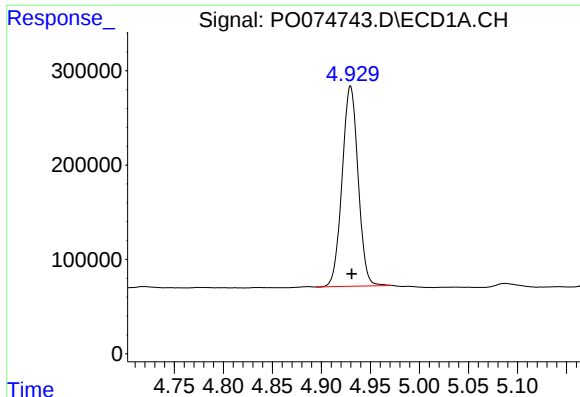


#1 Tetrachloro-m-xylene

R.T.: 4.930 min
Delta R.T.: -0.001 min
Response: 2410726
Conc: 22.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-32A


Manual Integrations
APPROVED

Ankita
1/18/2021 2:36:53 PM

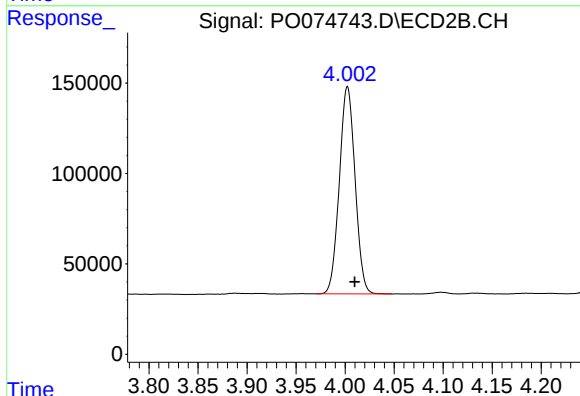


#1 Tetrachloro-m-xylene

R.T.: 4.002 min
Delta R.T.: -0.007 min
Response: 1280606
Conc: 22.77 ng/ml

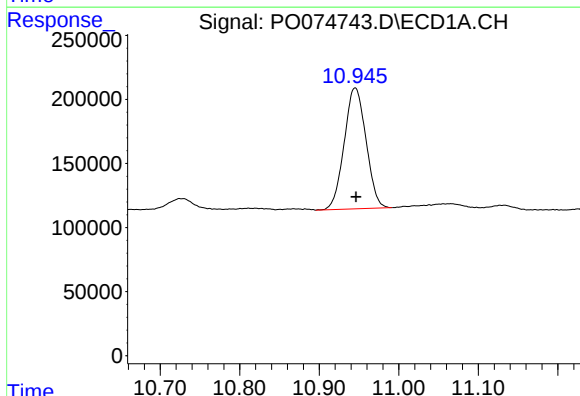


#2 Decachlorobiphenyl

R.T.: 10.945 min
Delta R.T.: -0.001 min
Response: 1798052
Conc: 17.72 ng/ml

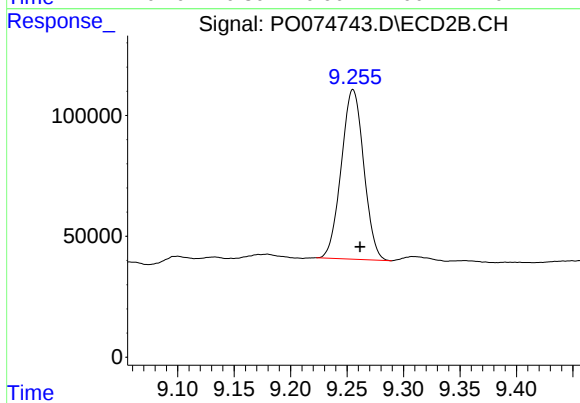

#2 Decachlorobiphenyl

R.T.: 9.255 min
Delta R.T.: -0.006 min
Response: 971266
Conc: 17.69 ng/ml

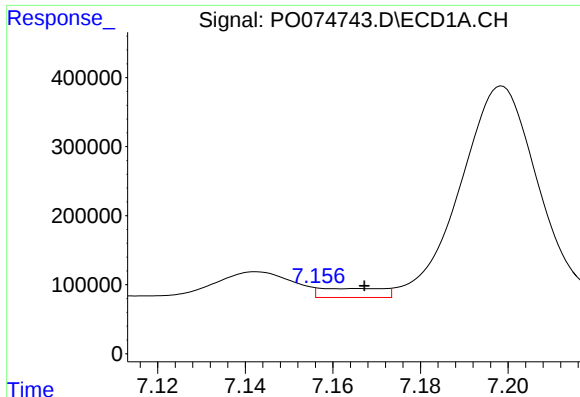


#26 AR-1254-1

R.T.: 7.156 min
Delta R.T.: -0.011 min
Response: 135641
Conc: 30.84 ng/ml m

Instrument :
ECD_O
ClientSampleId :
263K-32A


Manual Integrations
APPROVED

Ankita
1/18/2021 2:36:53 PM

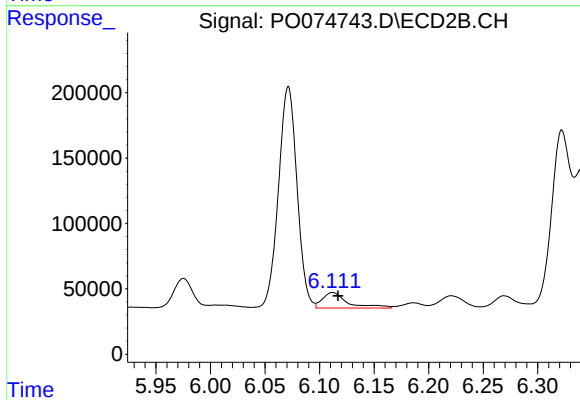


#26 AR-1254-1

R.T.: 6.112 min
Delta R.T.: -0.005 min
Response: 193893
Conc: 53.68 ng/ml

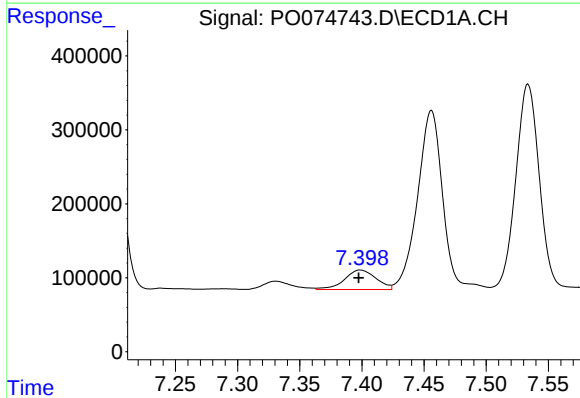


#27 AR-1254-2

R.T.: 7.399 min
Delta R.T.: 0.001 min
Response: 466009
Conc: 68.42 ng/ml

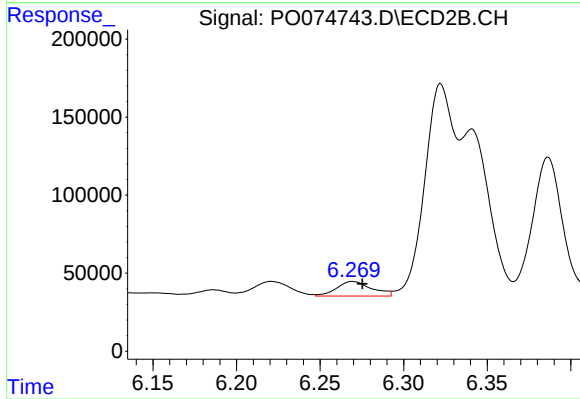

#27 AR-1254-2

R.T.: 6.269 min
Delta R.T.: -0.006 min
Response: 137235
Conc: 44.03 ng/ml

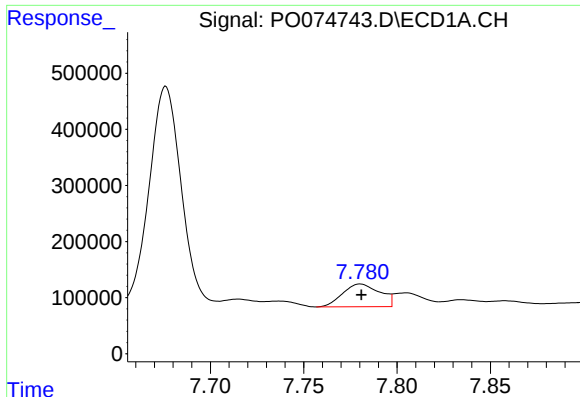


#28 AR-1254-3

R.T.: 7.780 min
Delta R.T.: 0.000 min
Response: 560368
Conc: 79.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-32A


Manual Integrations
APPROVED

Ankita
1/18/2021 2:36:53 PM

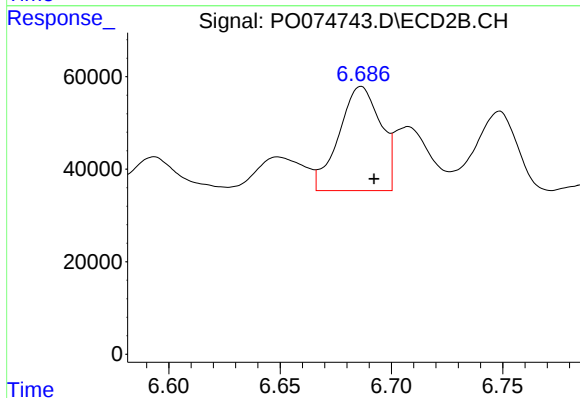


#28 AR-1254-3

R.T.: 6.686 min
Delta R.T.: -0.006 min
Response: 293498
Conc: 59.85 ng/ml

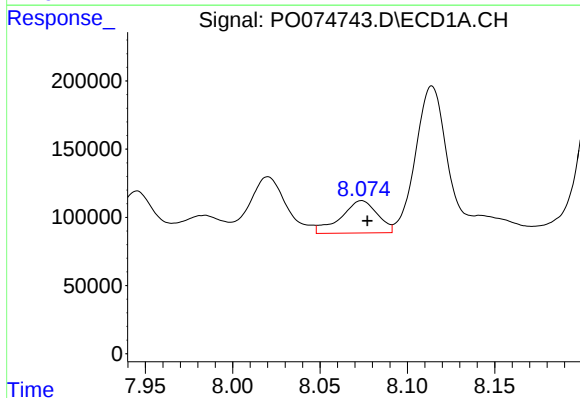


#29 AR-1254-4

R.T.: 8.074 min
Delta R.T.: -0.003 min
Response: 346739
Conc: 57.17 ng/ml

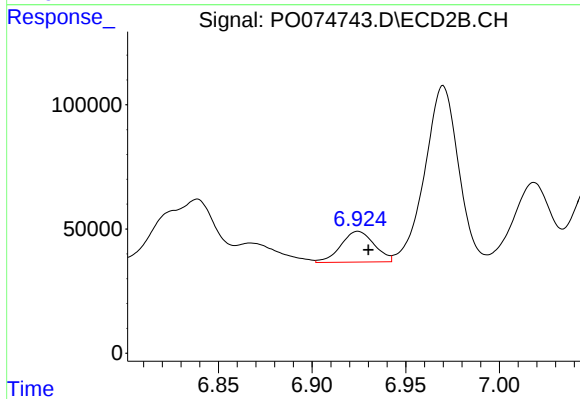

#29 AR-1254-4

R.T.: 6.925 min
Delta R.T.: -0.005 min
Response: 153951
Conc: 44.39 ng/ml

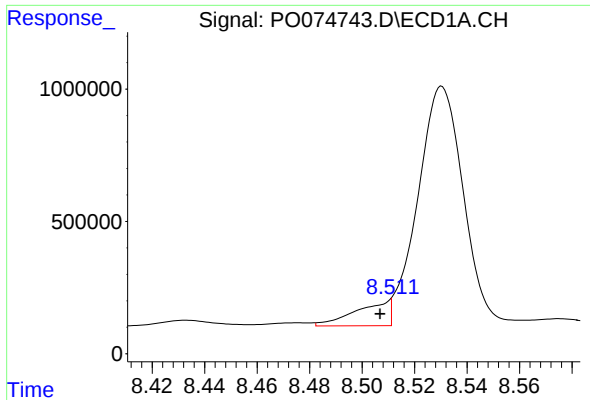


#30 AR-1254-5

R.T.: 8.511 min
Delta R.T.: 0.004 min
Response: 854073
Conc: 147.03 ng/ml m

Instrument :
ECD_O
ClientSampleId :
263K-32A

Manual Integrations
APPROVED

Ankita
1/18/2021 2:36:53 PM

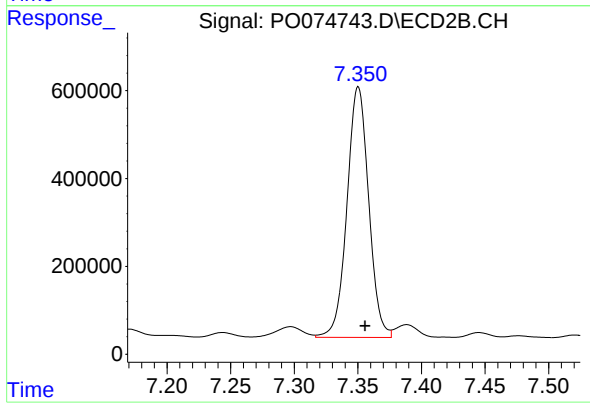

#30 AR-1254-5

R.T.: 7.350 min
Delta R.T.: -0.005 min
Response: 6776994
Conc: 1497.37 ng/ml