

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011521\
 Data File : P0074746.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Jan 2021 13:36
 Operator : AJ/MA
 Sample : M1096-10
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 263K-32B

Manual Integrations
 APPROVED

Ankita
 1/18/2021 2:36:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 10:13:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.931	4.004	2230768	1220325	21.141	21.694
2) SA Decachlor...	10.948	9.257	1353961	712141	13.341	12.971
Target Compounds						
26) L6 AR-1254-1	7.163	6.112	52654	122742	11.972m	33.982 #
27) L6 AR-1254-2	7.404	6.271	322900	104637	47.410	33.575 #
28) L6 AR-1254-3	7.783	6.687	790832	428897	112.745	87.460
29) L6 AR-1254-4	8.075	6.926	456382	188812	75.253	54.447 #
30) L6 AR-1254-5	8.508	7.352	1426658	3099081	245.597	684.737 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011521\
Data File : PO074746.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Jan 2021 13:36
Operator : AJ/MA
Sample : M1096-10
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
263K-32B


Manual Integrations
APPROVED

Ankita
1/18/2021 2:36:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 10:13:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

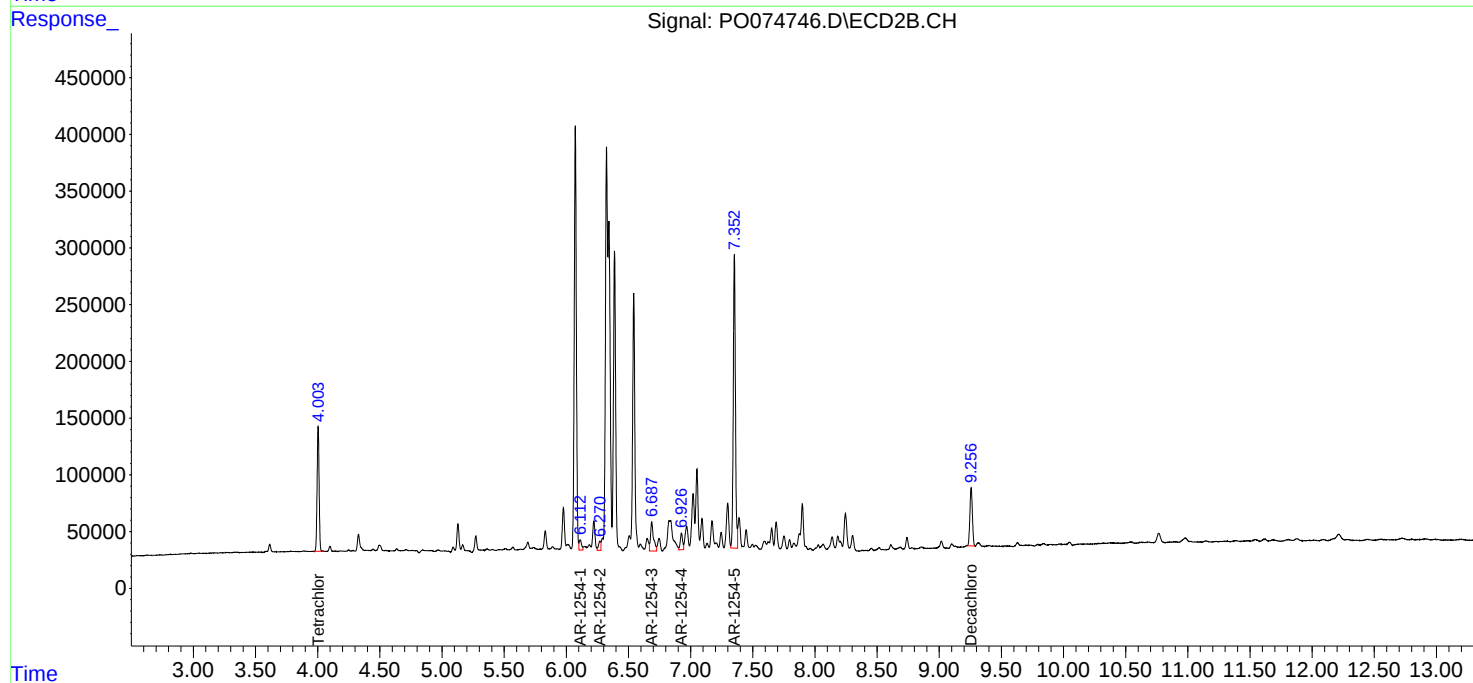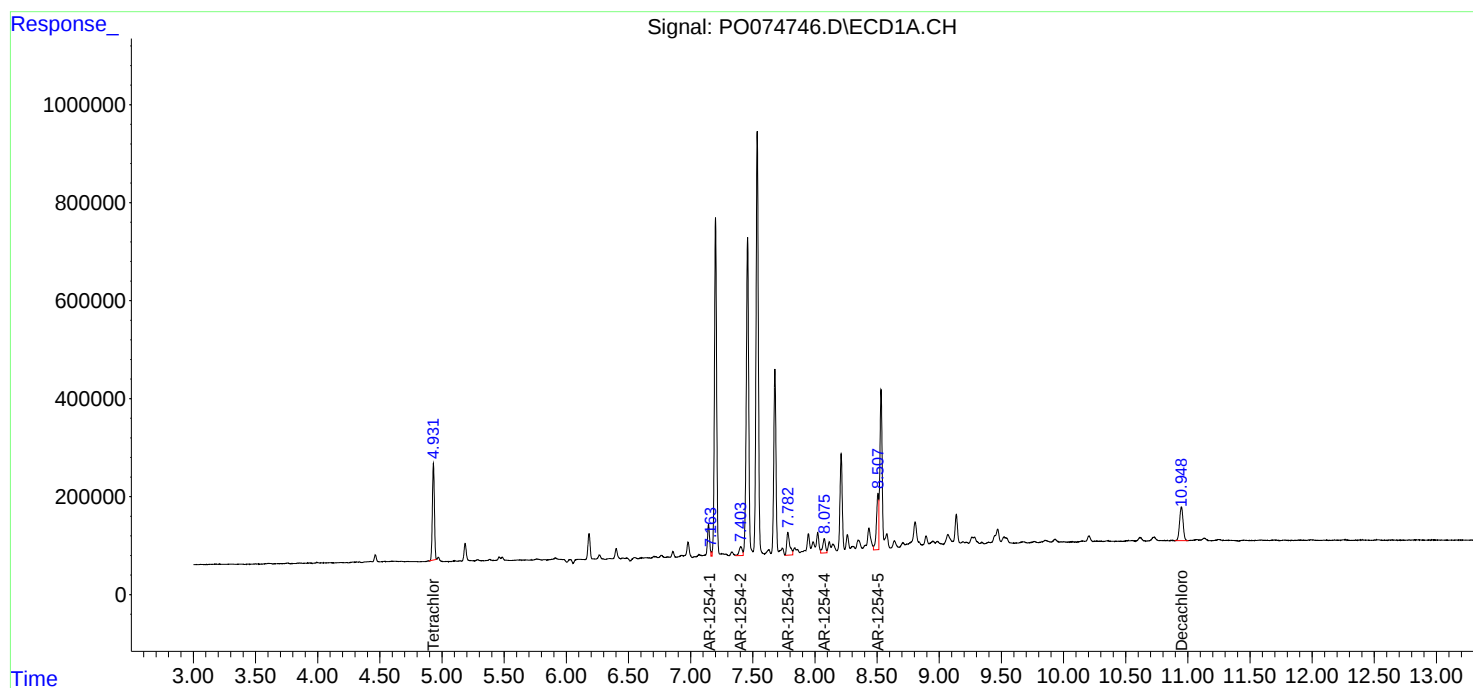

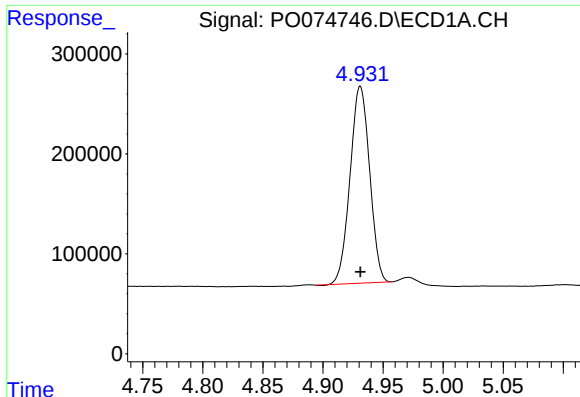


#1 Tetrachloro-m-xylene

R.T.: 4.931 min
Delta R.T.: 0.000 min
Response: 2230768
Conc: 21.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-32B


Manual Integrations
APPROVED

Ankita
1/18/2021 2:36:55 PM

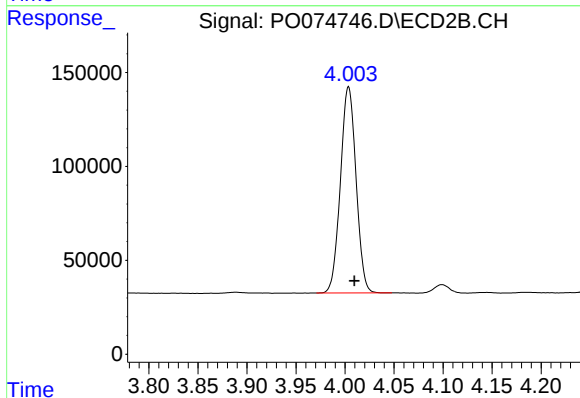


#1 Tetrachloro-m-xylene

R.T.: 4.004 min
Delta R.T.: -0.006 min
Response: 1220325
Conc: 21.69 ng/ml

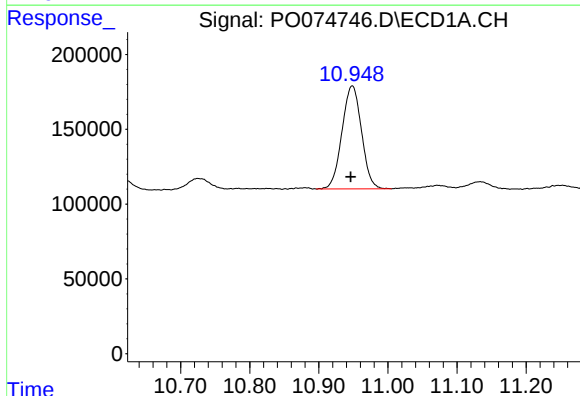


#2 Decachlorobiphenyl

R.T.: 10.948 min
Delta R.T.: 0.002 min
Response: 1353961
Conc: 13.34 ng/ml

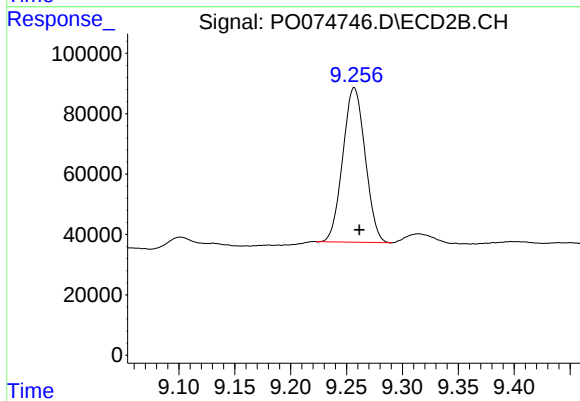

#2 Decachlorobiphenyl

R.T.: 9.257 min
Delta R.T.: -0.005 min
Response: 712141
Conc: 12.97 ng/ml

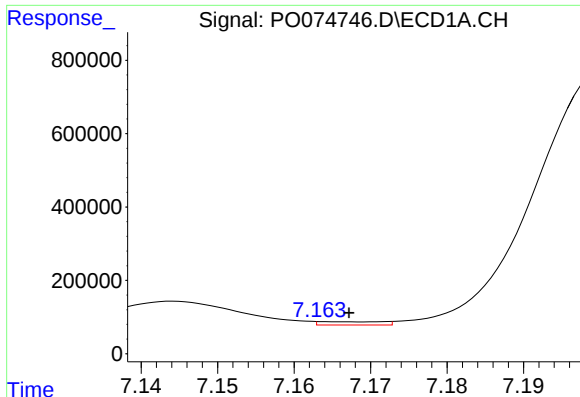


#26 AR-1254-1

R.T.: 7.163 min
Delta R.T.: -0.004 min
Response: 52654
Conc: 11.97 ng/ml m

Instrument :
ECD_O
ClientSampleId :
263K-32B


Manual Integrations
APPROVED

Ankita
1/18/2021 2:36:55 PM

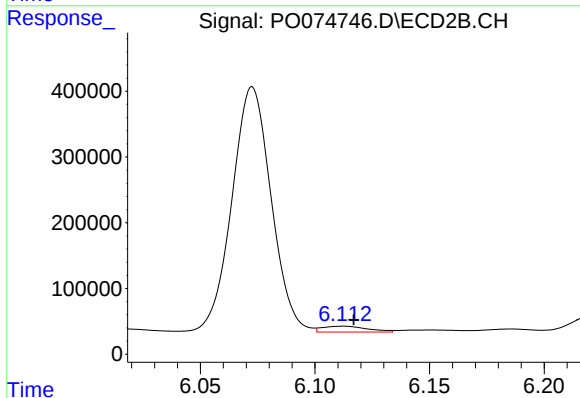


#26 AR-1254-1

R.T.: 6.112 min
Delta R.T.: -0.005 min
Response: 122742
Conc: 33.98 ng/ml

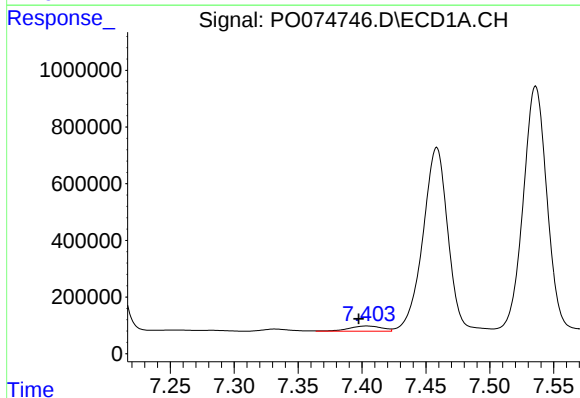


#27 AR-1254-2

R.T.: 7.404 min
Delta R.T.: 0.006 min
Response: 322900
Conc: 47.41 ng/ml

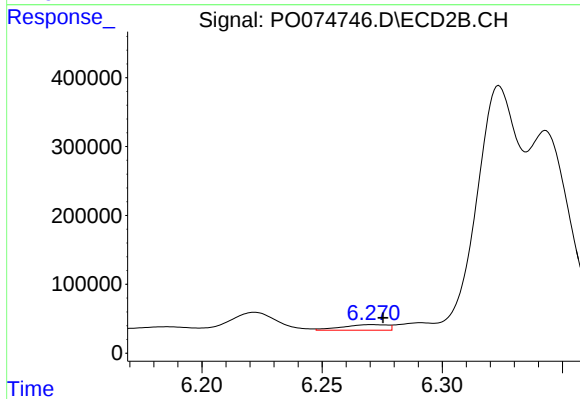

#27 AR-1254-2

R.T.: 6.271 min
Delta R.T.: -0.005 min
Response: 104637
Conc: 33.57 ng/ml

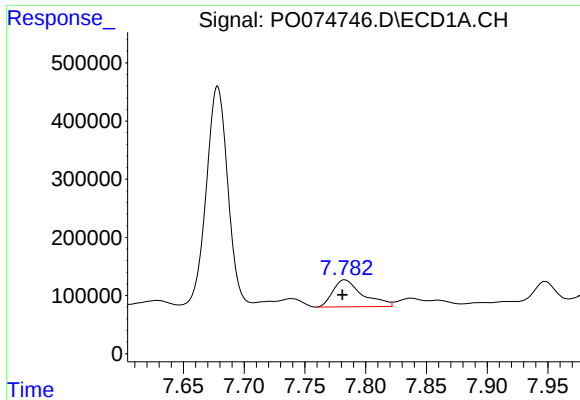


#28 AR-1254-3

R.T.: 7.783 min
Delta R.T.: 0.002 min
Response: 790832
Conc: 112.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-32B


Manual Integrations
APPROVED

Ankita
1/18/2021 2:36:55 PM

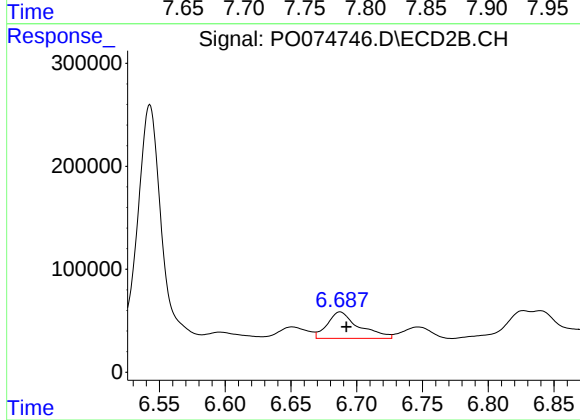


#28 AR-1254-3

R.T.: 6.687 min
Delta R.T.: -0.005 min
Response: 428897
Conc: 87.46 ng/ml

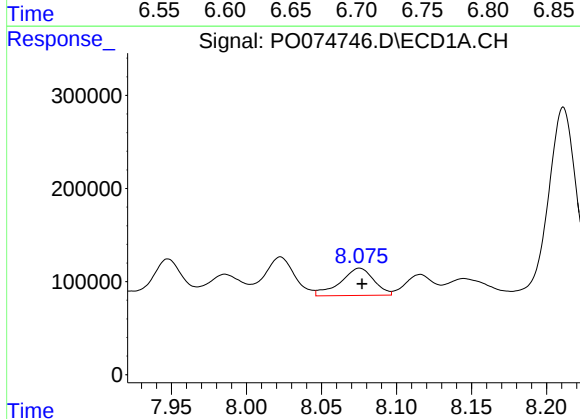


#29 AR-1254-4

R.T.: 8.075 min
Delta R.T.: -0.002 min
Response: 456382
Conc: 75.25 ng/ml

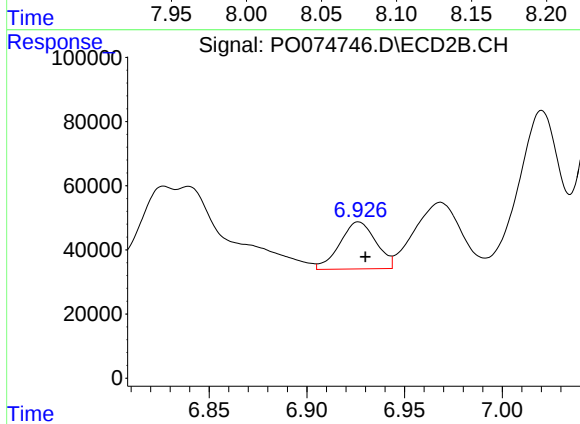

#29 AR-1254-4

R.T.: 6.926 min
Delta R.T.: -0.004 min
Response: 188812
Conc: 54.45 ng/ml

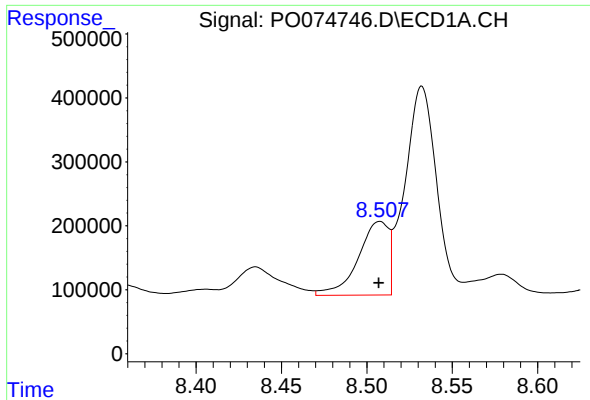


#30 AR-1254-5

R.T.: 8.508 min
Delta R.T.: 0.000 min
Response: 1426658
Conc: 245.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-32B

Manual Integrations
APPROVED

Ankita
1/18/2021 2:36:55 PM

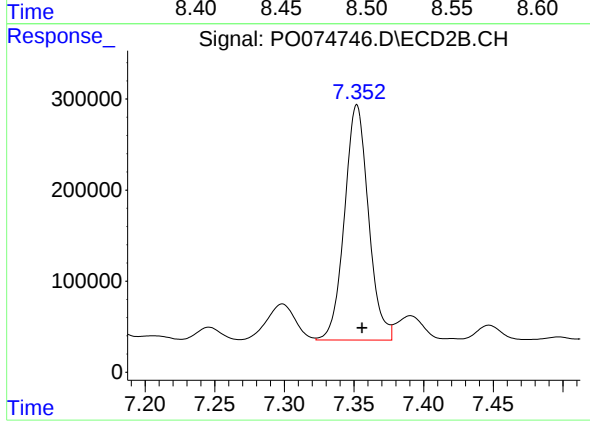

#30 AR-1254-5

R.T.: 7.352 min
Delta R.T.: -0.004 min
Response: 3099081
Conc: 684.74 ng/ml