

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011521\
 Data File : P0074750.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Jan 2021 14:45
 Operator : AJ/MA
 Sample : M1096-17
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 263K-35A

Manual Integrations
 APPROVED

Ankita
 1/18/2021 2:37:00 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 09:58:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.929	4.003	2242361	1121962	21.251	19.945
2) SA Decachlor...	10.947	9.254	1542973	875768	15.203	15.951
Target Compounds						
26) L6 AR-1254-1	7.166	6.112	242995	241181	55.250	66.772
27) L6 AR-1254-2	7.396	6.270	775166	267807	113.815	85.931
28) L6 AR-1254-3	7.779	6.686	1073448	753179	153.036	153.587
29) L6 AR-1254-4	8.075	6.925	705282	322491	116.294	92.996
30) L6 AR-1254-5	8.510	7.350	1830795	7743665	315.169m	1710.951 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011521\
Data File : PO074750.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Jan 2021 14:45
Operator : AJ/MA
Sample : M1096-17
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
263K-35A


Manual Integrations
APPROVED

Ankita
1/18/2021 2:37:00 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 09:58:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

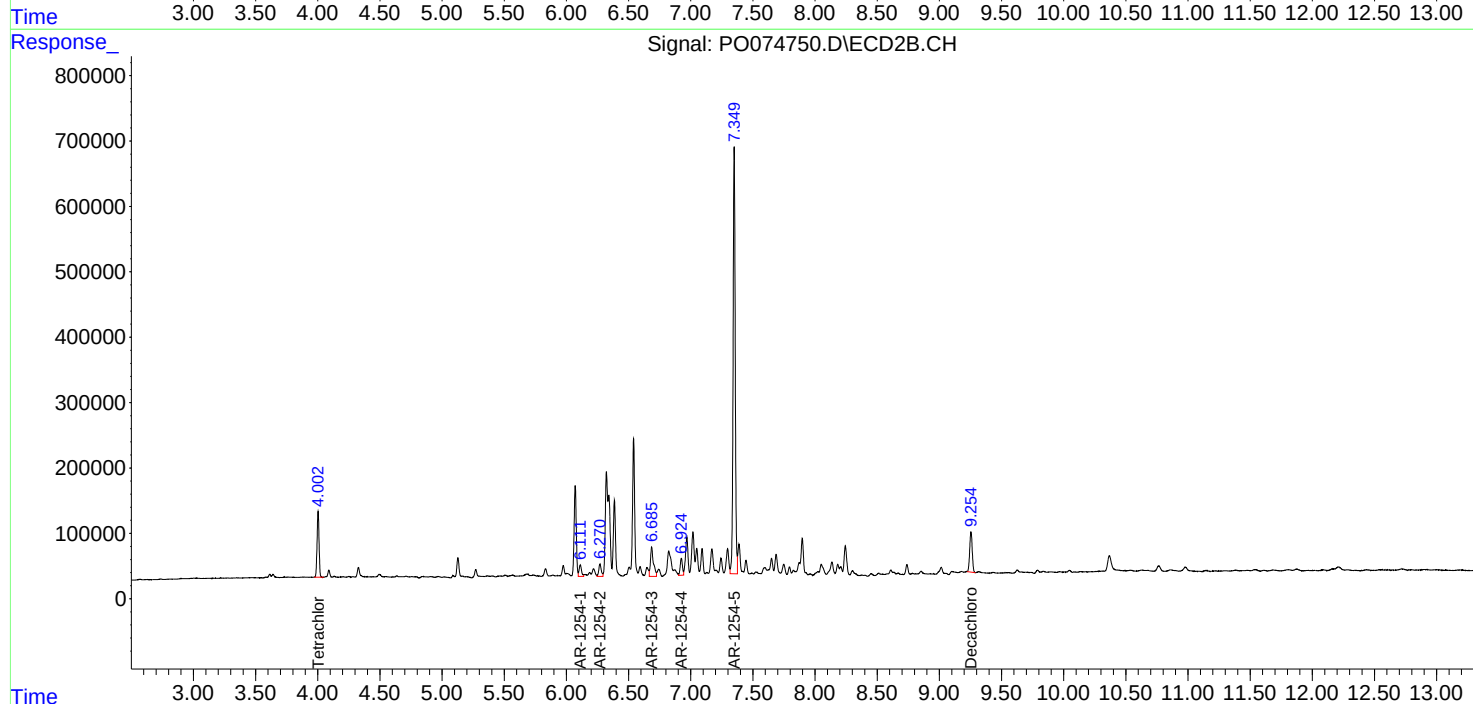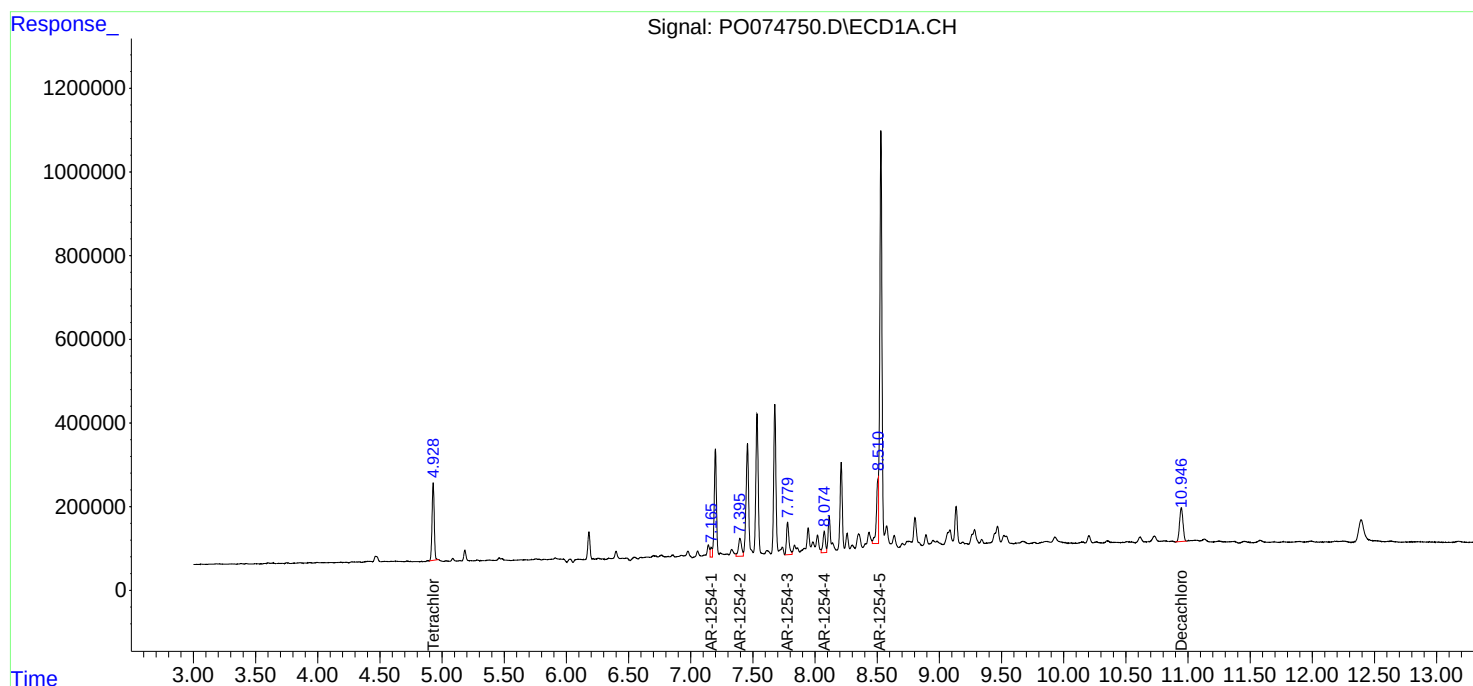

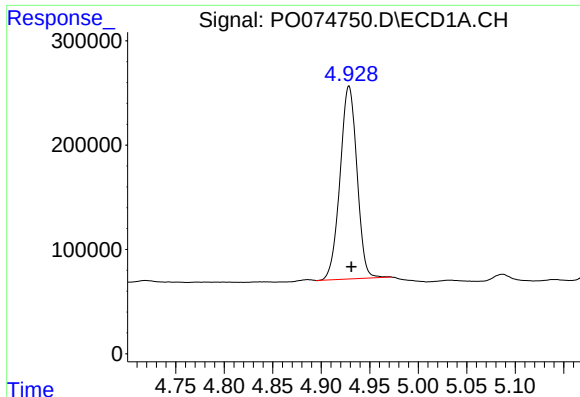


#1 Tetrachloro-m-xylene

R.T.: 4.929 min
Delta R.T.: -0.002 min
Response: 2242361
Conc: 21.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-35A


Manual Integrations
APPROVED

Ankita
1/18/2021 2:37:00 PM

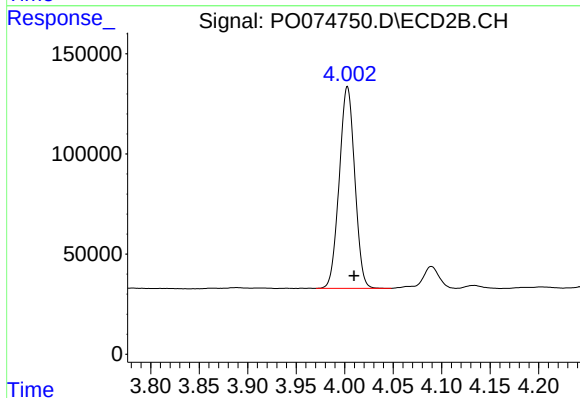


#1 Tetrachloro-m-xylene

R.T.: 4.003 min
Delta R.T.: -0.007 min
Response: 1121962
Conc: 19.95 ng/ml

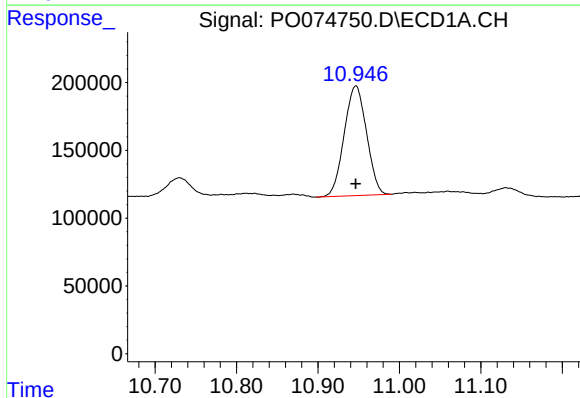


#2 Decachlorobiphenyl

R.T.: 10.947 min
Delta R.T.: 0.000 min
Response: 1542973
Conc: 15.20 ng/ml

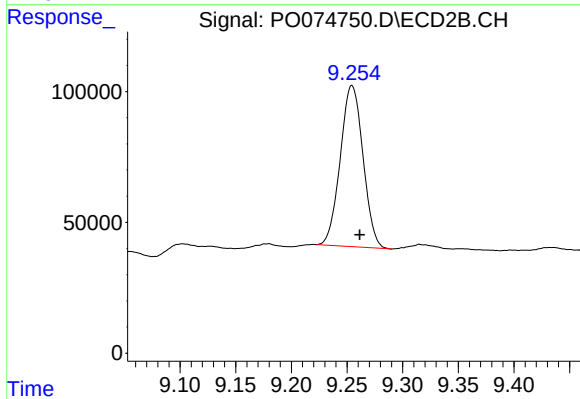

#2 Decachlorobiphenyl

R.T.: 9.254 min
Delta R.T.: -0.007 min
Response: 875768
Conc: 15.95 ng/ml

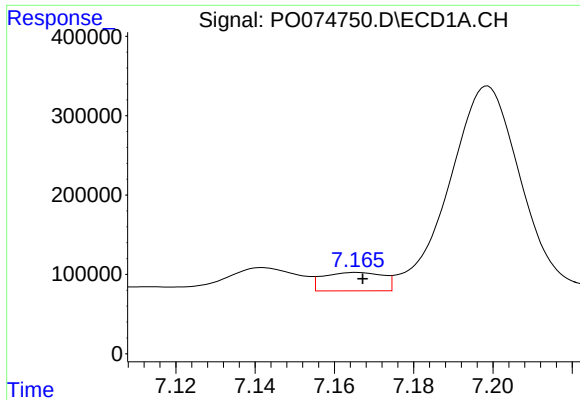


#26 AR-1254-1

R.T.: 7.166 min
Delta R.T.: -0.002 min
Response: 242995
Conc: 55.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-35A


Manual Integrations
APPROVED

Ankita
1/18/2021 2:37:00 PM

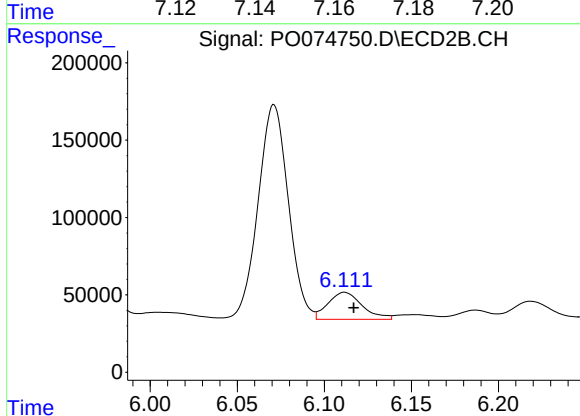


#26 AR-1254-1

R.T.: 6.112 min
Delta R.T.: -0.005 min
Response: 241181
Conc: 66.77 ng/ml

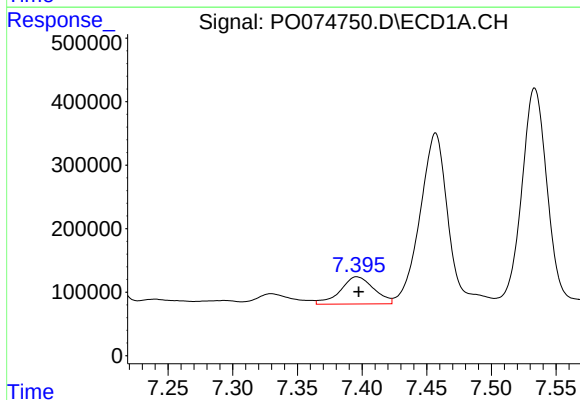


#27 AR-1254-2

R.T.: 7.396 min
Delta R.T.: -0.002 min
Response: 775166
Conc: 113.81 ng/ml

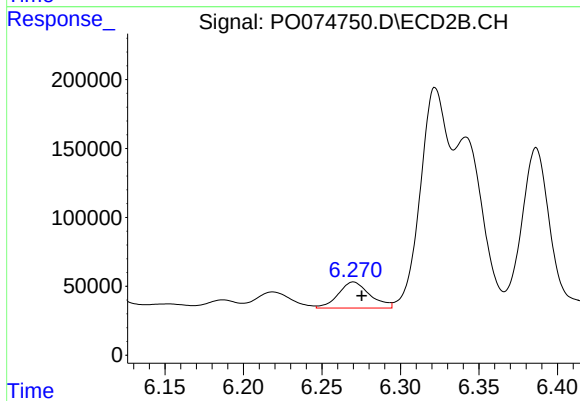

#27 AR-1254-2

R.T.: 6.270 min
Delta R.T.: -0.005 min
Response: 267807
Conc: 85.93 ng/ml

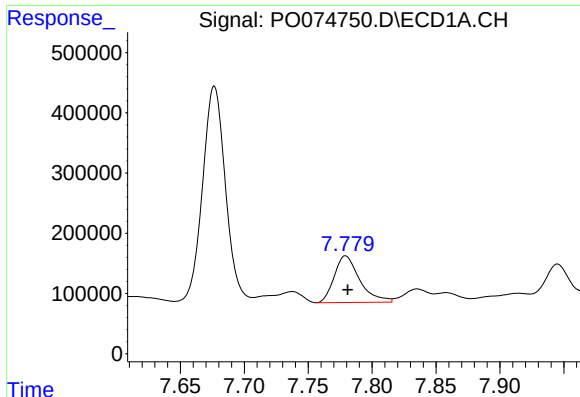


#28 AR-1254-3

R.T.: 7.779 min
Delta R.T.: -0.002 min
Response: 1073448
Conc: 153.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-35A


Manual Integrations
APPROVED

Ankita
1/18/2021 2:37:00 PM

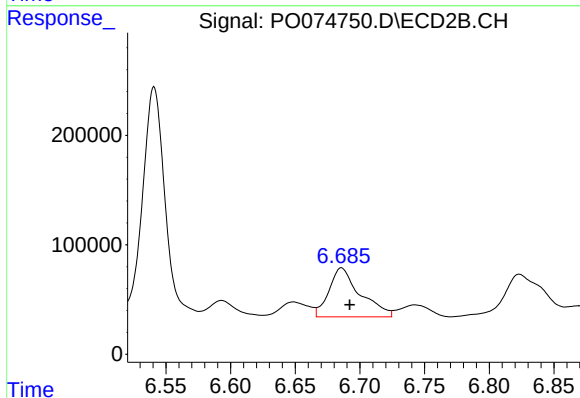


#28 AR-1254-3

R.T.: 6.686 min
Delta R.T.: -0.006 min
Response: 753179
Conc: 153.59 ng/ml

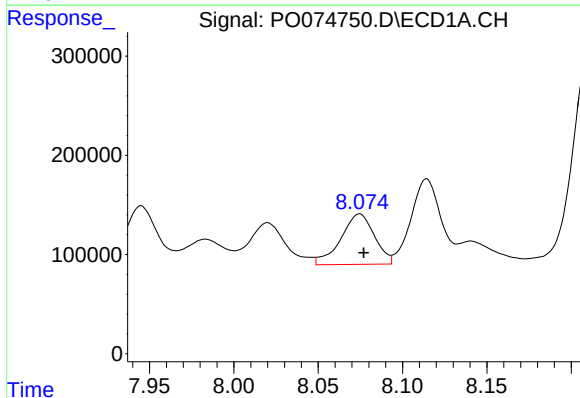


#29 AR-1254-4

R.T.: 8.075 min
Delta R.T.: -0.002 min
Response: 705282
Conc: 116.29 ng/ml

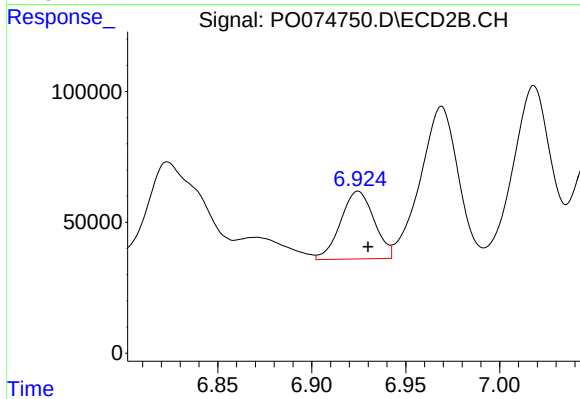

#29 AR-1254-4

R.T.: 6.925 min
Delta R.T.: -0.005 min
Response: 322491
Conc: 93.00 ng/ml

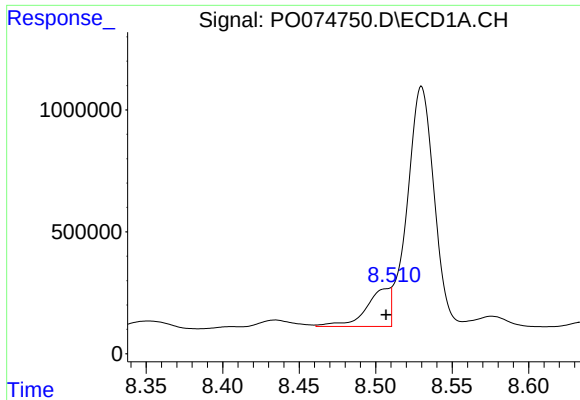


#30 AR-1254-5

R.T.: 8.510 min
Delta R.T.: 0.003 min
Response: 1830795
Conc: 315.17 ng/ml m

Instrument :
ECD_O
ClientSampleId :
263K-35A

Manual Integrations
APPROVED

Ankita
1/18/2021 2:37:00 PM

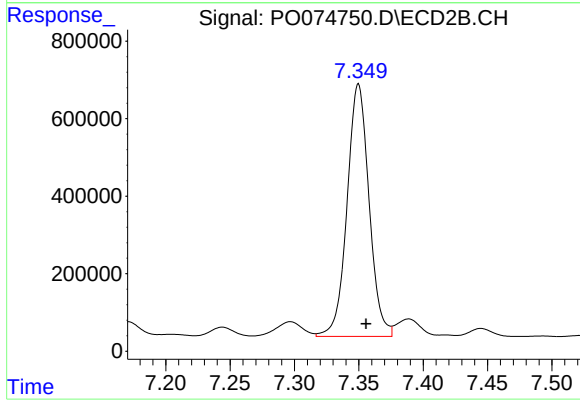

#30 AR-1254-5

R.T.: 7.350 min
Delta R.T.: -0.006 min
Response: 7743665
Conc: 1710.95 ng/ml