

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011521\
 Data File : P0074752.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Jan 2021 15:19
 Operator : AJ/MA
 Sample : M1096-20
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 263K-36B

Manual Integrations
 APPROVED

Ankita
 1/18/2021 2:37:04 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 10:04:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.930	4.002	2083123	1049697	19.742	18.661
2) SA Decachlor...	10.948	9.256	1175733	664330	11.584	12.100
Target Compounds						
26) L6 AR-1254-1	7.160	6.113	34986	34574	7.955m	9.572
27) L6 AR-1254-2	7.397	6.270	131128	94743	19.253	30.400 #
28) L6 AR-1254-3	7.781	6.686	430226	303989	61.335	61.989
29) L6 AR-1254-4	8.075	6.924	245109	148746	40.416	42.894
30) L6 AR-1254-5	8.505	7.350	998684	1316538	171.922	290.887 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011521\
Data File : PO074752.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Jan 2021 15:19
Operator : AJ/MA
Sample : M1096-20
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
263K-36B


Manual Integrations
APPROVED

Ankita
1/18/2021 2:37:04 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 10:04:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

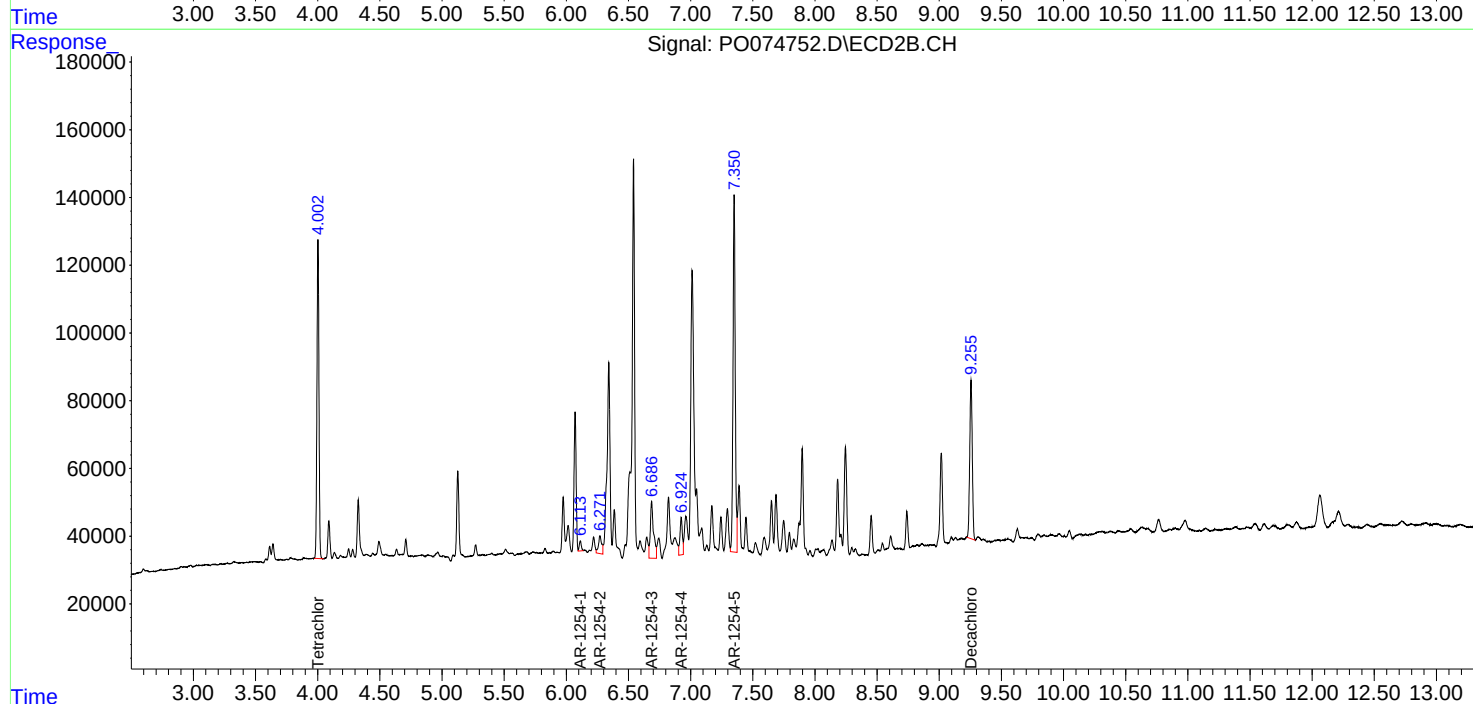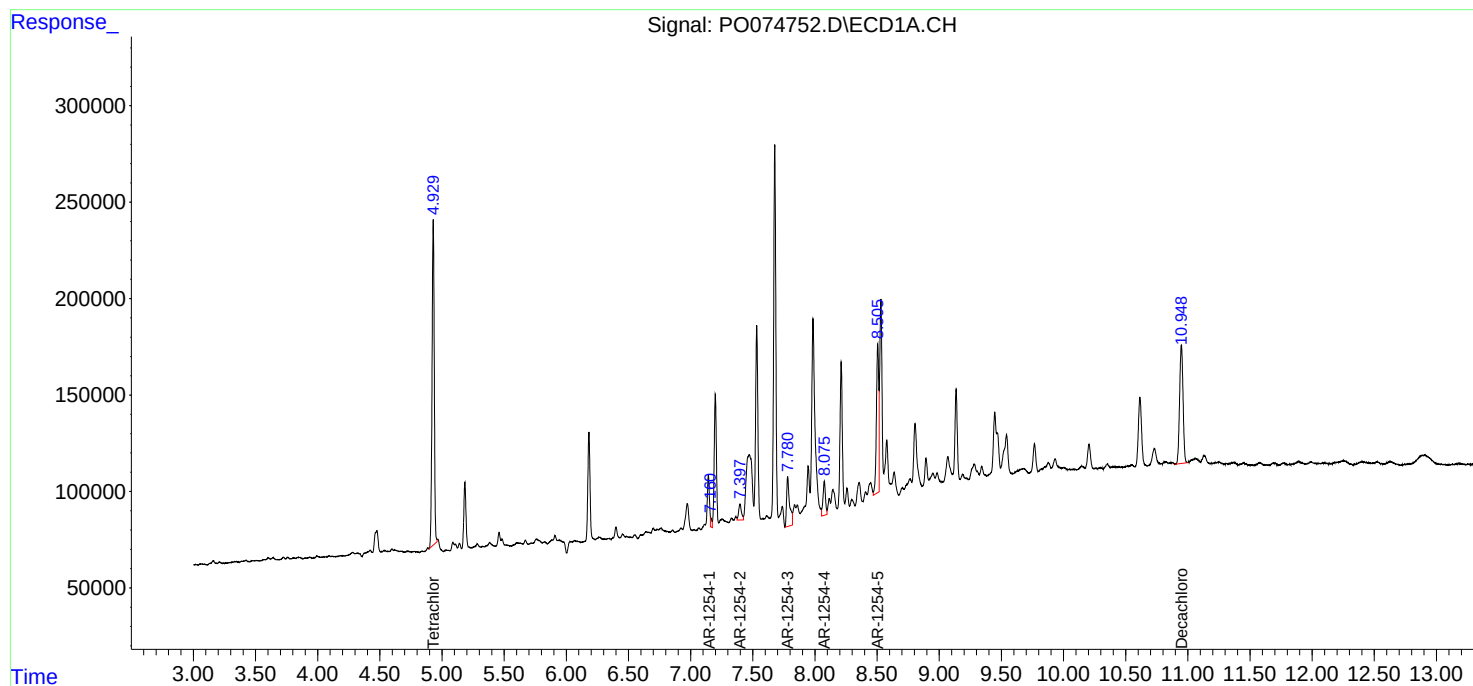

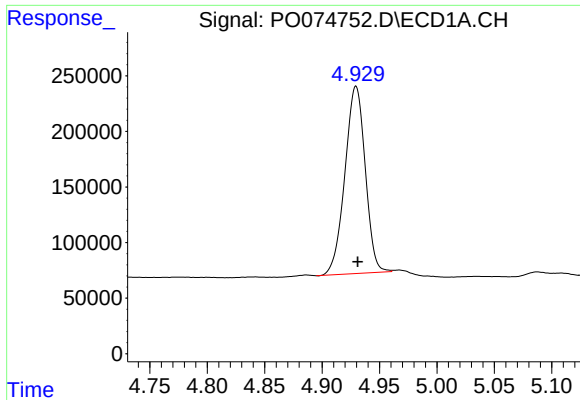


#1 Tetrachloro-m-xylene

R.T.: 4.930 min
Delta R.T.: -0.001 min
Response: 2083123
Conc: 19.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-36B


Manual Integrations
APPROVED

Ankita
1/18/2021 2:37:04 PM

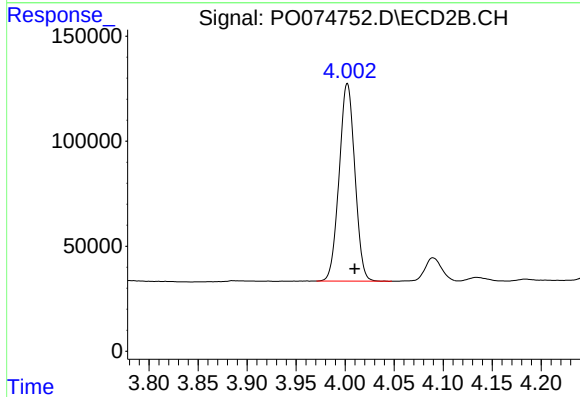


#1 Tetrachloro-m-xylene

R.T.: 4.002 min
Delta R.T.: -0.007 min
Response: 1049697
Conc: 18.66 ng/ml

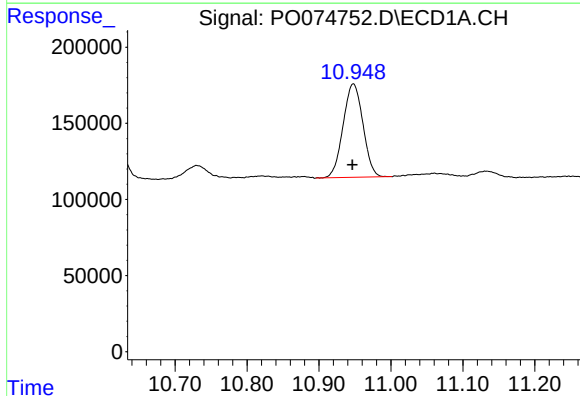


#2 Decachlorobiphenyl

R.T.: 10.948 min
Delta R.T.: 0.001 min
Response: 1175733
Conc: 11.58 ng/ml

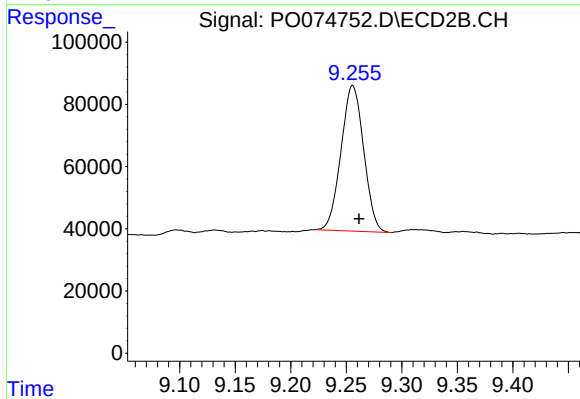

#2 Decachlorobiphenyl

R.T.: 9.256 min
Delta R.T.: -0.006 min
Response: 664330
Conc: 12.10 ng/ml

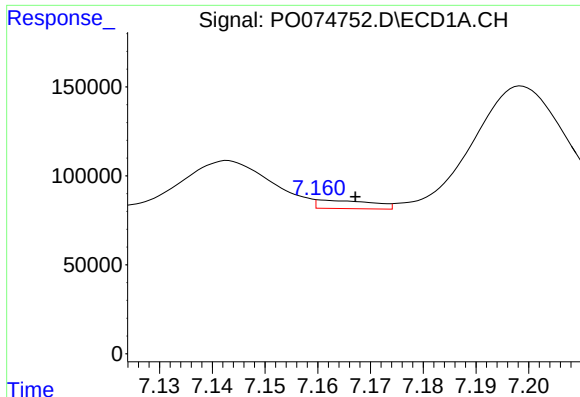


#26 AR-1254-1

R.T.: 7.160 min
Delta R.T.: -0.008 min
Response: 34986
Conc: 7.95 ng/ml m

Instrument :
ECD_O
ClientSampleId :
263K-36B


Manual Integrations
APPROVED

Ankita
1/18/2021 2:37:04 PM

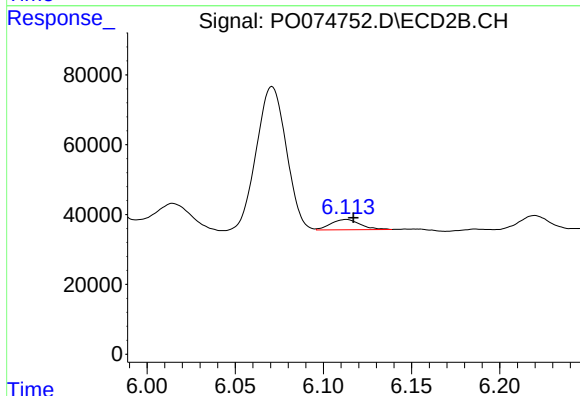


#26 AR-1254-1

R.T.: 6.113 min
Delta R.T.: -0.004 min
Response: 34574
Conc: 9.57 ng/ml

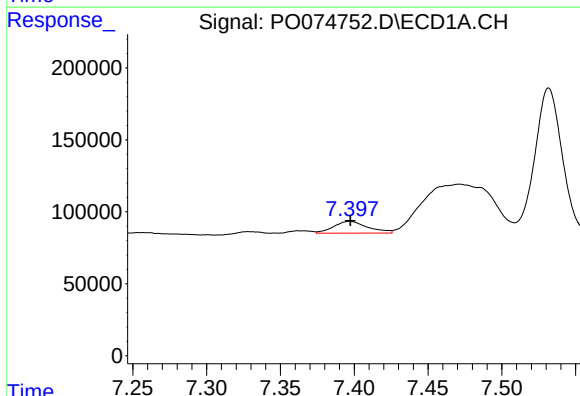


#27 AR-1254-2

R.T.: 7.397 min
Delta R.T.: 0.000 min
Response: 131128
Conc: 19.25 ng/ml

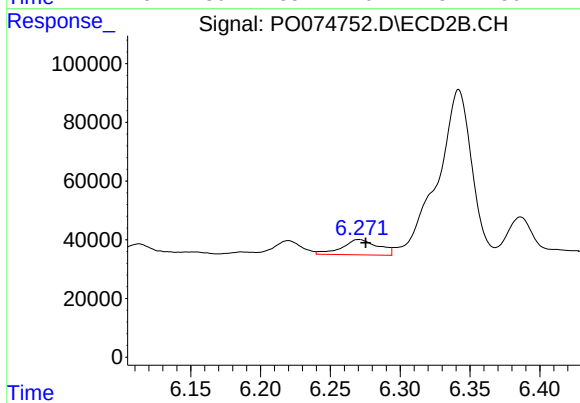

#27 AR-1254-2

R.T.: 6.270 min
Delta R.T.: -0.005 min
Response: 94743
Conc: 30.40 ng/ml

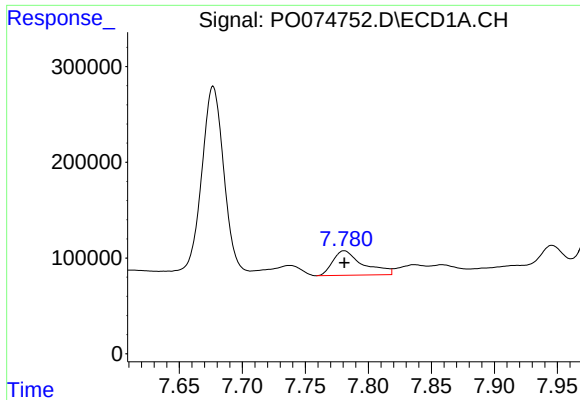


#28 AR-1254-3

R.T.: 7.781 min
Delta R.T.: 0.000 min
Response: 430226
Conc: 61.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-36B


Manual Integrations
APPROVED

Ankita
1/18/2021 2:37:04 PM

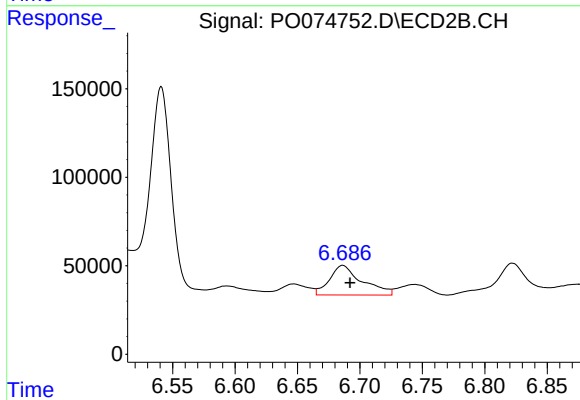


#28 AR-1254-3

R.T.: 6.686 min
Delta R.T.: -0.006 min
Response: 303989
Conc: 61.99 ng/ml

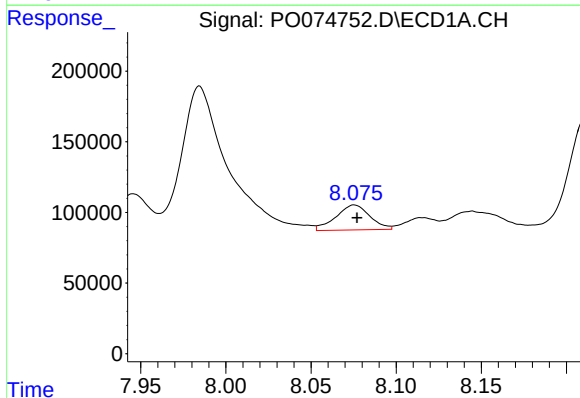


#29 AR-1254-4

R.T.: 8.075 min
Delta R.T.: -0.002 min
Response: 245109
Conc: 40.42 ng/ml

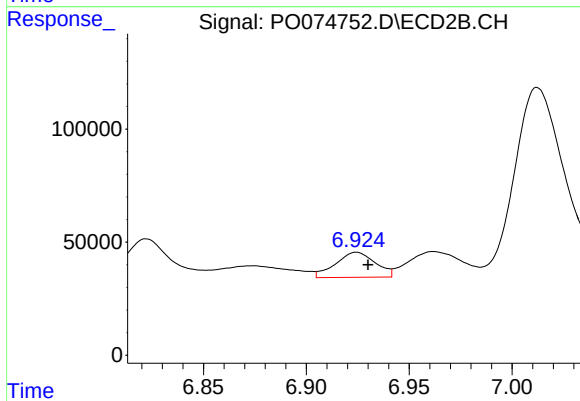

#29 AR-1254-4

R.T.: 6.924 min
Delta R.T.: -0.006 min
Response: 148746
Conc: 42.89 ng/ml

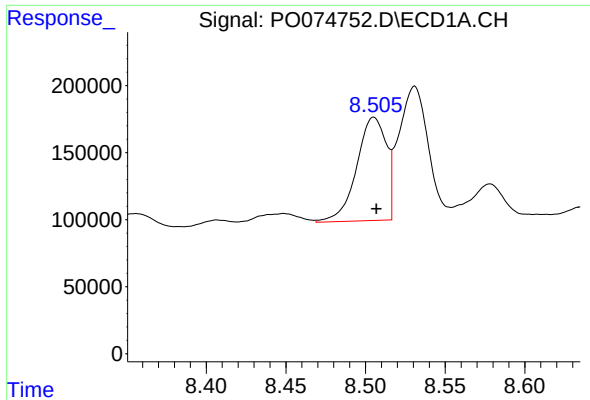


#30 AR-1254-5

R.T.: 8.505 min
Delta R.T.: -0.002 min
Response: 998684
Conc: 171.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-36B

Manual Integrations
APPROVED

Ankita
1/18/2021 2:37:04 PM

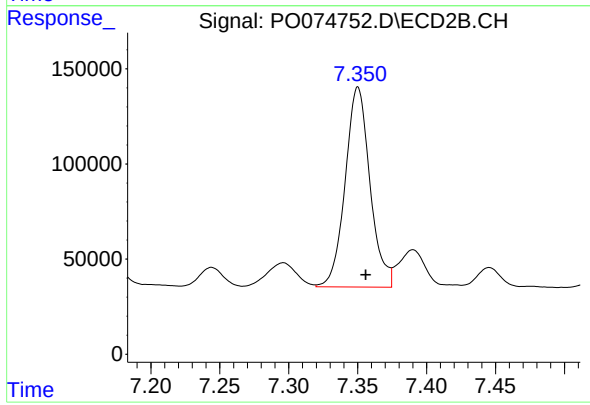

#30 AR-1254-5

R.T.: 7.350 min
Delta R.T.: -0.006 min
Response: 1316538
Conc: 290.89 ng/ml