

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011521\
 Data File : P0074758.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Jan 2021 17:31
 Operator : AJ/MA
 Sample : M1087-06
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S4-02-C

Manual Integrations
 APPROVED

Ankita
 1/18/2021 12:52:34 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 15 23:39:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.930	4.002	2402179	1383288	22.766m	24.591
2) SA Decachlor...	10.947	9.256	1854812	956824	18.275	17.427
Target Compounds						
26) L6 AR-1254-1	7.166	6.112	480940	291965	109.351	80.832 #
27) L6 AR-1254-2	7.395	6.270	1100305	430719	161.554	138.204
28) L6 AR-1254-3	7.779	6.687	1701147	1157411	242.525	236.017
29) L6 AR-1254-4	8.075	6.925	1407908	736494	232.149	212.382
30) L6 AR-1254-5	8.510	7.351	2559844	12113811	440.673m	2676.529 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011521\
Data File : PO074758.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Jan 2021 17:31
Operator : AJ/MA
Sample : M1087-06
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S4-02-C


Manual Integrations
APPROVED

Ankita
1/18/2021 12:52:34 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 15 23:39:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

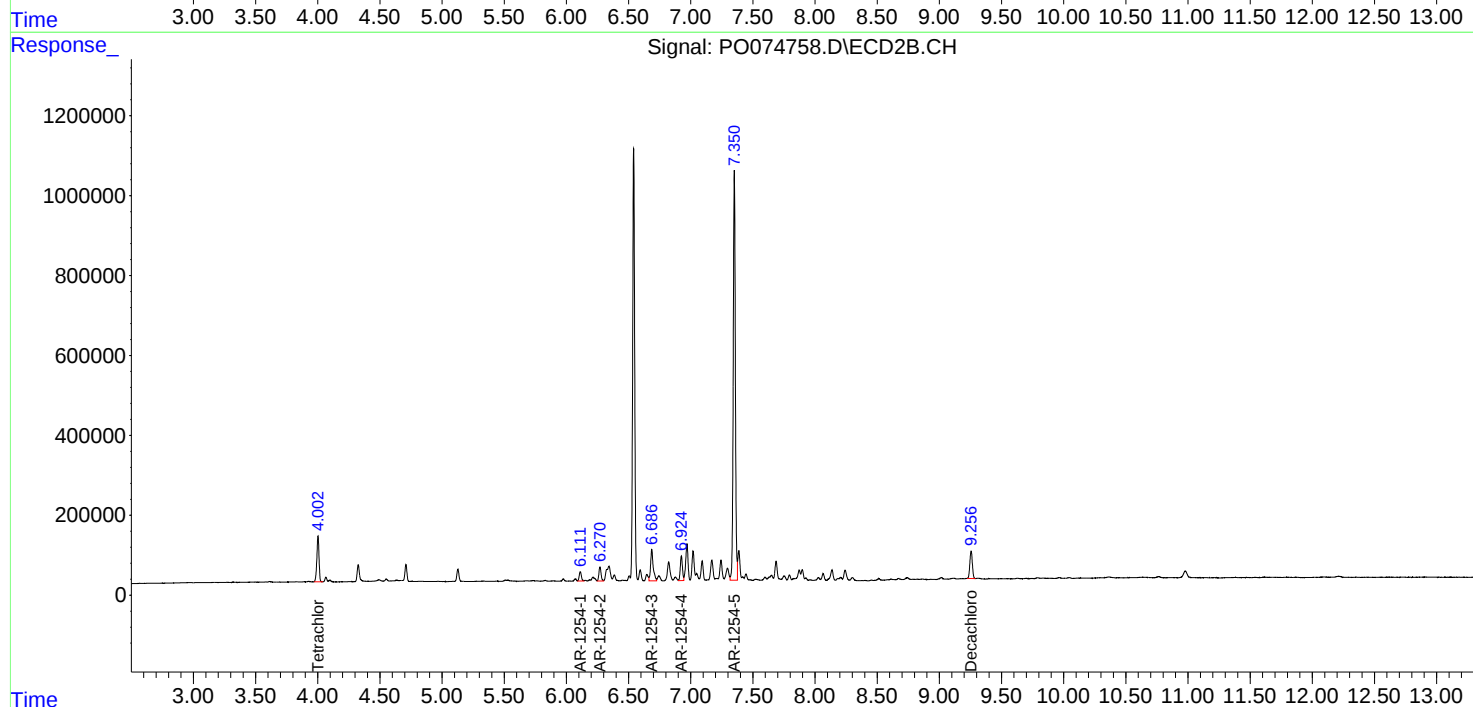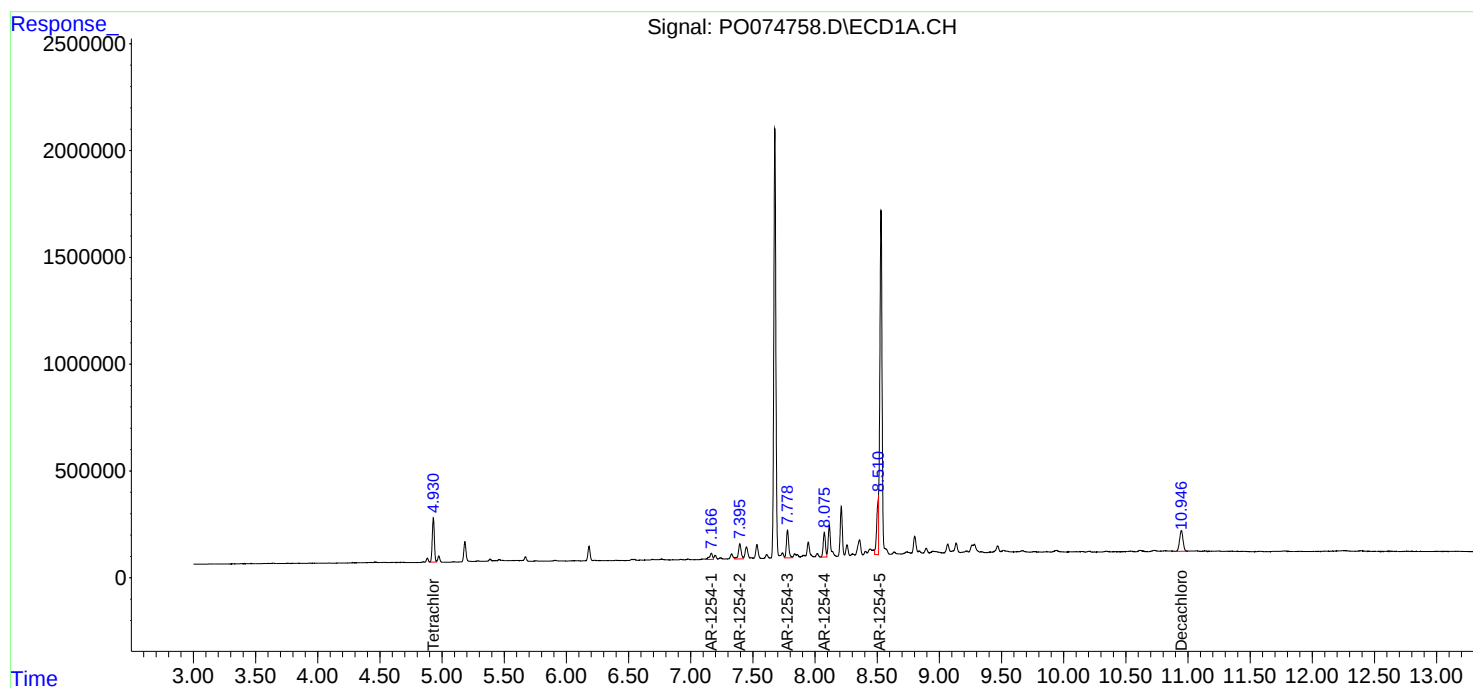

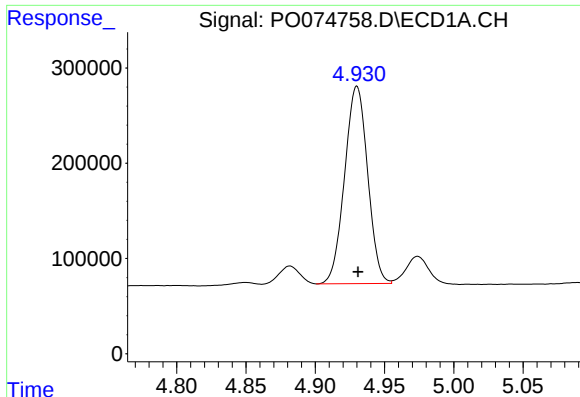


#1 Tetrachloro-m-xylene

R.T.: 4.930 min
Delta R.T.: -0.001 min
Response: 2402179
Conc: 22.77 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S4-02-C


Manual Integrations
APPROVED

Ankita
1/18/2021 12:52:34 PM

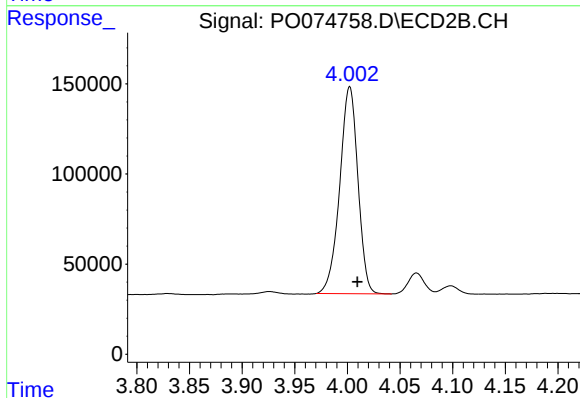


#1 Tetrachloro-m-xylene

R.T.: 4.002 min
Delta R.T.: -0.008 min
Response: 1383288
Conc: 24.59 ng/ml

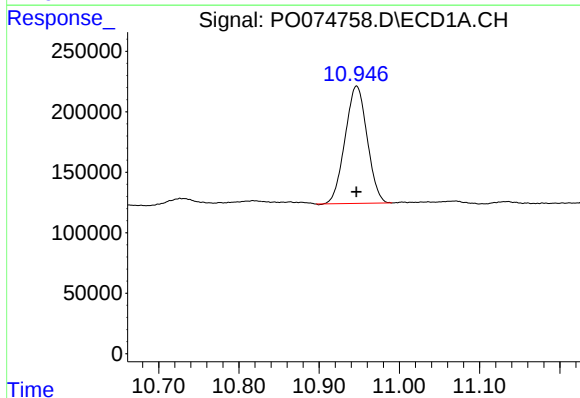


#2 Decachlorobiphenyl

R.T.: 10.947 min
Delta R.T.: 0.000 min
Response: 1854812
Conc: 18.28 ng/ml

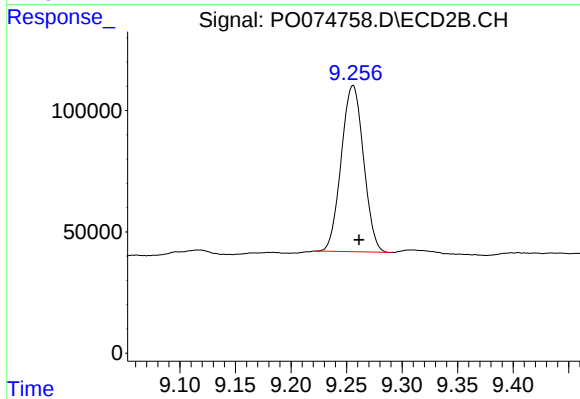

#2 Decachlorobiphenyl

R.T.: 9.256 min
Delta R.T.: -0.006 min
Response: 956824
Conc: 17.43 ng/ml

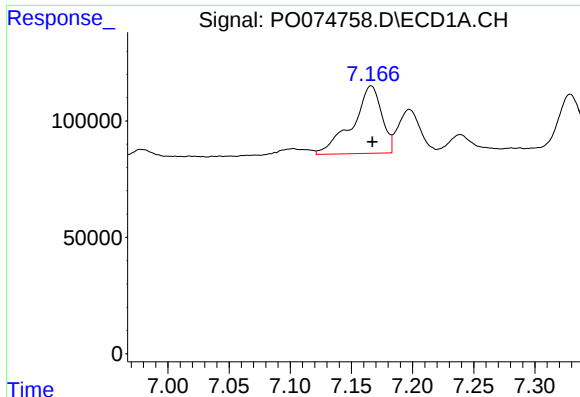


#26 AR-1254-1

R.T.: 7.166 min
Delta R.T.: -0.001 min
Response: 480940
Conc: 109.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
S4-02-C


Manual Integrations
APPROVED

Ankita
1/18/2021 12:52:34 PM

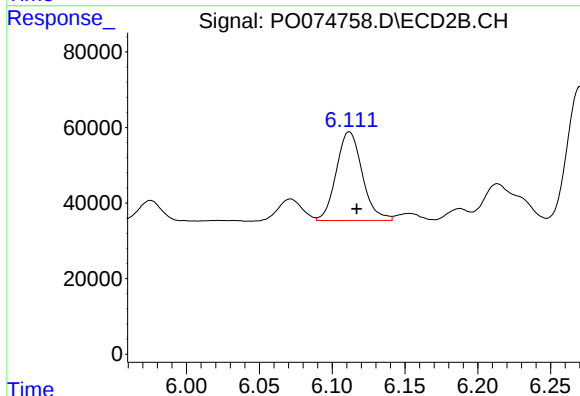


#26 AR-1254-1

R.T.: 6.112 min
Delta R.T.: -0.005 min
Response: 291965
Conc: 80.83 ng/ml

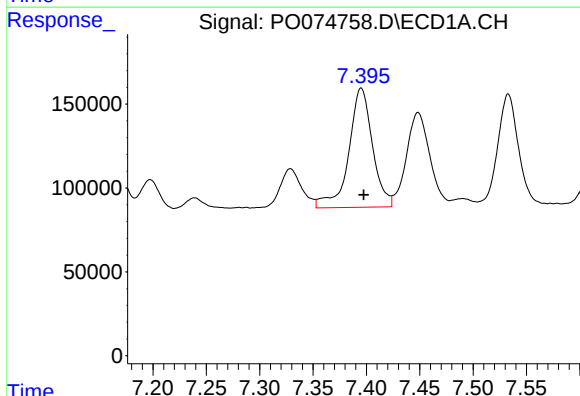


#27 AR-1254-2

R.T.: 7.395 min
Delta R.T.: -0.002 min
Response: 1100305
Conc: 161.55 ng/ml

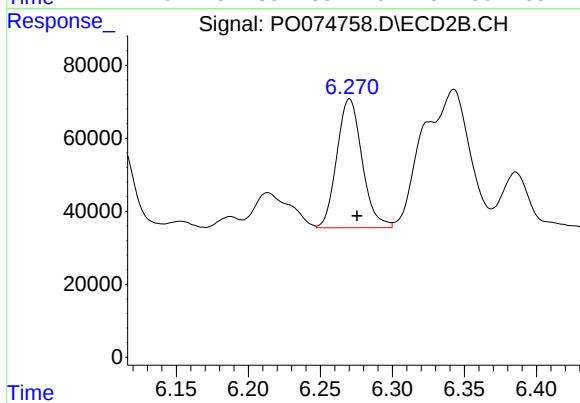

#27 AR-1254-2

R.T.: 6.270 min
Delta R.T.: -0.005 min
Response: 430719
Conc: 138.20 ng/ml

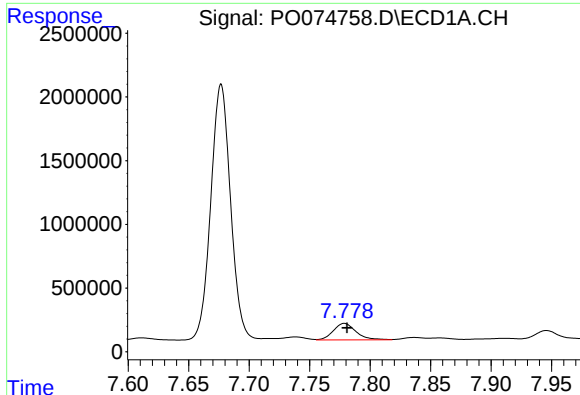


#28 AR-1254-3

R.T.: 7.779 min
Delta R.T.: -0.002 min
Response: 1701147
Conc: 242.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
S4-02-C


Manual Integrations
APPROVED

Ankita
1/18/2021 12:52:34 PM

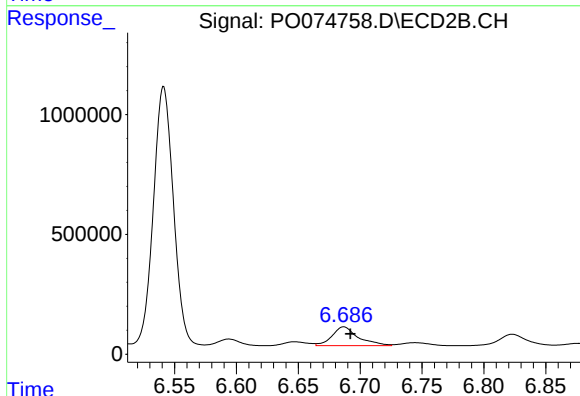


#28 AR-1254-3

R.T.: 6.687 min
Delta R.T.: -0.005 min
Response: 1157411
Conc: 236.02 ng/ml

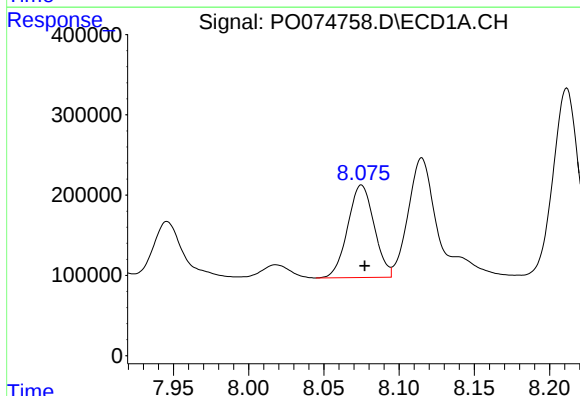


#29 AR-1254-4

R.T.: 8.075 min
Delta R.T.: -0.002 min
Response: 1407908
Conc: 232.15 ng/ml

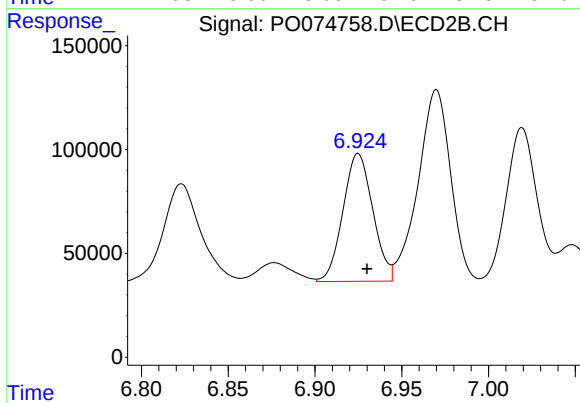

#29 AR-1254-4

R.T.: 6.925 min
Delta R.T.: -0.005 min
Response: 736494
Conc: 212.38 ng/ml

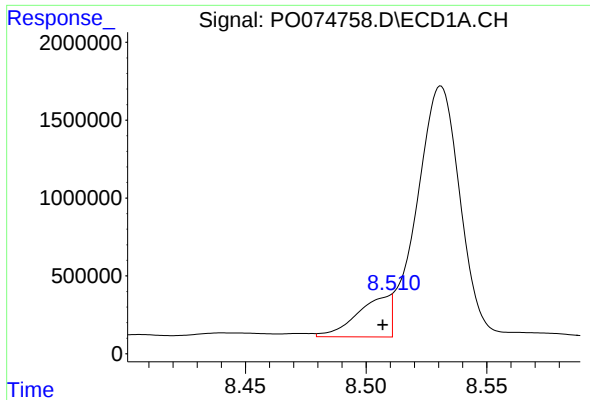


#30 AR-1254-5

R.T.: 8.510 min
Delta R.T.: 0.003 min
Response: 2559844
Conc: 440.67 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S4-02-C

Manual Integrations
APPROVED

Ankita
1/18/2021 12:52:34 PM

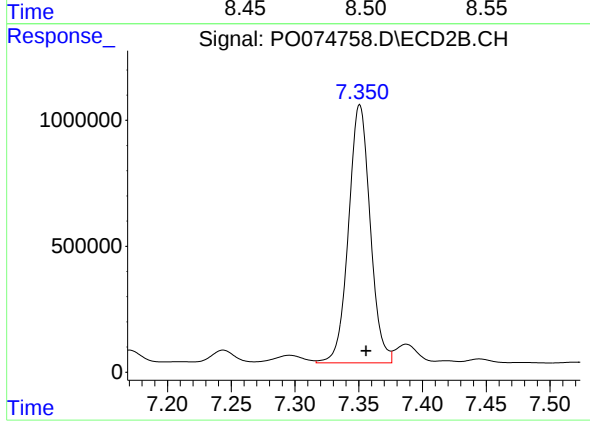

#30 AR-1254-5

R.T.: 7.351 min
Delta R.T.: -0.005 min
Response: 12113811
Conc: 2676.53 ng/ml