

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011521\
 Data File : P0074761.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Jan 2021 18:22
 Operator : AJ/MA
 Sample : M1089-06
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S6-02-C

Manual Integrations
 APPROVED

Ankita
 1/18/2021 12:52:36 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 15 23:40:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.930	4.003	2409550	1278300	22.835	22.724
2) SA Decachlor...	10.947	9.256	1607838	828271	15.842	15.086
Target Compounds						
26) L6 AR-1254-1	7.161	6.113	667888	633792	151.857m	175.468
27) L6 AR-1254-2	7.398	6.271	2102195	910767	308.657	292.237
28) L6 AR-1254-3	7.781	6.688	2502006	1550865	356.699	316.250
29) L6 AR-1254-4	8.075	6.926	2465946	1119092	406.608m	322.711
30) L6 AR-1254-5	8.506	7.352	4032473	5598358	694.184m	1236.949 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011521\
Data File : PO074761.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Jan 2021 18:22
Operator : AJ/MA
Sample : M1089-06
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S6-02-C


Manual Integrations
APPROVED

Ankita
1/18/2021 12:52:36 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 15 23:40:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

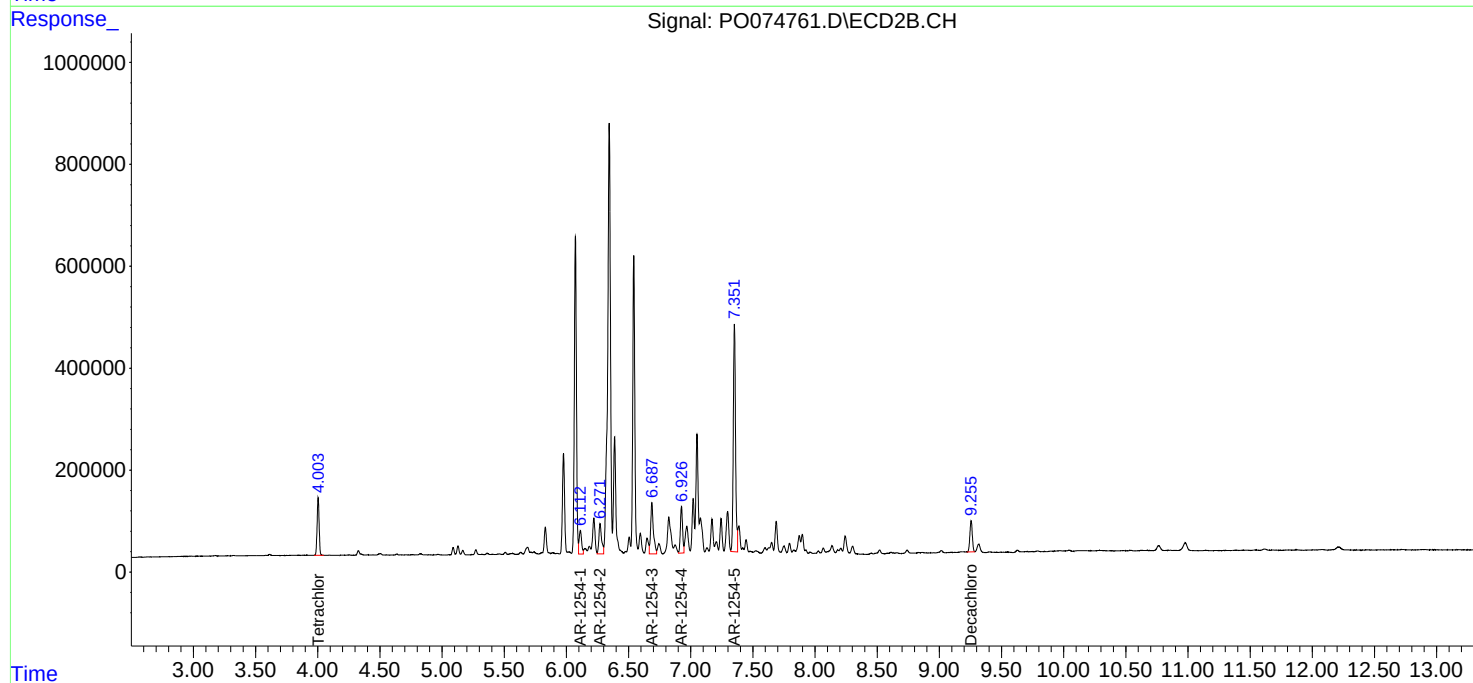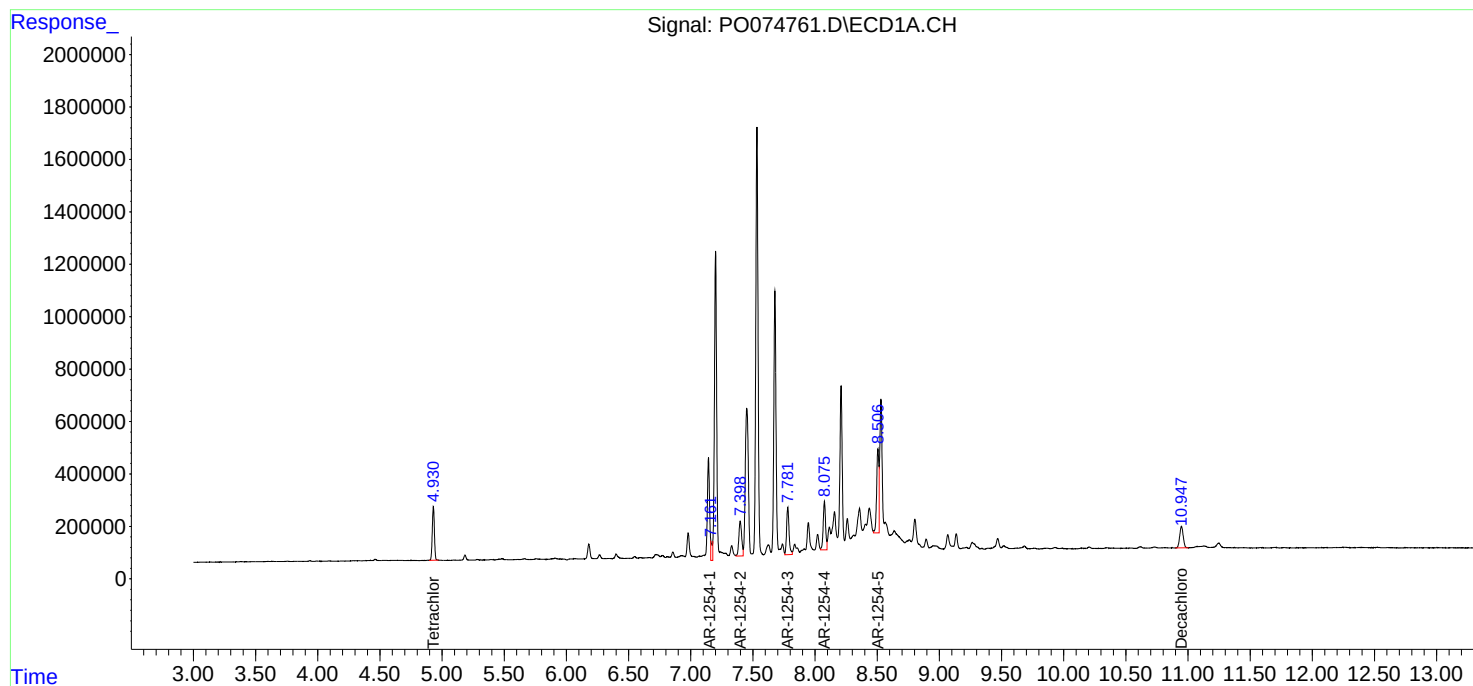

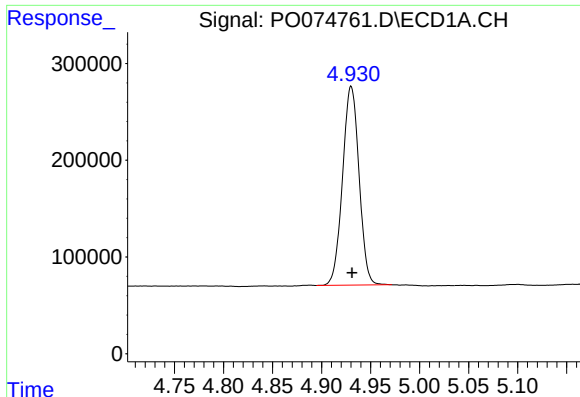


#1 Tetrachloro-m-xylene

R.T.: 4.930 min
Delta R.T.: 0.000 min
Response: 2409550
Conc: 22.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
S6-02-C


Manual Integrations
APPROVED

Ankita
1/18/2021 12:52:36 PM

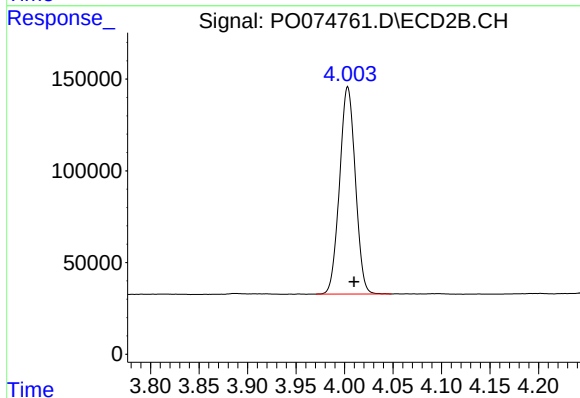


#1 Tetrachloro-m-xylene

R.T.: 4.003 min
Delta R.T.: -0.006 min
Response: 1278300
Conc: 22.72 ng/ml

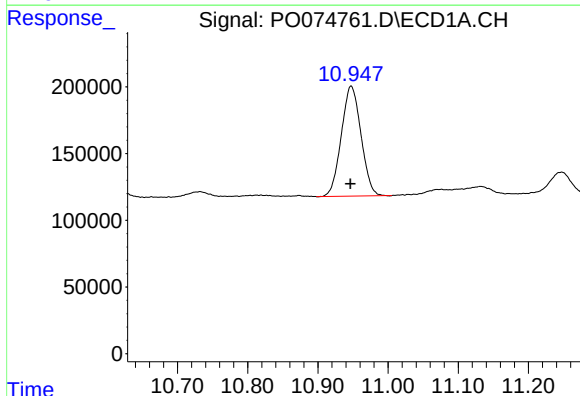


#2 Decachlorobiphenyl

R.T.: 10.947 min
Delta R.T.: 0.000 min
Response: 1607838
Conc: 15.84 ng/ml

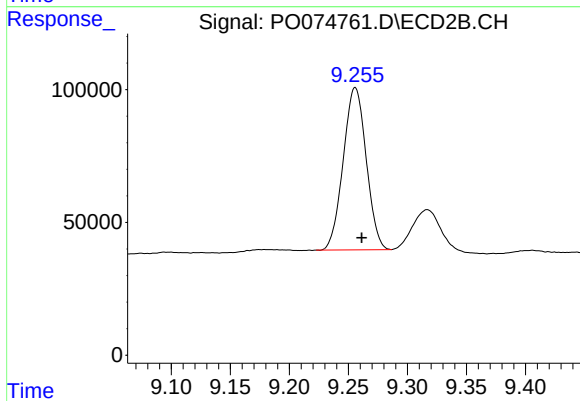

#2 Decachlorobiphenyl

R.T.: 9.256 min
Delta R.T.: -0.006 min
Response: 828271
Conc: 15.09 ng/ml

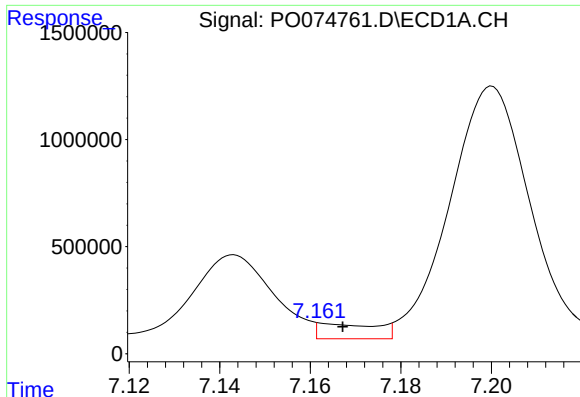


#26 AR-1254-1

R.T.: 7.161 min
Delta R.T.: -0.006 min
Response: 667888
Conc: 151.86 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S6-02-C


Manual Integrations
APPROVED

Ankita
1/18/2021 12:52:36 PM

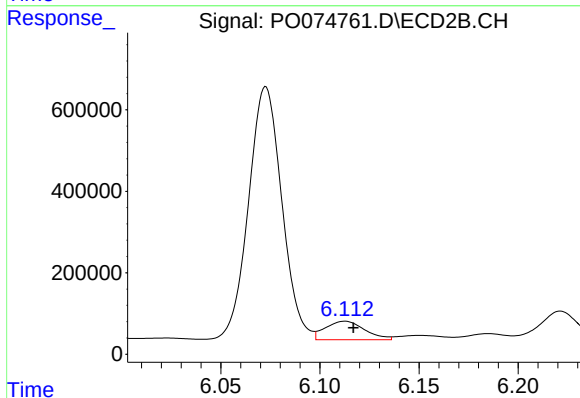


#26 AR-1254-1

R.T.: 6.113 min
Delta R.T.: -0.004 min
Response: 633792
Conc: 175.47 ng/ml

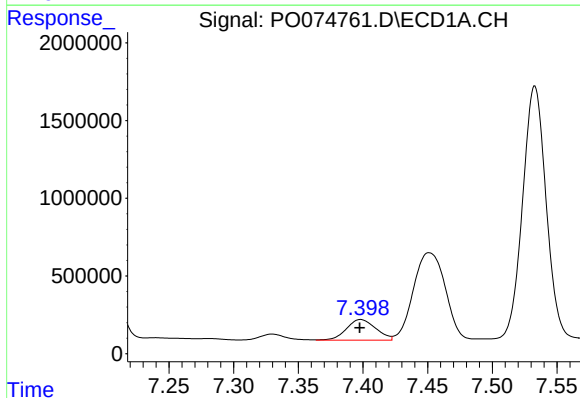


#27 AR-1254-2

R.T.: 7.398 min
Delta R.T.: 0.000 min
Response: 2102195
Conc: 308.66 ng/ml

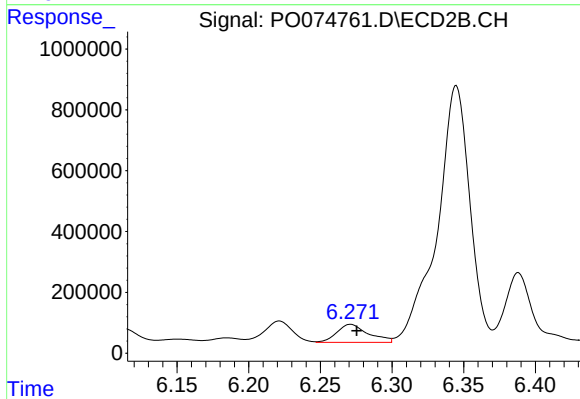

#27 AR-1254-2

R.T.: 6.271 min
Delta R.T.: -0.004 min
Response: 910767
Conc: 292.24 ng/ml

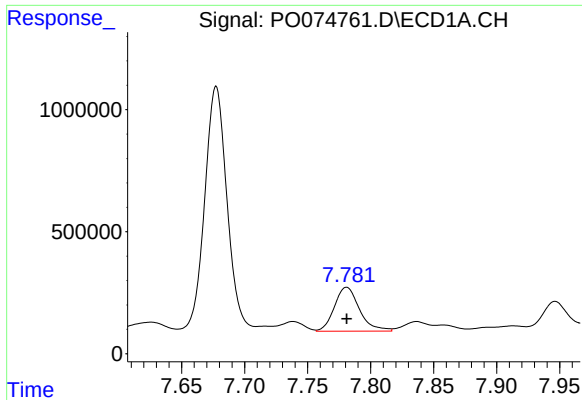


#28 AR-1254-3

R.T.: 7.781 min
Delta R.T.: 0.000 min
Response: 2502006
Conc: 356.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
S6-02-C


Manual Integrations
APPROVED

Ankita
1/18/2021 12:52:36 PM

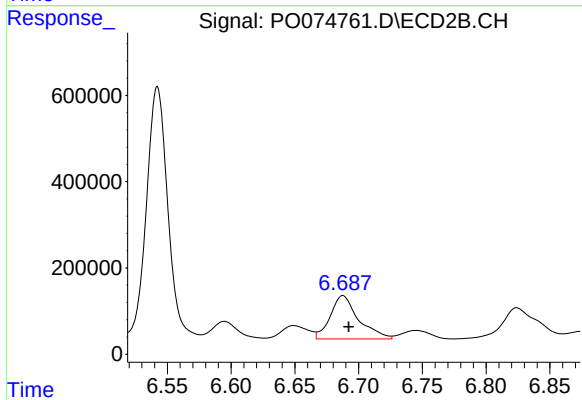


#28 AR-1254-3

R.T.: 6.688 min
Delta R.T.: -0.005 min
Response: 1550865
Conc: 316.25 ng/ml

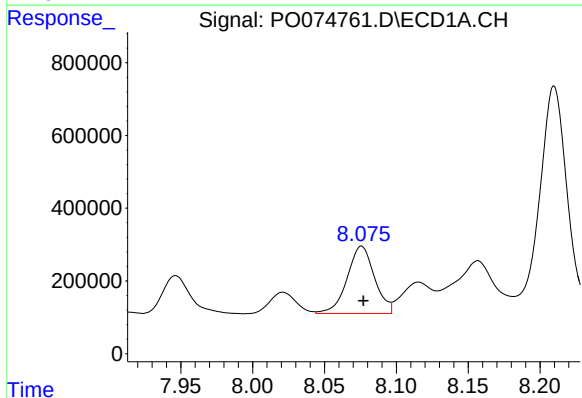


#29 AR-1254-4

R.T.: 8.075 min
Delta R.T.: -0.002 min
Response: 2465946
Conc: 406.61 ng/ml m

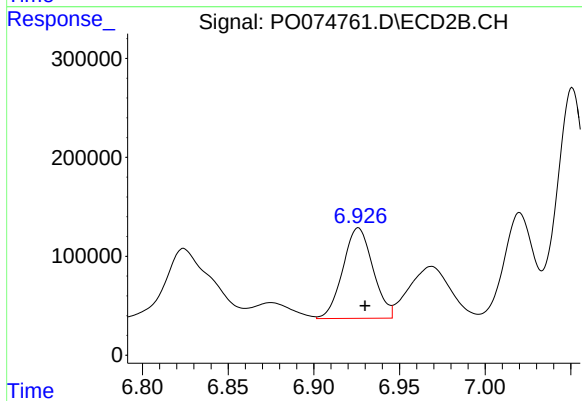

#29 AR-1254-4

R.T.: 6.926 min
Delta R.T.: -0.004 min
Response: 1119092
Conc: 322.71 ng/ml

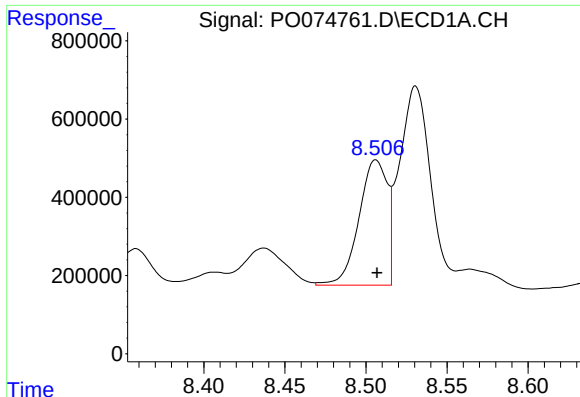


#30 AR-1254-5

R.T.: 8.506 min
Delta R.T.: -0.001 min
Response: 4032473
Conc: 694.18 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S6-02-C

Manual Integrations
APPROVED

Ankita
1/18/2021 12:52:36 PM

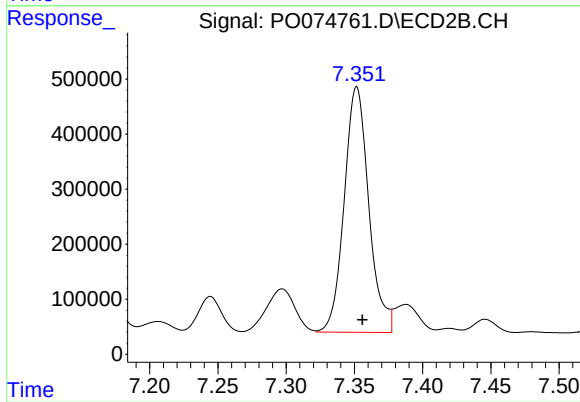

#30 AR-1254-5

R.T.: 7.352 min
Delta R.T.: -0.004 min
Response: 5598358
Conc: 1236.95 ng/ml