

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011521\
 Data File : P0074772.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Jan 2021 21:30
 Operator : AJ/MA
 Sample : M1084-12
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S1-06-C

Manual Integrations
 APPROVED

Ankita
 1/18/2021 12:52:54 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 15 23:45:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.931	4.004	2067463	1146681	19.593	20.385
2) SA Decachlor...	10.949	9.256	1484543	775806	14.627	14.130
Target Compounds						
26) L6 AR-1254-1	7.167	6.113	1457844	968797	331.468m	268.216
27) L6 AR-1254-2	7.397	6.272	3023210	1357777	443.887	435.669
28) L6 AR-1254-3	7.781	6.688	3748836	2610406	534.454	532.310
29) L6 AR-1254-4	8.077	6.926	3545691	1808099	584.647	521.400
30) L6 AR-1254-5	8.507	7.352	6272611	8724122	1079.821	1927.582 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011521\
Data File : PO074772.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Jan 2021 21:30
Operator : AJ/MA
Sample : M1084-12
Misc :
ALS Vial : 41 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S1-06-C


Manual Integrations
APPROVED

Ankita
1/18/2021 12:52:54 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 15 23:45:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

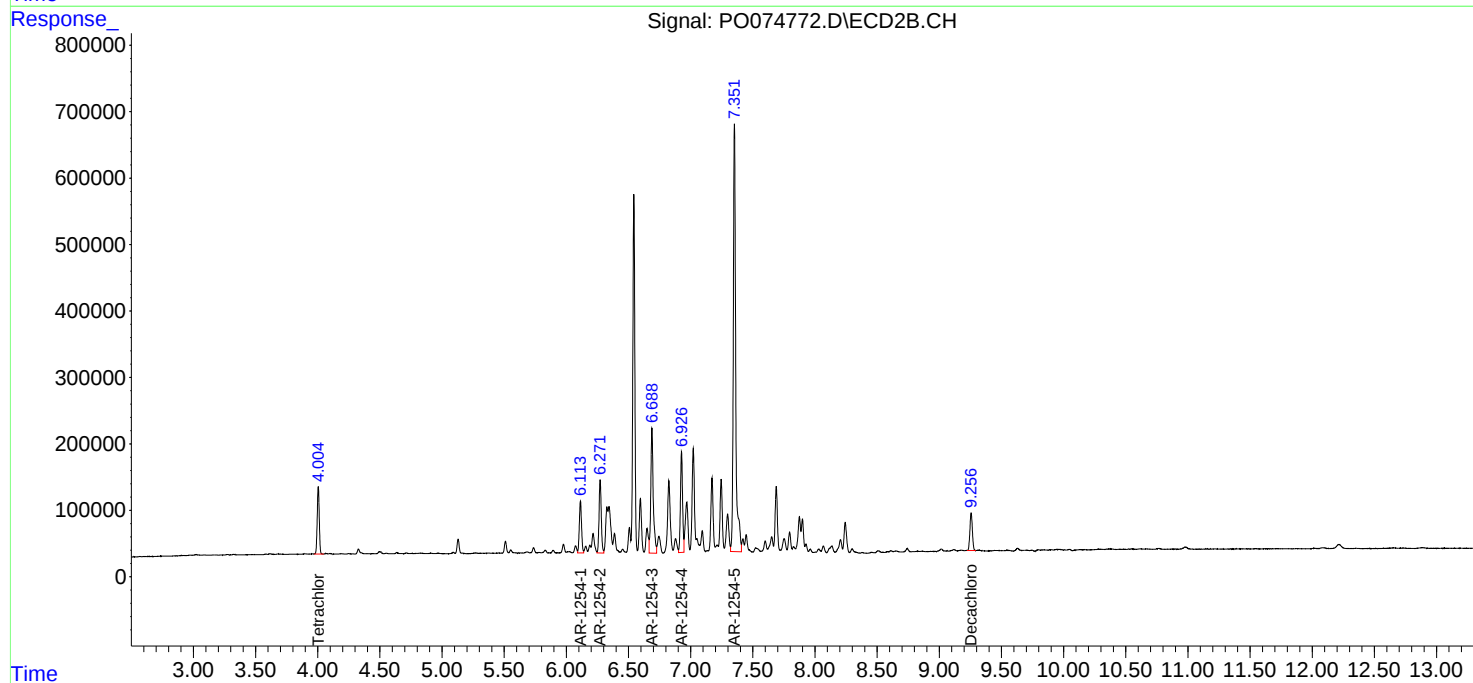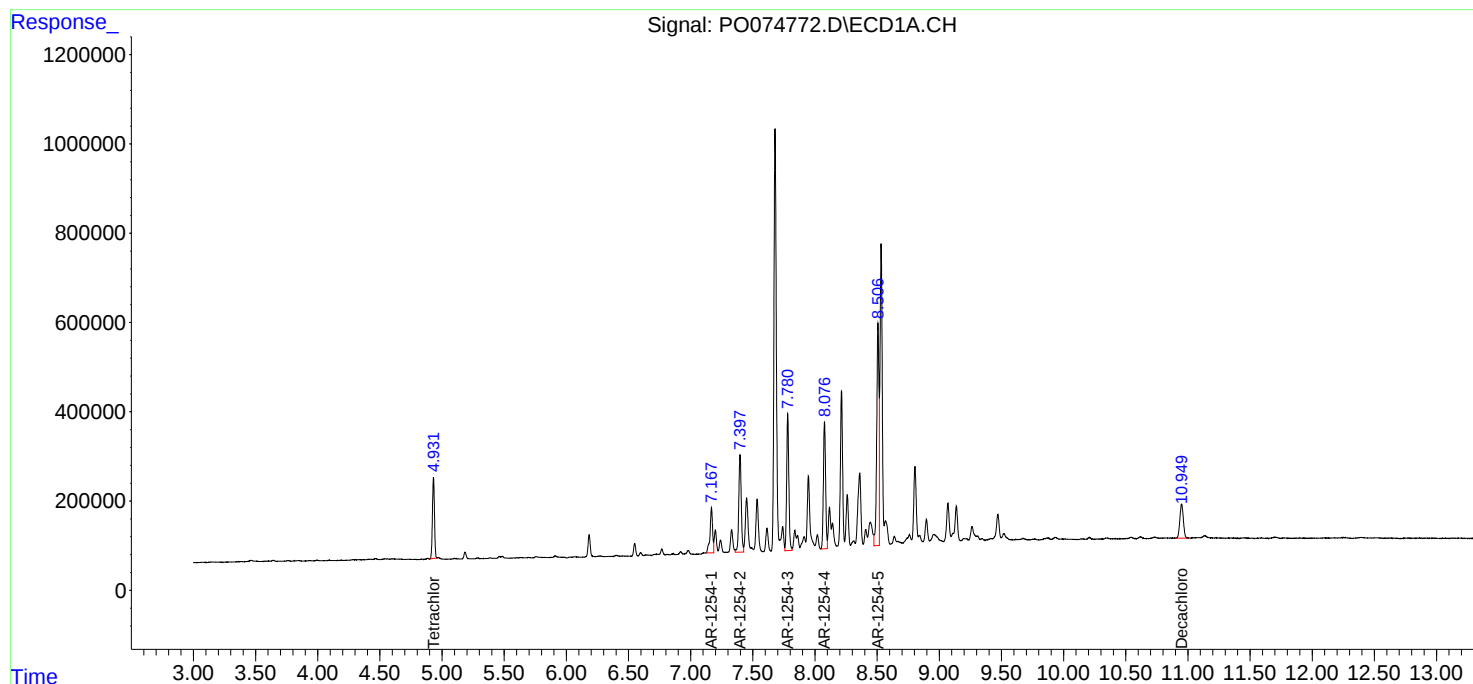

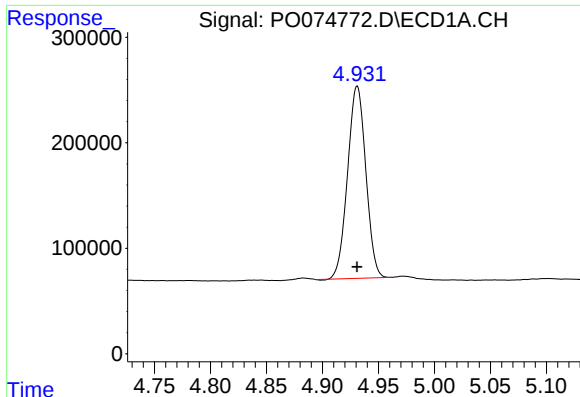


#1 Tetrachloro-m-xylene

R.T.: 4.931 min
Delta R.T.: 0.000 min
Response: 2067463
Conc: 19.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
S1-06-C


Manual Integrations
APPROVED

Ankita
1/18/2021 12:52:54 PM

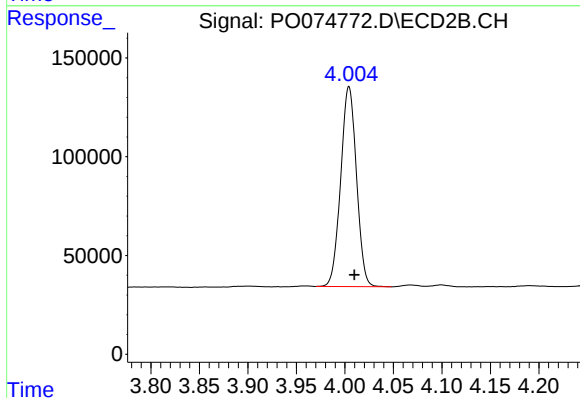


#1 Tetrachloro-m-xylene

R.T.: 4.004 min
Delta R.T.: -0.006 min
Response: 1146681
Conc: 20.38 ng/ml

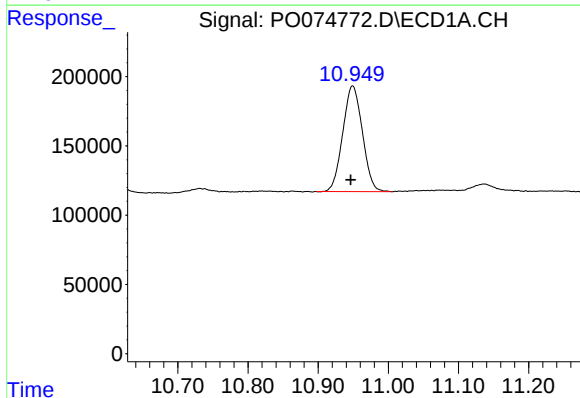


#2 Decachlorobiphenyl

R.T.: 10.949 min
Delta R.T.: 0.003 min
Response: 1484543
Conc: 14.63 ng/ml

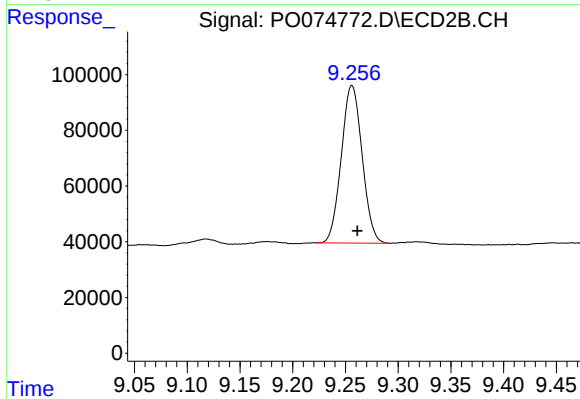

#2 Decachlorobiphenyl

R.T.: 9.256 min
Delta R.T.: -0.005 min
Response: 775806
Conc: 14.13 ng/ml

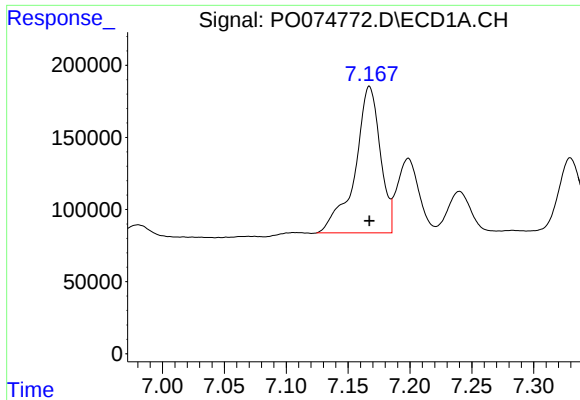


#26 AR-1254-1

R.T.: 7.167 min
Delta R.T.: 0.000 min
Response: 1457844
Conc: 331.47 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S1-06-C


Manual Integrations
APPROVED

Ankita
1/18/2021 12:52:54 PM

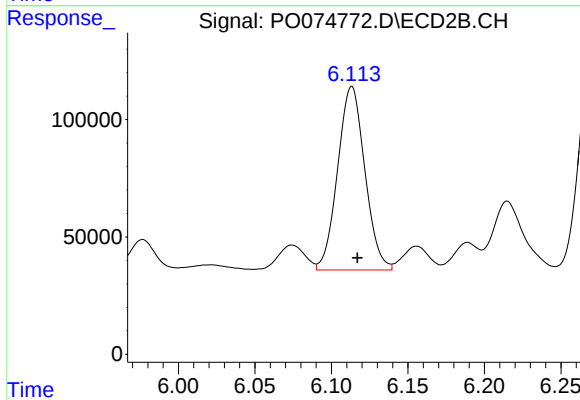


#26 AR-1254-1

R.T.: 6.113 min
Delta R.T.: -0.004 min
Response: 968797
Conc: 268.22 ng/ml

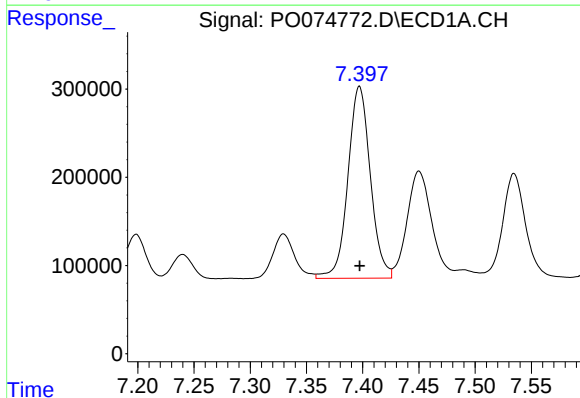


#27 AR-1254-2

R.T.: 7.397 min
Delta R.T.: 0.000 min
Response: 3023210
Conc: 443.89 ng/ml

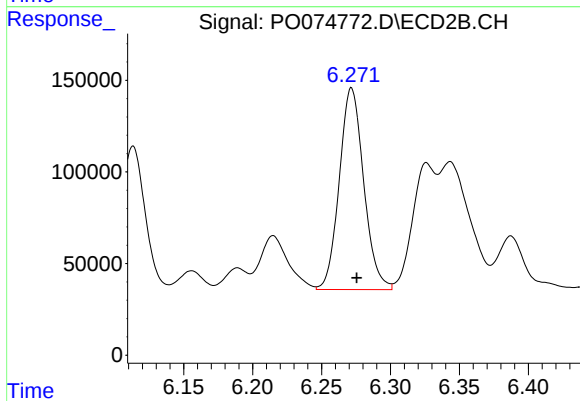

#27 AR-1254-2

R.T.: 6.272 min
Delta R.T.: -0.004 min
Response: 1357777
Conc: 435.67 ng/ml

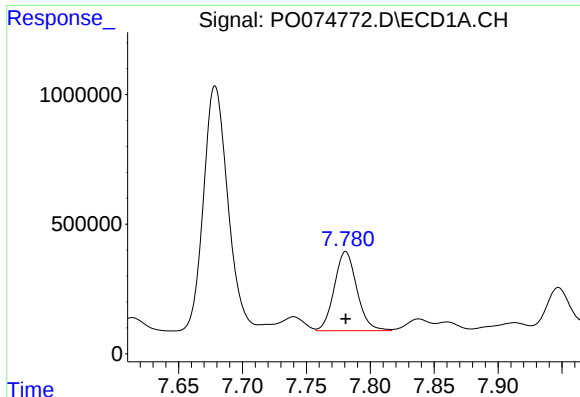


#28 AR-1254-3

R.T.: 7.781 min
Delta R.T.: 0.000 min
Response: 3748836
Conc: 534.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
S1-06-C


Manual Integrations
APPROVED

Ankita
1/18/2021 12:52:54 PM

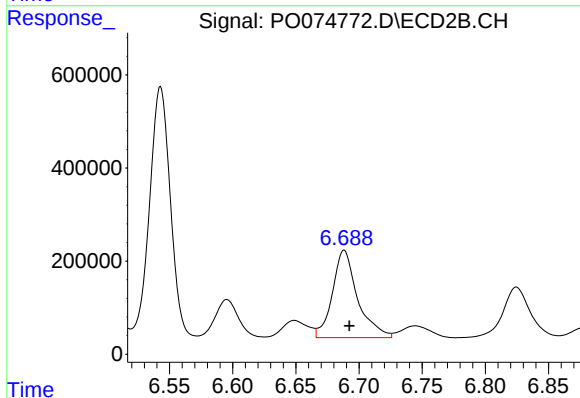


#28 AR-1254-3

R.T.: 6.688 min
Delta R.T.: -0.004 min
Response: 2610406
Conc: 532.31 ng/ml

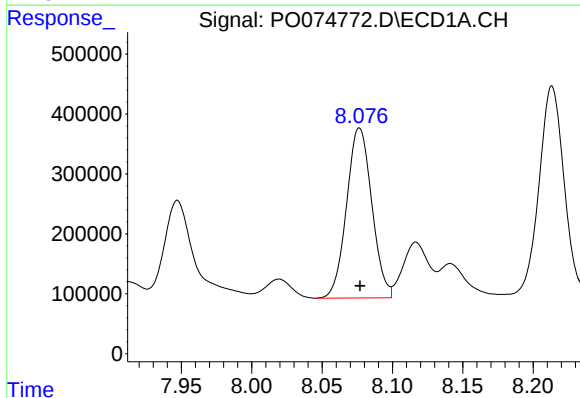


#29 AR-1254-4

R.T.: 8.077 min
Delta R.T.: 0.000 min
Response: 3545691
Conc: 584.65 ng/ml

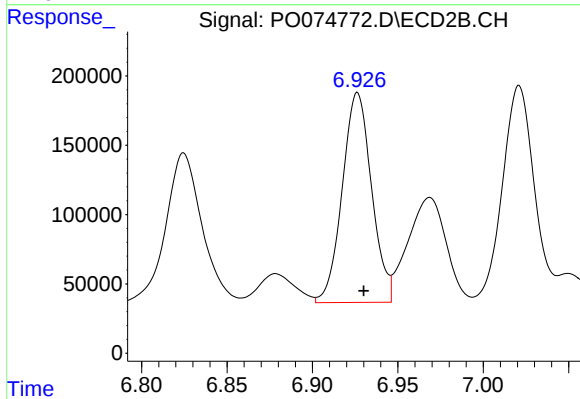

#29 AR-1254-4

R.T.: 6.926 min
Delta R.T.: -0.004 min
Response: 1808099
Conc: 521.40 ng/ml

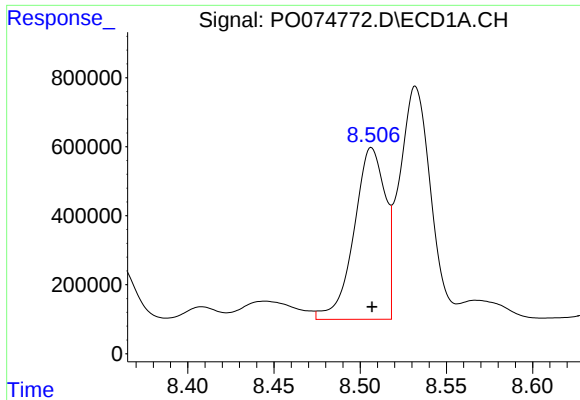


#30 AR-1254-5

R.T.: 8.507 min
Delta R.T.: 0.000 min
Response: 6272611
Conc: 1079.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
S1-06-C

Manual Integrations
APPROVED

Ankita
1/18/2021 12:52:54 PM

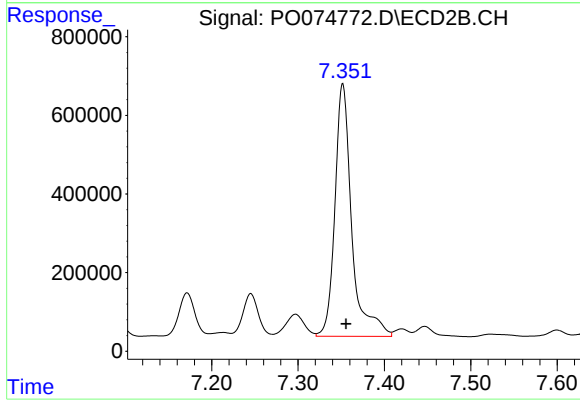

#30 AR-1254-5

R.T.: 7.352 min
Delta R.T.: -0.004 min
Response: 8724122
Conc: 1927.58 ng/ml