

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011521\
 Data File : P0074775.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Jan 2021 22:22
 Operator : AJ/MA
 Sample : M1088-09
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S5-01-C

Manual Integrations
 APPROVED

Ankita
 1/18/2021 12:53:09 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 15 23:46:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.931	4.004	2258191	1362067	21.401m	24.214
2) SA Decachlor...	10.952	9.259	1737494	949823	17.119	17.300
Target Compounds						
26) L6 AR-1254-1	7.167	6.114	2822743	2039500	641.804	564.645
27) L6 AR-1254-2	7.396	6.273	6136490	2958655	900.998	949.341
28) L6 AR-1254-3	7.781	6.689	7905388	5213874	1127.034	1063.205
29) L6 AR-1254-4	8.077	6.927	6985661	3491217	1151.861	1006.759
30) L6 AR-1254-5	8.507	7.353	10652559	17675825	1833.822	3905.447 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011521\
Data File : PO074775.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Jan 2021 22:22
Operator : AJ/MA
Sample : M1088-09
Misc :
ALS Vial : 44 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S5-01-C


Manual Integrations
APPROVED

Ankita
1/18/2021 12:53:09 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 15 23:46:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

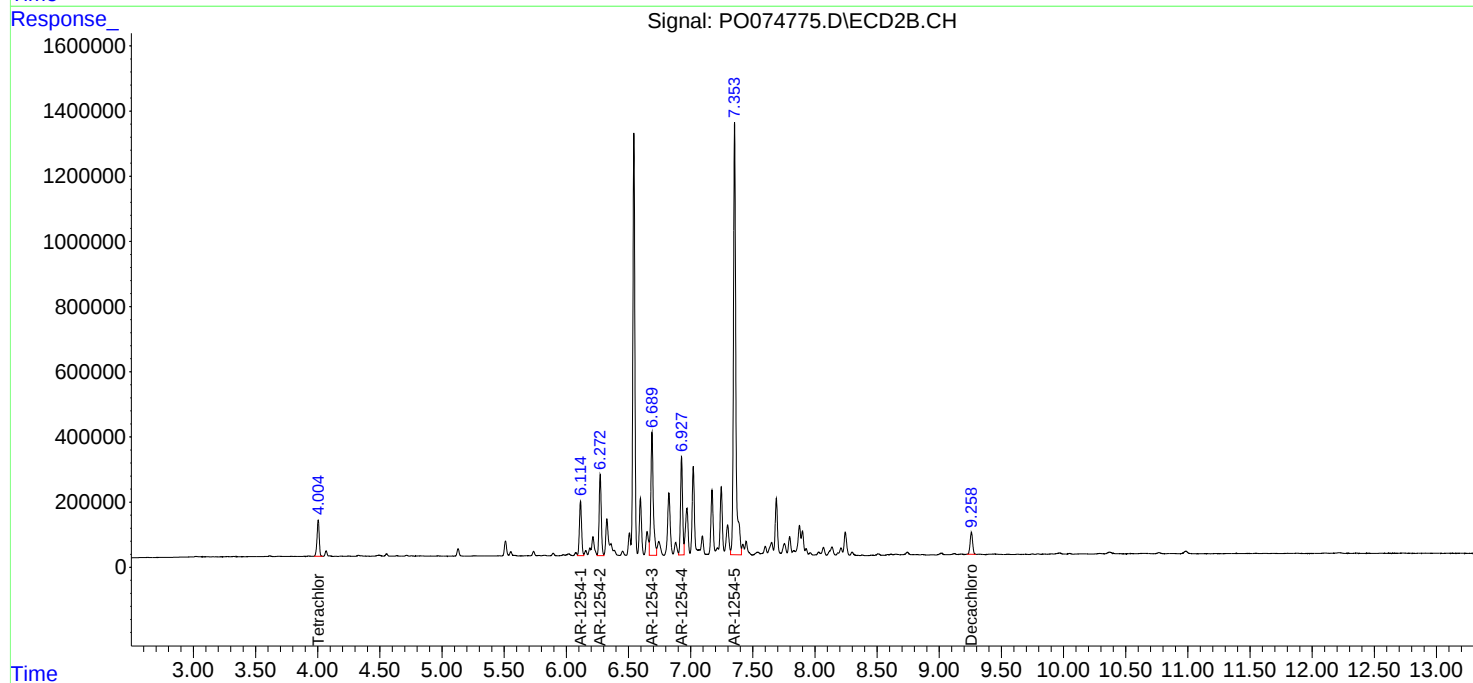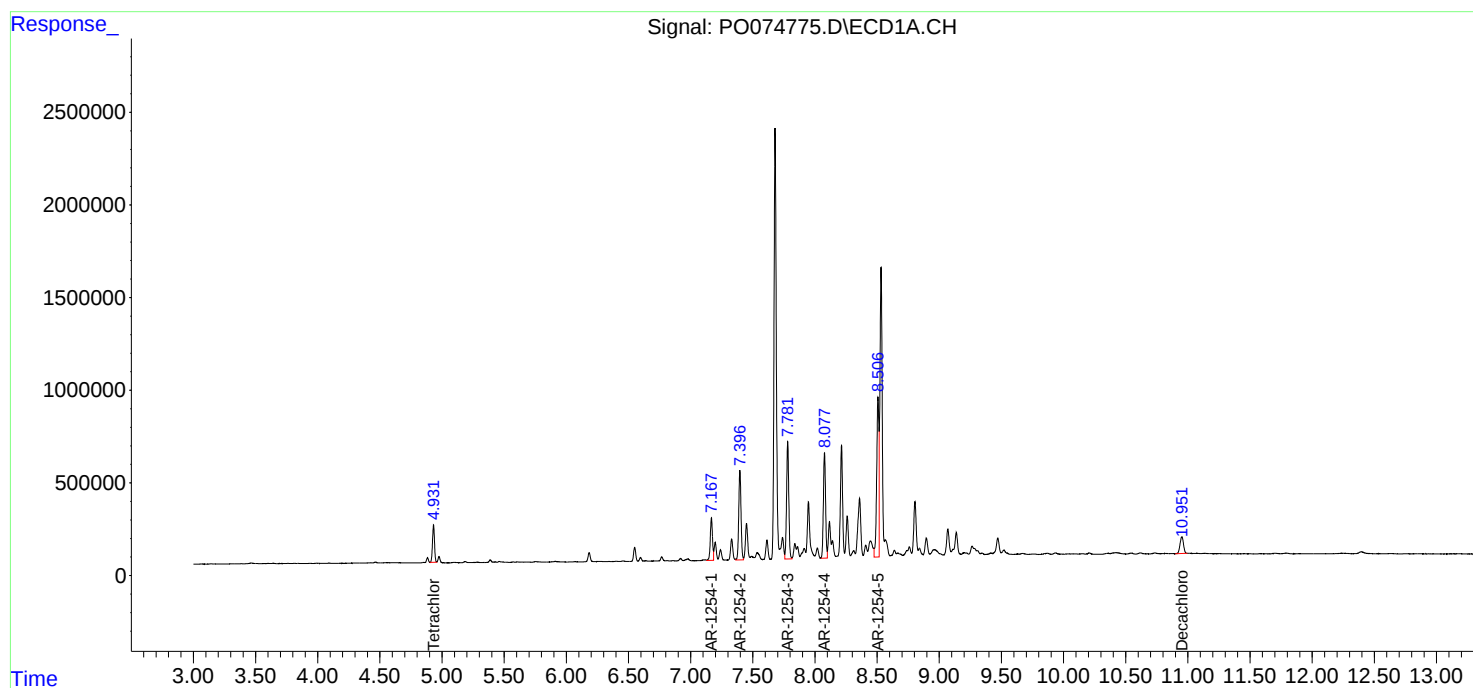

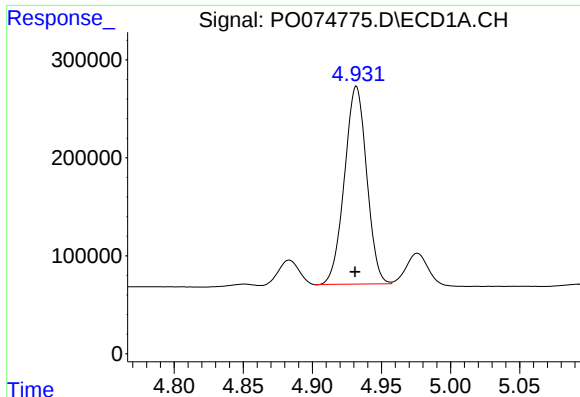


#1 Tetrachloro-m-xylene

R.T.: 4.931 min
Delta R.T.: 0.000 min
Response: 2258191
Conc: 21.40 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S5-01-C


Manual Integrations
APPROVED

Ankita
1/18/2021 12:53:09 PM

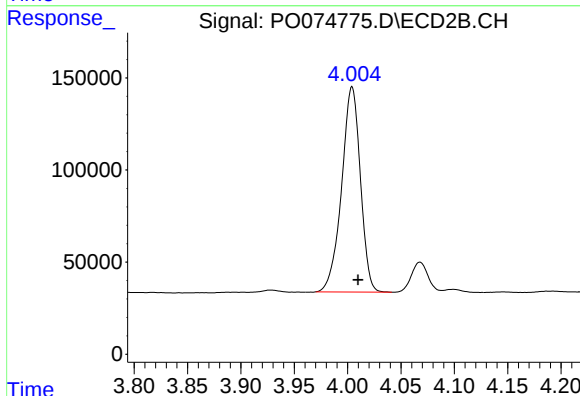


#1 Tetrachloro-m-xylene

R.T.: 4.004 min
Delta R.T.: -0.006 min
Response: 1362067
Conc: 24.21 ng/ml

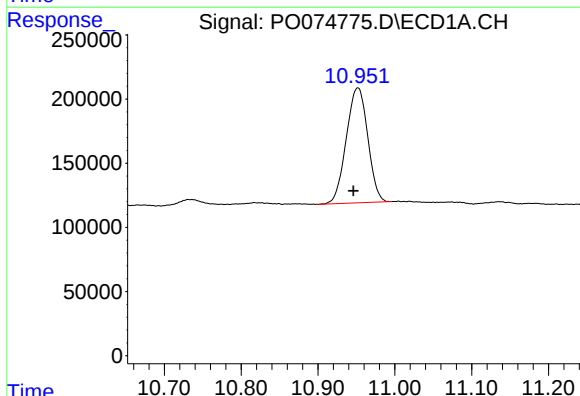


#2 Decachlorobiphenyl

R.T.: 10.952 min
Delta R.T.: 0.006 min
Response: 1737494
Conc: 17.12 ng/ml

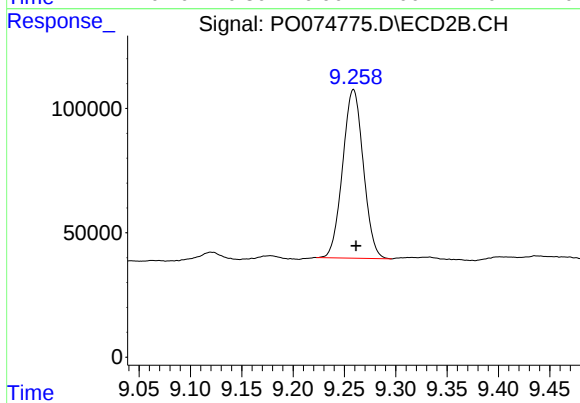

#2 Decachlorobiphenyl

R.T.: 9.259 min
Delta R.T.: -0.003 min
Response: 949823
Conc: 17.30 ng/ml

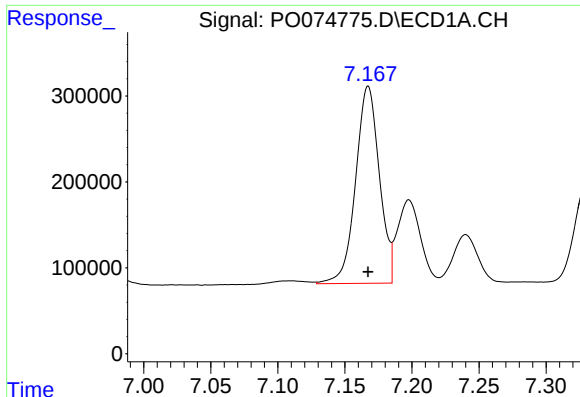


#26 AR-1254-1

R.T.: 7.167 min
Delta R.T.: 0.000 min
Response: 2822743
Conc: 641.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
S5-01-C


Manual Integrations
APPROVED

Ankita
1/18/2021 12:53:09 PM

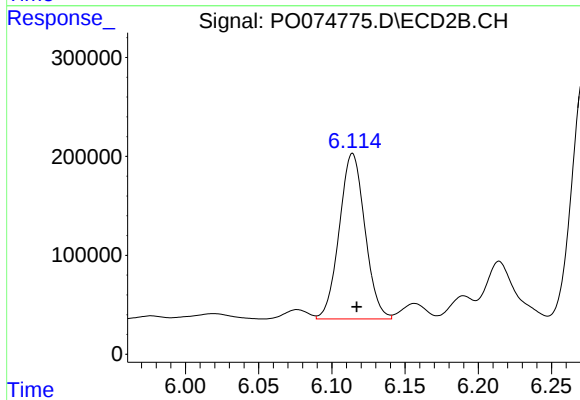


#26 AR-1254-1

R.T.: 6.114 min
Delta R.T.: -0.003 min
Response: 2039500
Conc: 564.64 ng/ml

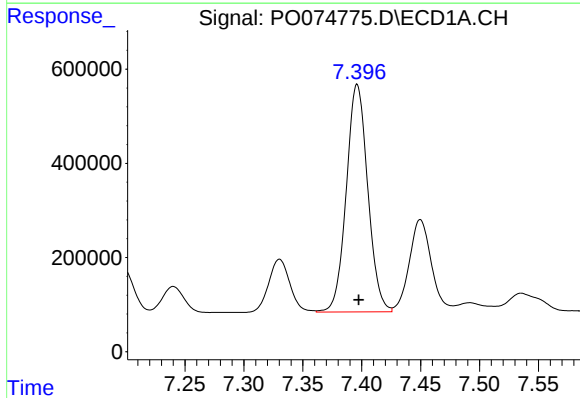


#27 AR-1254-2

R.T.: 7.396 min
Delta R.T.: -0.001 min
Response: 6136490
Conc: 901.00 ng/ml

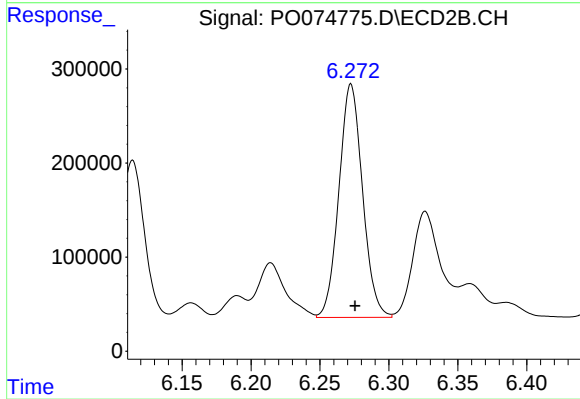

#27 AR-1254-2

R.T.: 6.273 min
Delta R.T.: -0.003 min
Response: 2958655
Conc: 949.34 ng/ml

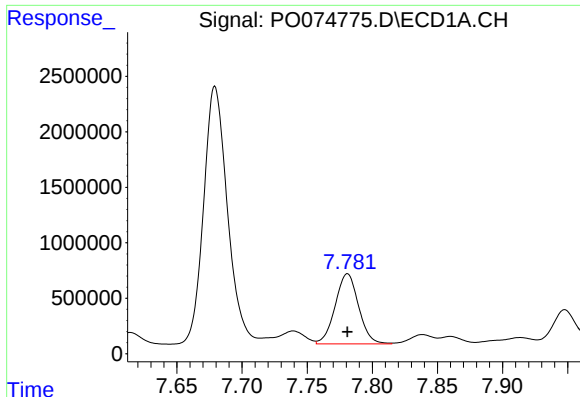


#28 AR-1254-3

R.T.: 7.781 min
Delta R.T.: 0.000 min
Response: 7905388
Conc: 1127.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
S5-01-C


Manual Integrations
APPROVED

Ankita
1/18/2021 12:53:09 PM

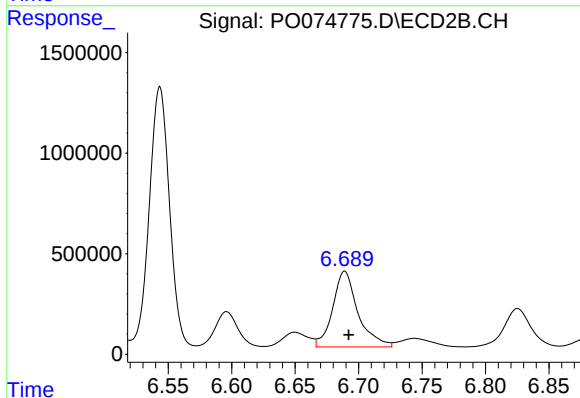


#28 AR-1254-3

R.T.: 6.689 min
Delta R.T.: -0.003 min
Response: 5213874
Conc: 1063.20 ng/ml

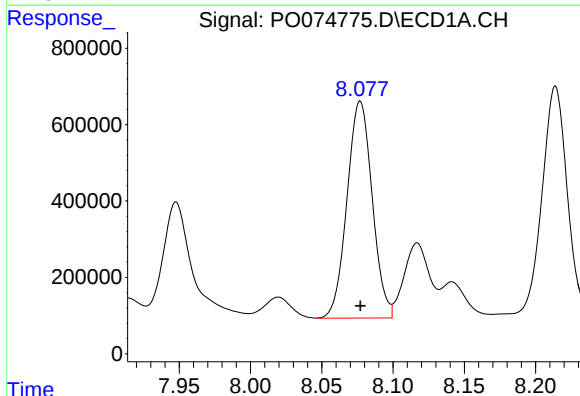


#29 AR-1254-4

R.T.: 8.077 min
Delta R.T.: 0.000 min
Response: 6985661
Conc: 1151.86 ng/ml

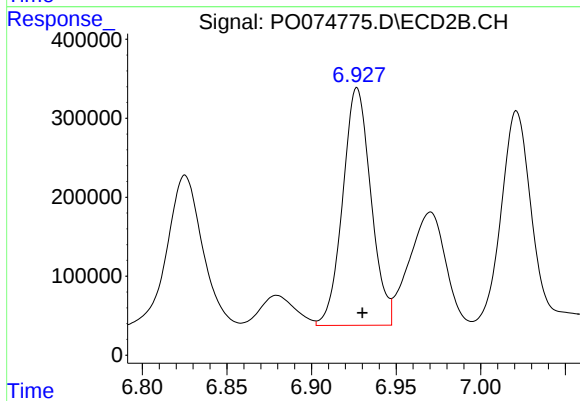

#29 AR-1254-4

R.T.: 6.927 min
Delta R.T.: -0.003 min
Response: 3491217
Conc: 1006.76 ng/ml

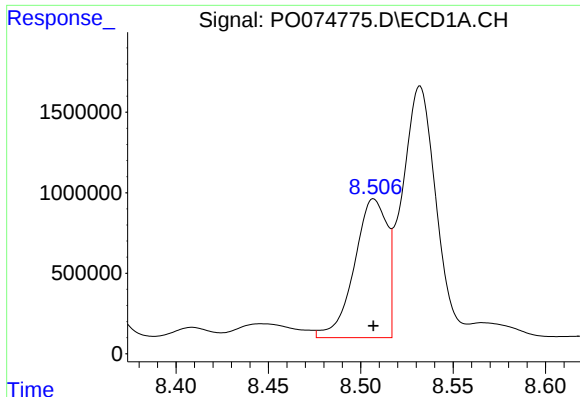


#30 AR-1254-5

R.T.: 8.507 min
Delta R.T.: 0.000 min
Response: 10652559
Conc: 1833.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
S5-01-C

Manual Integrations
APPROVED

Ankita
1/18/2021 12:53:09 PM

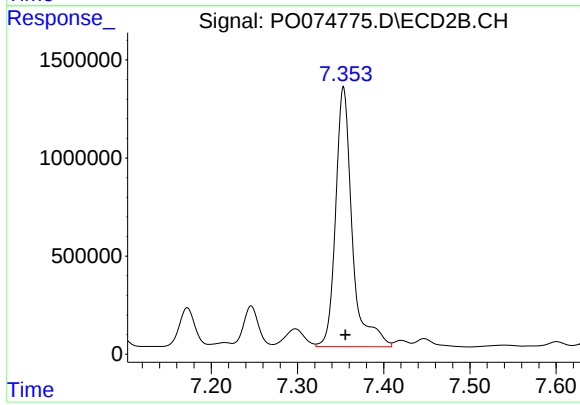

#30 AR-1254-5

R.T.: 7.353 min
Delta R.T.: -0.002 min
Response: 17675825
Conc: 3905.45 ng/ml