

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011521\
 Data File : P0074779.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Jan 2021 23:30
 Operator : AJ/MA
 Sample : M1088-13
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S5-05-C

Manual Integrations
 APPROVED

Ankita
 1/18/2021 12:53:13 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 16 00:33:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.929	4.002	2249930	1198568	21.323	21.307
2)	SA Decachlor...	10.946	9.256	1601174	850312	15.776	15.487
Target Compounds							
26)	L6 AR-1254-1	7.165	6.111	185185	169842	42.105	47.021
27)	L6 AR-1254-2	7.394	6.270	643090	348355	94.422	111.776
28)	L6 AR-1254-3	7.779	6.686	897894	709951	128.009	144.772
29)	L6 AR-1254-4	8.075	6.925	1126741	595008	185.788	171.582
30)	L6 AR-1254-5	8.504	7.351	2609564	2283984	449.233m	504.643

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011521\
Data File : PO074779.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Jan 2021 23:30
Operator : AJ/MA
Sample : M1088-13
Misc :
ALS Vial : 48 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S5-05-C


Manual Integrations
APPROVED

Ankita
1/18/2021 12:53:13 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 16 00:33:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

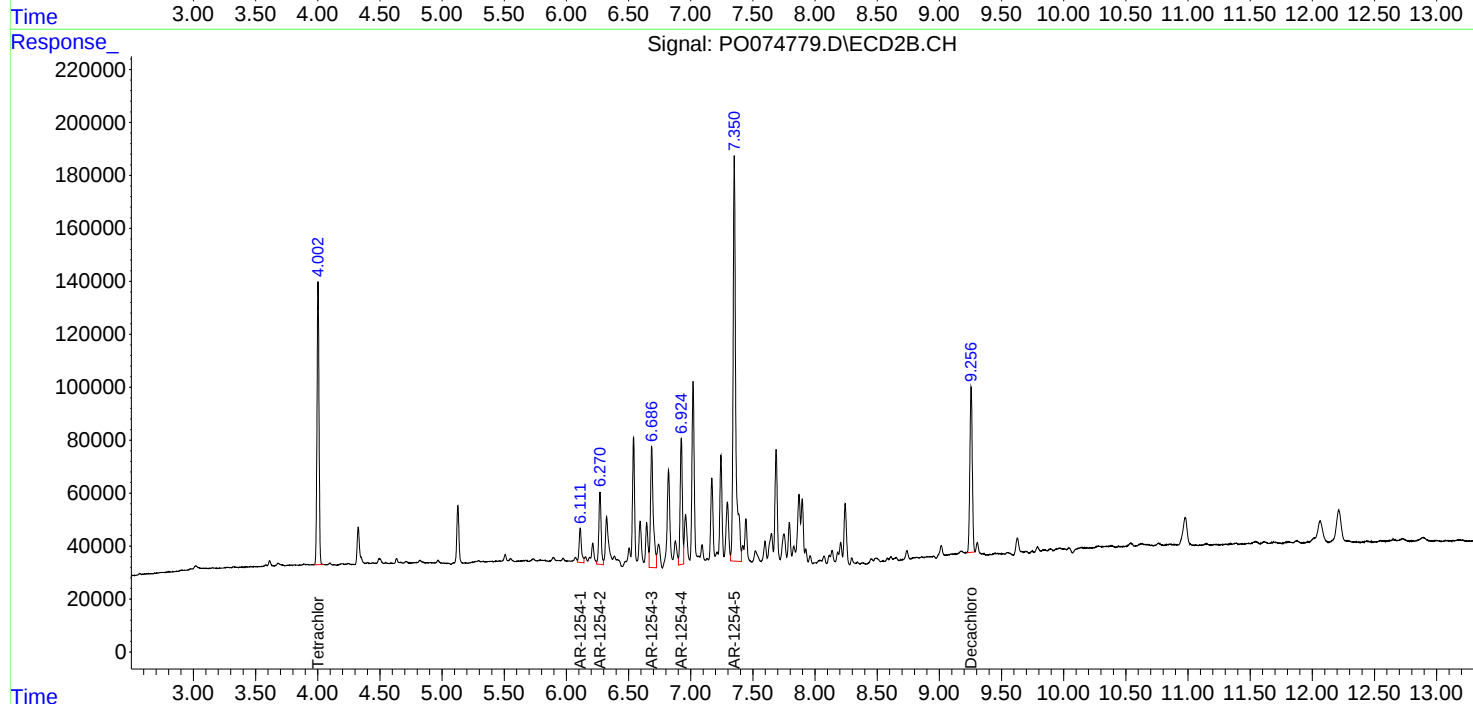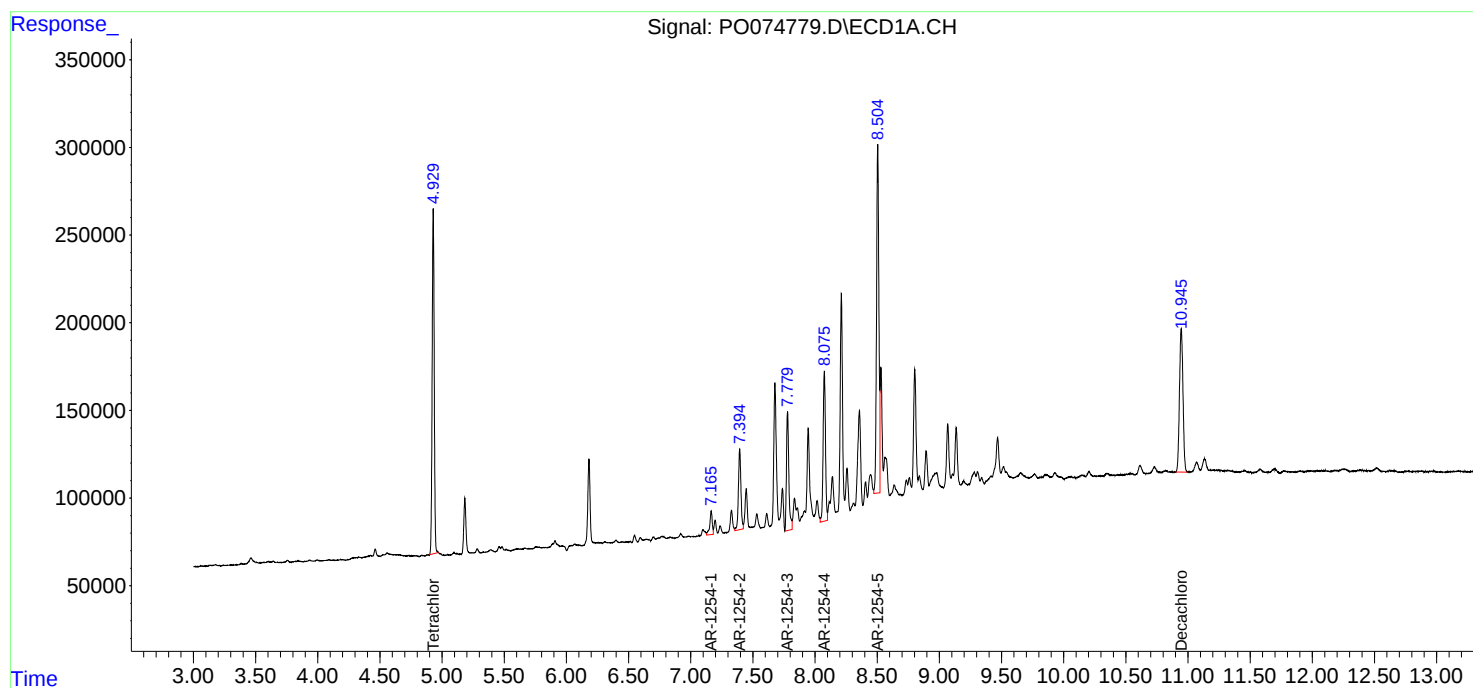

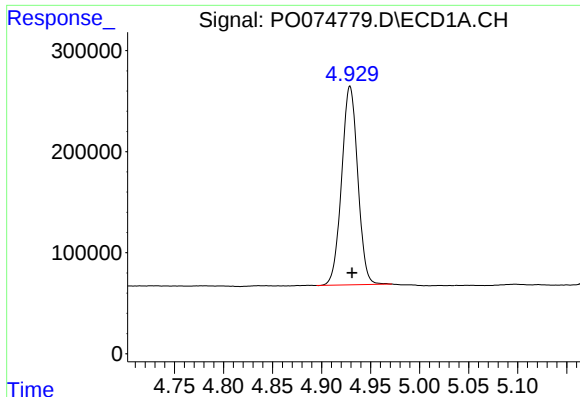


#1 Tetrachloro-m-xylene

R.T.: 4.929 min
Delta R.T.: -0.002 min
Response: 2249930
Conc: 21.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
S5-05-C


Manual Integrations
APPROVED

Ankita
1/18/2021 12:53:13 PM

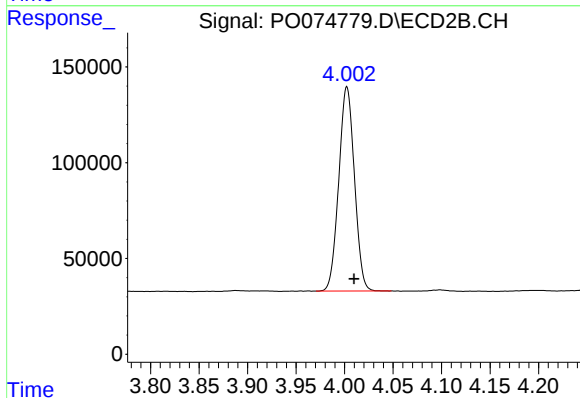


#1 Tetrachloro-m-xylene

R.T.: 4.002 min
Delta R.T.: -0.007 min
Response: 1198568
Conc: 21.31 ng/ml

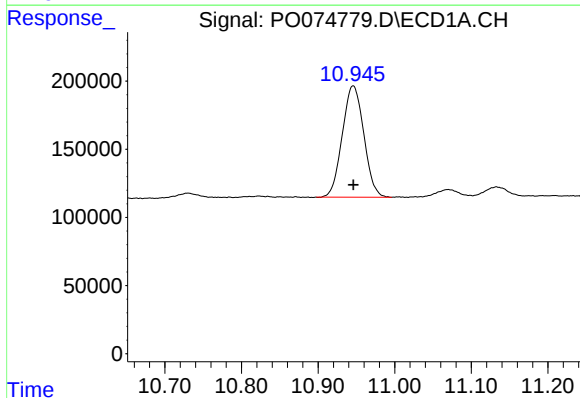


#2 Decachlorobiphenyl

R.T.: 10.946 min
Delta R.T.: 0.000 min
Response: 1601174
Conc: 15.78 ng/ml

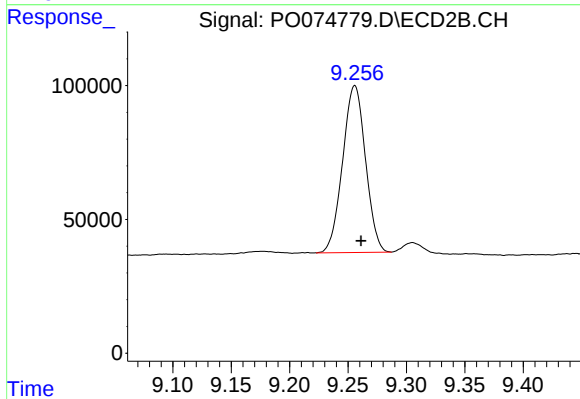

#2 Decachlorobiphenyl

R.T.: 9.256 min
Delta R.T.: -0.006 min
Response: 850312
Conc: 15.49 ng/ml

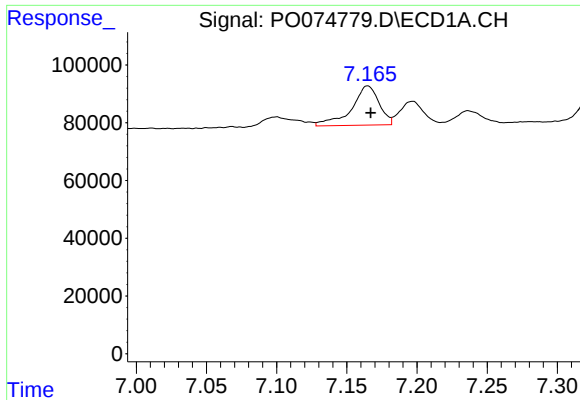


#26 AR-1254-1

R.T.: 7.165 min
Delta R.T.: -0.002 min
Response: 185185
Conc: 42.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
S5-05-C


Manual Integrations
APPROVED

Ankita
1/18/2021 12:53:13 PM

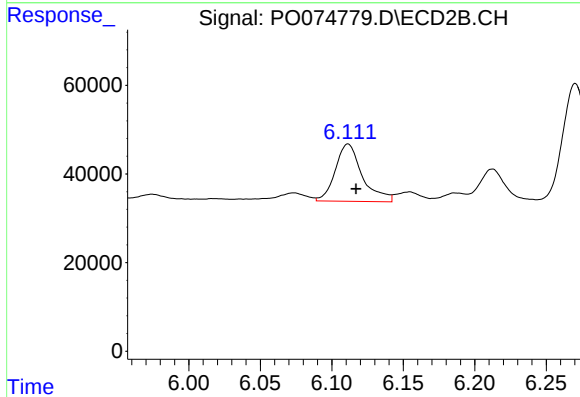


#26 AR-1254-1

R.T.: 6.111 min
Delta R.T.: -0.006 min
Response: 169842
Conc: 47.02 ng/ml

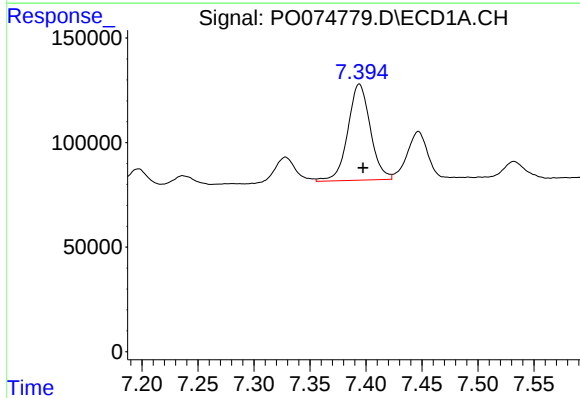


#27 AR-1254-2

R.T.: 7.394 min
Delta R.T.: -0.003 min
Response: 643090
Conc: 94.42 ng/ml

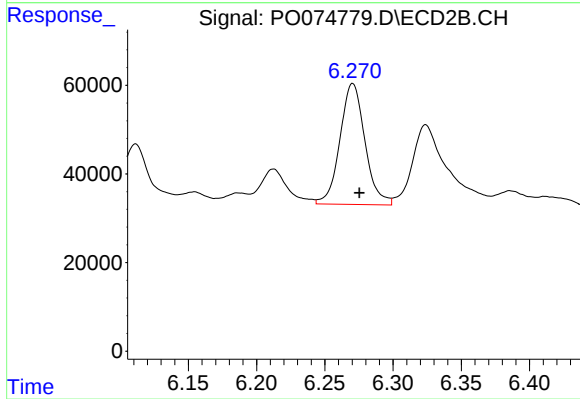

#27 AR-1254-2

R.T.: 6.270 min
Delta R.T.: -0.005 min
Response: 348355
Conc: 111.78 ng/ml

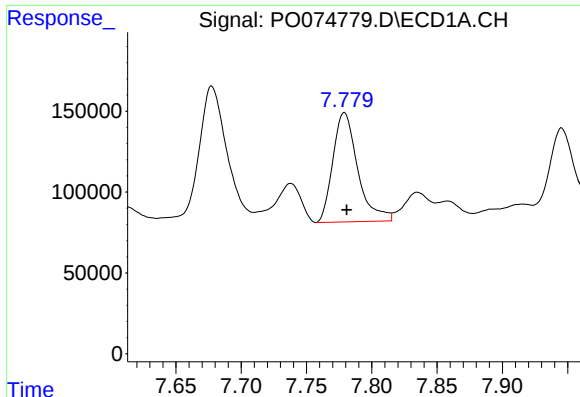


#28 AR-1254-3

R.T.: 7.779 min
Delta R.T.: -0.002 min
Response: 897894
Conc: 128.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
S5-05-C


Manual Integrations
APPROVED

Ankita
1/18/2021 12:53:13 PM

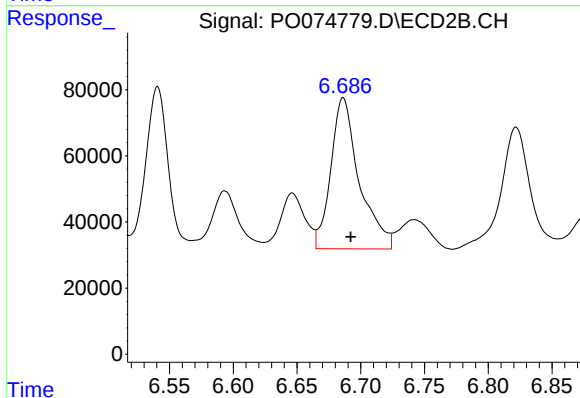


#28 AR-1254-3

R.T.: 6.686 min
Delta R.T.: -0.006 min
Response: 709951
Conc: 144.77 ng/ml

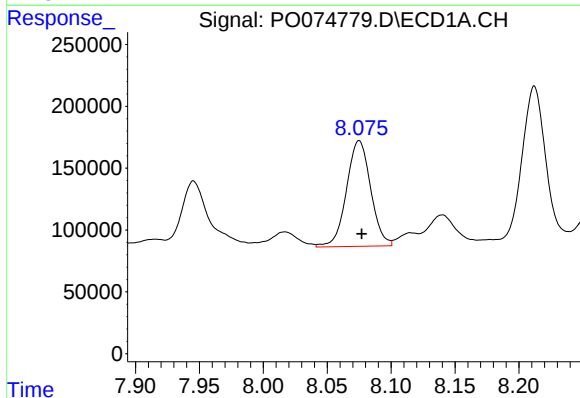


#29 AR-1254-4

R.T.: 8.075 min
Delta R.T.: -0.002 min
Response: 1126741
Conc: 185.79 ng/ml

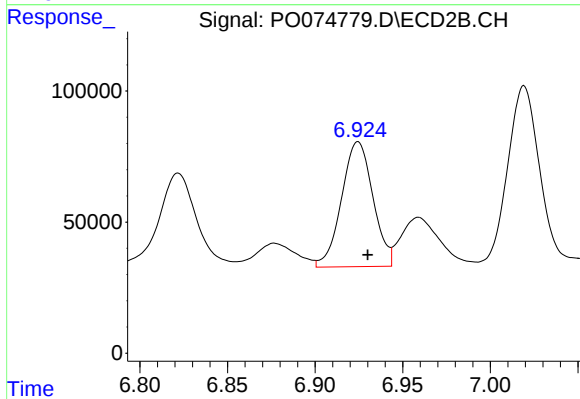

#29 AR-1254-4

R.T.: 6.925 min
Delta R.T.: -0.006 min
Response: 595008
Conc: 171.58 ng/ml

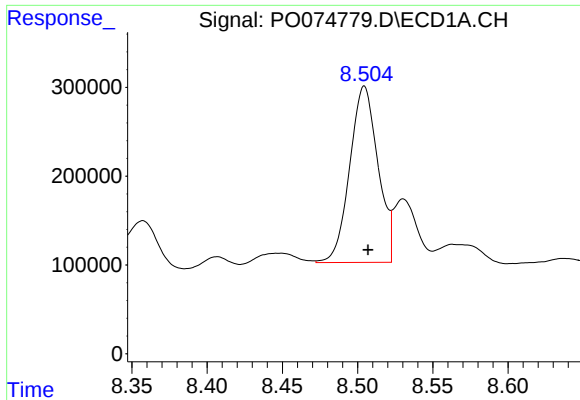


#30 AR-1254-5

R.T.: 8.504 min
Delta R.T.: -0.003 min
Response: 2609564
Conc: 449.23 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S5-05-C

Manual Integrations
APPROVED

Ankita
1/18/2021 12:53:13 PM

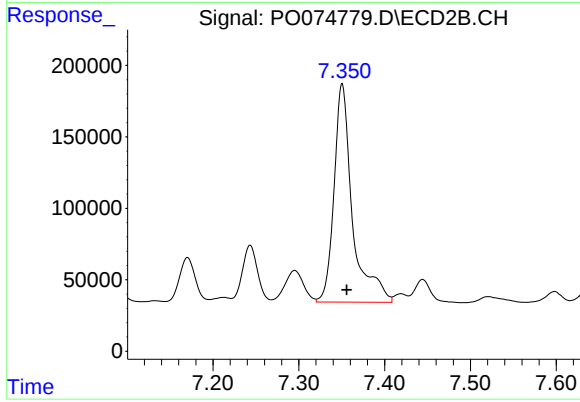

#30 AR-1254-5

R.T.: 7.351 min
Delta R.T.: -0.005 min
Response: 2283984
Conc: 504.64 ng/ml