

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011521\
 Data File : P0074827.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Jan 2021 14:21
 Operator : AJ/MA
 Sample : M1139-01
 Misc :
 ALS Vial : 84 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PL-01-011421

Manual Integrations
 APPROVED

Ankita
 1/18/2021 12:54:13 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 00:42:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.931	4.003	2201938	1235687	20.868m	21.967
2) SA Decachlor...	10.954	9.259	2157785	1024776	21.261	18.665
Target Compounds						
31) L7 AR-1260-1	7.948	6.823	172320	169669	34.542	53.183 #
32) L7 AR-1260-2	8.216	7.021	698496	120415	102.688	28.326 #
33) L7 AR-1260-3	8.582	7.173	134383	134266	23.446	37.260m#
34) L7 AR-1260-4	8.811	7.653	149856	80451	27.389m	25.692
35) L7 AR-1260-5	9.139	7.899	284026	180426	22.731	22.699

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011521\
Data File : PO074827.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Jan 2021 14:21
Operator : AJ/MA
Sample : M1139-01
Misc :
ALS Vial : 84 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
PL-01-011421


Manual Integrations
APPROVED

Ankita
1/18/2021 12:54:13 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 00:42:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

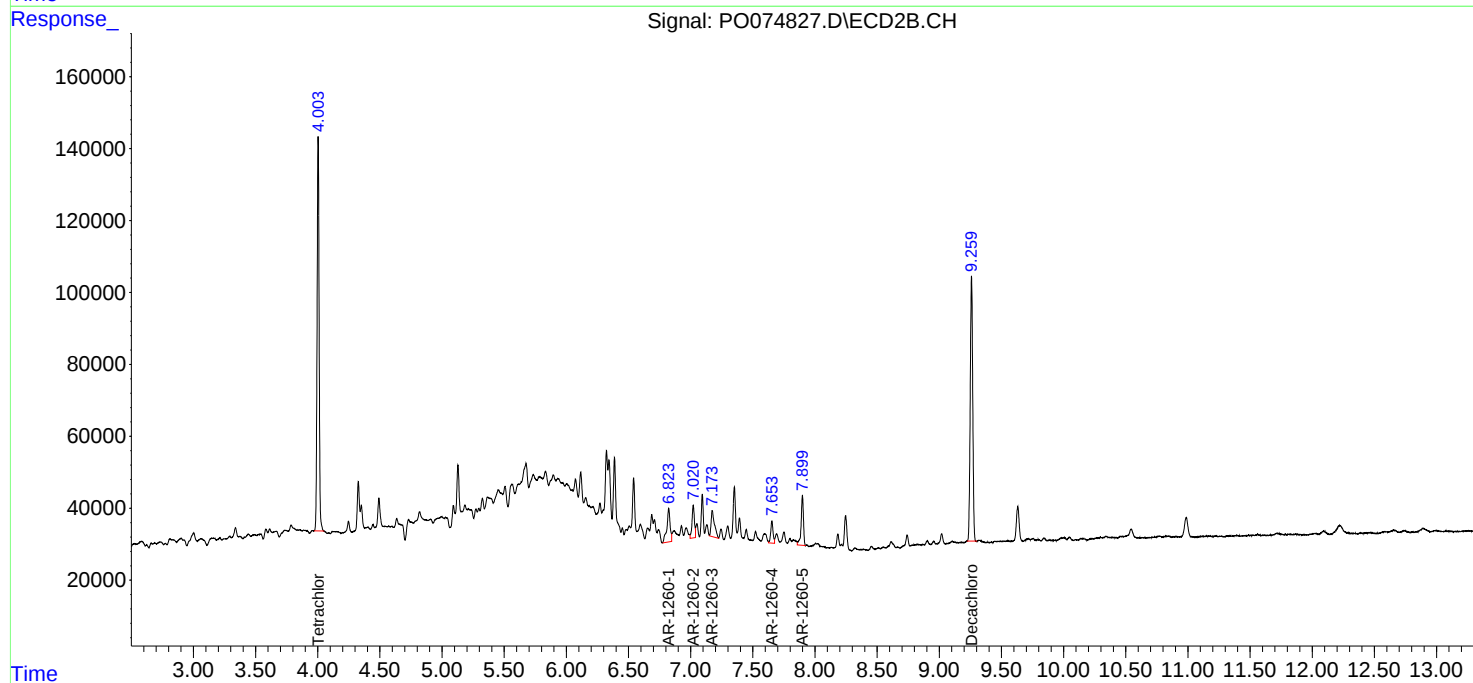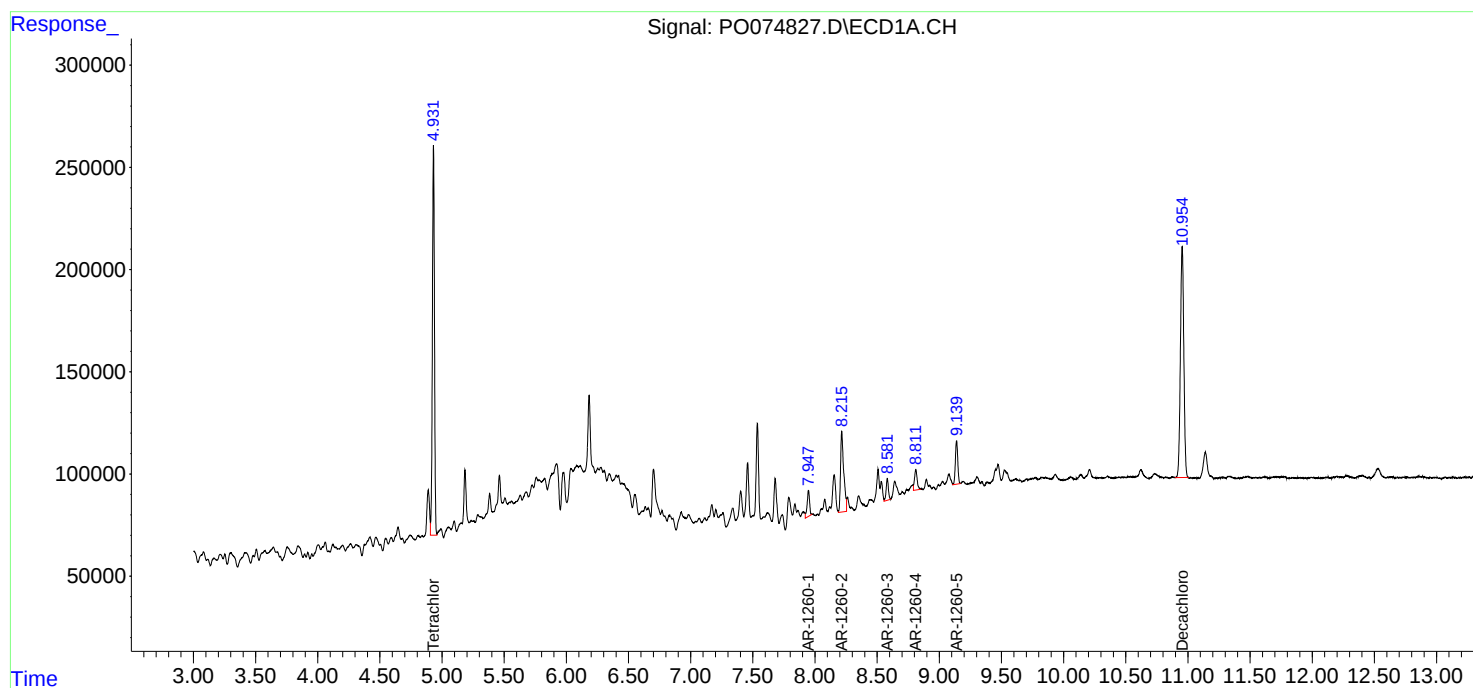

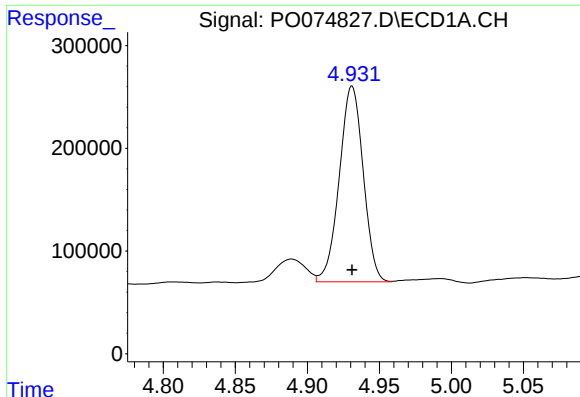


#1 Tetrachloro-m-xylene

R.T.: 4.931 min
Delta R.T.: 0.000 min
Response: 2201938
Conc: 20.87 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PL-01-011421


Manual Integrations
APPROVED

Ankita
1/18/2021 12:54:13 PM

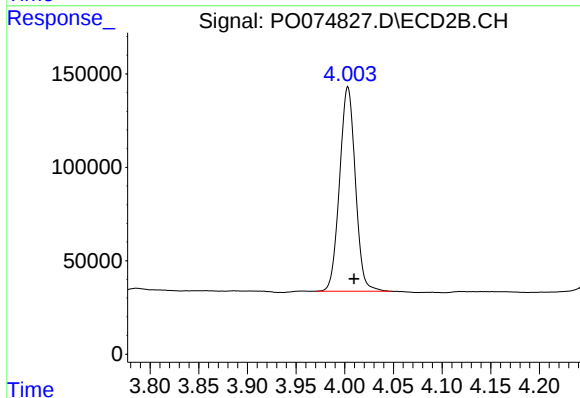


#1 Tetrachloro-m-xylene

R.T.: 4.003 min
Delta R.T.: -0.006 min
Response: 1235687
Conc: 21.97 ng/ml

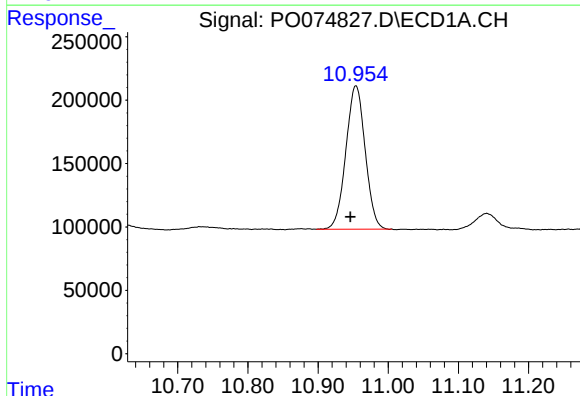


#2 Decachlorobiphenyl

R.T.: 10.954 min
Delta R.T.: 0.008 min
Response: 2157785
Conc: 21.26 ng/ml

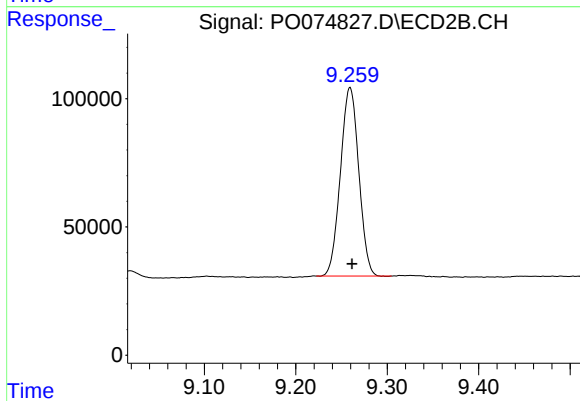

#2 Decachlorobiphenyl

R.T.: 9.259 min
Delta R.T.: -0.002 min
Response: 1024776
Conc: 18.66 ng/ml

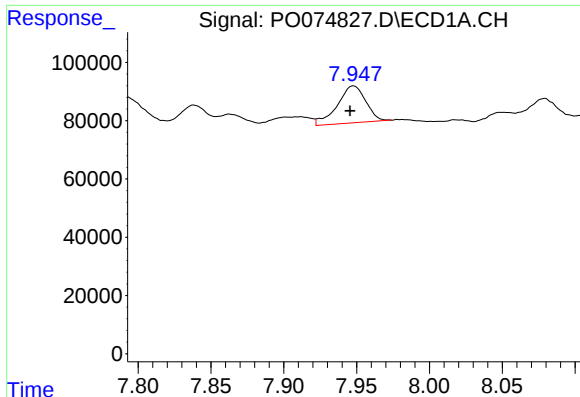


#31 AR-1260-1

R.T.: 7.948 min
Delta R.T.: 0.002 min
Response: 172320
Conc: 34.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
PL-01-011421


Manual Integrations
APPROVED

Ankita
1/18/2021 12:54:13 PM

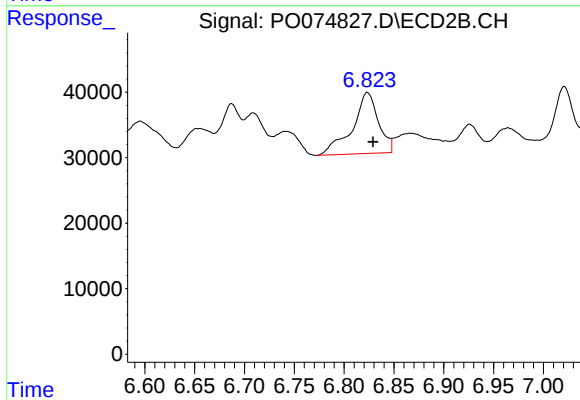


#31 AR-1260-1

R.T.: 6.823 min
Delta R.T.: -0.006 min
Response: 169669
Conc: 53.18 ng/ml

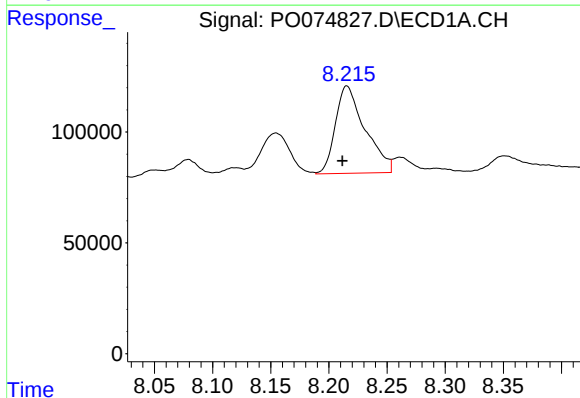


#32 AR-1260-2

R.T.: 8.216 min
Delta R.T.: 0.004 min
Response: 698496
Conc: 102.69 ng/ml

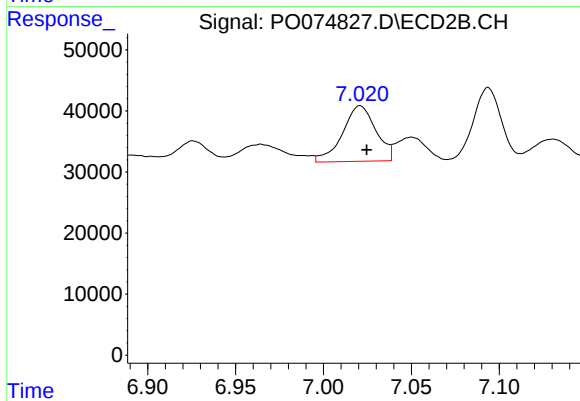

#32 AR-1260-2

R.T.: 7.021 min
Delta R.T.: -0.004 min
Response: 120415
Conc: 28.33 ng/ml

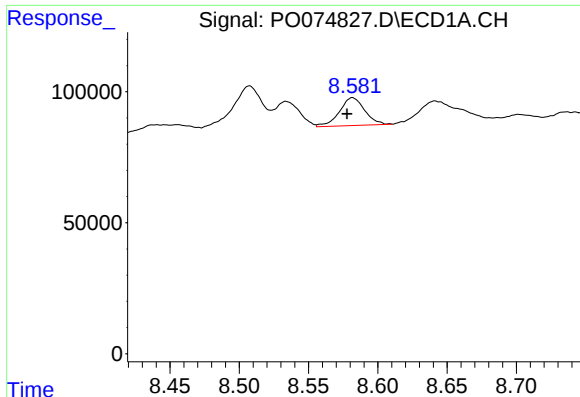


#33 AR-1260-3

R.T.: 8.582 min
Delta R.T.: 0.004 min
Response: 134383
Conc: 23.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
PL-01-011421


Manual Integrations
APPROVED

Ankita
1/18/2021 12:54:13 PM

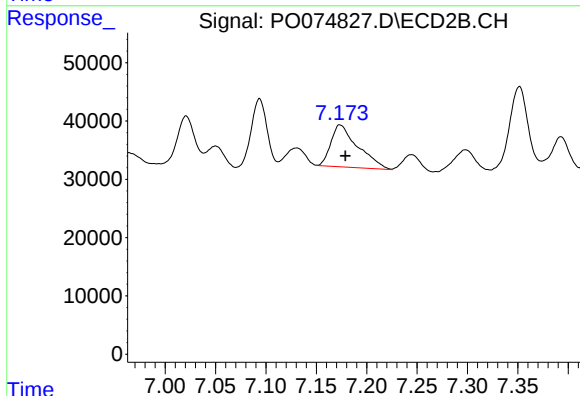


#33 AR-1260-3

R.T.: 7.173 min
Delta R.T.: -0.006 min
Response: 134266
Conc: 37.26 ng/ml m

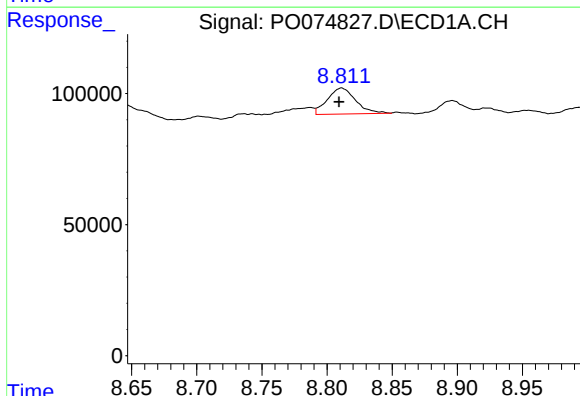


#34 AR-1260-4

R.T.: 8.811 min
Delta R.T.: 0.002 min
Response: 149856
Conc: 27.39 ng/ml m

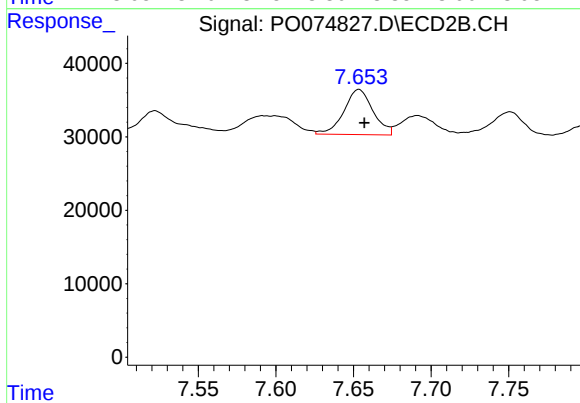

#34 AR-1260-4

R.T.: 7.653 min
Delta R.T.: -0.003 min
Response: 80451
Conc: 25.69 ng/ml

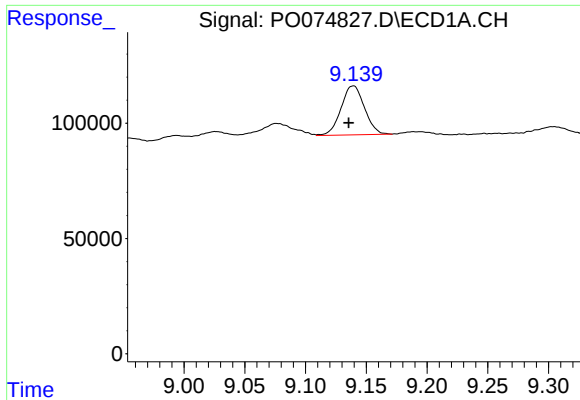


#35 AR-1260-5

R.T.: 9.139 min
Delta R.T.: 0.004 min
Response: 284026
Conc: 22.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
PL-01-011421

Manual Integrations
APPROVED

Ankita
1/18/2021 12:54:13 PM

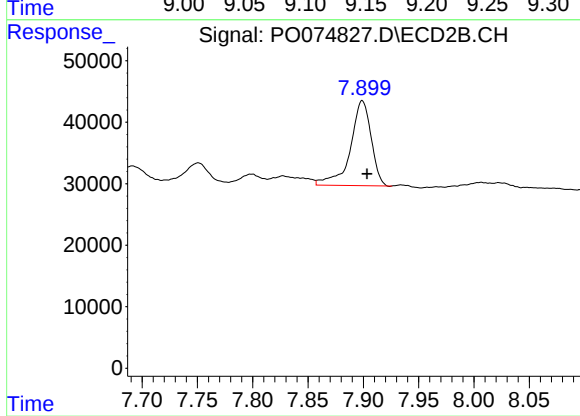

#35 AR-1260-5

R.T.: 7.899 min
Delta R.T.: -0.004 min
Response: 180426
Conc: 22.70 ng/ml