

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011521\
 Data File : P0074831.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Jan 2021 15:30
 Operator : AJ/MA
 Sample : M1141-22
 Misc :
 ALS Vial : 88 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ETGI-354

Manual Integrations
 APPROVED

Ankita
 1/18/2021 12:53:57 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 00:44:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.931	4.003	2034384	1106816	19.280	19.676
2) SA Decachlor...	10.955	9.259	1956664	962463	19.279	17.530
Target Compounds						
31) L7 AR-1260-1	7.948	6.824	119893	89997	24.033	28.210
32) L7 AR-1260-2	8.214	7.021	496182	107398	72.945	25.264 #
33) L7 AR-1260-3	8.581	7.173	149415	100607	26.068	27.920m
34) L7 AR-1260-4	8.813	7.653	178756	85305	32.672	27.243
35) L7 AR-1260-5	9.139	7.900	290575	200626	23.255	25.240

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011521\
Data File : PO074831.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Jan 2021 15:30
Operator : AJ/MA
Sample : M1141-22
Misc :
ALS Vial : 88 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
ETGI-354


Manual Integrations
APPROVED

Ankita
1/18/2021 12:53:57 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 00:44:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

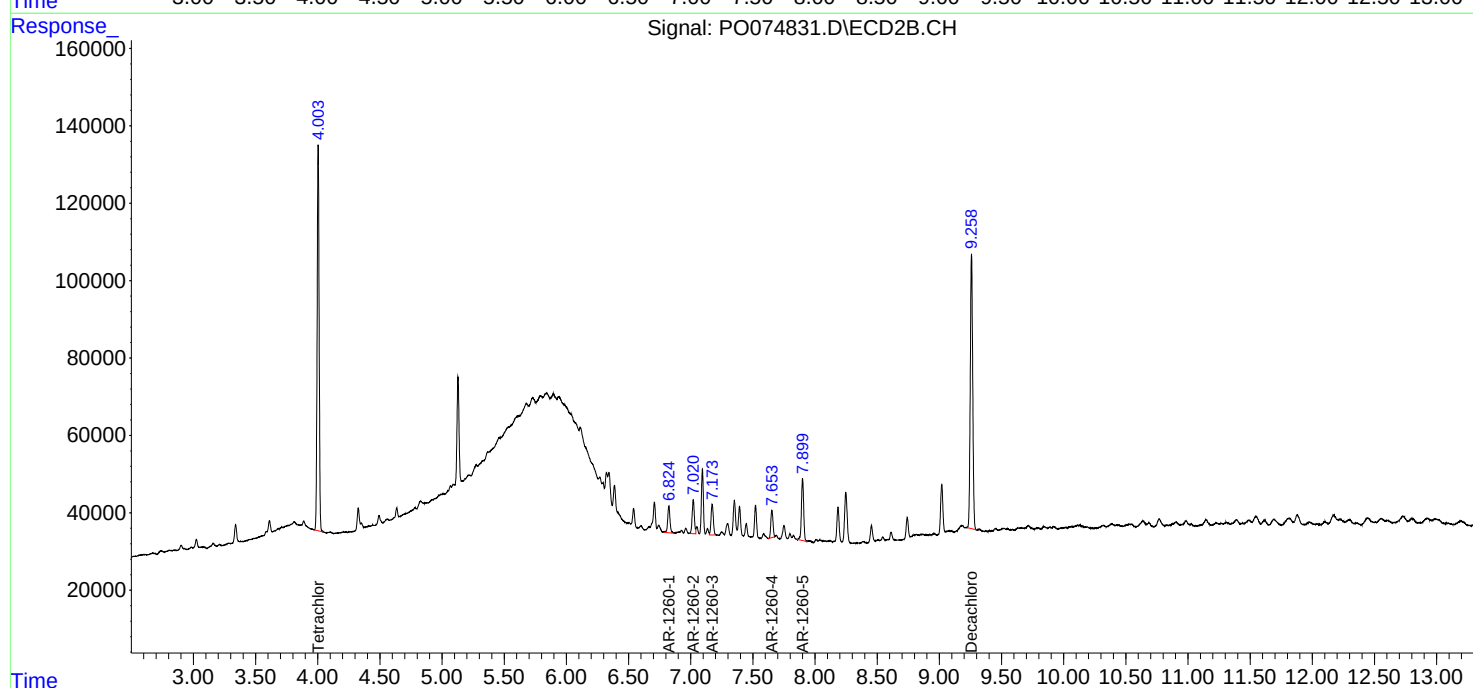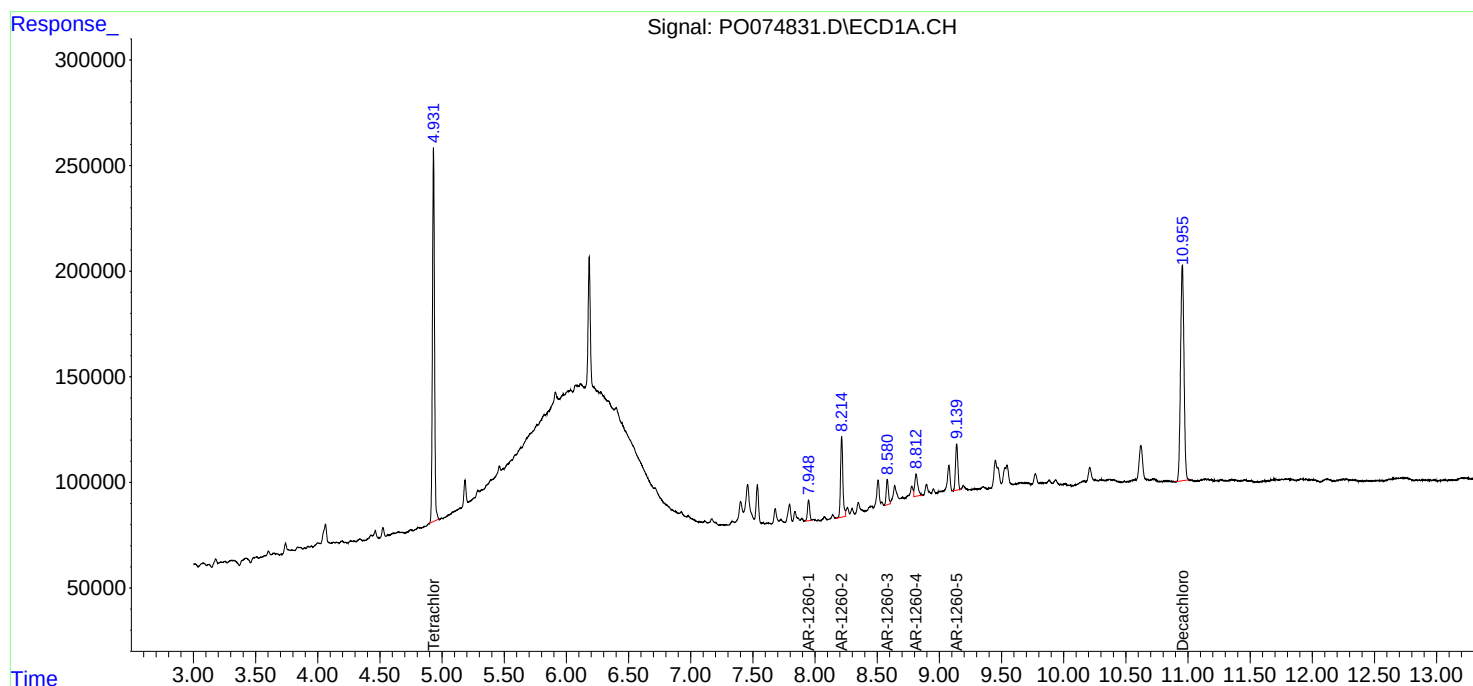

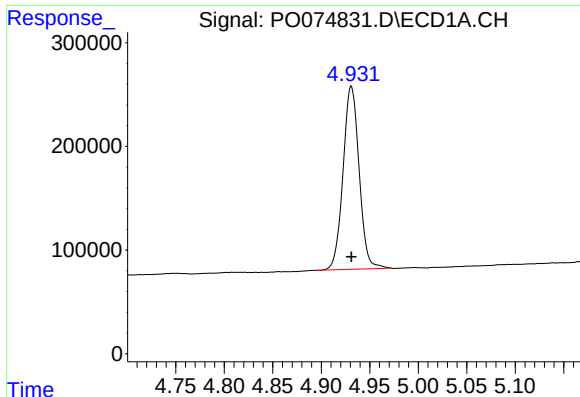


#1 Tetrachloro-m-xylene

R.T.: 4.931 min
Delta R.T.: 0.000 min
Response: 2034384
Conc: 19.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
ETGI-354


Manual Integrations
APPROVED

Ankita
1/18/2021 12:53:57 PM

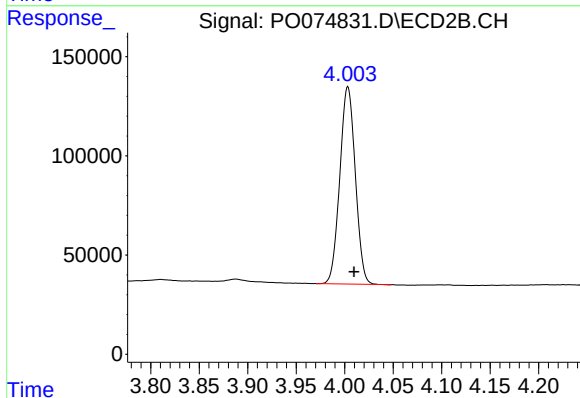


#1 Tetrachloro-m-xylene

R.T.: 4.003 min
Delta R.T.: -0.006 min
Response: 1106816
Conc: 19.68 ng/ml

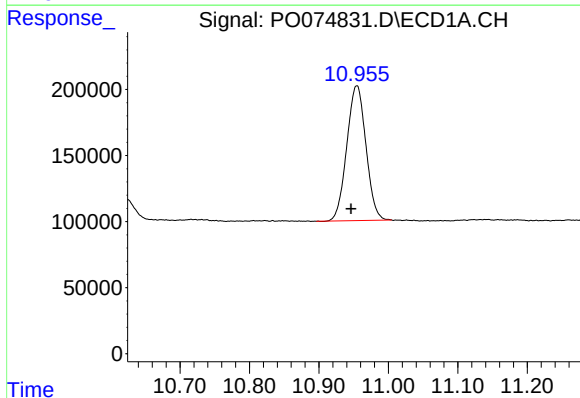


#2 Decachlorobiphenyl

R.T.: 10.955 min
Delta R.T.: 0.008 min
Response: 1956664
Conc: 19.28 ng/ml

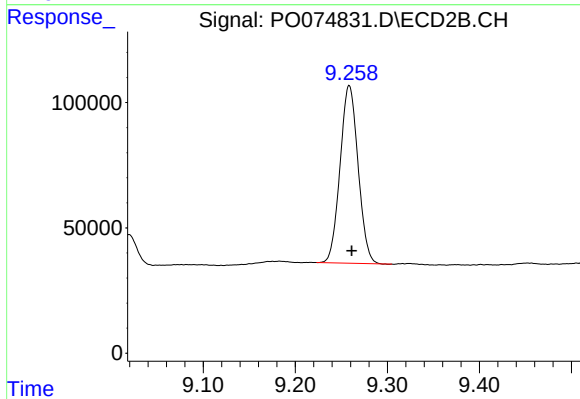

#2 Decachlorobiphenyl

R.T.: 9.259 min
Delta R.T.: -0.003 min
Response: 962463
Conc: 17.53 ng/ml

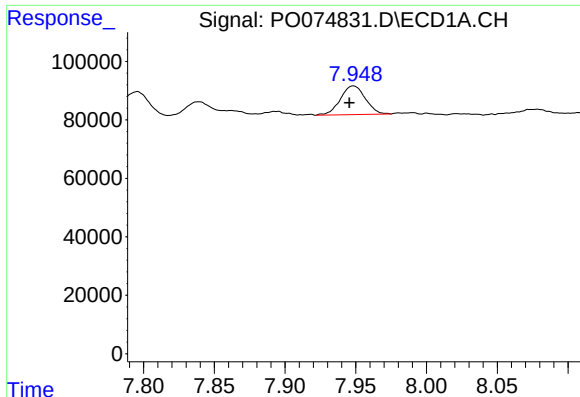


#31 AR-1260-1

R.T.: 7.948 min
Delta R.T.: 0.003 min
Response: 119893
Conc: 24.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
ETGI-354


Manual Integrations
APPROVED

Ankita
1/18/2021 12:53:57 PM

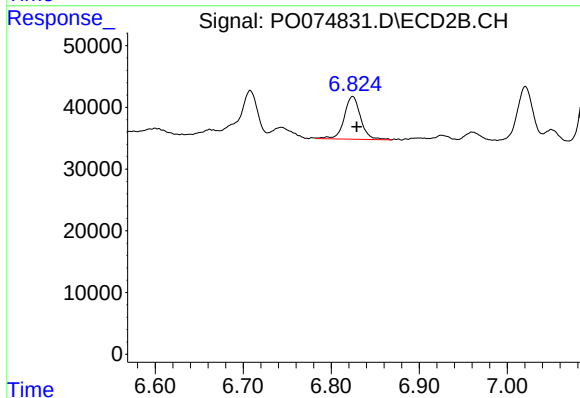


#31 AR-1260-1

R.T.: 6.824 min
Delta R.T.: -0.004 min
Response: 89997
Conc: 28.21 ng/ml

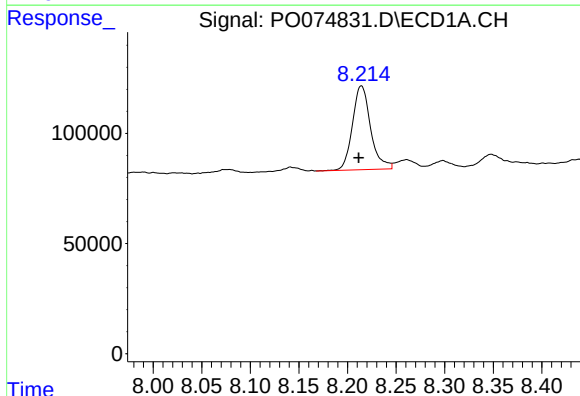


#32 AR-1260-2

R.T.: 8.214 min
Delta R.T.: 0.003 min
Response: 496182
Conc: 72.95 ng/ml

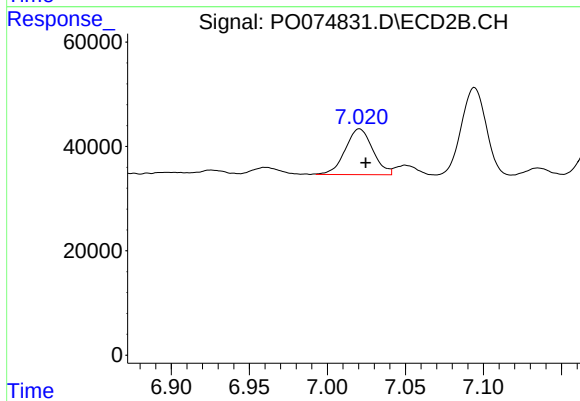

#32 AR-1260-2

R.T.: 7.021 min
Delta R.T.: -0.004 min
Response: 107398
Conc: 25.26 ng/ml

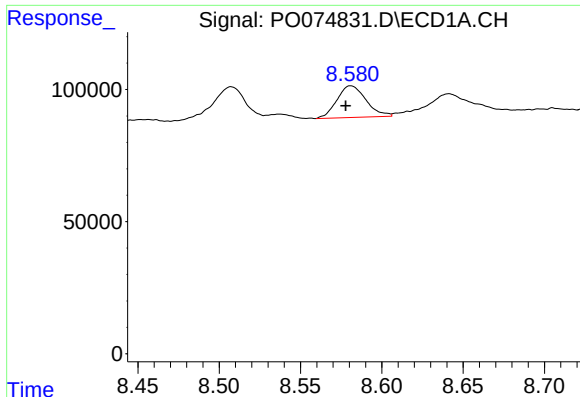


#33 AR-1260-3

R.T.: 8.581 min
Delta R.T.: 0.003 min
Response: 149415
Conc: 26.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
ETGI-354


Manual Integrations
APPROVED

Ankita
1/18/2021 12:53:57 PM

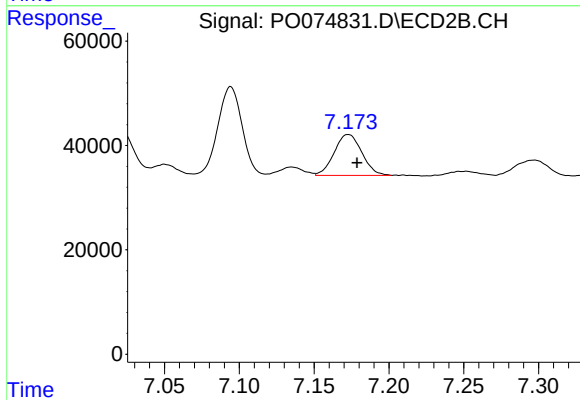


#33 AR-1260-3

R.T.: 7.173 min
Delta R.T.: -0.006 min
Response: 100607
Conc: 27.92 ng/ml m

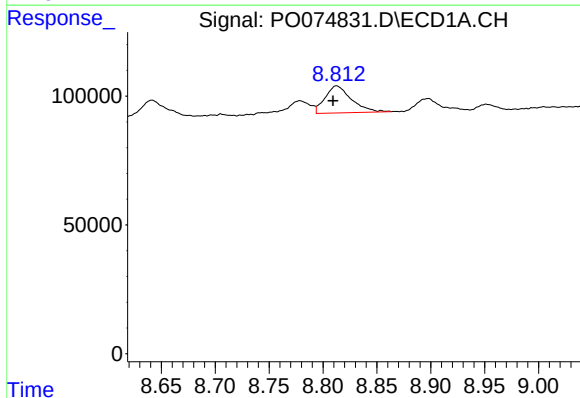


#34 AR-1260-4

R.T.: 8.813 min
Delta R.T.: 0.003 min
Response: 178756
Conc: 32.67 ng/ml

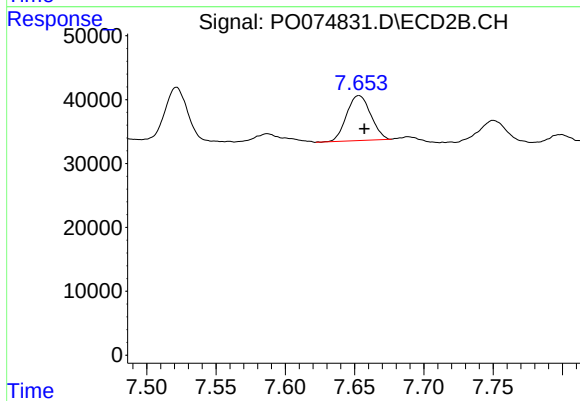

#34 AR-1260-4

R.T.: 7.653 min
Delta R.T.: -0.004 min
Response: 85305
Conc: 27.24 ng/ml

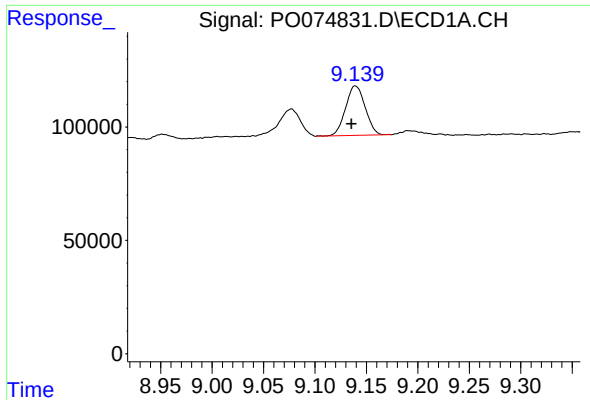


#35 AR-1260-5

R.T.: 9.139 min
Delta R.T.: 0.004 min
Response: 290575
Conc: 23.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
ETGI-354

Manual Integrations
APPROVED

Ankita
1/18/2021 12:53:57 PM

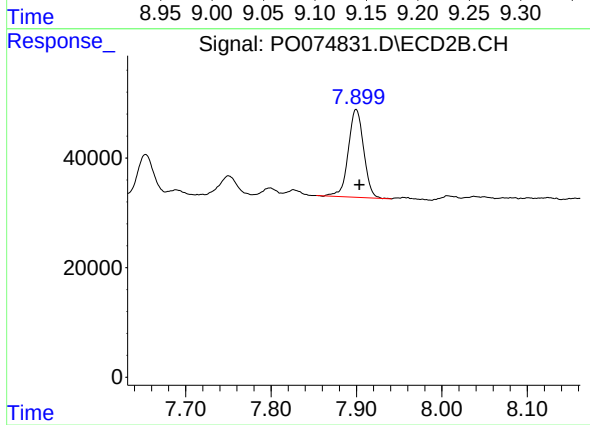

#35 AR-1260-5

R.T.: 7.900 min
Delta R.T.: -0.004 min
Response: 200626
Conc: 25.24 ng/ml