

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\P0011521\  
 Data File : P0074840.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 16 Jan 2021 18:21  
 Operator : AJ/MA  
 Sample : M1153-01  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 FK-PS-01-068

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jan 18 00:49:28 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\P0011121.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Jan 12 06:02:45 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1   | RT#2  | Resp#1  | Resp#2  | ng/ml  | ng/ml  |
|-----------------------------|--------|-------|---------|---------|--------|--------|
| -----                       |        |       |         |         |        |        |
| System Monitoring Compounds |        |       |         |         |        |        |
| 1) SA Tetrachlo...          | 4.930  | 4.002 | 2462906 | 1276228 | 23.341 | 22.688 |
| 2) SA Decachlor...          | 10.953 | 9.259 | 1642089 | 861672  | 16.179 | 15.694 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\PO011521\  
Data File : PO074840.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 16 Jan 2021 18:21  
Operator : AJ/MA  
Sample : M1153-01  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
ECD\_O  
ClientSampleId :  
FK-PS-01-068

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jan 18 00:49:28 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\PO011121.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Tue Jan 12 06:02:45 2021  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

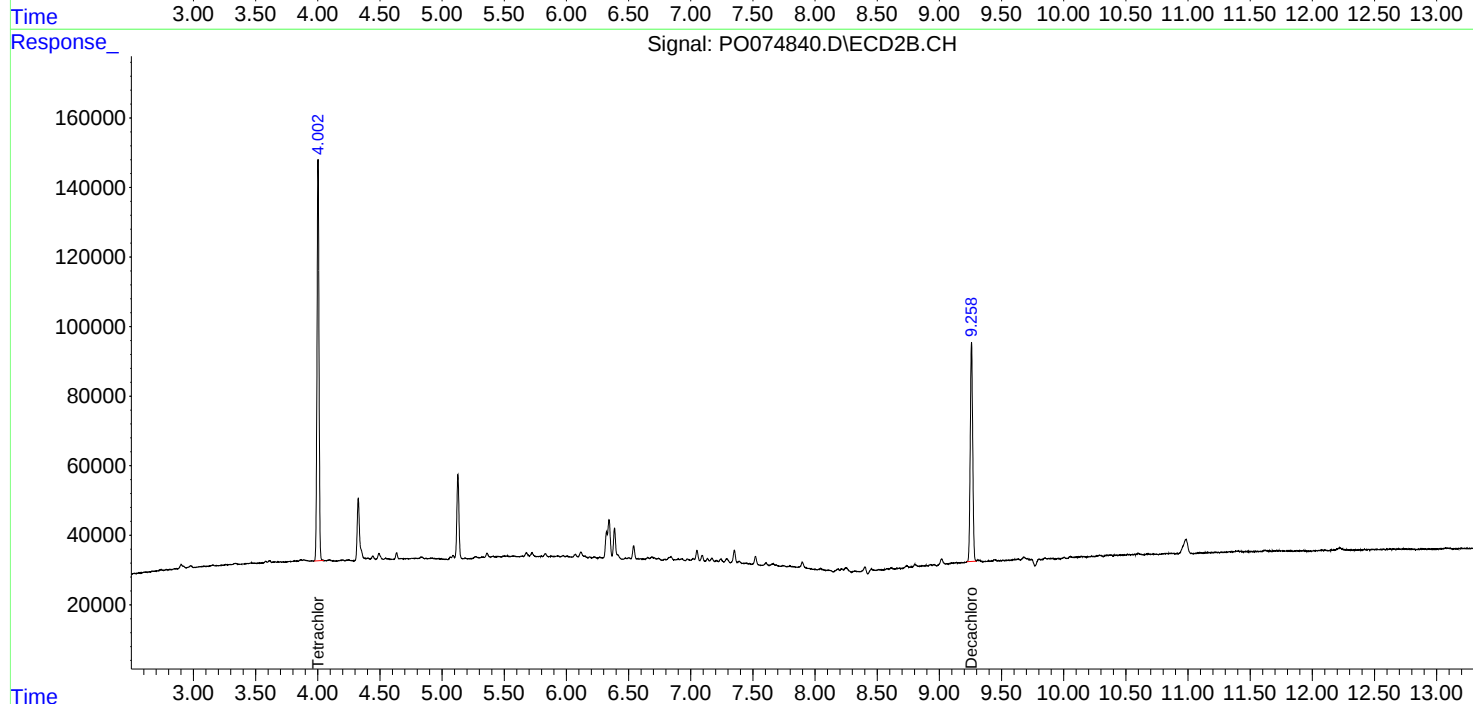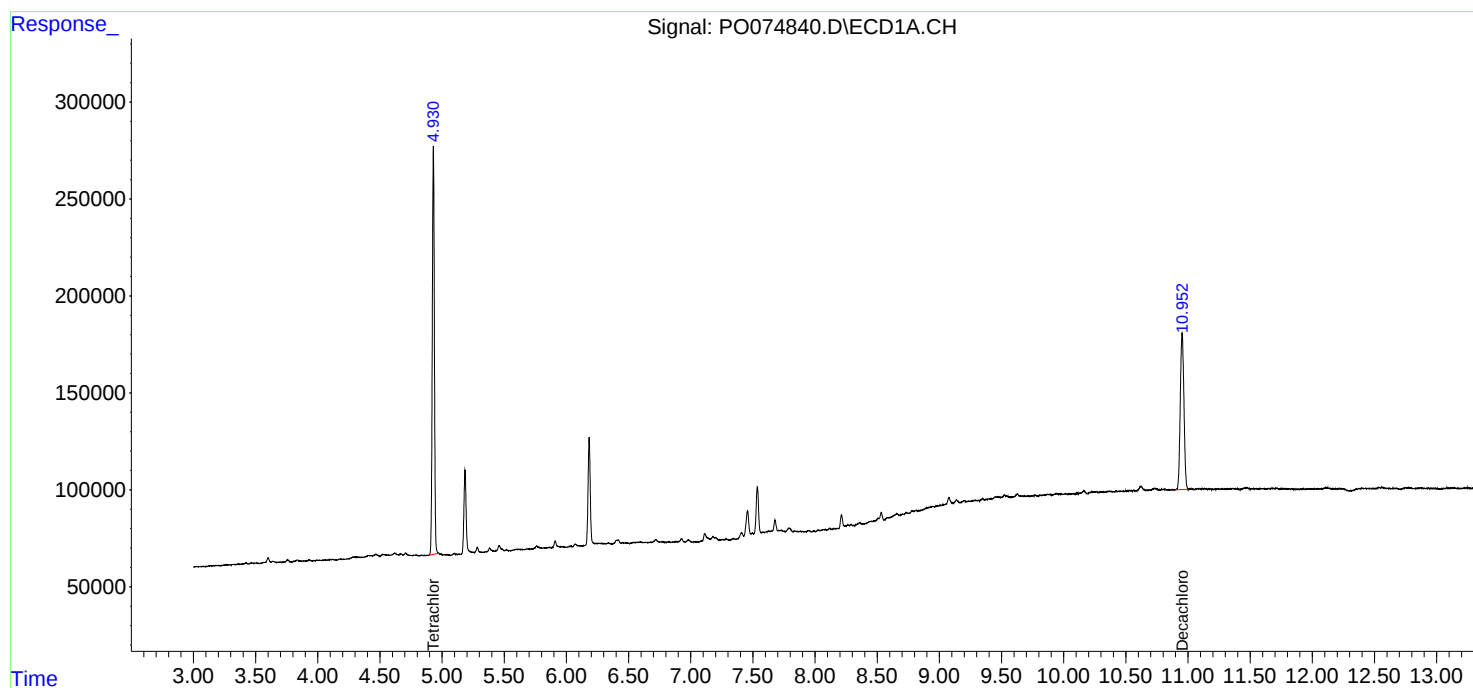


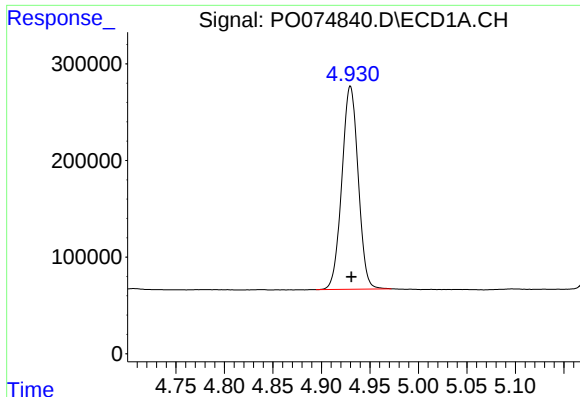

#1 Tetrachloro-m-xylene


R.T.: 4.930 min  
Delta R.T.: -0.001 min  
Response: 2462906  
Conc: 23.34 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
FK-PS-01-068

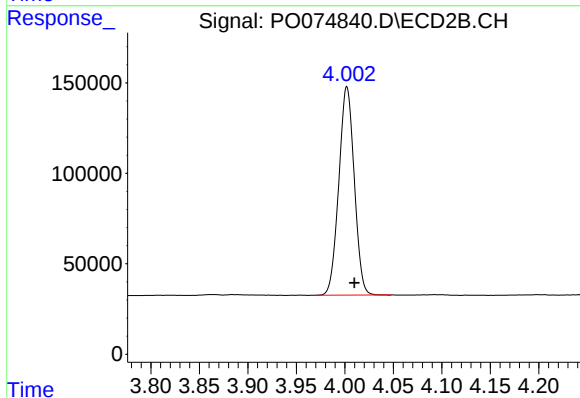


#1 Tetrachloro-m-xylene

R.T.: 4.002 min  
Delta R.T.: -0.008 min  
Response: 1276228  
Conc: 22.69 ng/ml

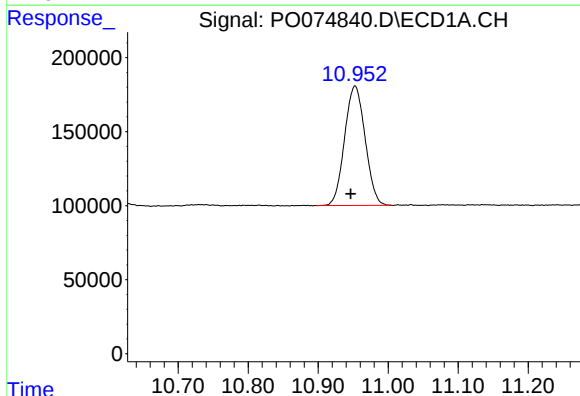

#2 Decachlorobiphenyl

R.T.: 10.953 min  
Delta R.T.: 0.006 min  
Response: 1642089  
Conc: 16.18 ng/ml

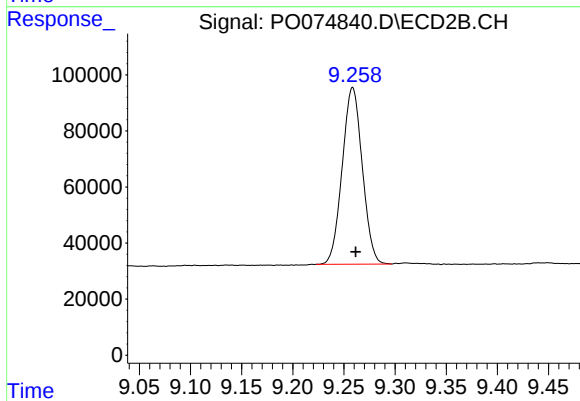

#2 Decachlorobiphenyl

R.T.: 9.259 min  
Delta R.T.: -0.003 min  
Response: 861672  
Conc: 15.69 ng/ml