

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011521\
 Data File : P0074846.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Jan 2021 20:04
 Operator : AJ/MA
 Sample : M1041-04 10X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 30712

Manual Integrations
 APPROVED

Ankita
 1/18/2021 2:36:12 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 00:51:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.930	4.003	181390	104927	1.719m	1.865
2) SA Decachlor...	10.961	9.263	172142	59389	1.696	1.082 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011521\
Data File : P0074846.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Jan 2021 20:04
Operator : AJ/MA
Sample : M1041-04 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
30712


Manual Integrations
APPROVED

Ankita
1/18/2021 2:36:12 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 00:51:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

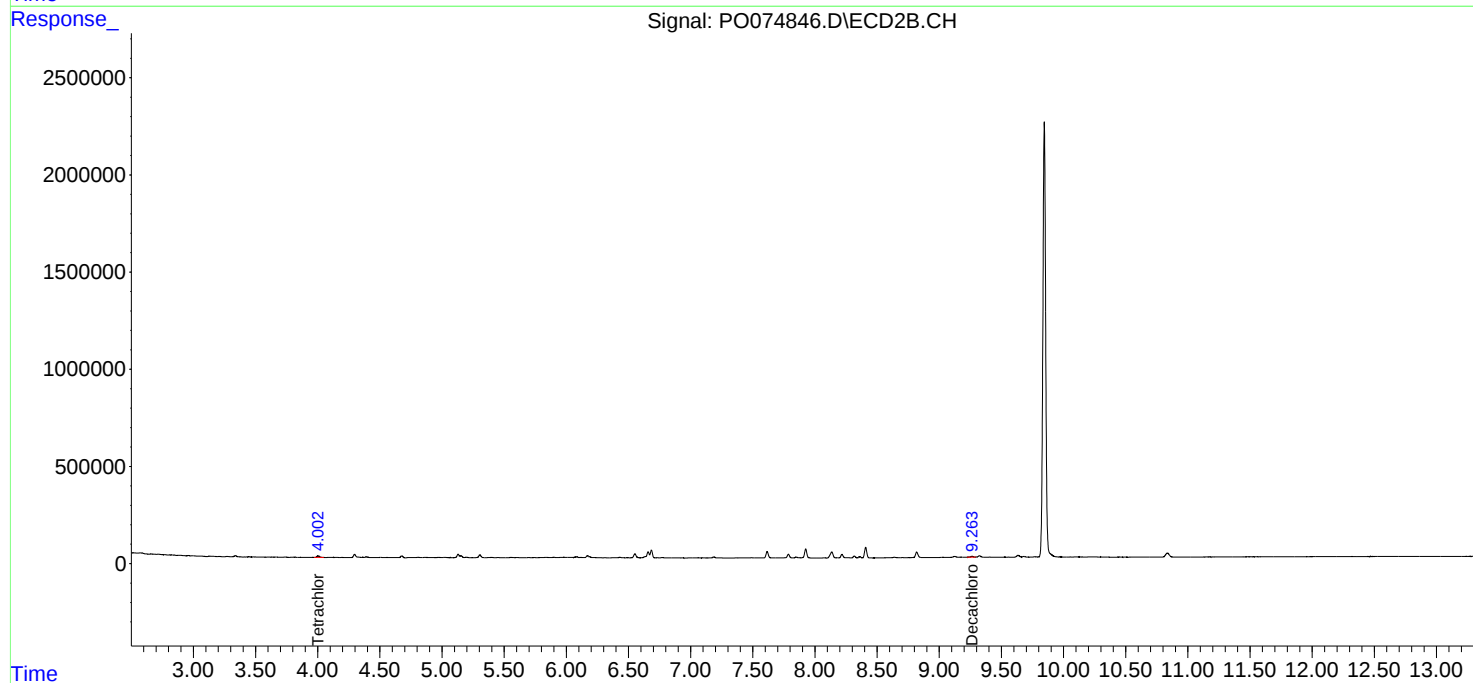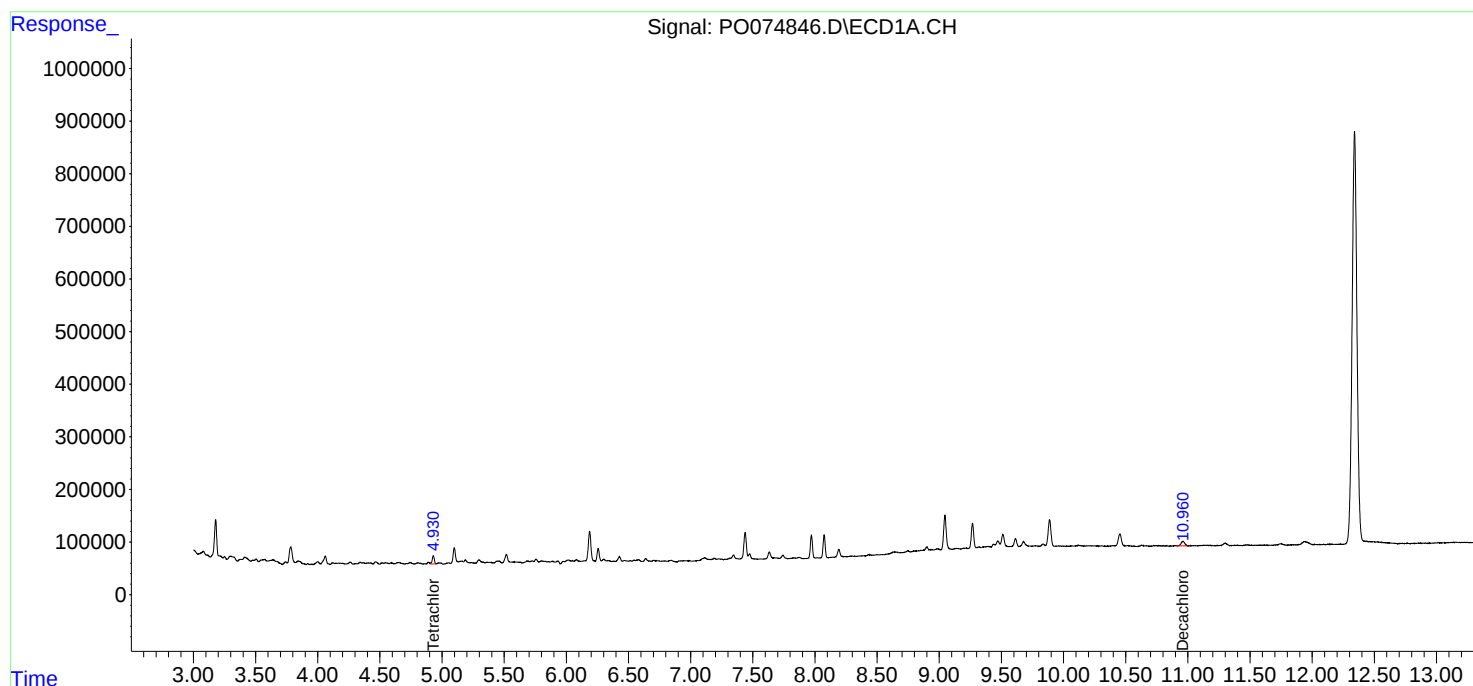

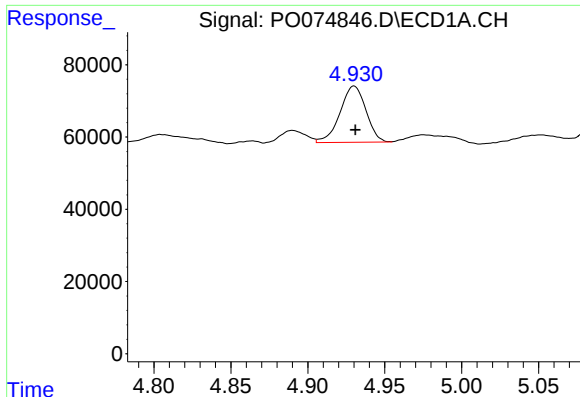


#1 Tetrachloro-m-xylene

R.T.: 4.930 min
Delta R.T.: -0.001 min
Response: 181390
Conc: 1.72 ng/ml m

Instrument :
ECD_O
ClientSampleId :
30712


Manual Integrations
APPROVED

Ankita
1/18/2021 2:36:12 PM

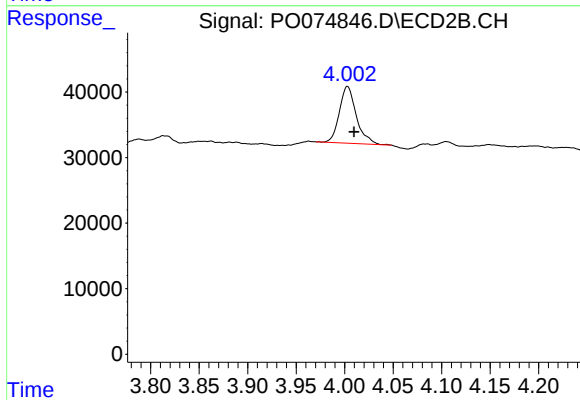


#1 Tetrachloro-m-xylene

R.T.: 4.003 min
Delta R.T.: -0.007 min
Response: 104927
Conc: 1.87 ng/ml

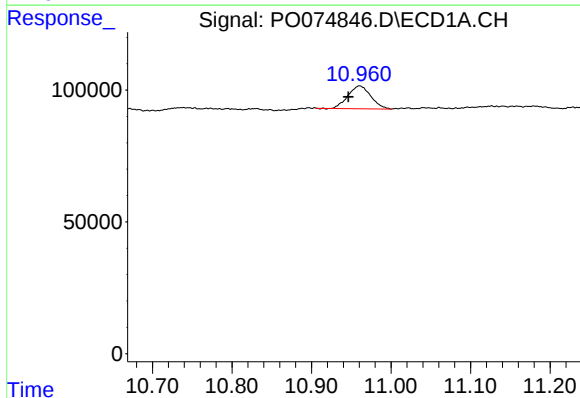

#2 Decachlorobiphenyl

R.T.: 10.961 min
Delta R.T.: 0.014 min
Response: 172142
Conc: 1.70 ng/ml

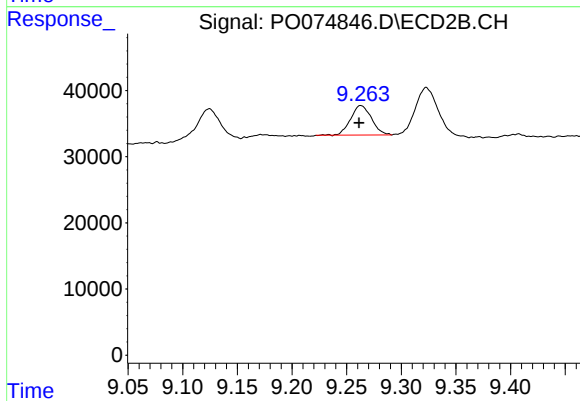

#2 Decachlorobiphenyl

R.T.: 9.263 min
Delta R.T.: 0.002 min
Response: 59389
Conc: 1.08 ng/ml