

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011524\
 Data File : P0101167.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jan 2024 14:31
 Operator : YP/AJ
 Sample : P1125-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MIXED-DEMO

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/16/2024
 Supervised By :Sohil Jodhani 01/16/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 15 20:41:25 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 11 11:52:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.341	3.637	95221868	57101716	23.508	21.661
2) SA Decachlor...	10.078	8.690	60478034	43105660	30.621m	26.101

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011524\
Data File : PO101167.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jan 2024 14:31
Operator : YP/AJ
Sample : P1125-01
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MIXED-DEMO


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/16/2024
Supervised By :Sohil Jodhani 01/16/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 15 20:41:25 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011024.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 11 11:52:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

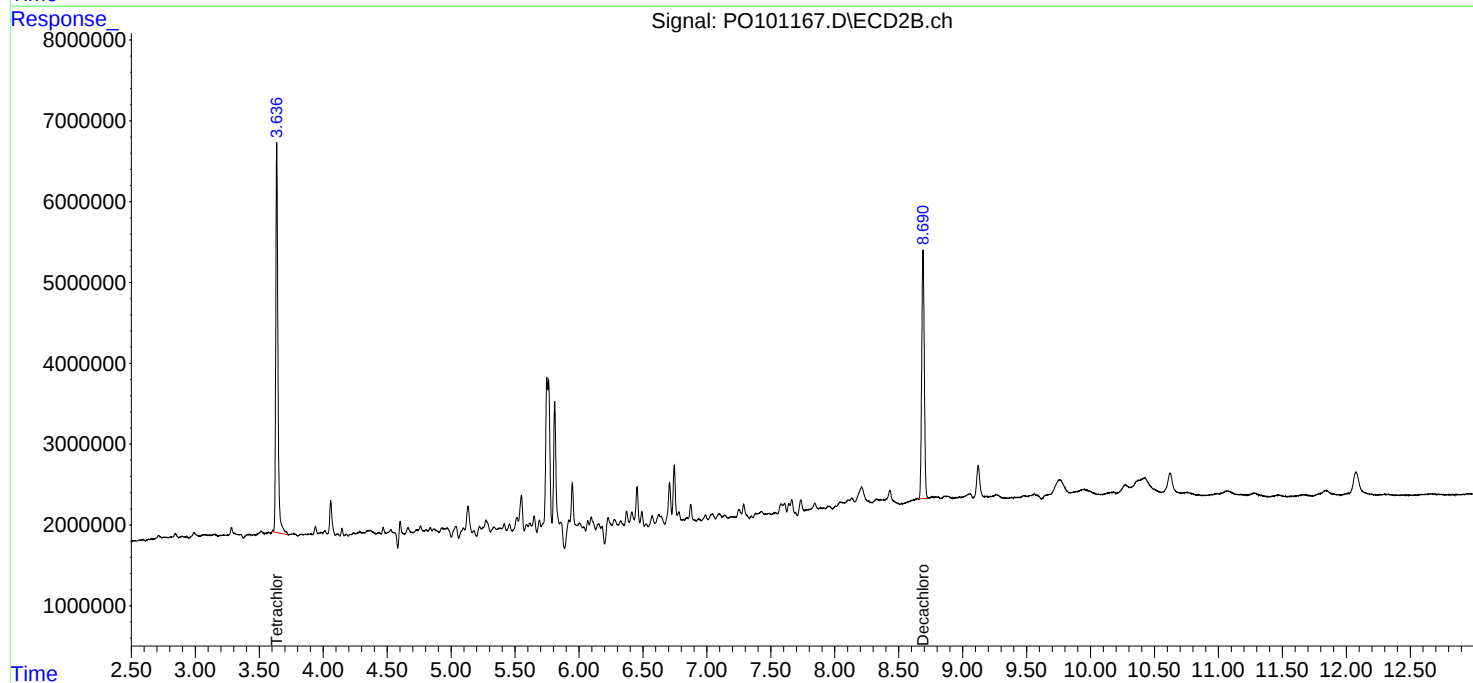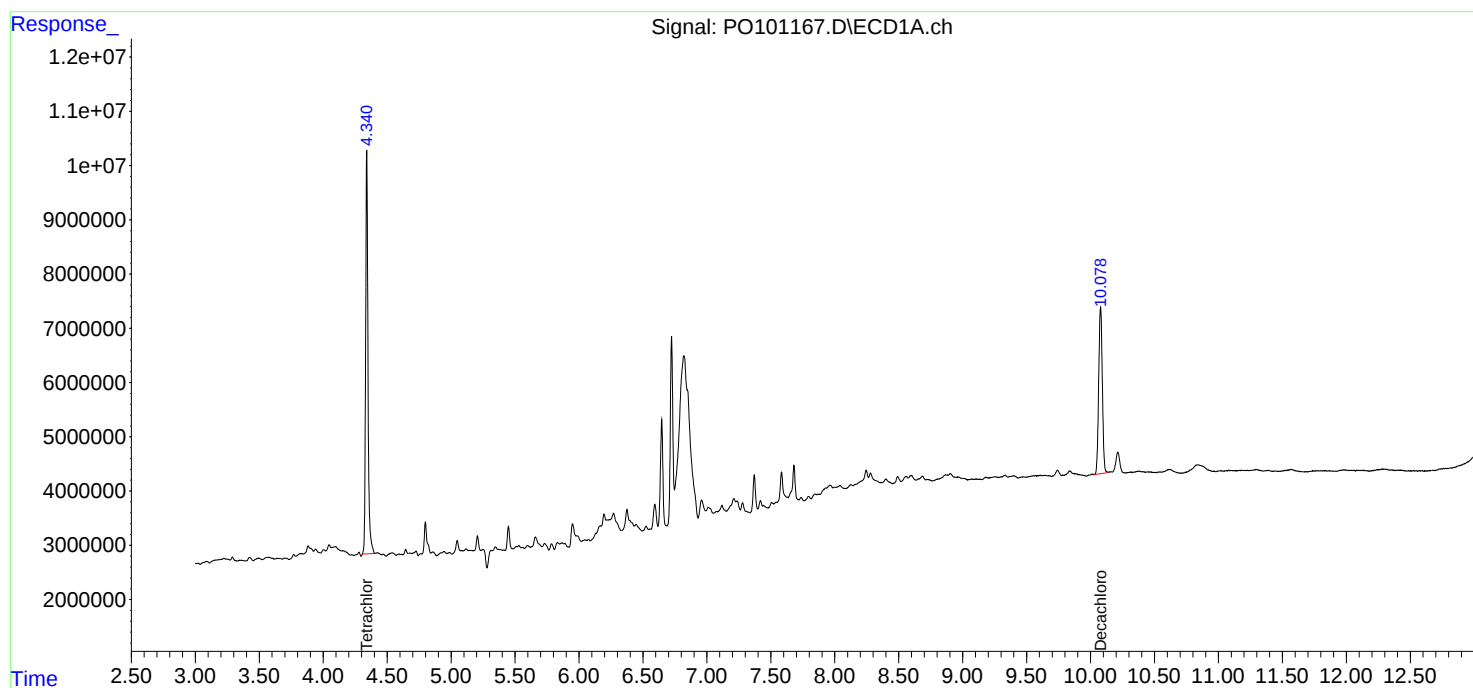

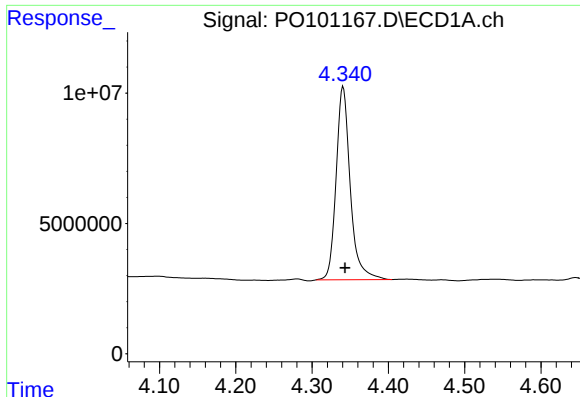

#1 Tetrachloro-m-xylene

R.T.: 4.341 min
Delta R.T.: -0.002 min
Response: 95221868
Conc: 23.51 ng/ml

Instrument :

ECD_O

ClientSampleId :


MIXED-DEMO

Manual Integrations

APPROVED


Reviewed By :Ankita Jodhani 01/16/2024

Supervised By :Sohil Jodhani 01/16/2024

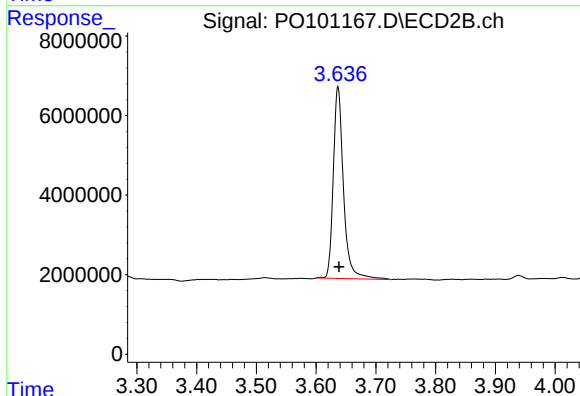


#1 Tetrachloro-m-xylene

R.T.: 3.637 min
Delta R.T.: -0.002 min
Response: 57101716
Conc: 21.66 ng/ml

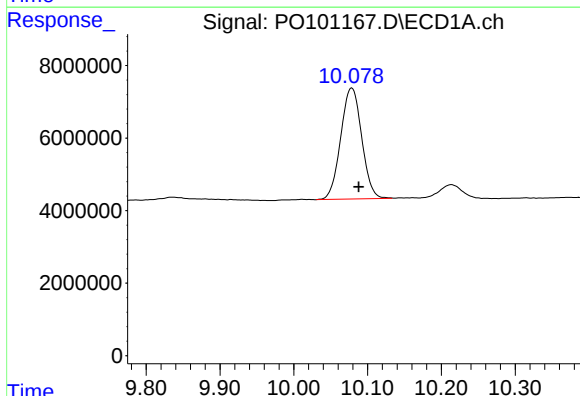

#2 Decachlorobiphenyl

R.T.: 10.078 min
Delta R.T.: -0.010 min
Response: 60478034
Conc: 30.62 ng/ml m

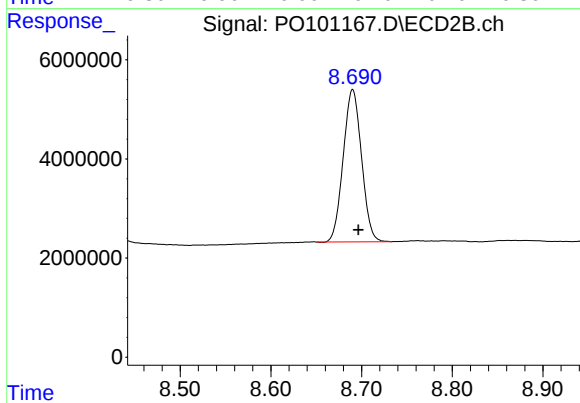

#2 Decachlorobiphenyl

R.T.: 8.690 min
Delta R.T.: -0.006 min
Response: 43105660
Conc: 26.10 ng/ml