

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011524\
 Data File : P0101187.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jan 2024 20:06
 Operator : YP/AJ
 Sample : P1079-06RE
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LS-3RE

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/16/2024
 Supervised By :Sohil Jodhani 01/16/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 15 20:58:06 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 11 11:52:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.339	3.635	5335112	1951236	1.317	0.740m#
2) SA Decachlor...	10.082	8.678	953515	1612012	0.483	0.976 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011524\
Data File : PO101187.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jan 2024 20:06
Operator : YP/AJ
Sample : P1079-06RE
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LS-3RE


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/16/2024
Supervised By :Sohil Jodhani 01/16/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 15 20:58:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011024.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 11 11:52:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

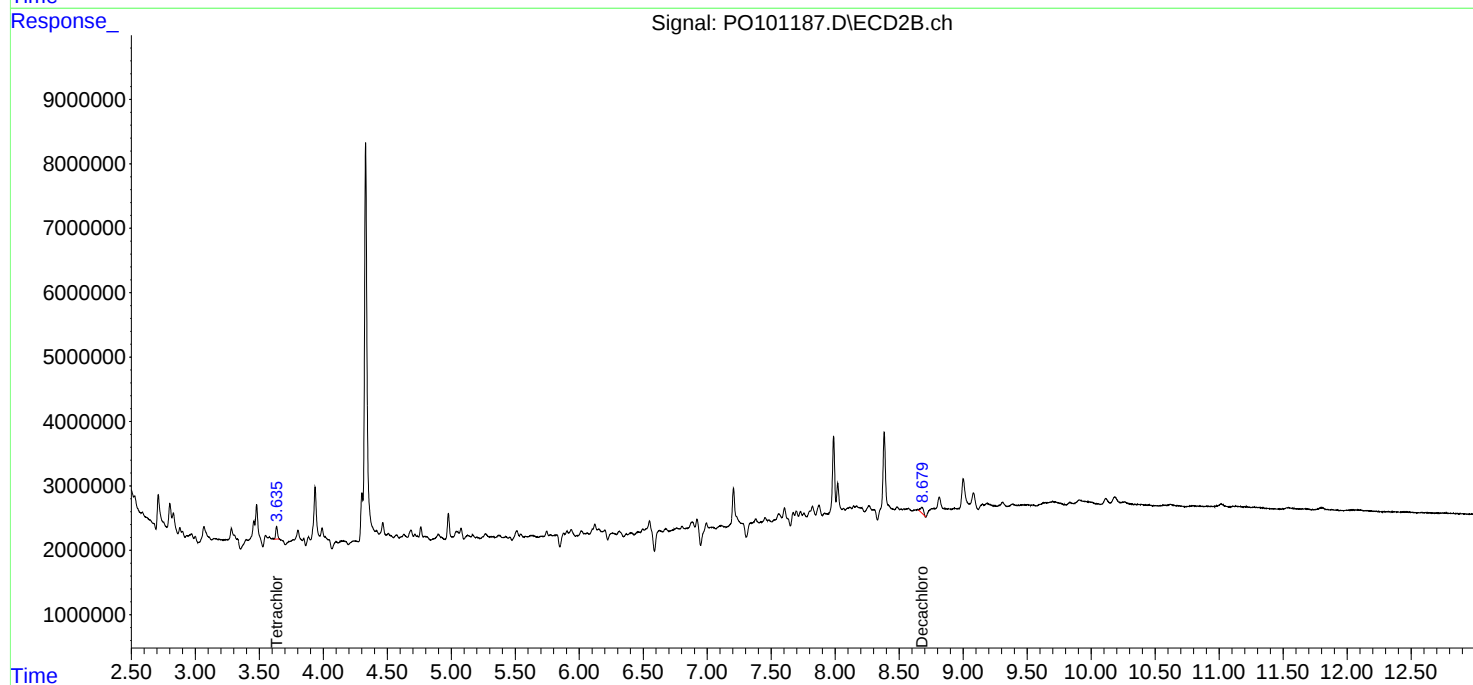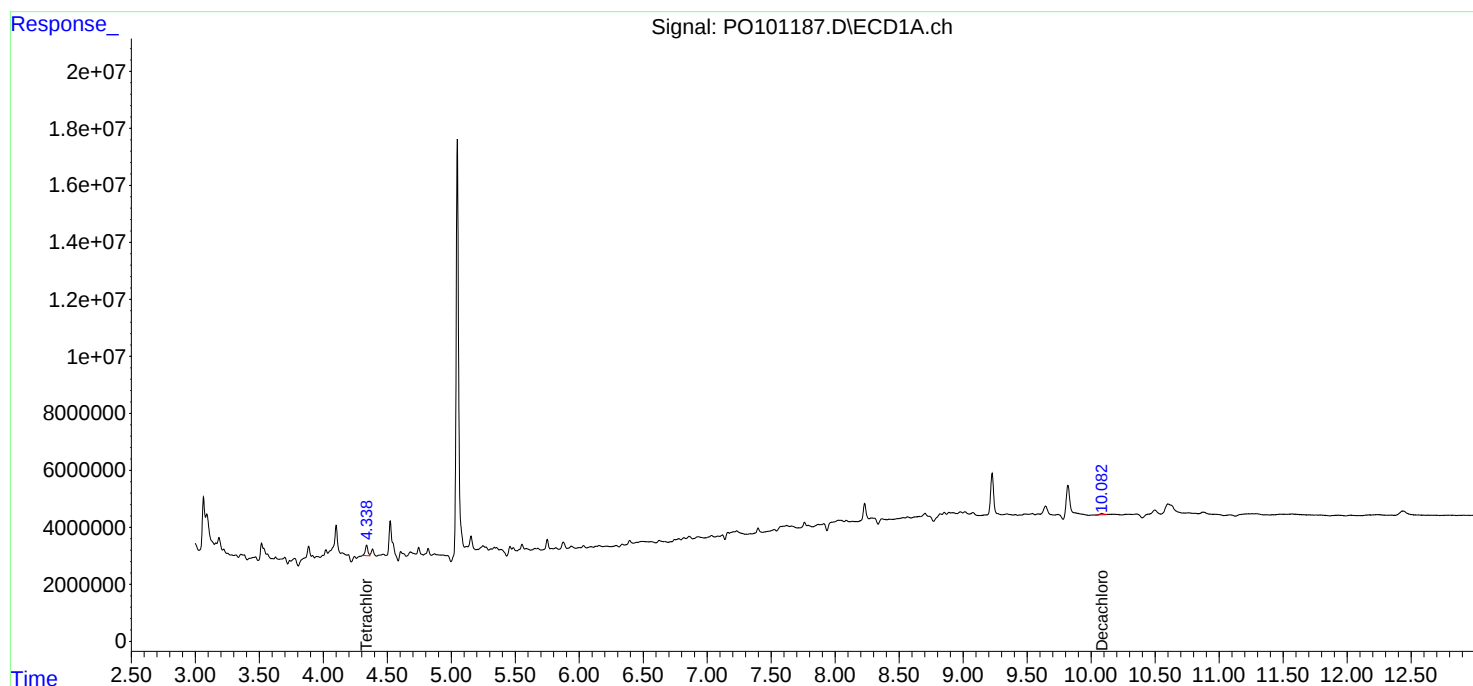

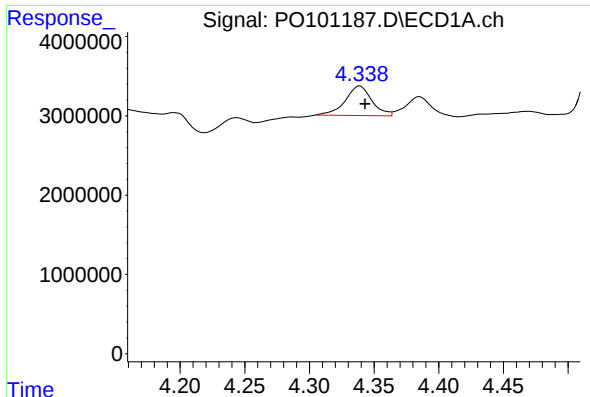


#1 Tetrachloro-m-xylene

R.T.: 4.339 min
Delta R.T.: -0.004 min
Response: 5335112
Conc: 1.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
LS-3RE


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/16/2024
Supervised By :Sohil Jodhani 01/16/2024

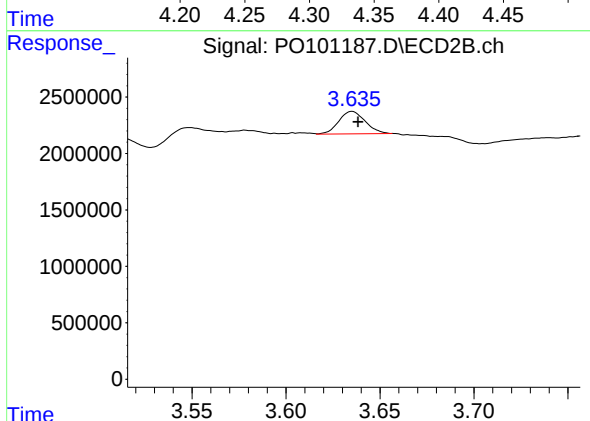


#1 Tetrachloro-m-xylene

R.T.: 3.635 min
Delta R.T.: -0.003 min
Response: 1951236
Conc: 0.74 ng/ml m

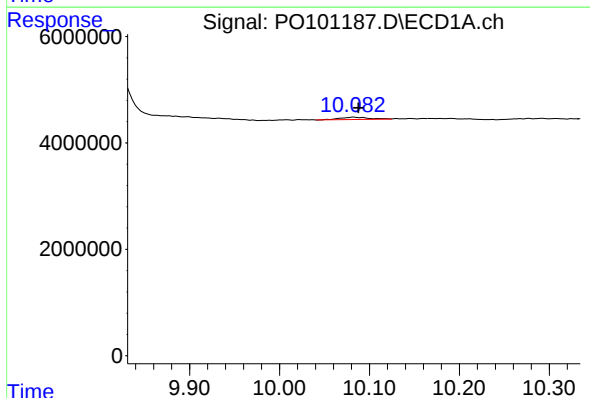

#2 Decachlorobiphenyl

R.T.: 10.082 min
Delta R.T.: -0.006 min
Response: 953515
Conc: 0.48 ng/ml

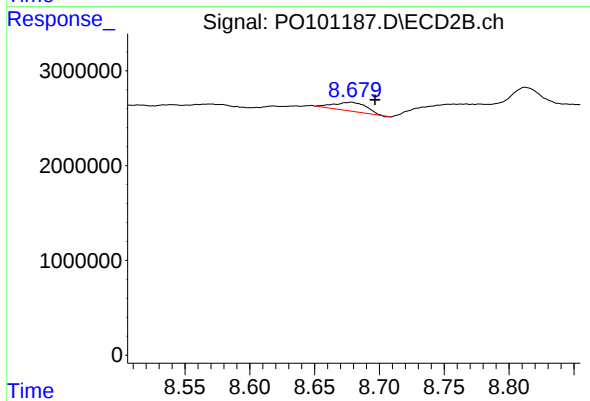

#2 Decachlorobiphenyl

R.T.: 8.678 min
Delta R.T.: -0.018 min
Response: 1612012
Conc: 0.98 ng/ml