

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011524\
 Data File : P0101193.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jan 2024 22:03
 Operator : YP/AJ
 Sample : PB158455BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB158455BL

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/16/2024
 Supervised By :Sohil Jodhani 01/16/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 16 00:09:02 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 11 11:52:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.341	3.637	92958374	57980534	22.949	21.994
2) SA Decachlor...	10.079	8.689	56891781	45053112	28.805m	27.280

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011524\
Data File : PO101193.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jan 2024 22:03
Operator : YP/AJ
Sample : PB158455BL
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB158455BL


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/16/2024
Supervised By :Sohil Jodhani 01/16/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 16 00:09:02 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011024.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 11 11:52:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

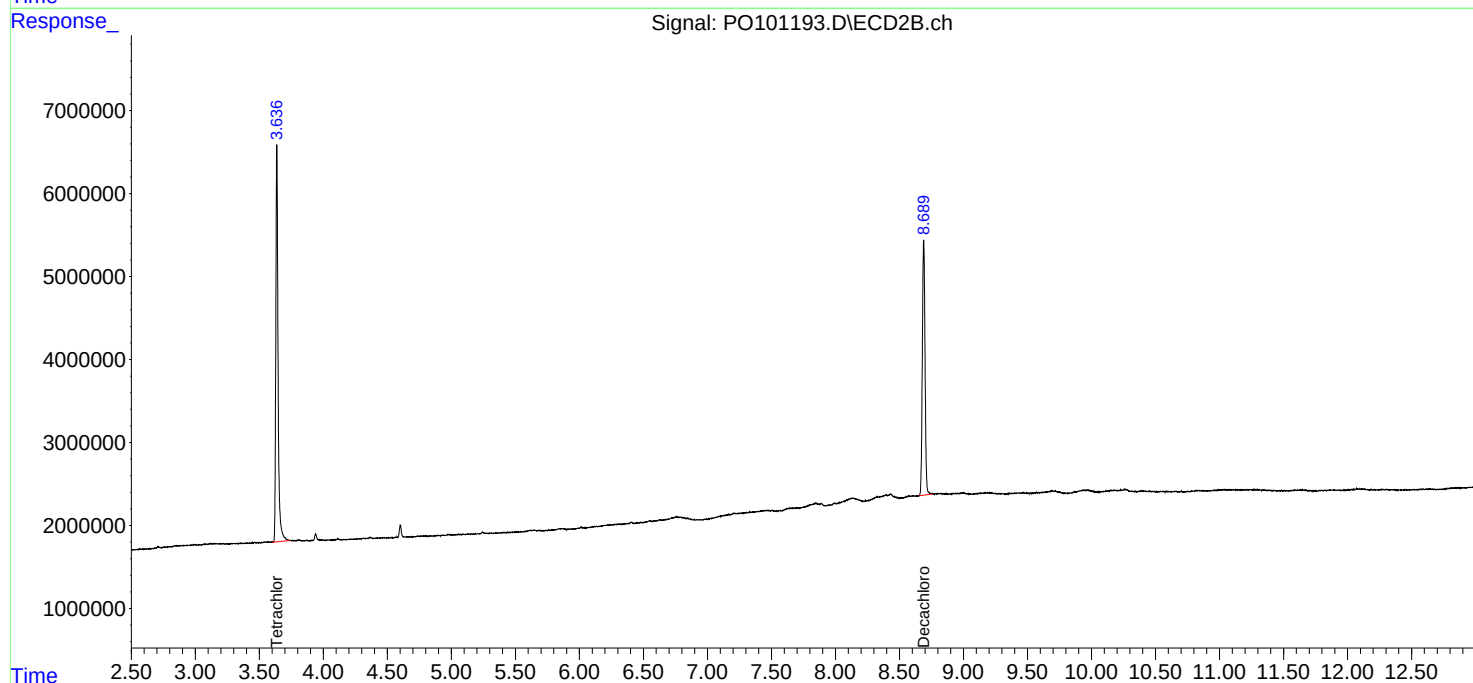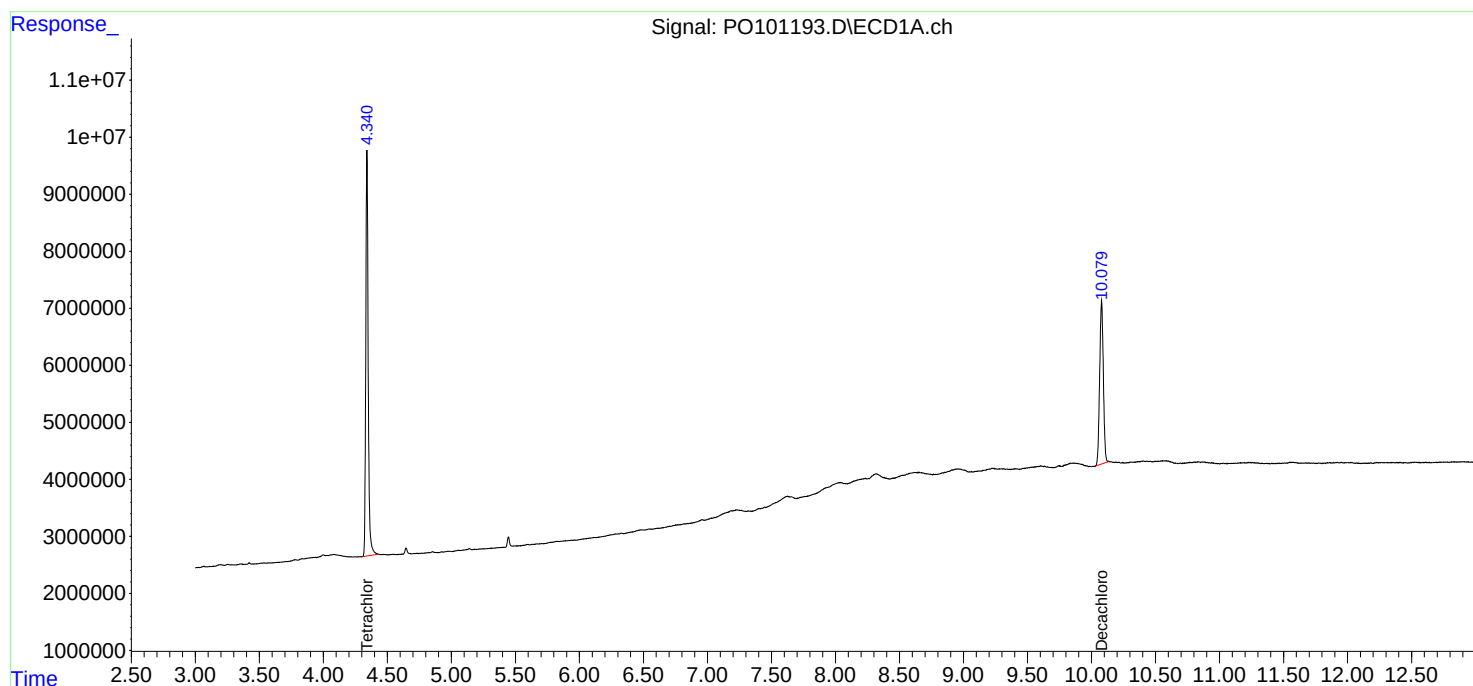

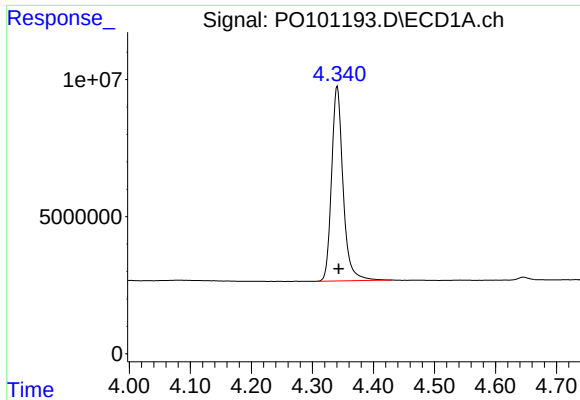


#1 Tetrachloro-m-xylene

R.T.: 4.341 min
Delta R.T.: -0.002 min
Response: 92958374
Conc: 22.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB158455BL


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/16/2024
Supervised By :Sohil Jodhani 01/16/2024

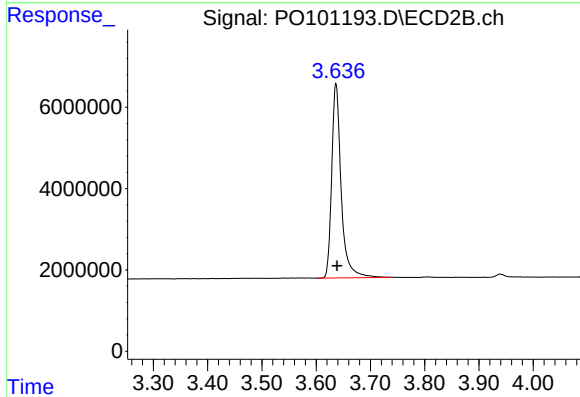


#1 Tetrachloro-m-xylene

R.T.: 3.637 min
Delta R.T.: -0.002 min
Response: 57980534
Conc: 21.99 ng/ml

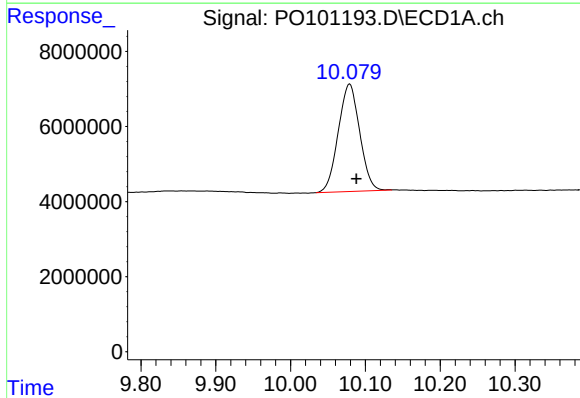

#2 Decachlorobiphenyl

R.T.: 10.079 min
Delta R.T.: -0.009 min
Response: 56891781
Conc: 28.81 ng/ml m

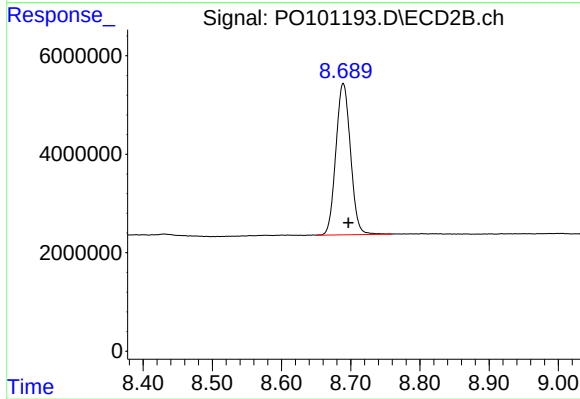

#2 Decachlorobiphenyl

R.T.: 8.689 min
Delta R.T.: -0.007 min
Response: 45053112
Conc: 27.28 ng/ml