

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011524\
 Data File : P0101196.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jan 2024 22:54
 Operator : YP/AJ
 Sample : P1133-01 10X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TOTE-6579

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/16/2024
 Supervised By :Sohil Jodhani 01/16/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 16 00:11:10 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 11 11:52:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.343	3.643	3953843	2230366	0.976	0.846
2) SA Decachlor...	10.079	8.690	4449570	3199841	2.253	1.938m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011524\
Data File : PO101196.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jan 2024 22:54
Operator : YP/AJ
Sample : P1133-01 10X
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TOTE-6579


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/16/2024
Supervised By :Sohil Jodhani 01/16/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 16 00:11:10 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011024.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 11 11:52:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

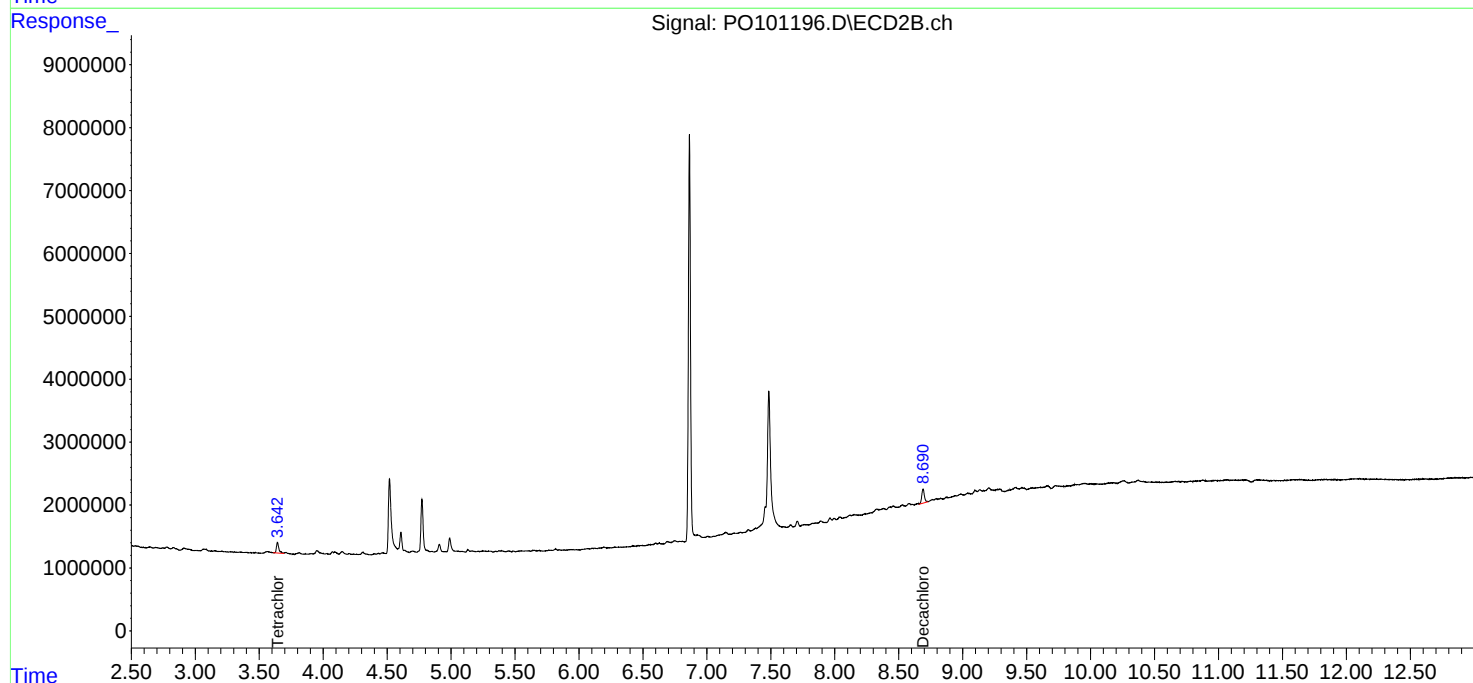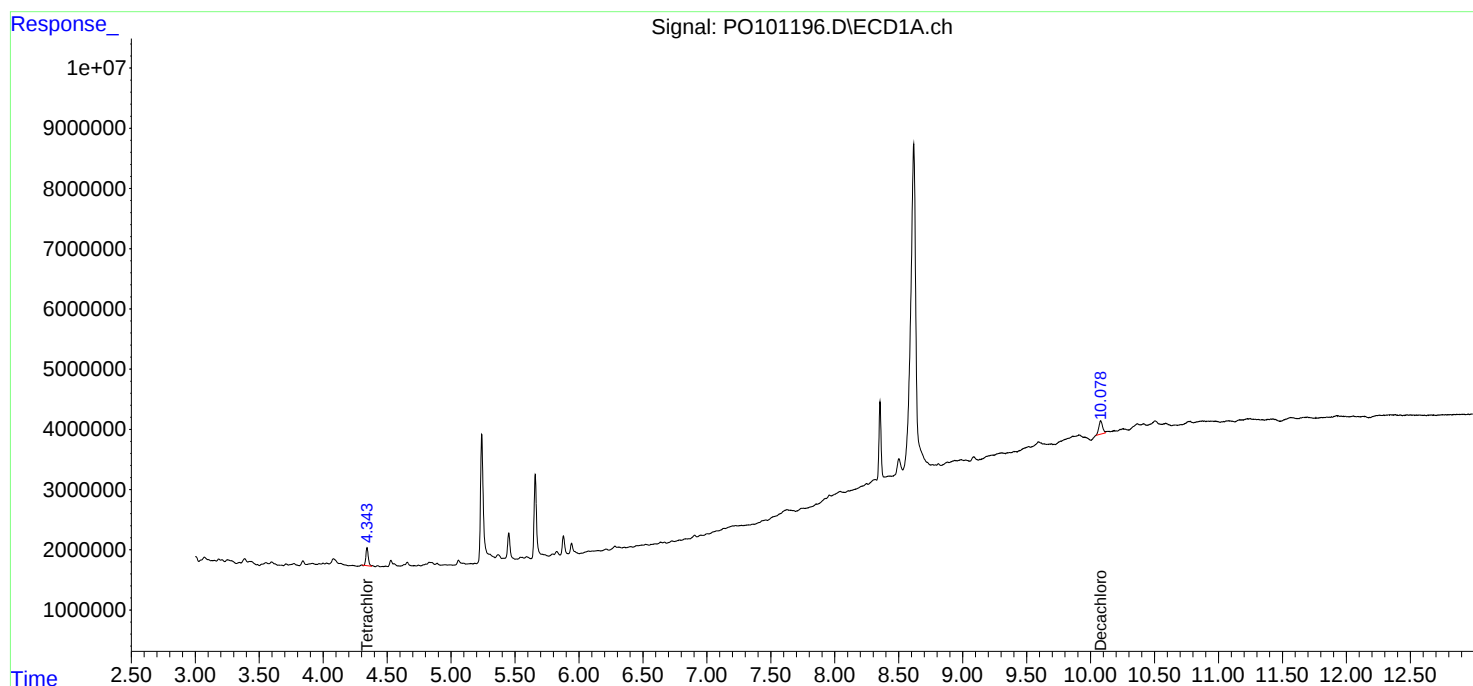

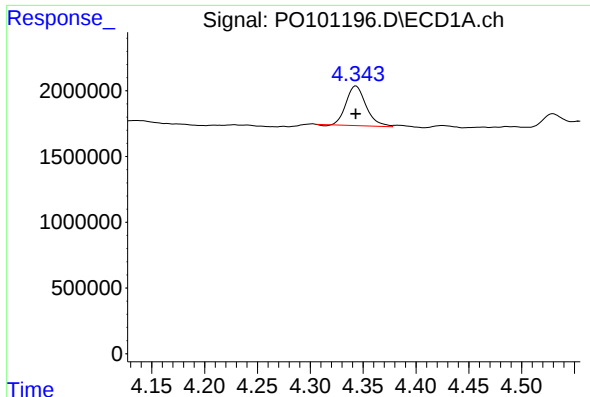


#1 Tetrachloro-m-xylene

R.T.: 4.343 min
Delta R.T.: 0.000 min
Response: 3953843
Conc: 0.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
TOTE-6579


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/16/2024
Supervised By :Sohil Jodhani 01/16/2024

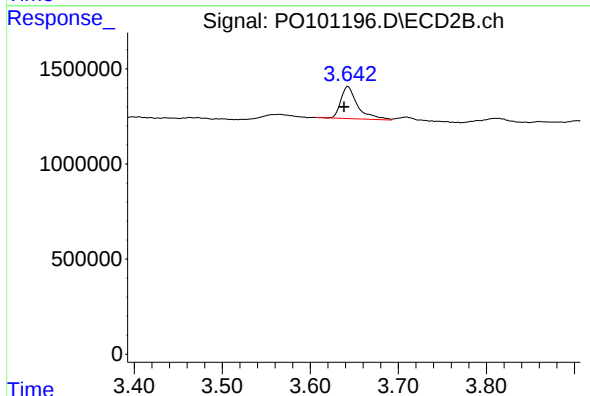


#1 Tetrachloro-m-xylene

R.T.: 3.643 min
Delta R.T.: 0.004 min
Response: 2230366
Conc: 0.85 ng/ml

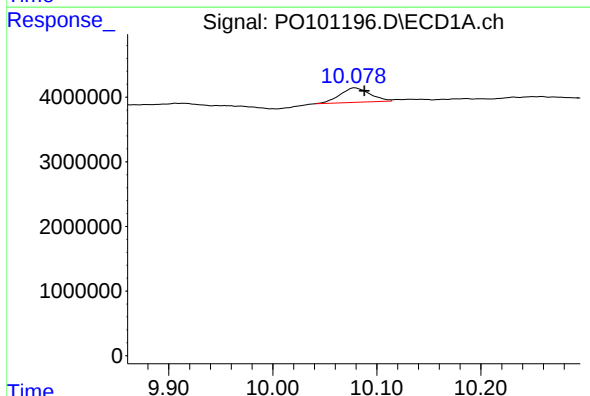

#2 Decachlorobiphenyl

R.T.: 10.079 min
Delta R.T.: -0.009 min
Response: 4449570
Conc: 2.25 ng/ml

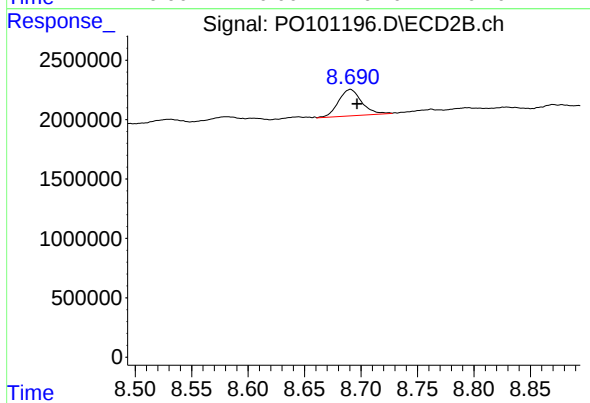

#2 Decachlorobiphenyl

R.T.: 8.690 min
Delta R.T.: -0.006 min
Response: 3199841
Conc: 1.94 ng/ml m