

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011619\
 Data File : P0053460.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Jan 2019 11:45
 Operator : SM/SJ
 Sample : K1127-01RE
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 23832RE

Manual Integrations
 APPROVED

Sohil
 1/17/2019 2:05:08 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 16 12:01:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 09 03:34:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.172	3.202	25612502	2748495	19.167m	10.992 #
2) SA Decachlor...	9.627	7.844	4000354	1087186	5.065	4.747m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011619\
Data File : P0053460.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Jan 2019 11:45
Operator : SM/SJ
Sample : K1127-01RE
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
23832RE


Manual Integrations
APPROVED

Sohil
1/17/2019 2:05:08 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 16 12:01:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010819.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 09 03:34:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

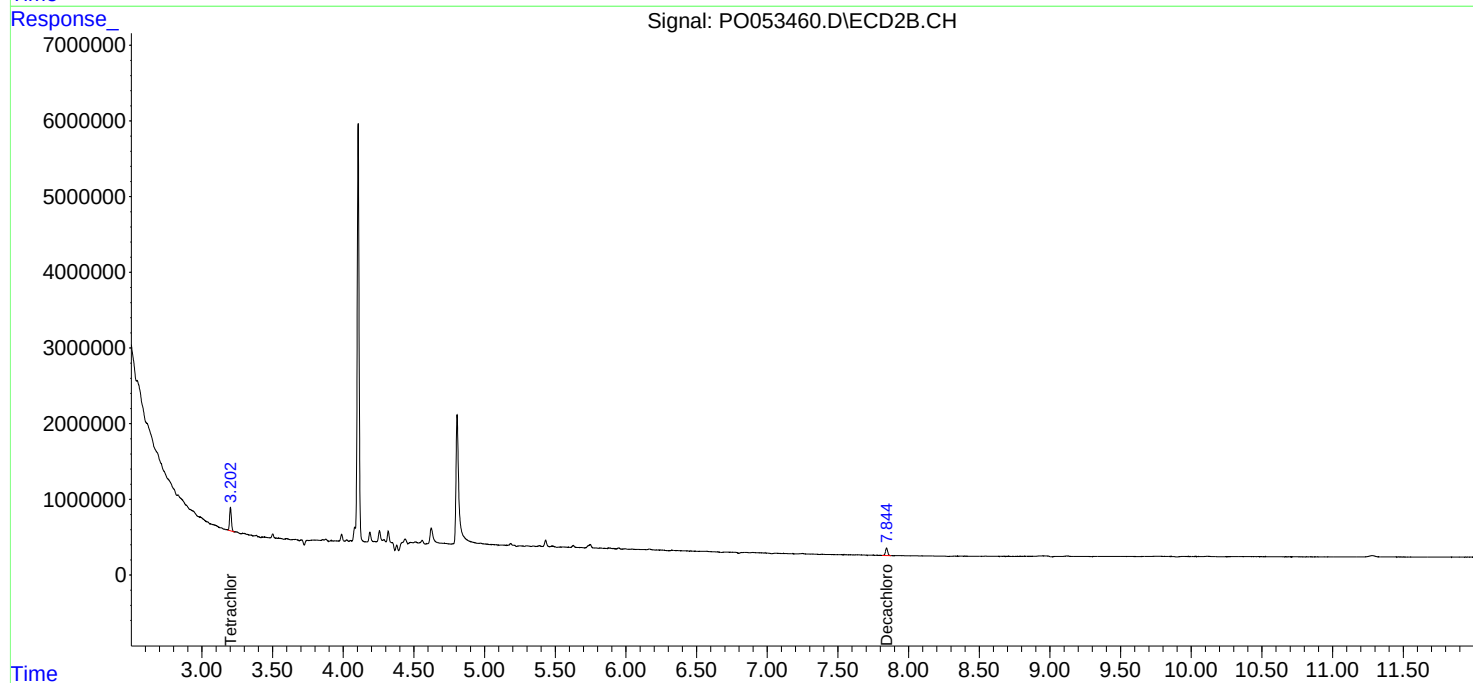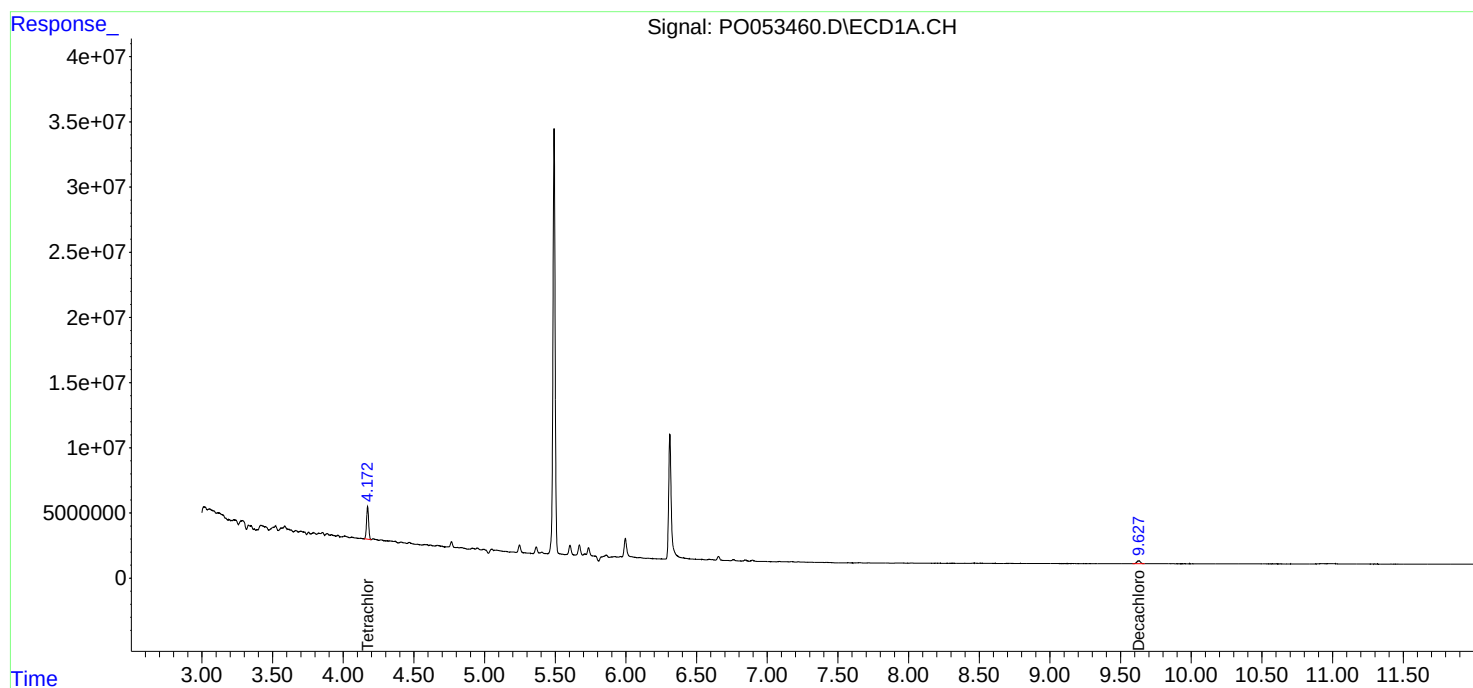

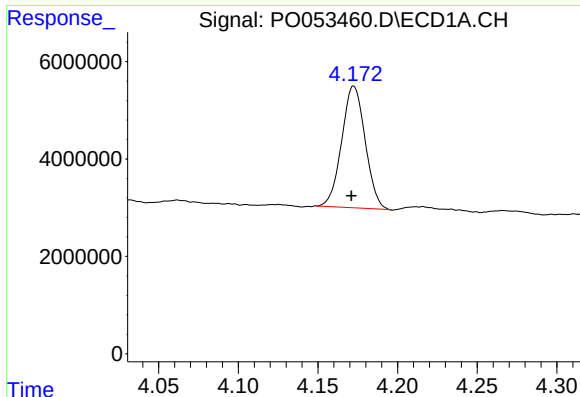


#1 Tetrachloro-m-xylene

R.T.: 4.172 min
Delta R.T.: 0.000 min
Response: 25612502
Conc: 19.17 ng/ml m

Instrument :
ECD_O
ClientSampleId :
23832RE


Manual Integrations
APPROVED

Sohil
1/17/2019 2:05:08 PM

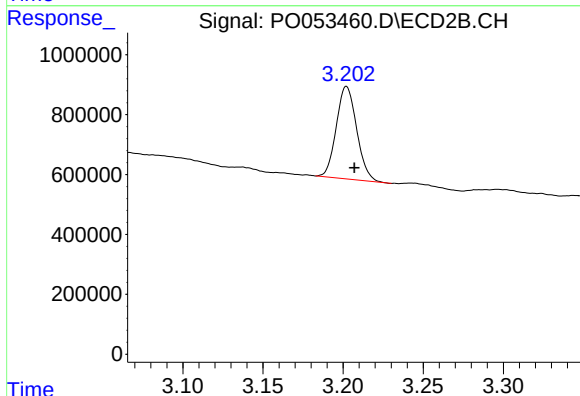


#1 Tetrachloro-m-xylene

R.T.: 3.202 min
Delta R.T.: -0.005 min
Response: 2748495
Conc: 10.99 ng/ml

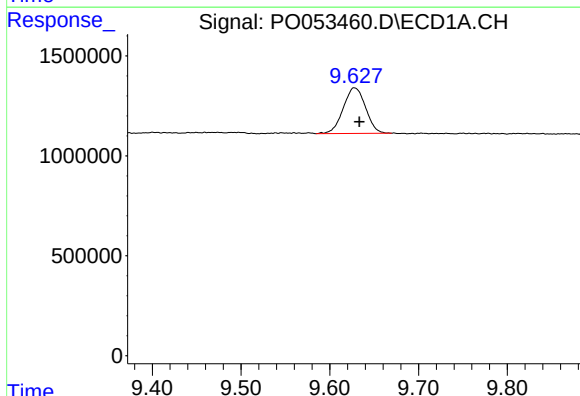

#2 Decachlorobiphenyl

R.T.: 9.627 min
Delta R.T.: -0.006 min
Response: 4000354
Conc: 5.06 ng/ml

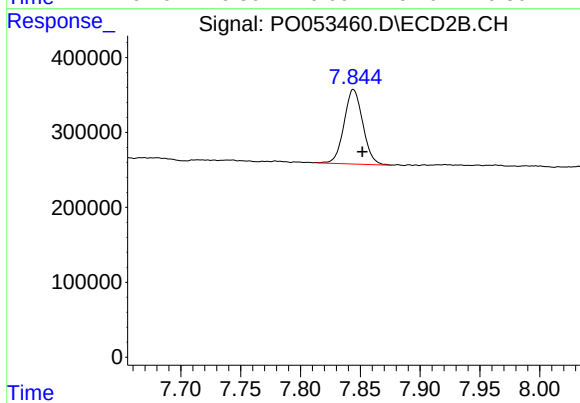

#2 Decachlorobiphenyl

R.T.: 7.844 min
Delta R.T.: -0.008 min
Response: 1087186
Conc: 4.75 ng/ml m